
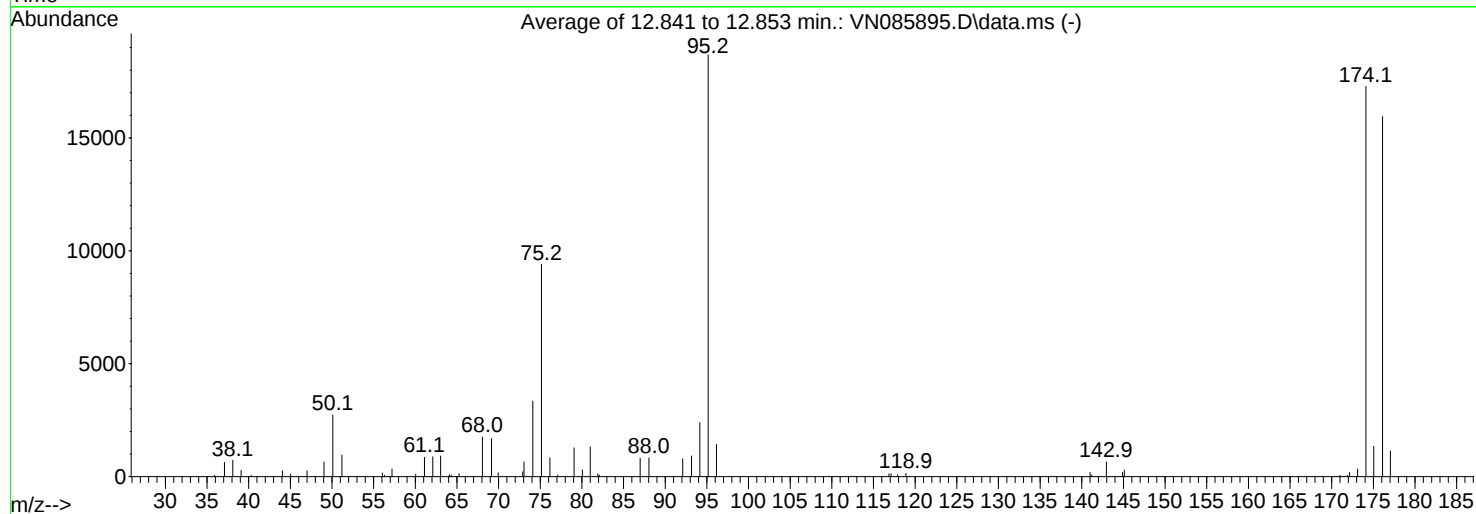


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030625\
Data File : VN085895.D
Acq On : 06 Mar 2025 11:02
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Title : SW846 8260
Last Update : Wed Feb 19 03:43:32 2025

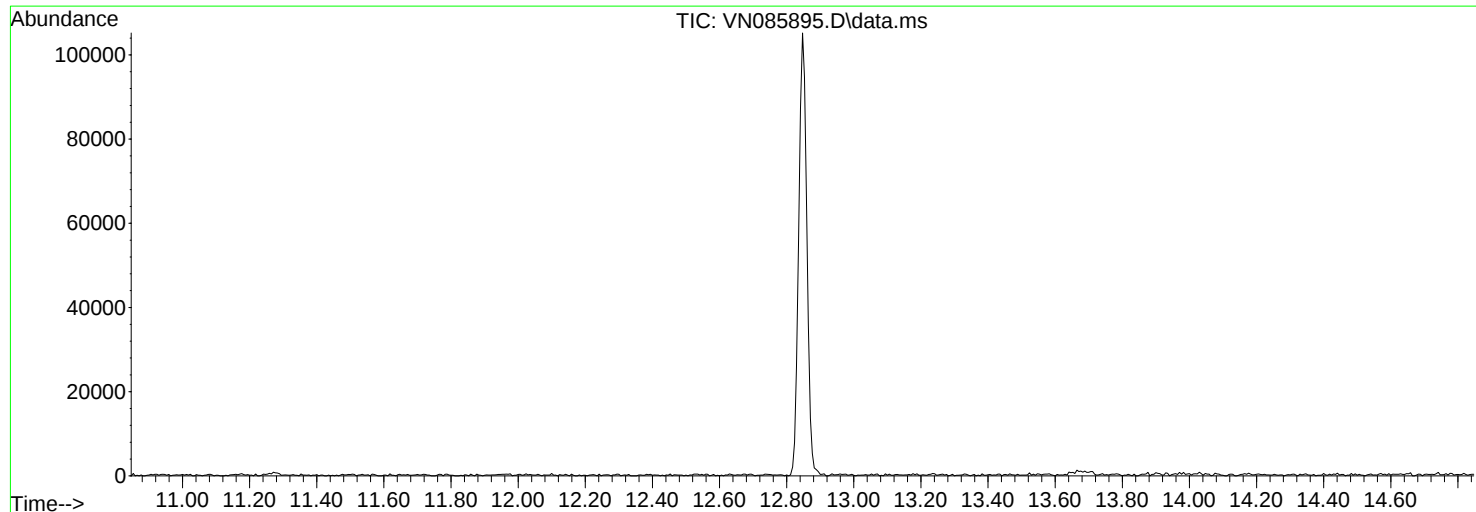

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	14.6	2731	FAIL*
75	95	30	60	50.3	9394	PASS
95	95	100	100	100.0	18678	PASS
96	95	5	9	7.6	1424	PASS
173	174	0.00	2	2.0	339	PASS
174	95	50	100	92.5	17280	PASS
175	174	5	9	7.7	1337	PASS
176	174	95	101	92.2	15939	FAIL*
177	176	5	9	7.2	1141	PASS

Average of 12.841 to 12.853 min.: VN085895.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	54	56.05	163	69.15	1685	81.90	111
37.10	638	56.30	56	69.95	170	82.10	64
38.10	721	57.20	336	72.90	211	87.00	81
39.10	278	60.05	108	73.05	654	88.05	82
40.30	55	61.10	855	74.10	3346	92.10	794
44.05	262	62.10	882	75.15	9394	93.15	915
45.05	120	63.05	915	76.15	827	94.15	2395
47.00	265	64.10	75	77.10	69	95.15	18678
49.05	643	64.30	73	79.05	1275	96.15	1424
50.10	2731	65.25	138	80.05	300	116.85	130
51.20	960	68.05	1748	81.00	1318	117.10	126

Average of 12.841 to 12.853 min.: VN085895.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
117.90	79	174.10	17280				
118.90	149	175.05	1337				
141.00	182	176.10	15939				
141.20	73	177.05	1141				
142.95	655						
144.90	182						
145.10	287						
171.00	62						
171.90	51						
172.15	185						
173.10	339						

Instrument :

MSVOA_N

ClientSampleId :

BFB