


Chloromethane

Response Ratio

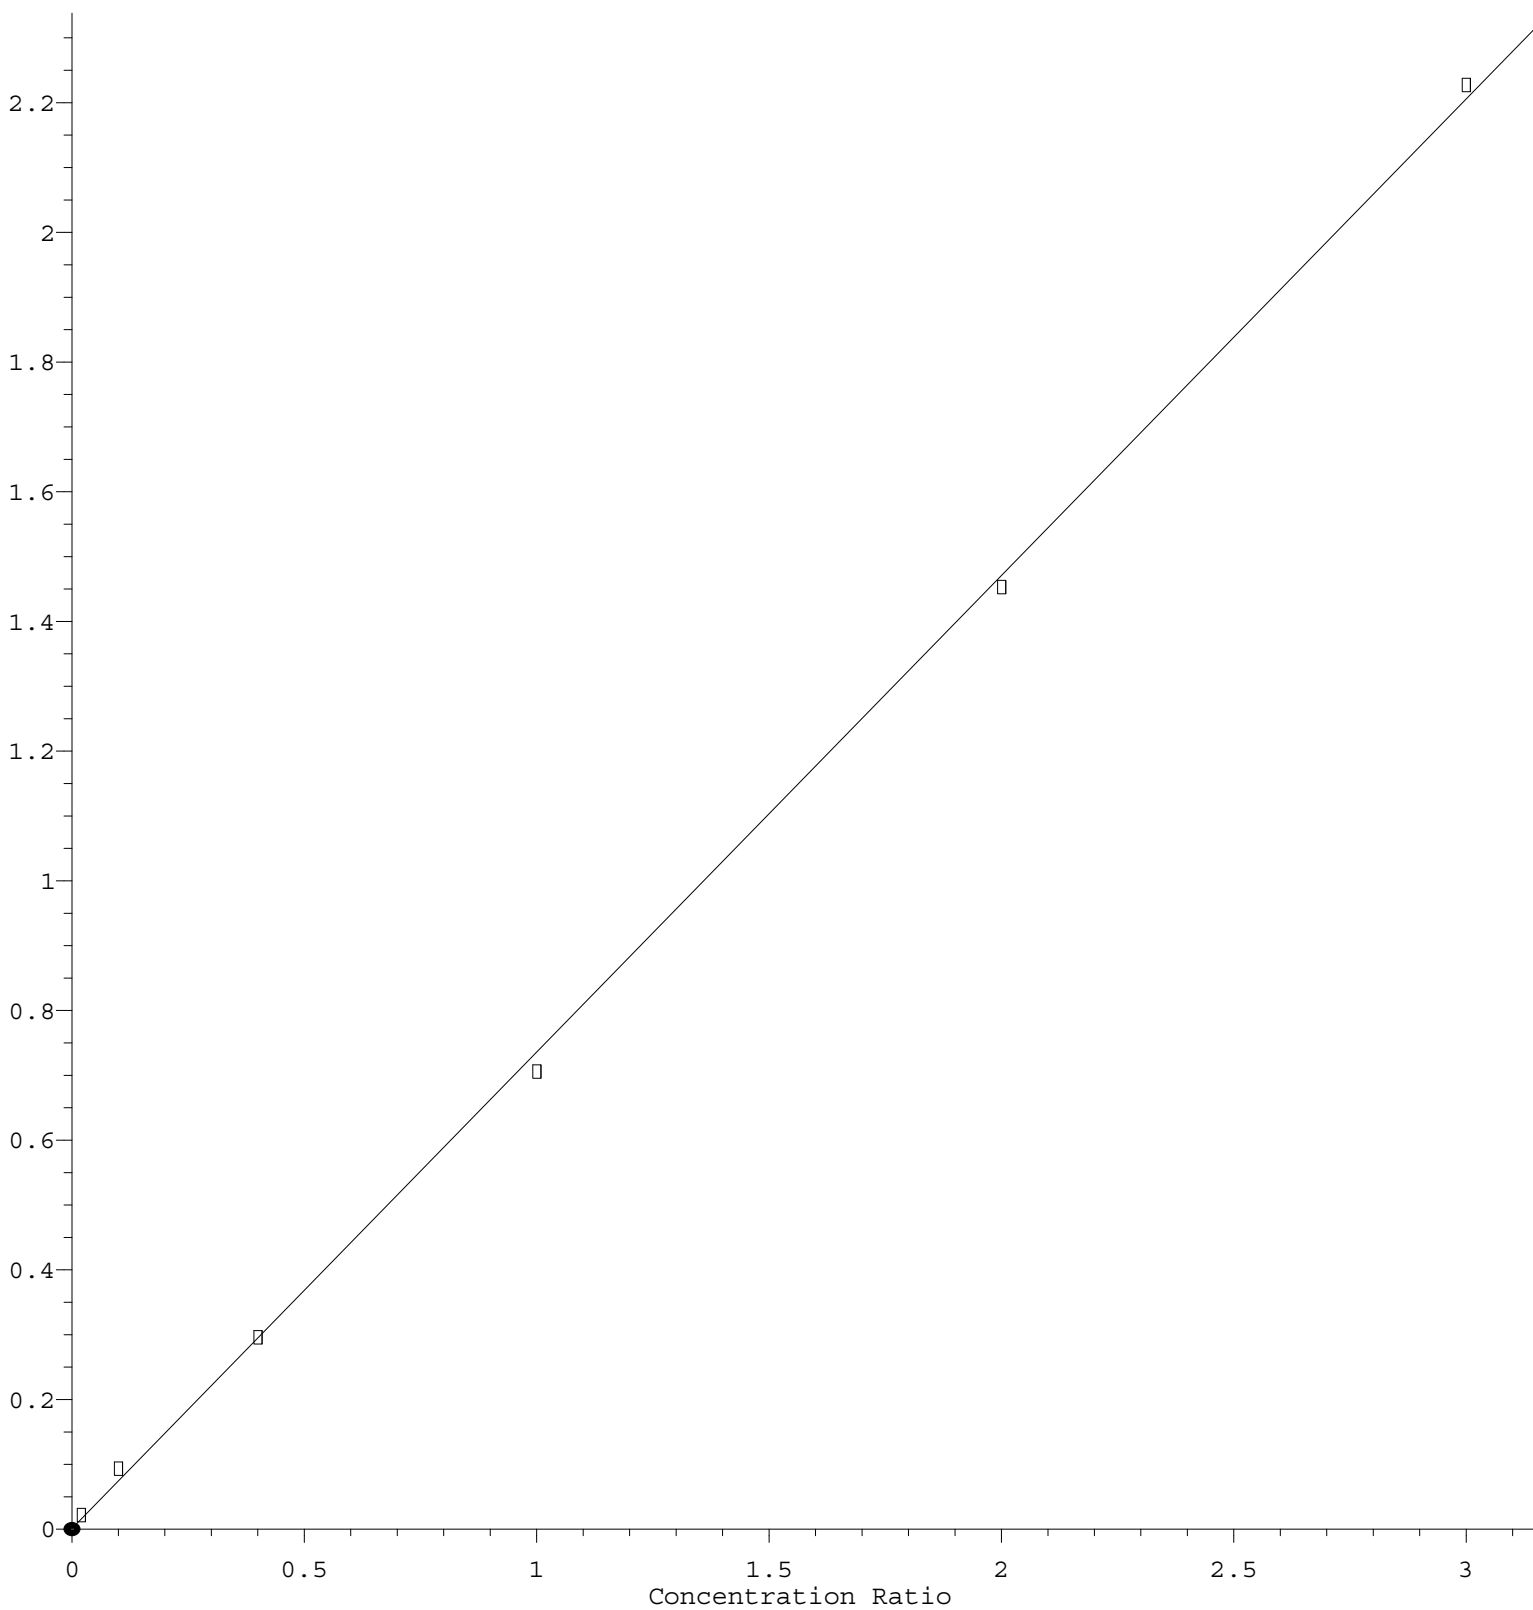


$$\text{Response} = 7.352\text{e-}001 * \text{Amt} + 5.091\text{e-}004$$

Coef of Det (r^2) = 0.999455 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N030722W.M

Calibration Table Last Updated: Tue Mar 08 06:52:46 2022


Bromomethane

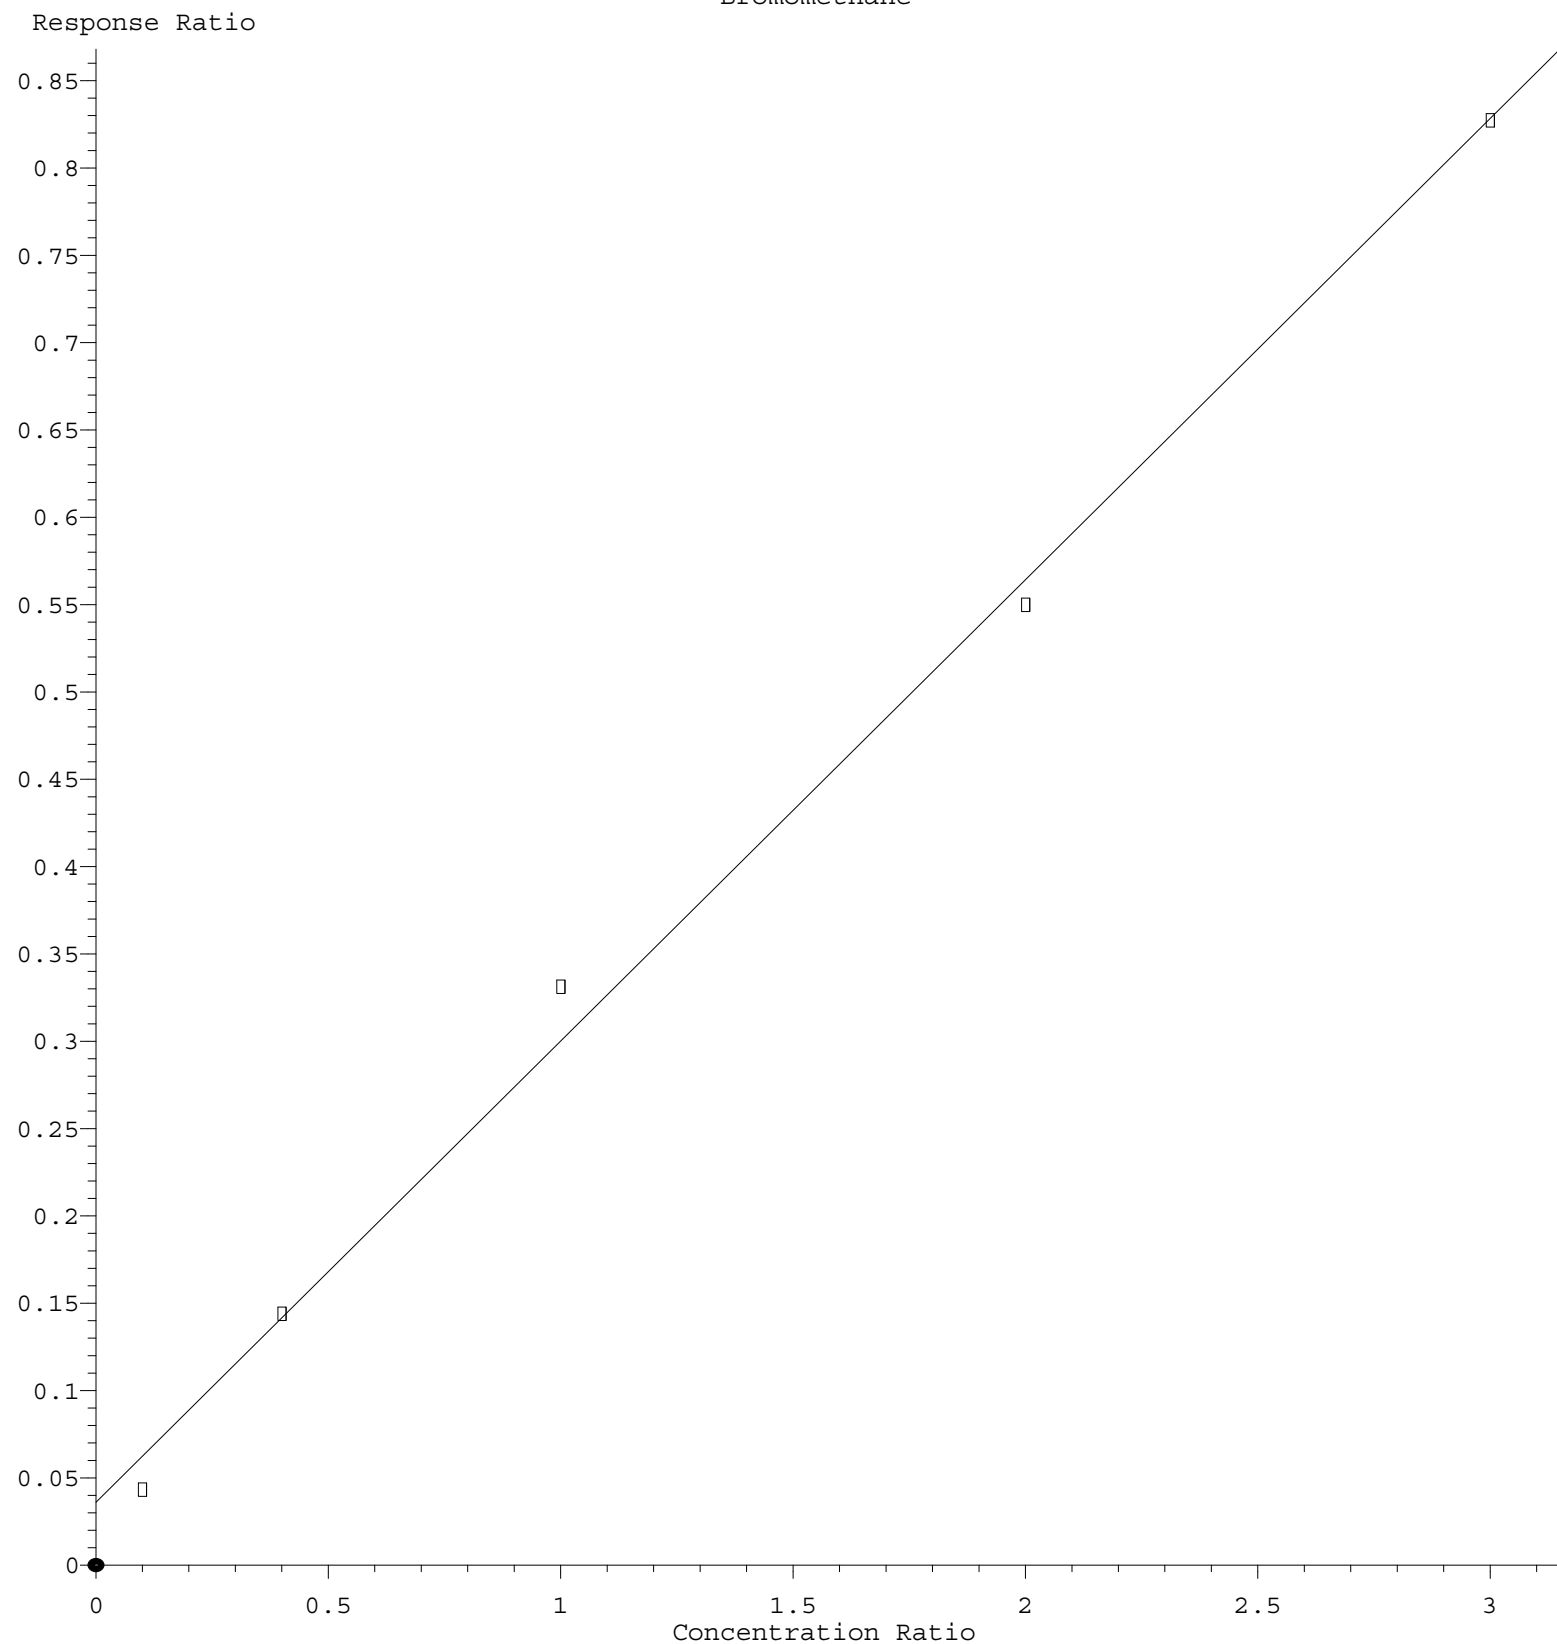

Response = 2.640e-001 * Amt + 3.584e-002
 Coef of Det (r^2) = 0.996140 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N030722W.M
 Calibration Table Last Updated: Tue Mar 08 06:52:46 2022

Methyl Acetate

Response Ratio

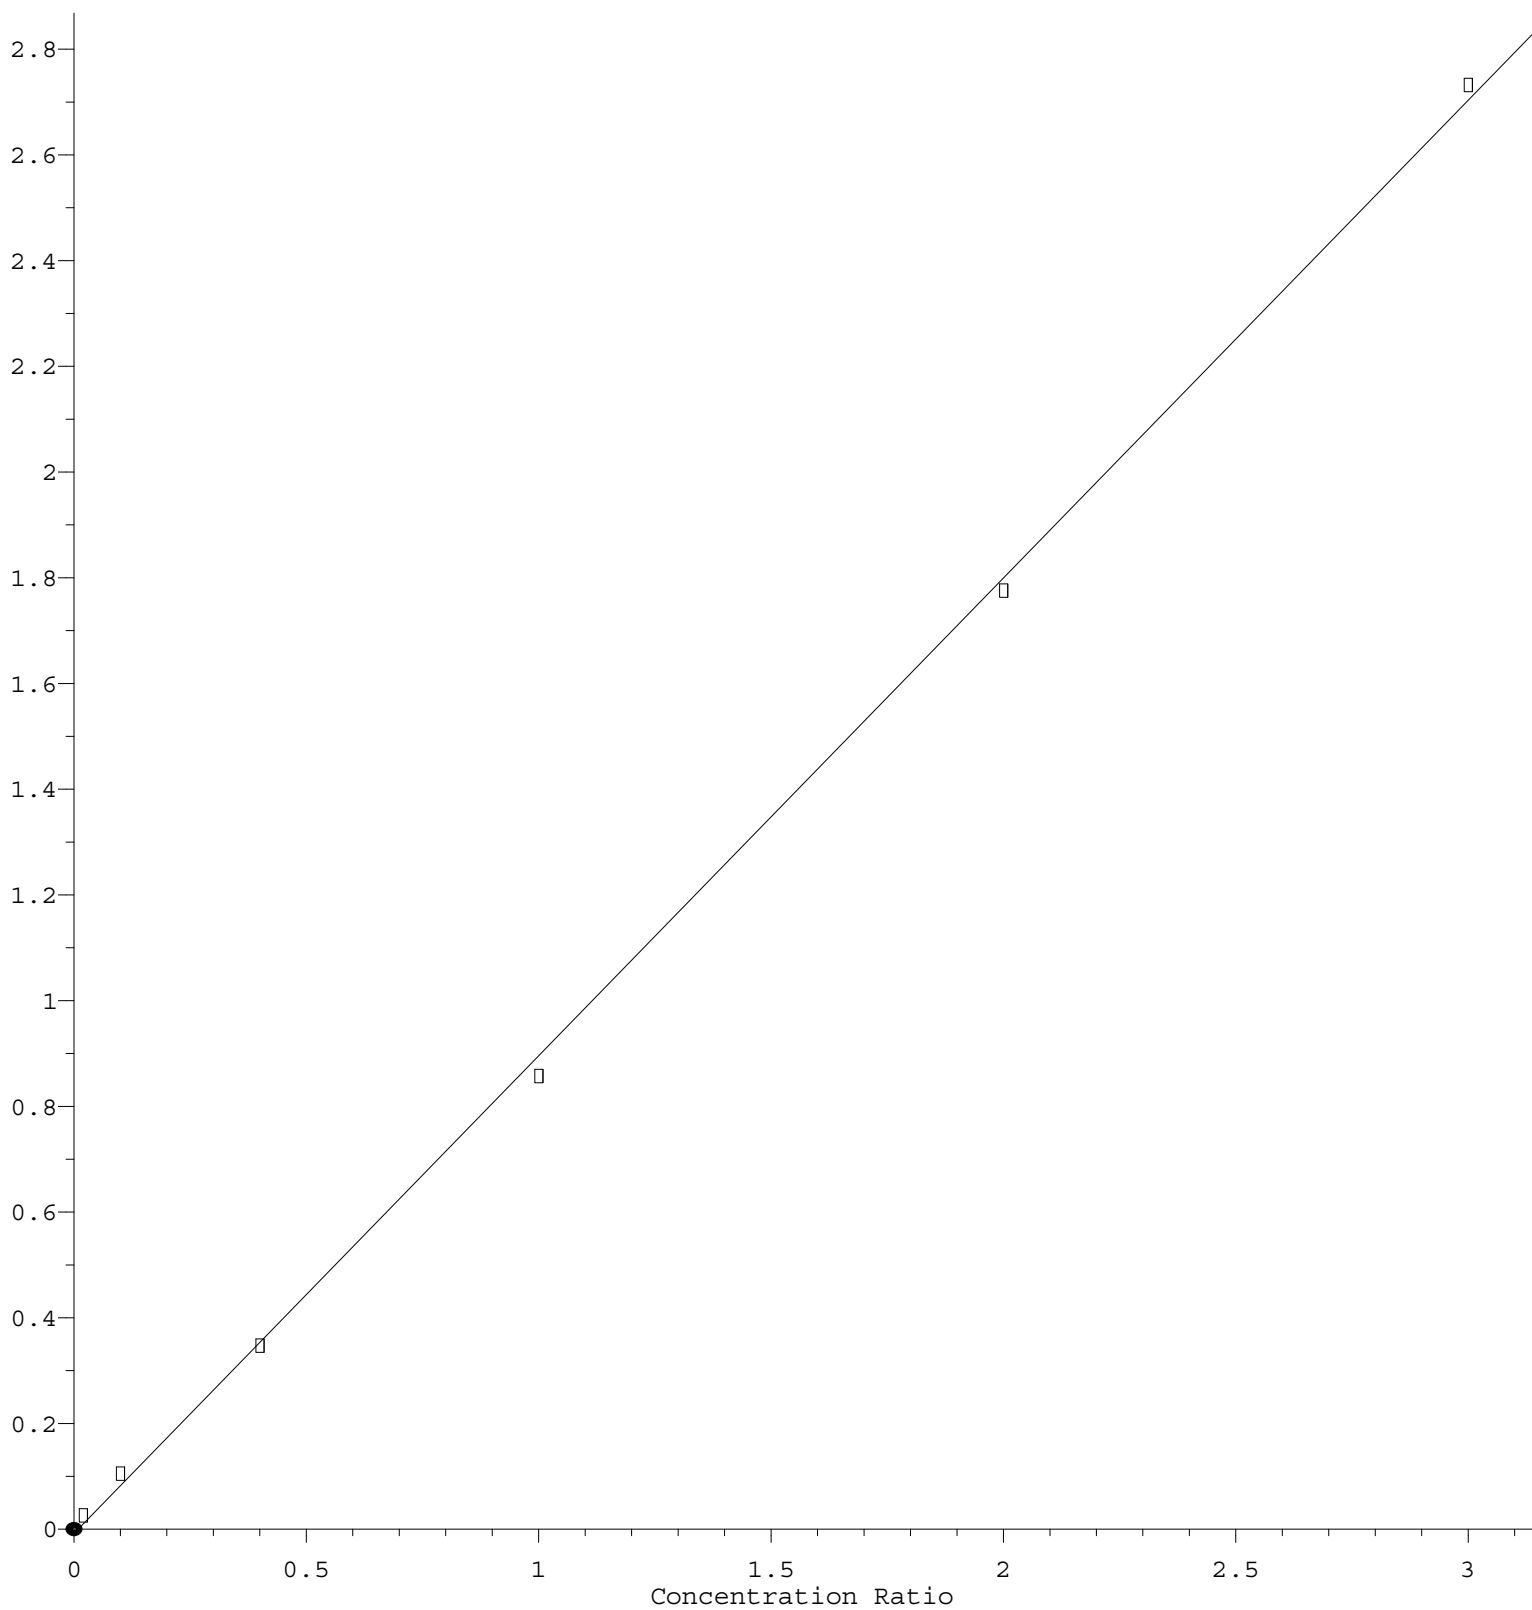

$$\text{Response} = 9.040\text{e-}001 * \text{Amt} - 8.498\text{e-}003$$


Coef of Det (r^2) = 0.999361 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N030722W.M

Calibration Table Last Updated: Tue Mar 08 06:52:46 2022

Methylene Chloride

Response Ratio

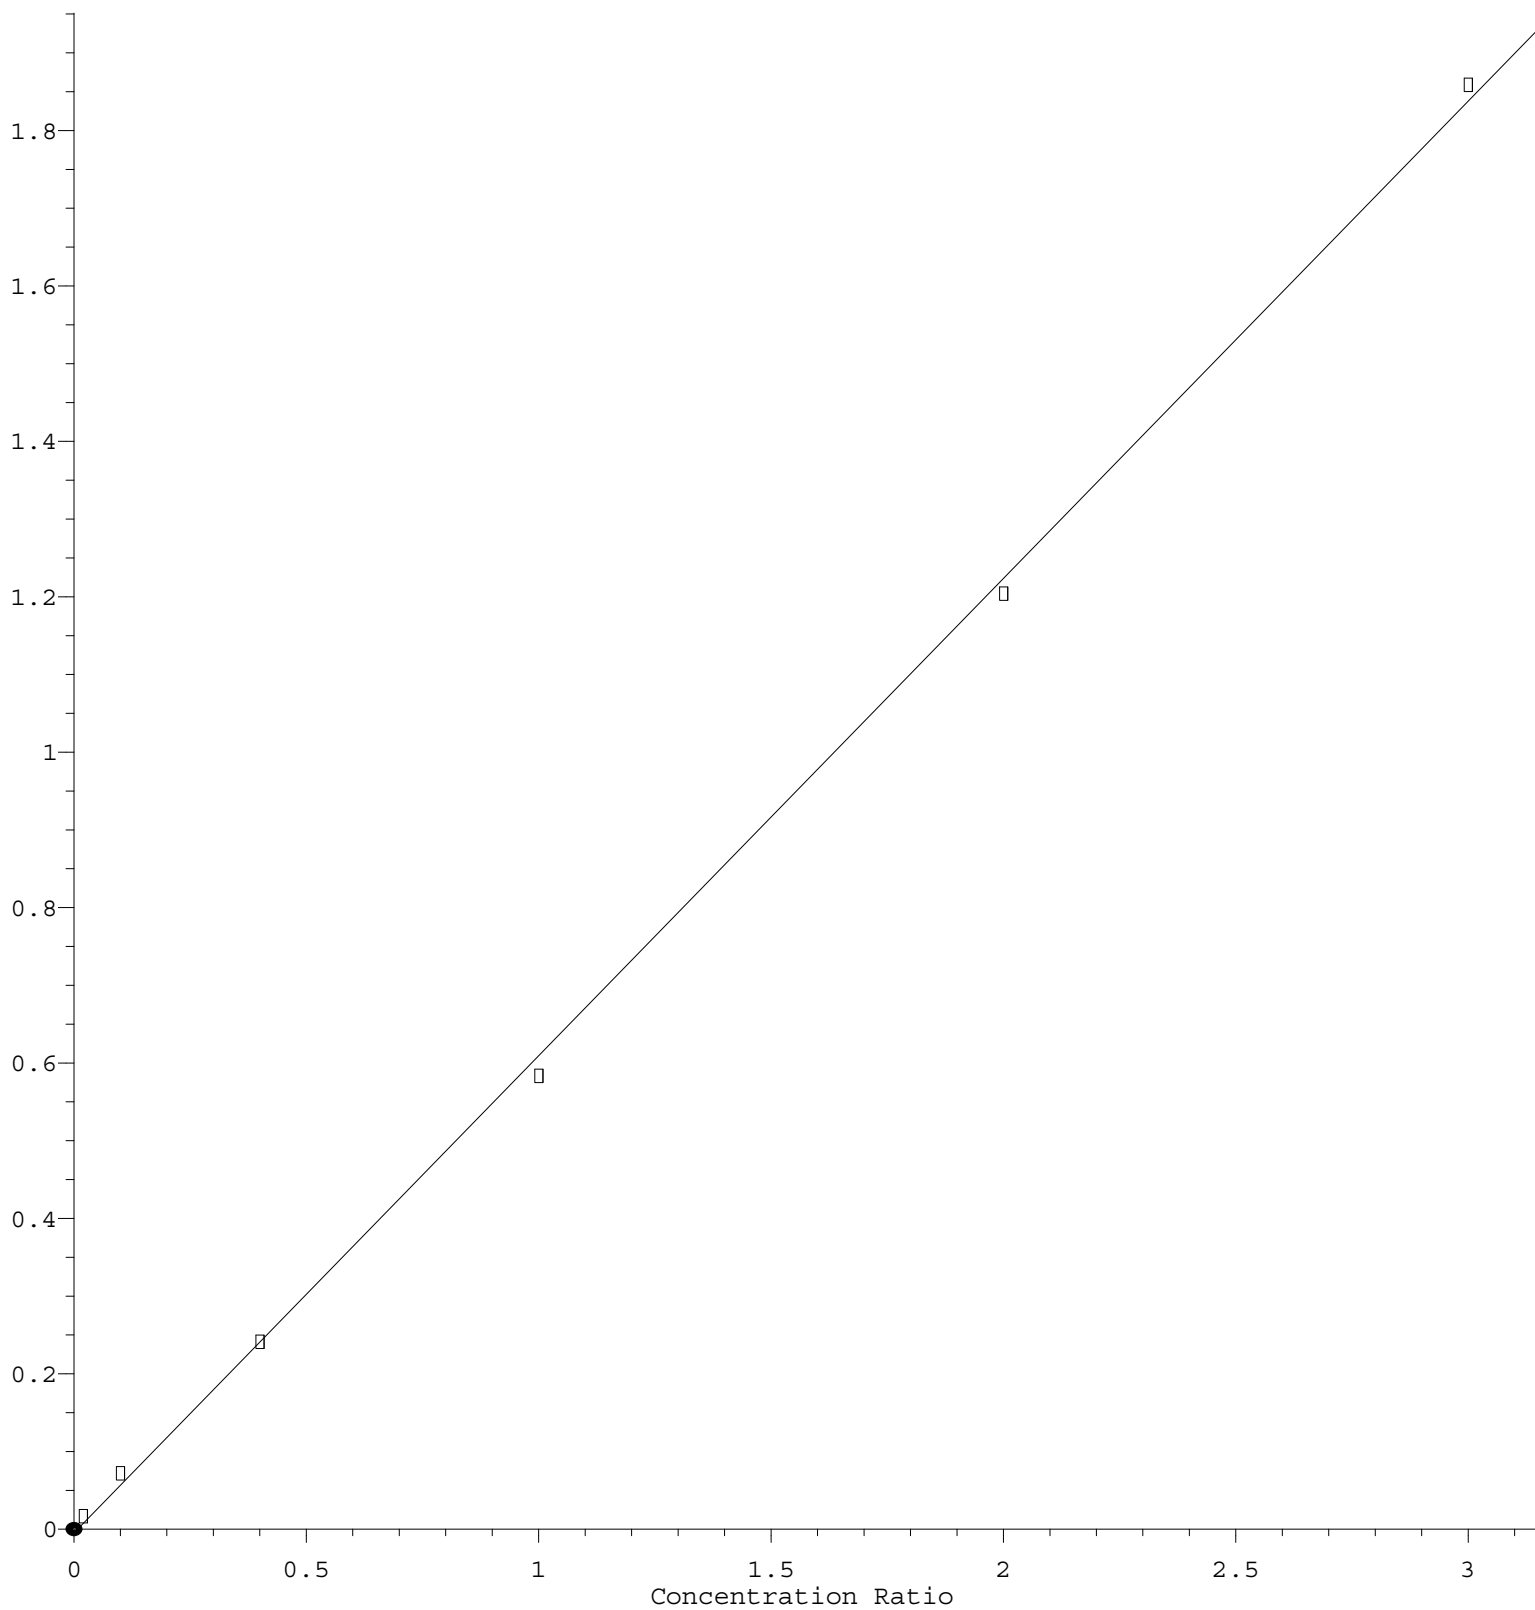

$$\text{Response} = 6.141\text{e-}001 * \text{Amt} - 4.690\text{e-}003$$


Coef of Det (r^2) = 0.999317 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N030722W.M

Calibration Table Last Updated: Tue Mar 08 06:52:46 2022

2-Chloroethyl Vinyl ether


Response Ratio

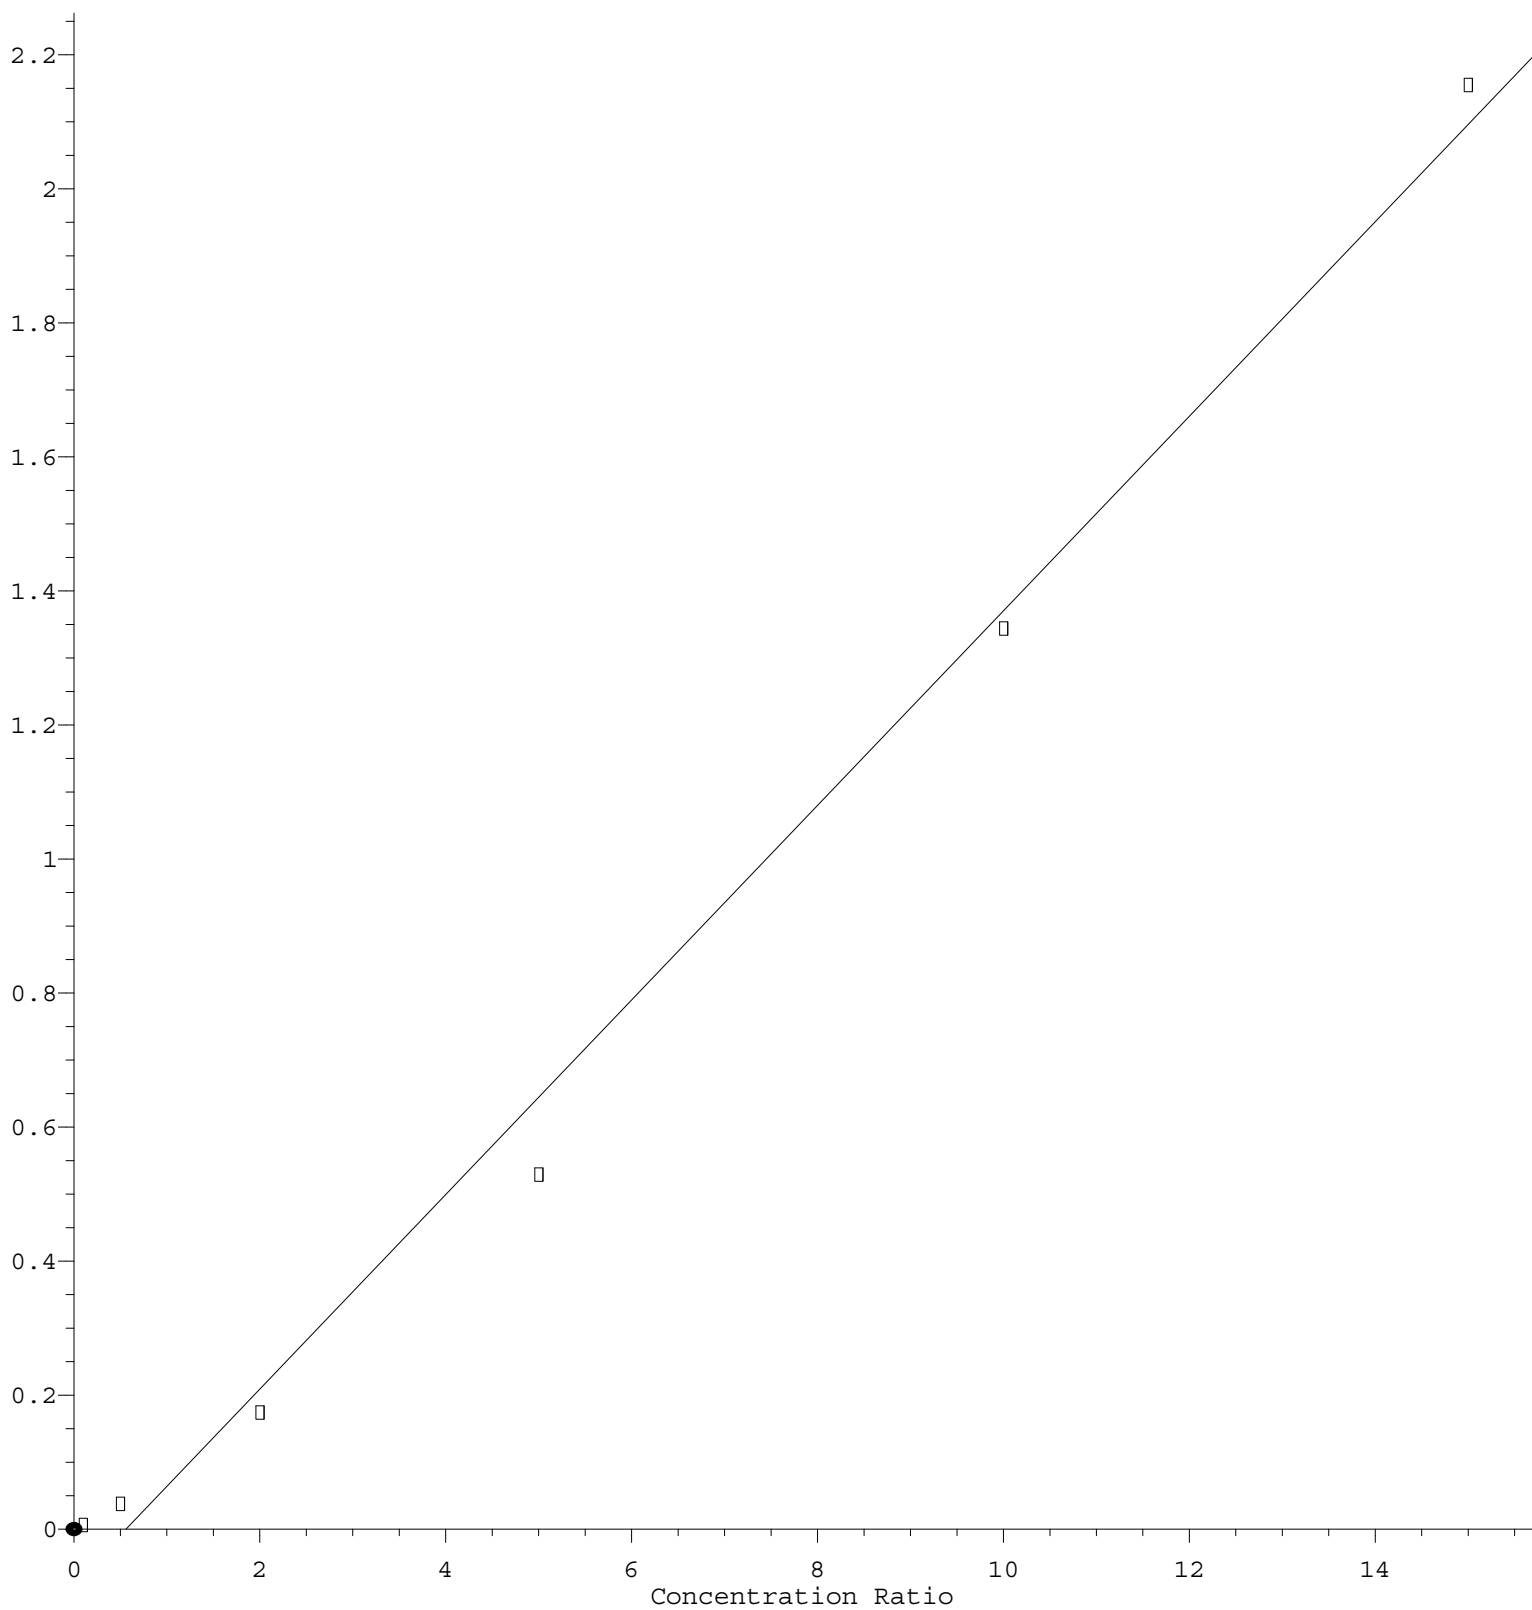

Response = $1.451\text{e-}001 * \text{Amt} - 8.088\text{e-}002$
Coef of Det (r^2) = 0.993037 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N030722W.M
Calibration Table Last Updated: Tue Mar 08 06:52:46 2022

1,1,2,2-Tetrachloroethane

Response Ratio

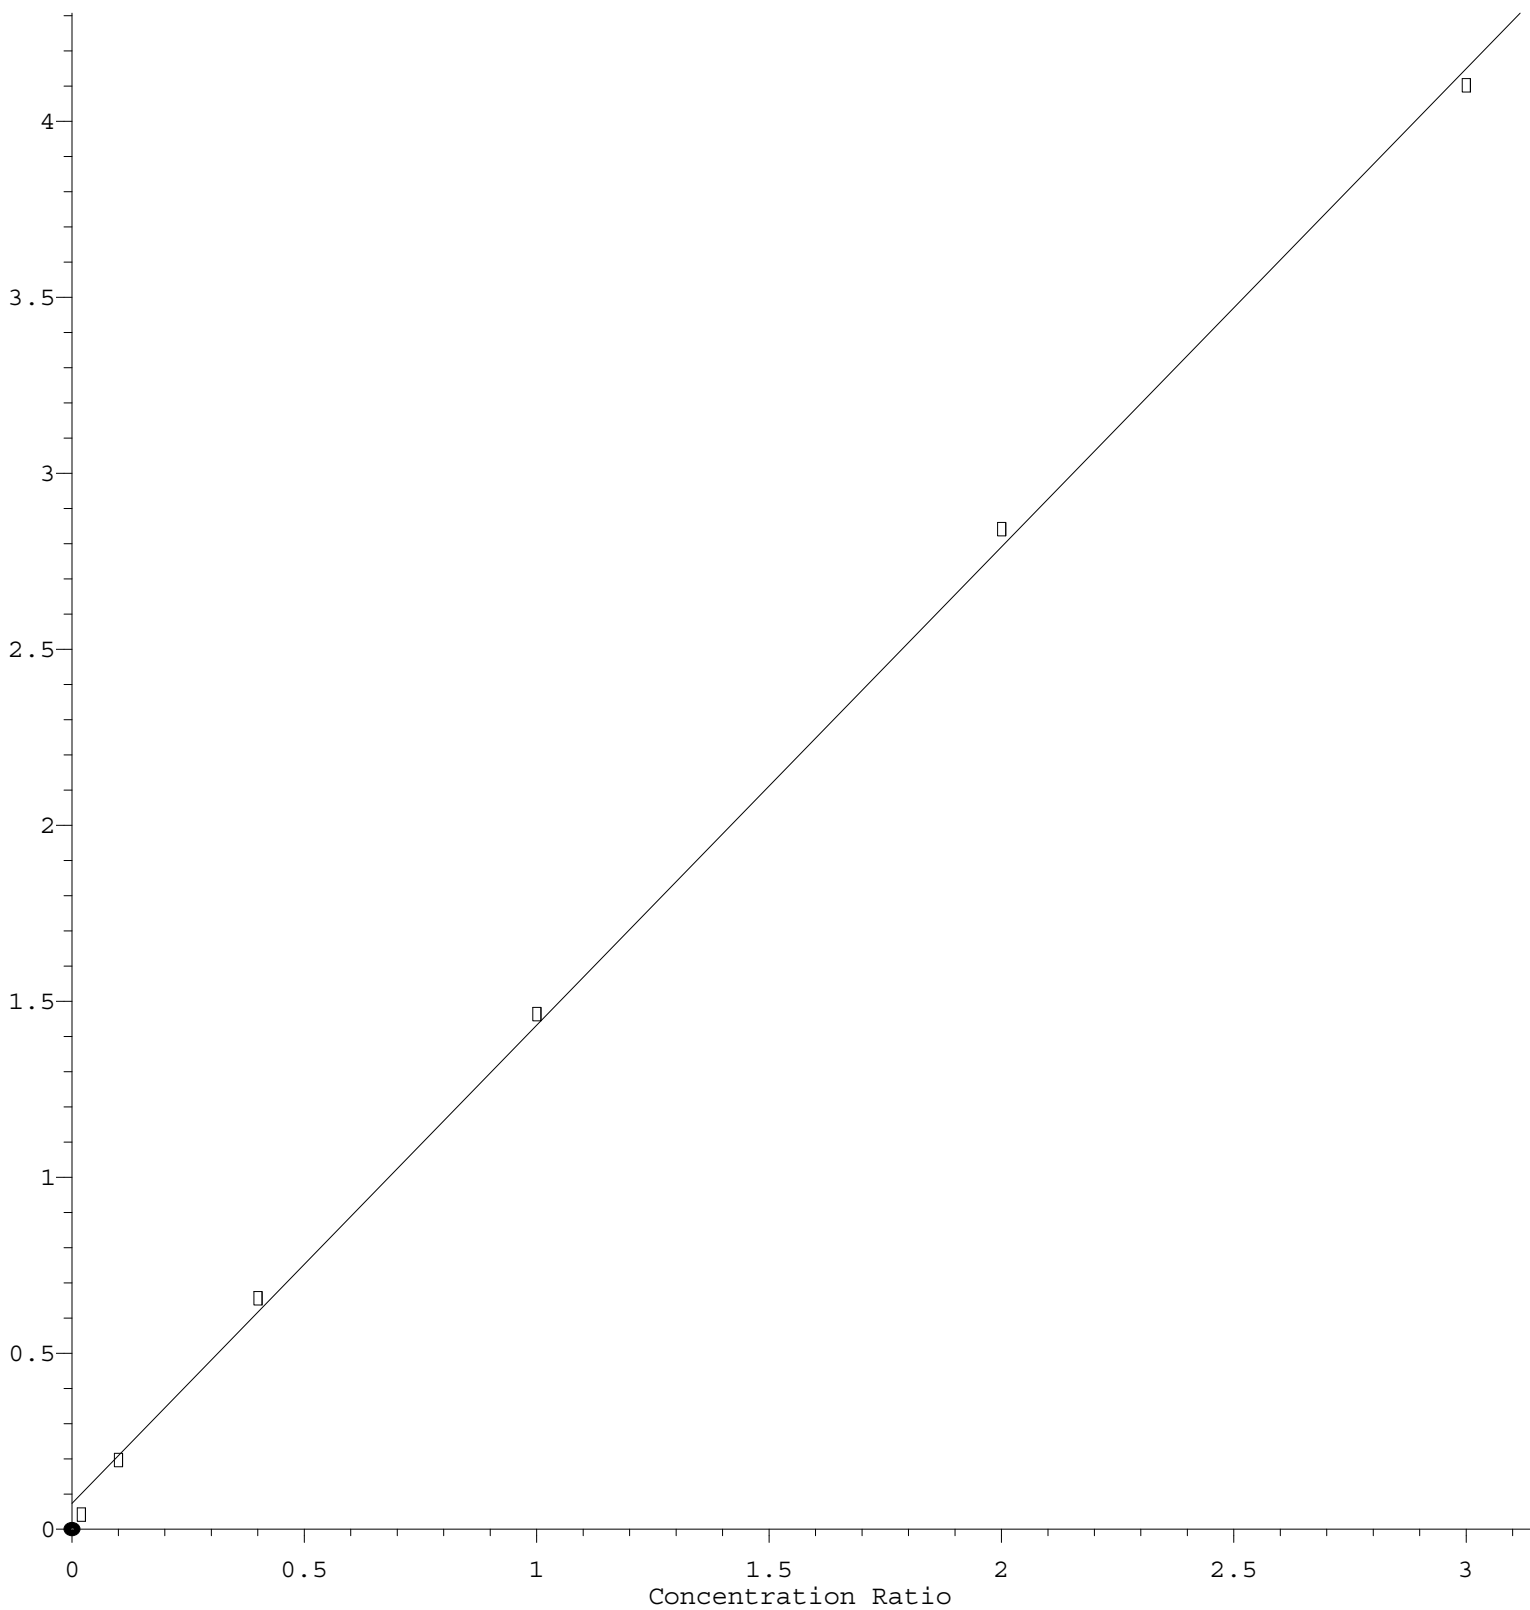

$$\text{Response} = 1.359\text{e}+000 * \text{Amt} + 7.340\text{e}-002$$


Coef of Det (r^2) = 0.999166 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N030722W.M

Calibration Table Last Updated: Tue Mar 08 06:52:46 2022

1,2,3-Trichloropropane

Response Ratio

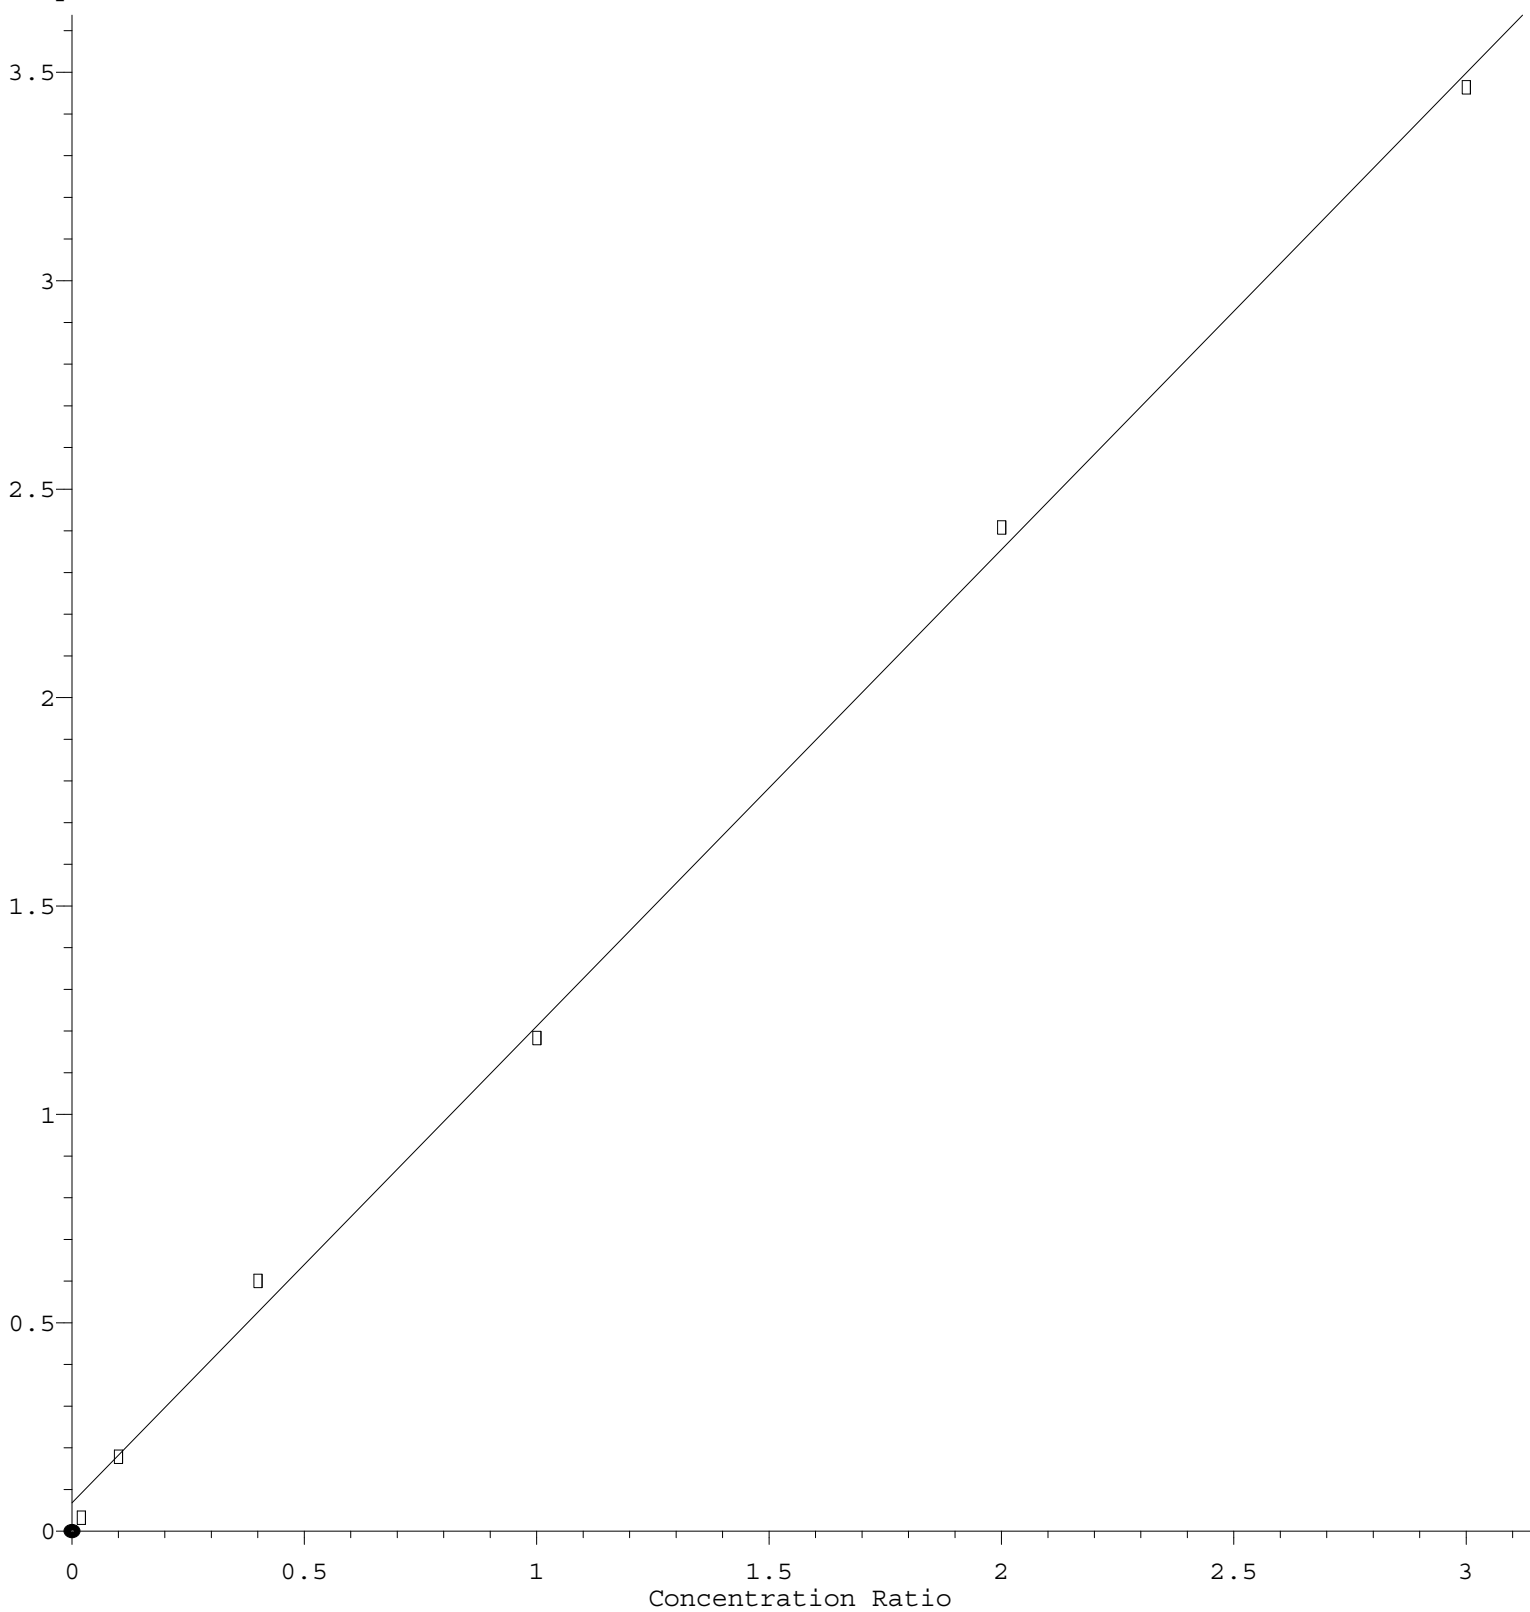

$$\text{Response} = 1.143\text{e}+000 * \text{Amt} + 6.840\text{e}-002$$


Coef of Det (r^2) = 0.998508 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N030722W.M

Calibration Table Last Updated: Tue Mar 08 06:52:46 2022

1,2,4-Trichlorobenzene

Response Ratio

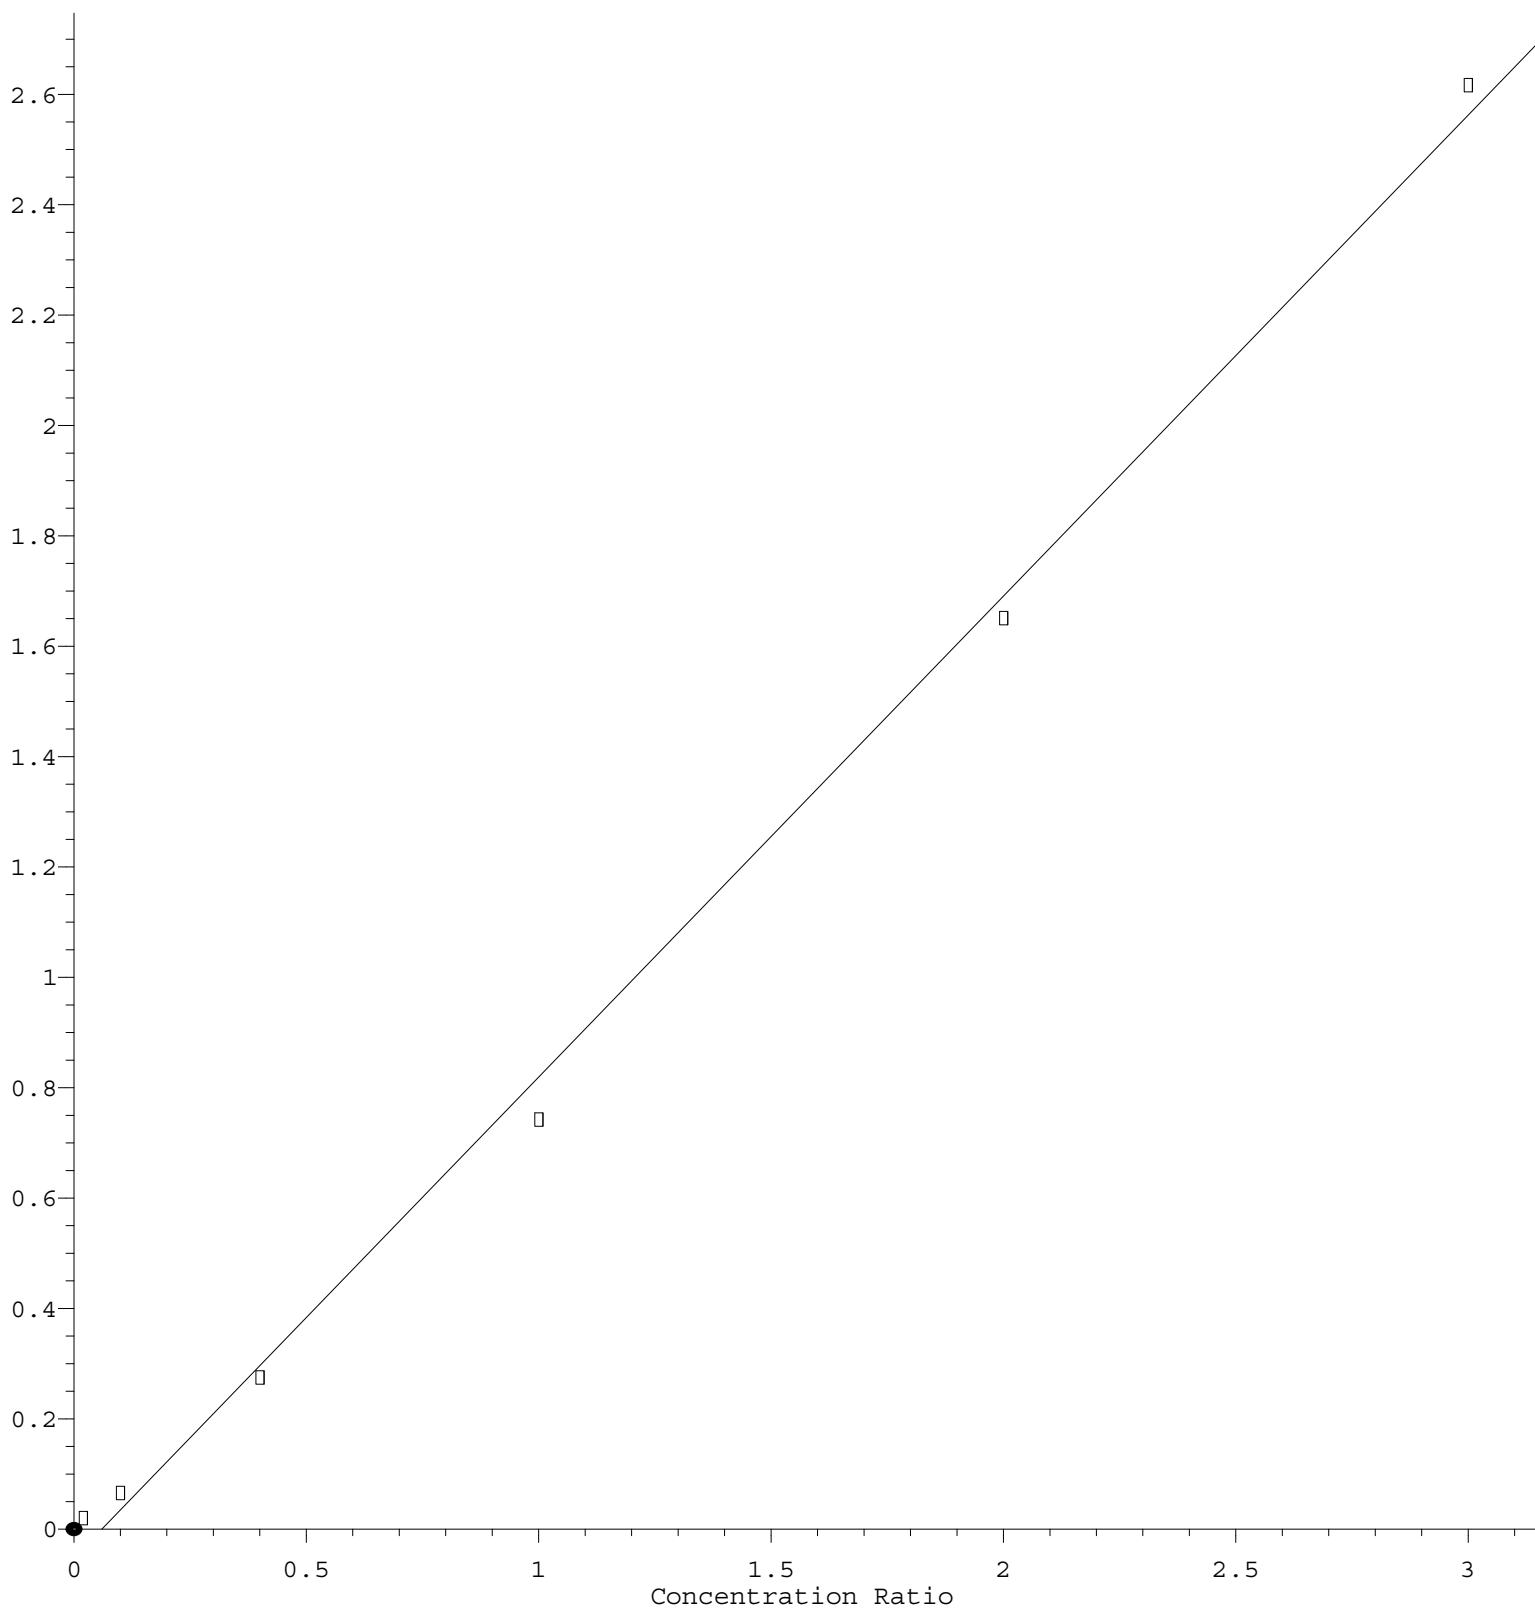

$$\text{Response} = 8.715\text{e-}001 * \text{Amt} - 5.210\text{e-}002$$


Coef of Det (r^2) = 0.997242 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N030722W.M

Calibration Table Last Updated: Tue Mar 08 06:52:46 2022

Naphthalene


Response Ratio

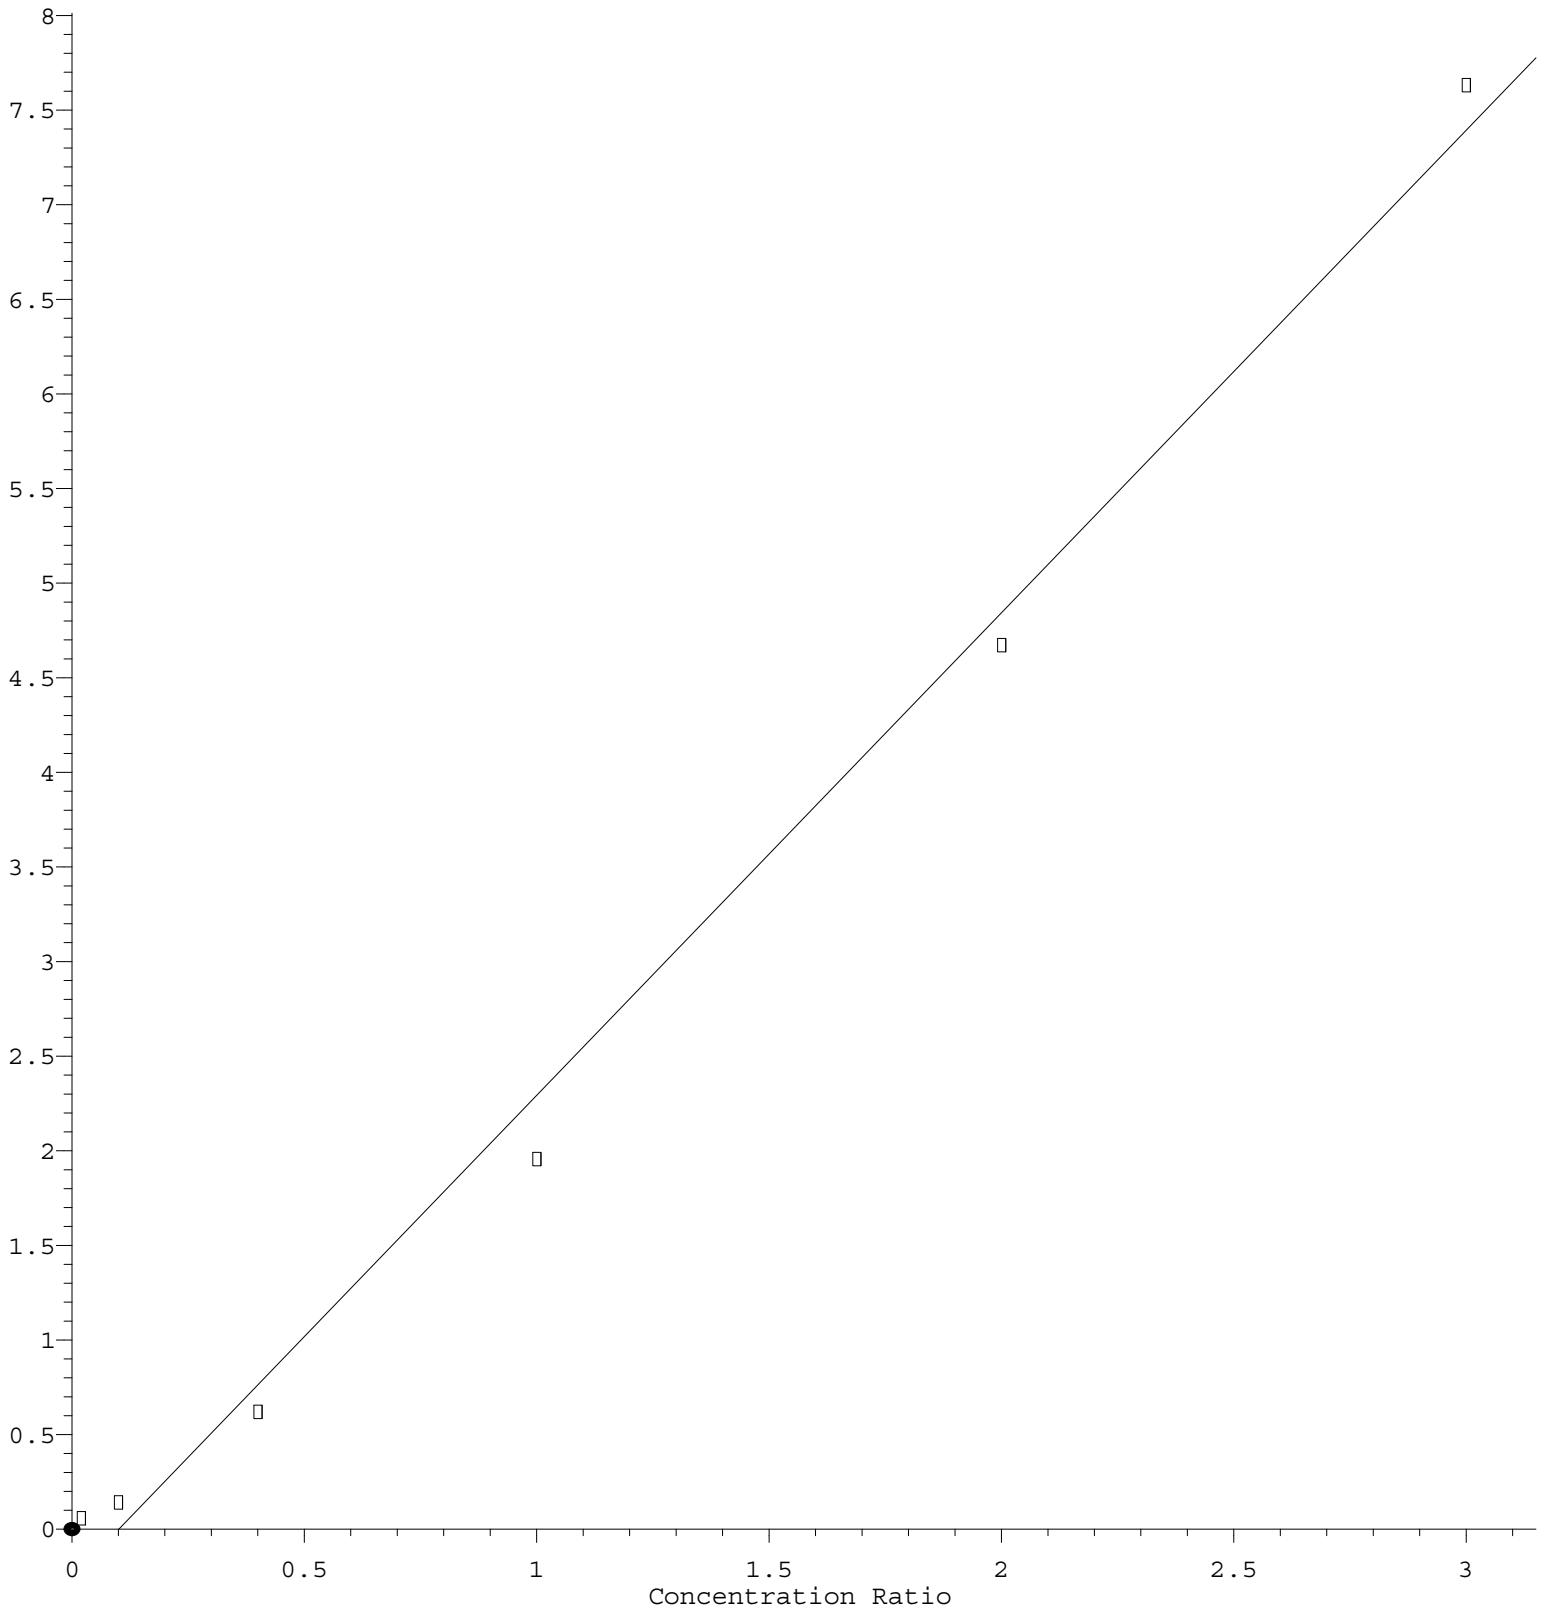

$\text{Response} = 2.551\text{e}+000 * \text{Amt} - 2.585\text{e}-001$
 Coef of Det (r^2) = 0.993318 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N030722W.M
 Calibration Table Last Updated: Tue Mar 08 06:52:46 2022

1,2,3-Trichlorobenzene

Response Ratio

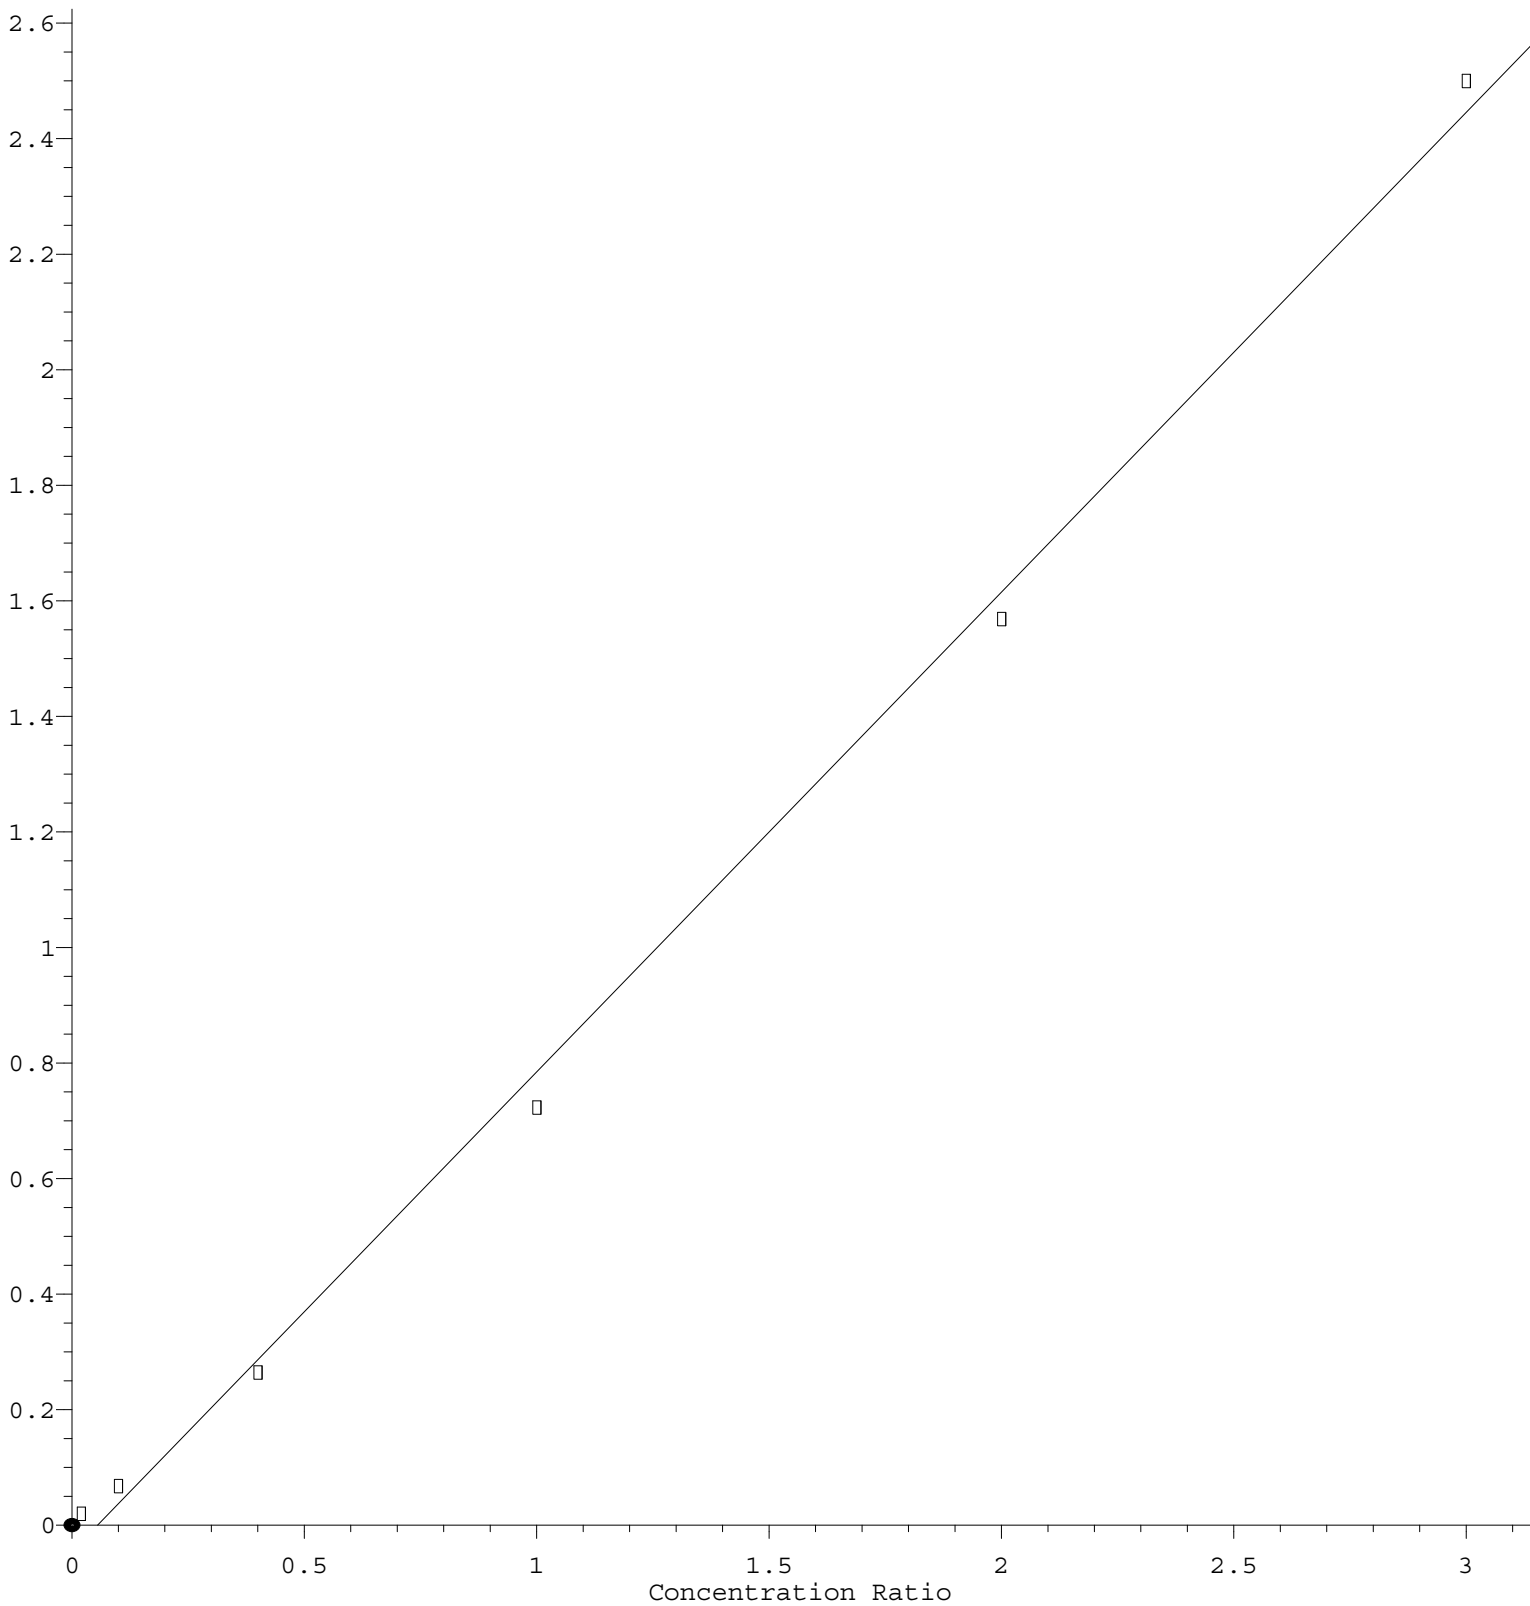

$$\text{Response} = 8.304\text{e-}001 * \text{Amt} - 4.537\text{e-}002$$

Coef of Det (r^2) = 0.997398 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N030722W.M

Calibration Table Last Updated: Tue Mar 08 06:52:46 2022