
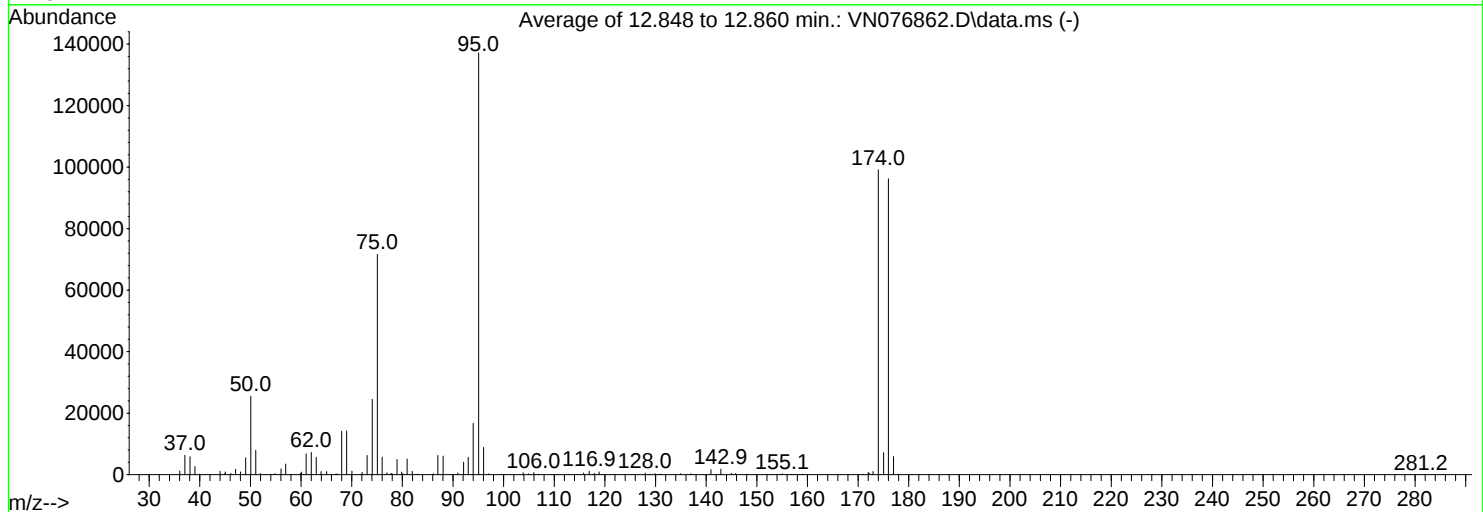


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030723\
Data File : VN076862.D
Acq On : 07 Mar 2023 10:00
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030623W.M
Title : SW846 8260
Last Update : Tue Mar 07 08:45:33 2023

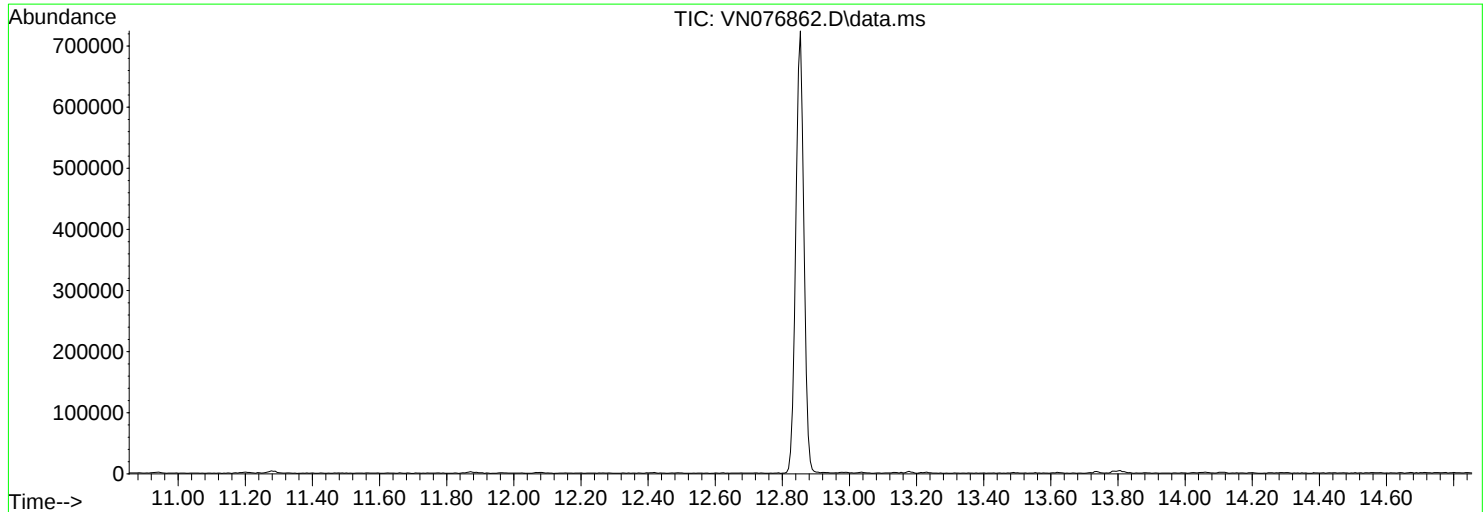

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	25488	PASS
75	95	30	60	52.3	71675	PASS
95	95	100	100	100.0	137171	PASS
96	95	5	9	6.5	8875	PASS
173	174	0.00	2	1.1	1053	PASS
174	95	50	100	72.3	99117	PASS
175	174	5	9	7.2	7114	PASS
176	174	95	101	97.1	96221	PASS
177	176	5	9	6.1	5857	PASS

Average of 12.848 to 12.860 min.: VN076862.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	1220	48.05	903	59.90	433	69.00	1421
37.05	6310	49.05	5469	60.05	835	70.05	114
38.05	5828	50.05	25488	61.00	6762	71.80	15
39.05	2663	51.05	7894	62.00	7262	72.05	75
39.90	236	51.95	350	63.00	5601	73.05	6227
40.80	61	53.05	115	63.95	988	74.05	24499
44.00	1090	54.00	57	65.05	980	75.05	71675
44.90	316	54.85	344	65.95	174	76.00	5707
45.05	904	56.05	1862	66.80	146	76.95	617
46.15	374	56.95	3429	67.10	280	77.75	410
47.05	1717	58.05	126	68.00	14111	77.95	403

Average of 12.848 to 12.860 min.: VN076862.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	4935	93.00	5615	110.90	76	129.95	287
79.85	855	94.00	16717	112.90	71	130.60	59
80.10	325	95.05	137171	114.90	73	131.05	186
80.95	5086	96.05	8875	115.80	507	134.95	294
81.95	1102	97.05	254	116.90	1111	137.00	338
83.00	164	103.85	650	117.70	160	140.95	1673
86.15	263	104.90	287	117.95	349	141.80	89
87.00	6224	105.95	710	118.85	903	142.90	1809
88.05	6019	106.80	55	127.95	531	144.95	431
90.95	571	107.00	56	128.90	157	145.85	383
92.10	4066	109.90	63	129.80	185	147.60	75

Average of 12.848 to 12.860 min.: VN076862.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
148.00	169	172.20	473				
148.20	60	172.95	1053				
149.70	58	174.00	99117				
152.90	107	175.05	7114				
154.80	101	176.00	96221				
155.05	246	177.00	5857				
156.80	64	177.95	170				
157.20	50	281.20	77				
159.00	155						
171.05	108						
172.00	794						

Instrument :

MSVOA_N

ClientSampleId :

BFB