
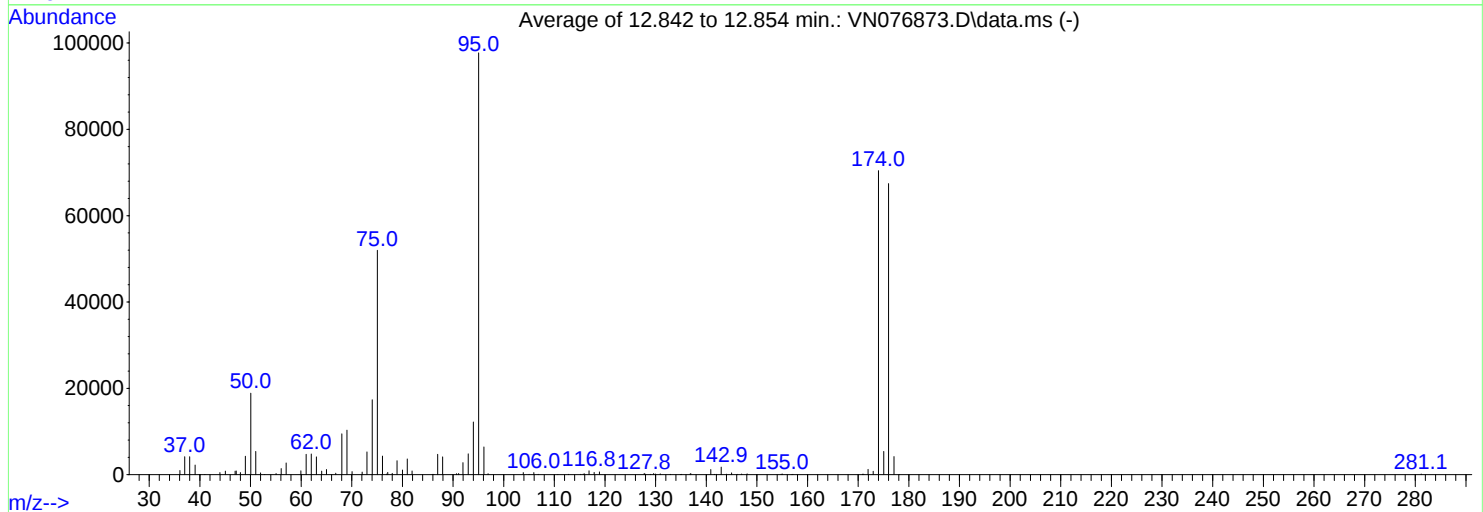


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030823\
Data File : VN076873.D
Acq On : 08 Mar 2023 09:26
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030623W.M
Title : SW846 8260
Last Update : Tue Mar 07 08:45:33 2023

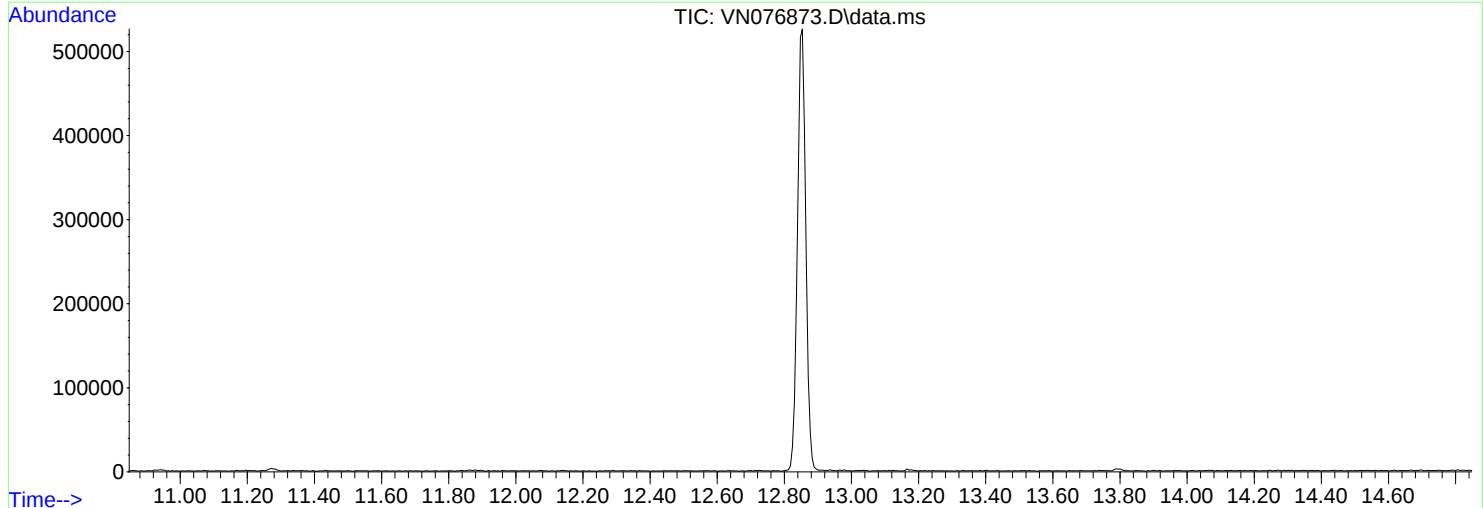

AutoFind: Scans 1854, 1855, 1856; Background Corrected with Scan 1846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	18855	PASS
75	95	30	60	53.2	51973	PASS
95	95	100	100	100.0	97728	PASS
96	95	5	9	6.6	6421	PASS
173	174	0.00	2	1.1	790	PASS
174	95	50	100	72.1	70421	PASS
175	174	5	9	7.6	5387	PASS
176	174	95	101	95.7	67419	PASS
177	176	5	9	6.2	4172	PASS

Average of 12.842 to 12.854 min.: VN076873.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	960	49.00	4279	63.00	4106	76.05	4311
37.00	4161	50.05	18855	64.05	815	76.90	163
38.00	4144	51.05	5364	65.00	1194	77.10	52
39.05	2231	52.00	416	66.85	347	78.00	29
39.90	12	52.80	58	68.05	9455	78.95	3214
41.00	59	55.05	271	69.05	10311	80.00	1092
43.95	494	56.05	1413	70.05	693	80.95	3632
45.05	807	57.05	2700	72.05	605	81.90	866
46.95	831	59.95	883	73.00	5272	85.90	64
47.20	841	61.00	4711	74.05	17337	86.20	87
48.00	490	62.00	4774	75.05	51973	86.95	4700

Average of 12.842 to 12.854 min.: VN076873.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.95	4134	105.95	477	128.00	130	141.60	95
90.70	235	106.80	65	129.00	63	142.00	61
91.10	253	110.70	51	129.60	245	142.95	1756
91.95	2799	112.80	76	130.00	142	144.00	119
93.00	4814	115.20	73	130.90	197	145.00	394
94.00	12212	115.70	144	132.90	70	146.10	68
95.05	97728	115.95	186	134.90	50	147.00	163
96.10	6421	116.85	879	135.10	82	148.05	190
96.90	223	117.85	516	136.80	132	150.00	51
103.85	469	118.90	632	136.95	279	154.80	96
105.00	61	127.75	293	140.90	1196	155.00	134

Average of 12.842 to 12.854 min.: VN076873.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.90	55	281.15	161				
157.10	72						
170.85	128						
171.10	101						
171.95	1209						
172.95	790						
174.00	70421						
175.05	5387						
176.00	67419						
177.05	4172						
178.10	53						

Instrument :

MSVOA_N

ClientSampleId :

BFB