


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030823\
Data File : VN076882.D
Acq On : 08 Mar 2023 16:47
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N030823W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Mar 09 04:16:54 2023

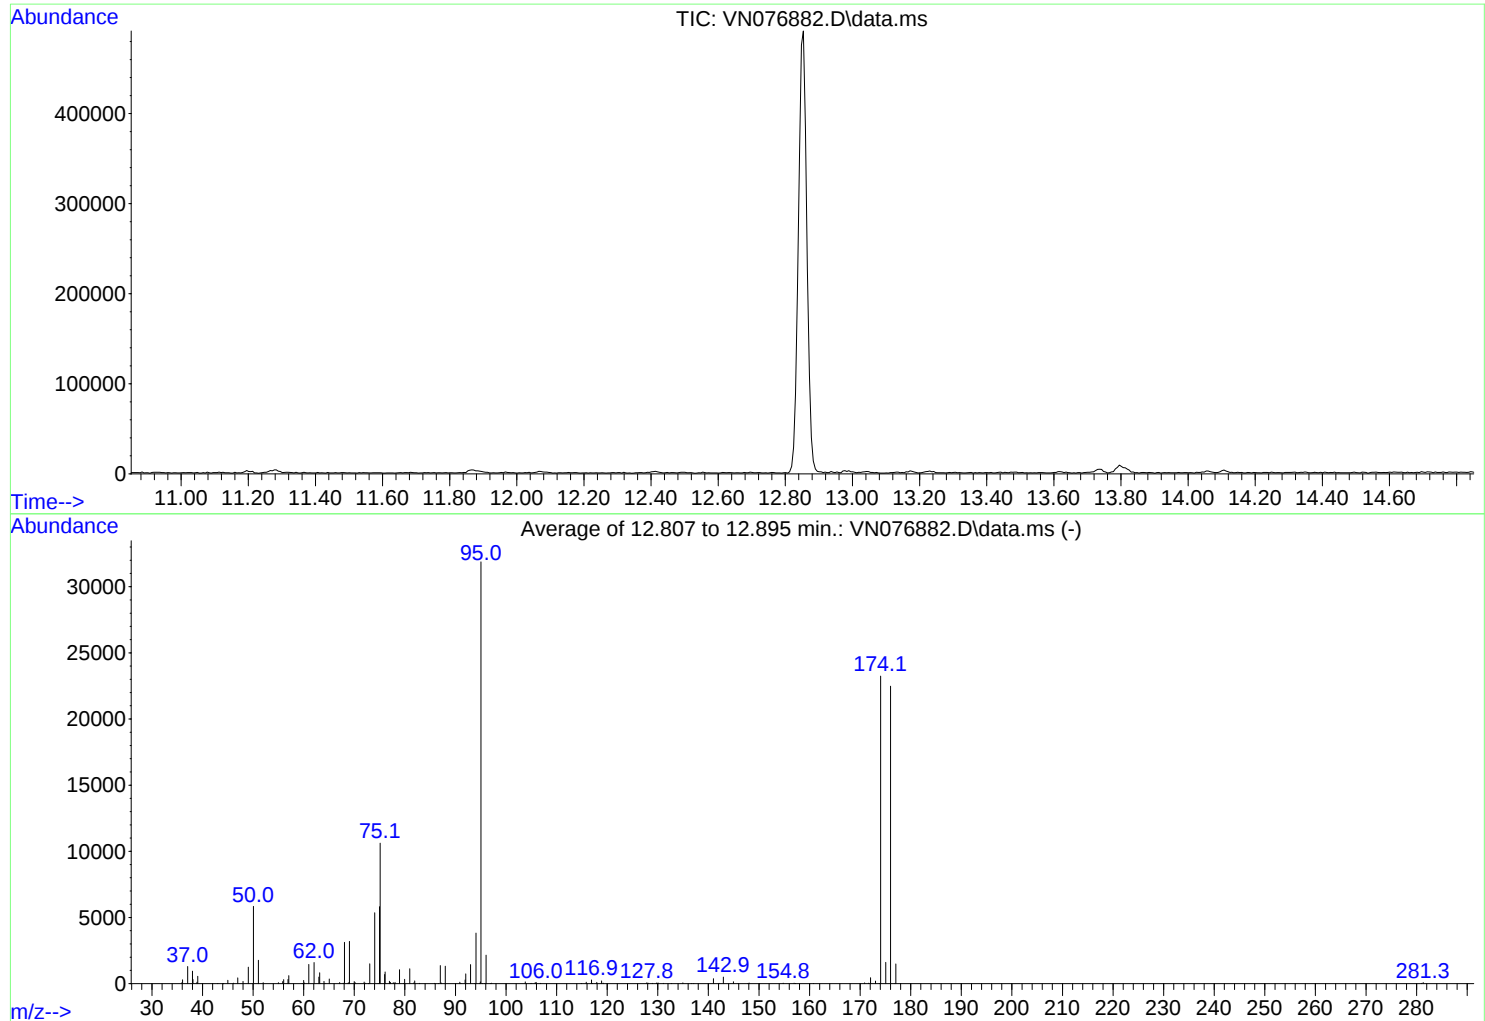

AutoFind: Averaged scan 1848 to 1863; Bkg corrected with scan 1847

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	5839	PASS
75	95	30	60	33.3	10619	PASS
95	95	100	100	100.0	31878	PASS
96	95	5	9	6.8	2157	PASS
173	174	0.00	2	0.8	195	PASS
174	95	50	100	72.9	23248	PASS
175	174	5	9	6.9	1604	PASS
176	174	95	101	96.7	22477	PASS
177	176	5	9	6.6	1491	PASS