
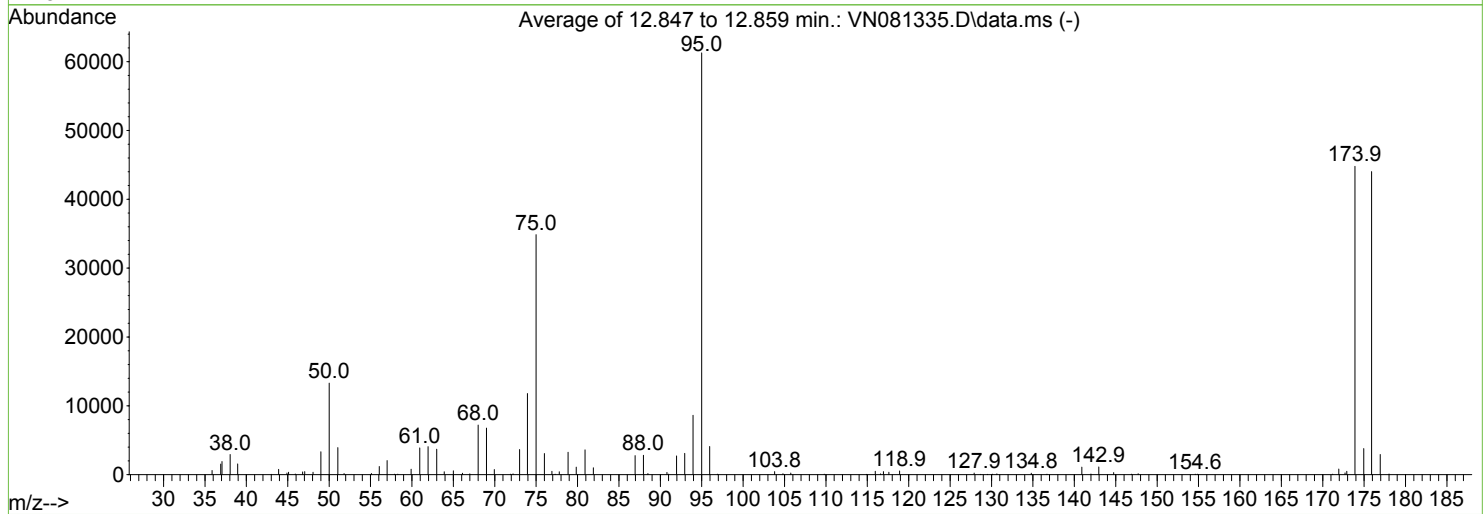


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030824\
Data File : VN081335.D
Acq On : 08 Mar 2024 08:17
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030524W.M
Title : SW846 8260
Last Update : Wed Mar 06 03:12:57 2024

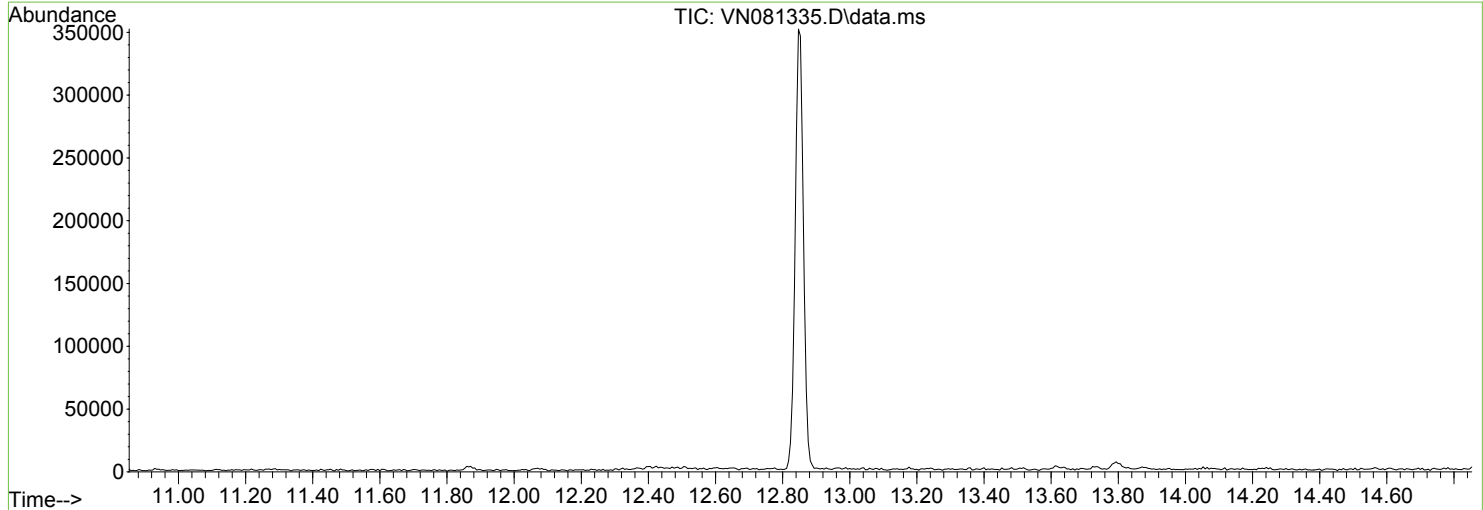

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.7	13309	PASS
75	95	30	60	56.9	34864	PASS
95	95	100	100	100.0	61277	PASS
96	95	5	9	6.7	4101	PASS
173	174	0.00	2	1.1	494	PASS
174	95	50	100	73.1	44803	PASS
175	174	5	9	8.5	3801	PASS
176	174	95	101	98.3	44021	PASS
177	176	5	9	6.7	2928	PASS

Average of 12.847 to 12.859 min.: VN081335.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	604	47.05	442	59.90	791	71.90	611
36.90	1533	48.05	341	60.95	3887	72.20	1178
37.05	1916	49.00	3337	61.95	4075	73.00	365
38.05	2940	50.00	13309	63.00	3697	73.95	1178
38.95	1567	51.05	3930	63.90	420	75.00	34864
43.00	59	51.80	156	65.00	562	76.00	3072
43.90	766	55.10	152	66.10	207	76.90	490
44.90	236	56.05	1195	67.00	113	77.30	73
45.10	358	57.00	2039	68.00	7200	77.80	422
45.90	105	57.90	74	69.00	6765	78.85	3259
46.80	399	58.30	71	69.95	735	79.85	1092

Average of 12.847 to 12.859 min.: VN081335.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.90	3593	95.95	4101	118.90	539	144.75	308
81.90	990	96.90	70	127.90	226	146.90	65
86.95	2769	103.80	444	128.70	59	147.70	150
87.95	2825	104.80	137	129.50	55	154.60	65
88.50	157	105.75	245	130.10	72	154.90	62
90.80	330	109.80	70	130.65	114	171.20	74
91.00	63	114.90	58	134.80	205	171.95	809
91.95	2728	115.95	487	136.70	69	172.70	257
92.95	3102	116.60	123	140.90	1104	172.90	494
93.95	8616	116.95	432	142.00	88	173.90	44803
95.00	61277	117.60	349	142.95	1125	174.95	3801

Average of 12.847 to 12.859 min.: VN081335.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
175.90	44021						
176.95	2928						
178.00	101						

Instrument :

MSVOA_N

ClientSampleId :

BFB