
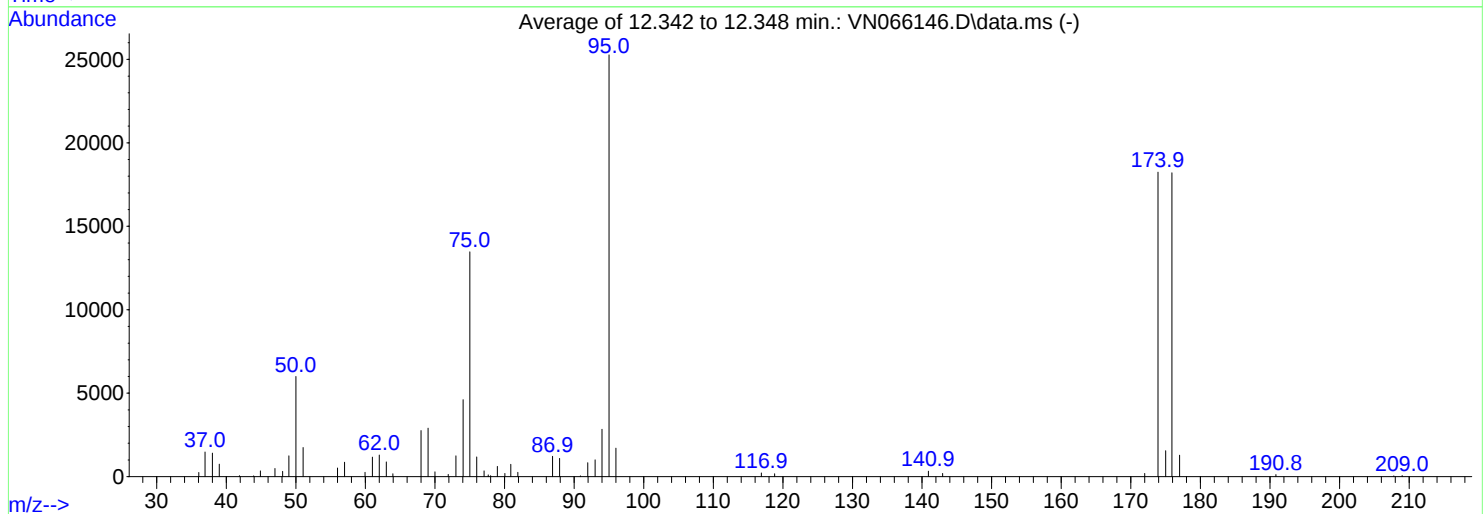


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030921\
 Data File : VN066146.D
 Acq On : 9 Mar 2021 8:42
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030921W.M
 Title : SW846 8260
 Last Update : Tue Mar 09 14:48:21 2021

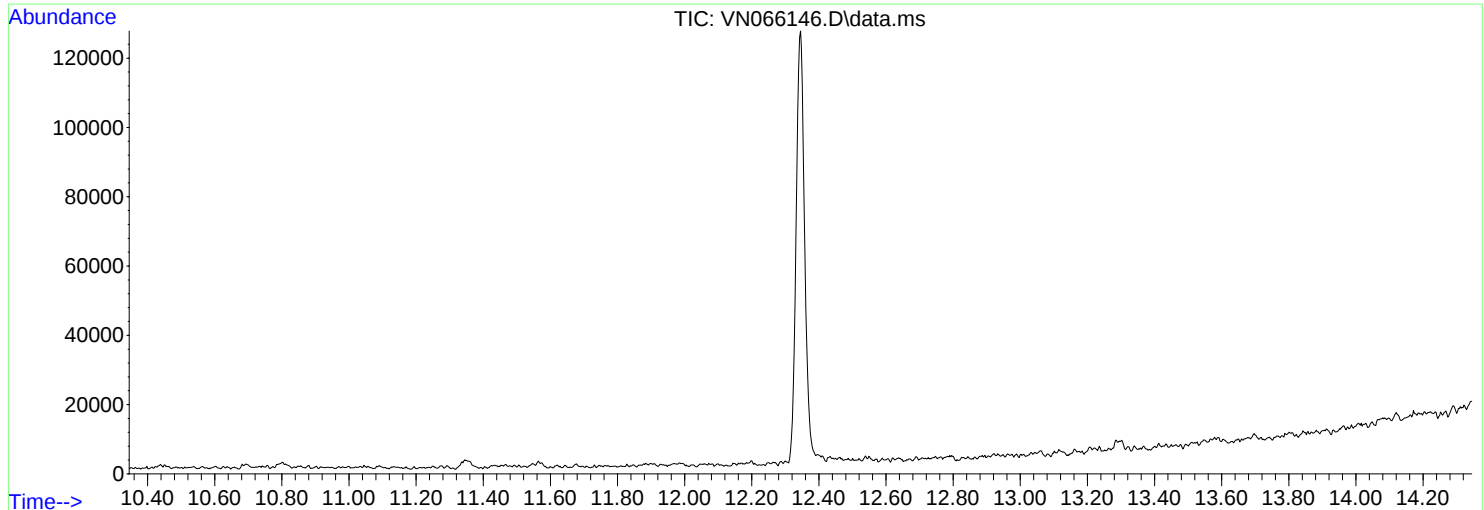

AutoFind: Scans 3972, 3973, 3974; Background Corrected with Scan 3958

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	5998	PASS
75	95	30	60	53.3	13469	PASS
95	95	100	100	100.0	25272	PASS
96	95	5	9	6.8	1709	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.2	18243	PASS
175	174	5	9	8.5	1553	PASS
176	174	95	101	99.8	18205	PASS
177	176	5	9	7.1	1286	PASS