

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030923\
 Data File : VN076909.D
 Acq On : 09 Mar 2023 18:04
 Operator : JC\MD
 Sample : PB151321ZHE#02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB151321ZHE#02

Quant Time: Mar 10 03:49:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030623W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 07 08:45:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.231	168	450019	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.107	114	754094	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.866	117	671057	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.795	152	273298	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.584	65	306585	48.592	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	97.180%		
35) Dibromofluoromethane	8.172	113	234537	49.717	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	99.440%		
50) Toluene-d8	10.572	98	909023	50.015	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	100.040%		
62) 4-Bromofluorobenzene	12.854	95	320571	50.902	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	101.800%		
Target Compounds						Qvalue
5) Bromomethane	2.990	94	1217	0.293	ug/l	90
6) Chloroethane	3.113	64	752	Below Cal	#	42
11) Tert butyl alcohol	5.525	59	1699	1.813	ug/l #	72
16) Acetone	4.449	43	44638	16.208	ug/l	99
18) Methyl Acetate	5.043	43	3629	0.385	ug/l #	75
20) Methylene Chloride	5.296	84	19615	3.053	ug/l	98
25) 2-Butanone	7.501	43	8210	2.041	ug/l #	72
29) Tetrahydrofuran	7.848	42	662	0.255	ug/l #	30
31) Cyclohexane	8.231	56	10006	0.939	ug/l #	1
36) 1,1-Dichloropropene	8.237	75	38891	5.129	ug/l #	49
37) Ethyl Acetate	7.572	43	81689	10.496	ug/l	97
38) Carbon Tetrachloride	8.231	117	50443	6.549	ug/l #	16
42) 1,2-Dichloroethane	8.695	62	2911	0.362	ug/l #	71
43) Isopropyl Acetate	8.695	43	382116	32.072	ug/l #	82
48) Methyl methacrylate	9.672	41	9500	1.641	ug/l #	27
49) 1,4-Dioxane	9.689	88	58	0.547	ug/l #	1
51) 4-Methyl-2-Pentanone	10.448	43	15417	2.051	ug/l	93
53) t-1,3-Dichloropropene	10.736	75	2831	0.375	ug/l #	61
54) cis-1,3-Dichloropropene	10.360	75	144476	16.650	ug/l #	65
56) Ethyl methacrylate	10.995	69	3611	0.443	ug/l #	1
57) 1,3-Dichloropropane	11.201	76	19505	2.053	ug/l #	42
59) 2-Hexanone	11.172	43	320661	58.885	ug/l #	17
71) Bromoform	12.848	173	1293	0.362	ug/l #	1
74) N-amyl acetate	12.495	43	3255	0.349	ug/l #	47
76) 1,2,3-Trichloropropane	12.854	75	174713	25.348	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.854	75	174713	83.599	ug/l #	15
93) 1,2,4-Trichlorobenzene	15.401	180	1722	0.353	ug/l	83
95) Naphthalene	15.648	128	5532	0.354	ug/l #	93
96) 1,2,3-Trichlorobenzene	15.842	180	1337	0.279	ug/l	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030923\
Data File : VN076909.D
Acq On : 09 Mar 2023 18:04
Operator : JC\MD
Sample : PB151321ZHE#02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB151321ZHE#02

Quant Time: Mar 10 03:49:12 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030623W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 07 08:45:33 2023
Response via : Initial Calibration




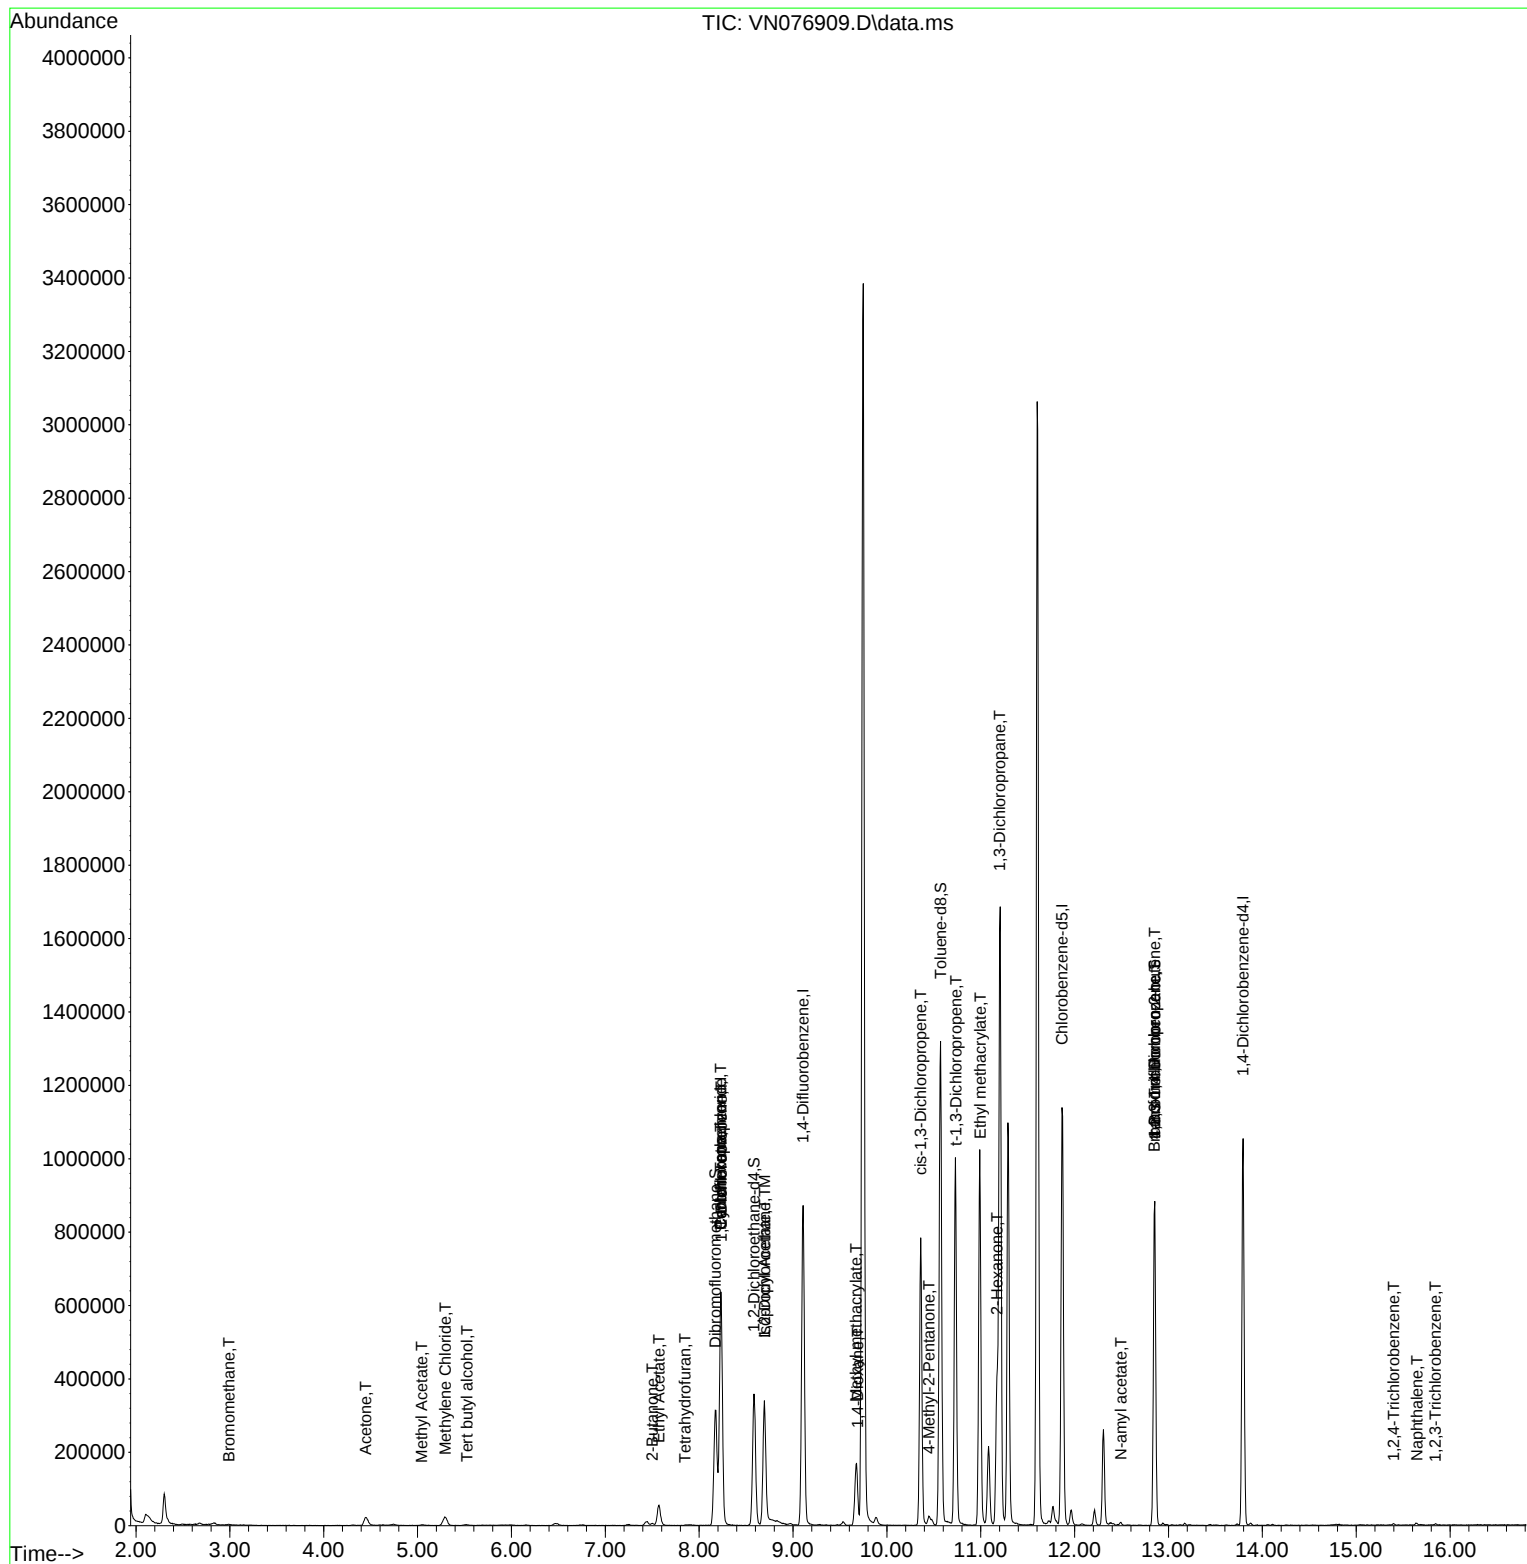




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.231 min Scan# 1070
Delta R.T. -0.000 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
PB151321ZHE#02


Tgt Ion:168 Resp: 450019
Ion Ratio Lower Upper
168 100
99 67.1 48.6 73.0

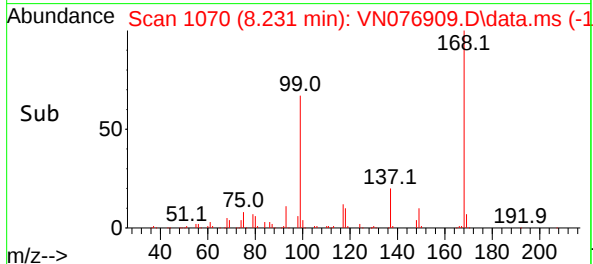

#5
Bromomethane
Concen: 0.293 ug/l
RT: 2.990 min Scan# 179
Delta R.T. 0.036 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04

Tgt Ion: 94 Resp: 1217
Ion Ratio Lower Upper
94 100
96 109.1 79.0 118.6



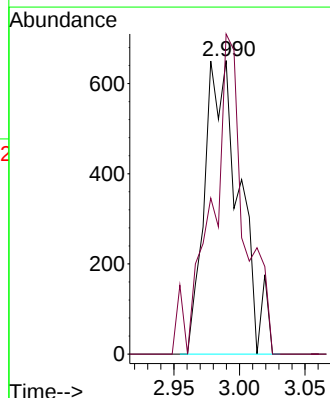
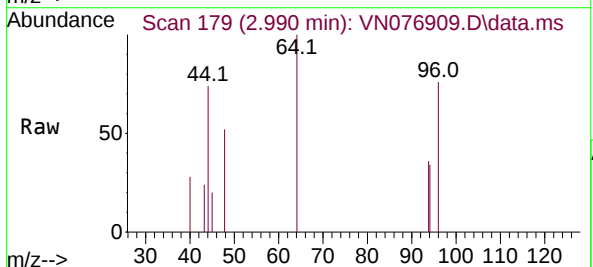


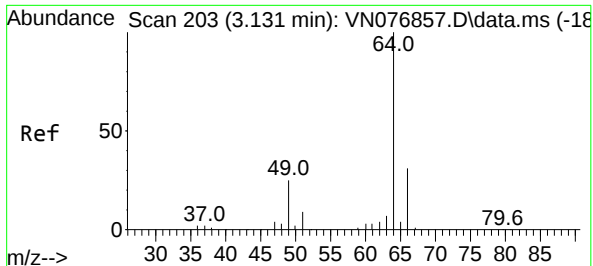

#6
Chloroethane
Concen: Below Cal
RT: 3.113 min Scan# 203
Delta R.T. -0.018 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
PB151321ZHE#02


Tgt Ion: 64 Resp: 752
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#

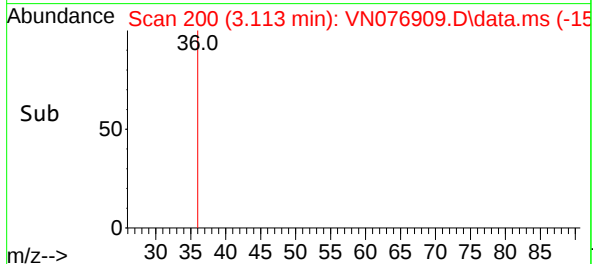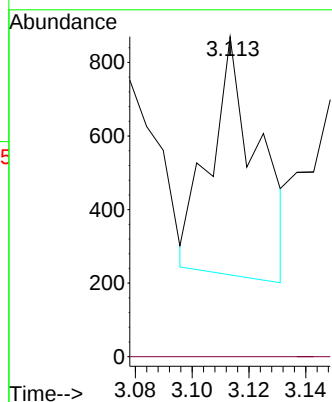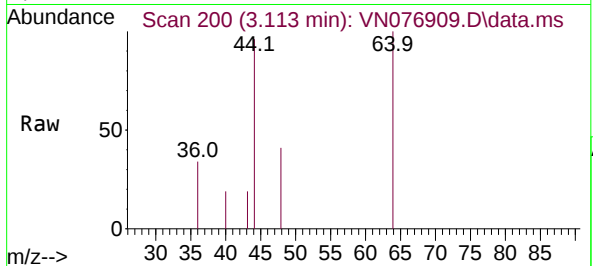

#11
Tert butyl alcohol
Concen: 1.813 ug/l
RT: 5.525 min Scan# 610
Delta R.T. -0.012 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04

Tgt Ion: 59 Resp: 1699
Ion Ratio Lower Upper
59 100
57 0.0 8.6 12.8#


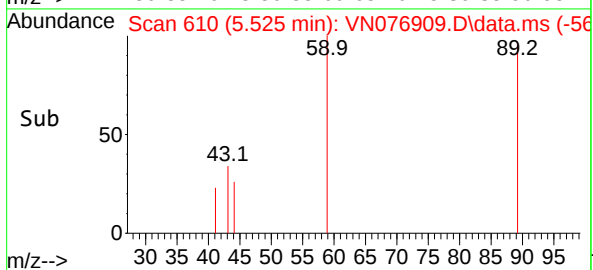
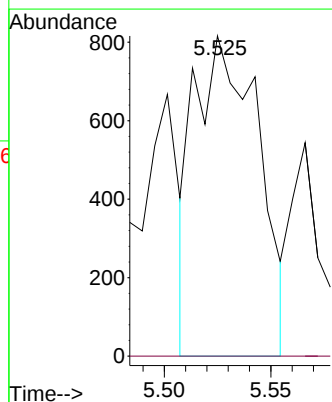
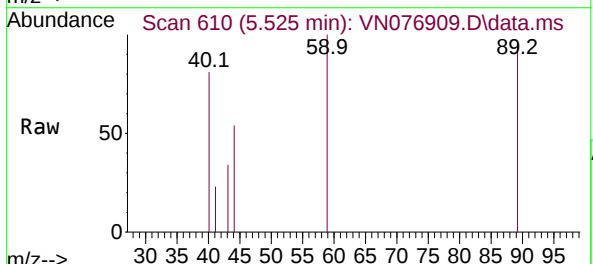




#16
Acetone
Concen: 16.208 ug/l
RT: 4.449 min Scan# 41
Delta R.T. 0.012 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
PB151321ZHE#02


Tgt Ion: 43 Resp: 44638
Ion Ratio Lower Upper
43 100
58 36.1 28.2 42.2

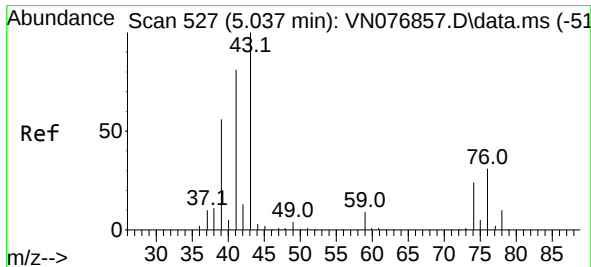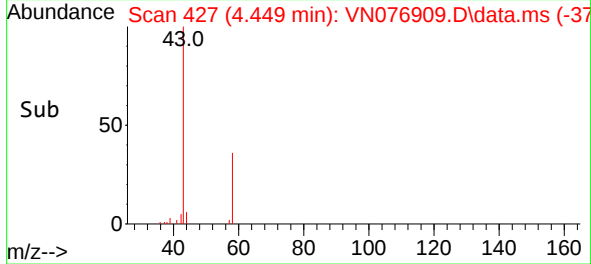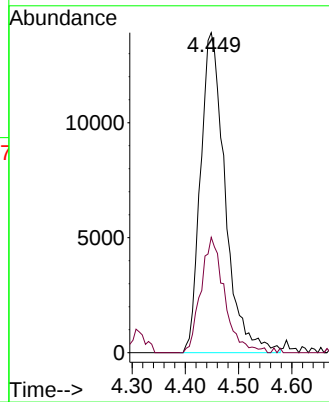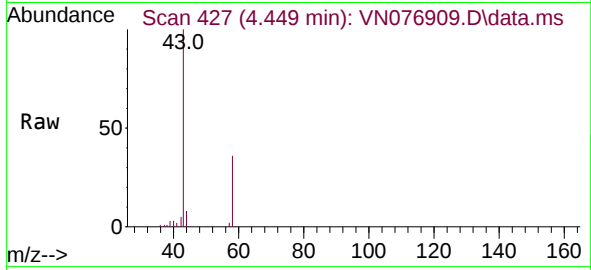

#18
Methyl Acetate
Concen: 0.385 ug/l
RT: 5.043 min Scan# 528
Delta R.T. 0.006 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04

Tgt Ion: 43 Resp: 3629
Ion Ratio Lower Upper
43 100
74 18.3 25.9 38.9#


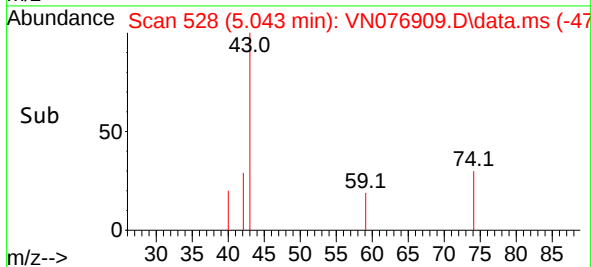
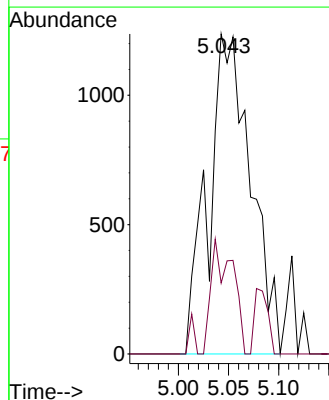
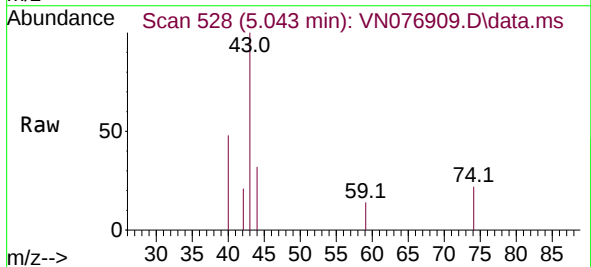


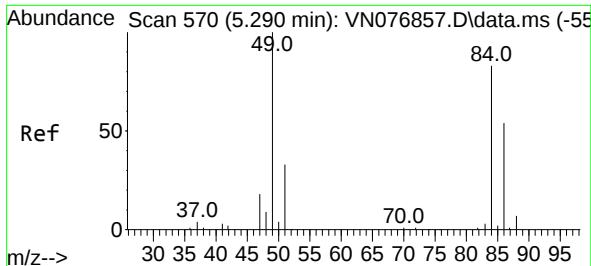

#20
Methylene Chloride
Concen: 3.053 ug/l
RT: 5.296 min Scan# 51
Delta R.T. 0.006 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
PB151321ZHE#02


Tgt Ion: 84	Resp:	19615	
Ion	Ratio	Lower	Upper
84	100		
49	96.8	76.6	114.8
51	32.6	25.4	38.2
86	60.2	51.1	76.7

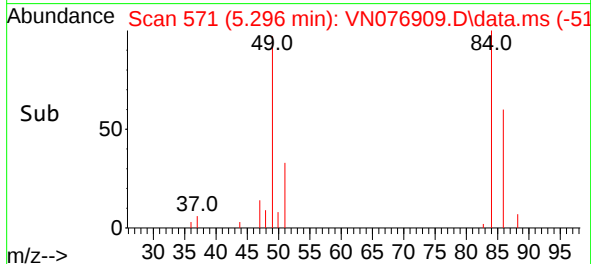

#25
2-Butanone
Concen: 2.041 ug/l
RT: 7.501 min Scan# 946
Delta R.T. 0.012 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04

Tgt Ion: 43	Resp:	8210	
Ion	Ratio	Lower	Upper
43	100		
72	19.5	28.8	43.2#

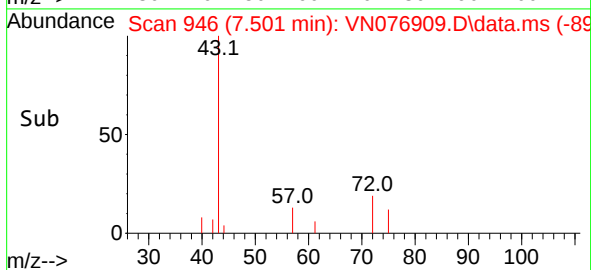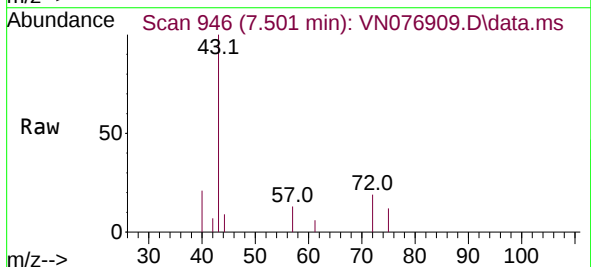

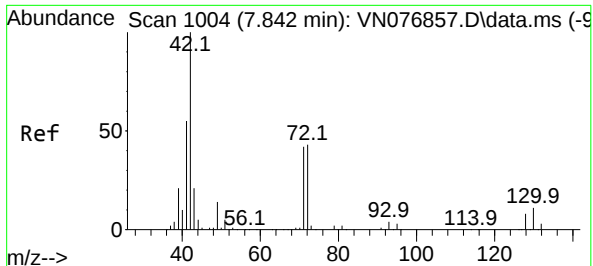

#29

Tetrahydrofuran

Concen: 0.255 ug/l

RT: 7.848 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN076909.D

Acq: 09 Mar 2023 18:04

Instrument :

MSVOA_N

ClientSampleId :

PB151321ZHE#02





Tgt Ion: 42 Resp: 662

Ion Ratio Lower Upper

42 100

72 12.4 48.6 73.0#

71 0.0 45.1 67.7#

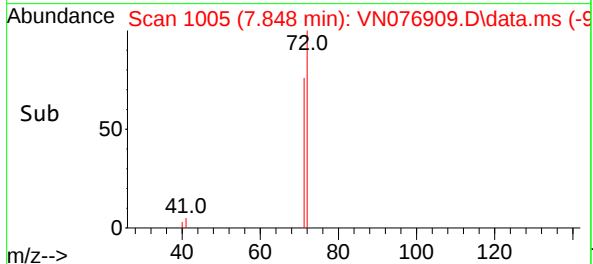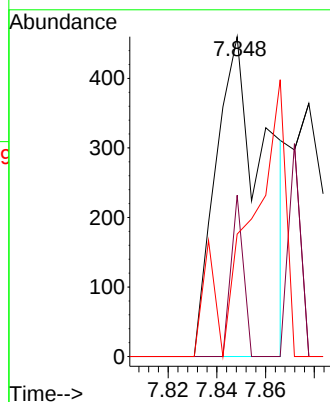

#31

Cyclohexane

Concen: 0.939 ug/l

RT: 8.231 min Scan# 1070

Delta R.T. -0.035 min

Lab File: VN076909.D

Acq: 09 Mar 2023 18:04




Tgt Ion: 56 Resp: 10006


Ion Ratio Lower Upper

56 100

69 186.9 27.0 40.6#

84 154.9 82.9 124.3#

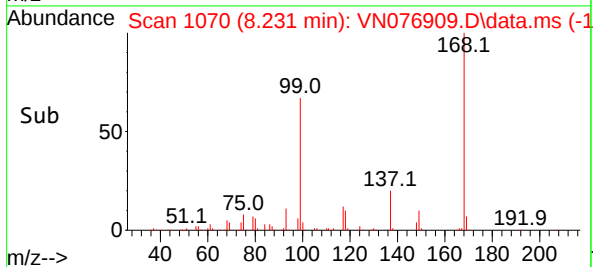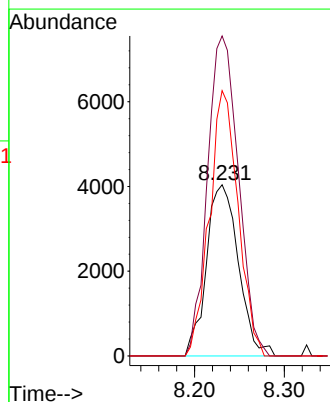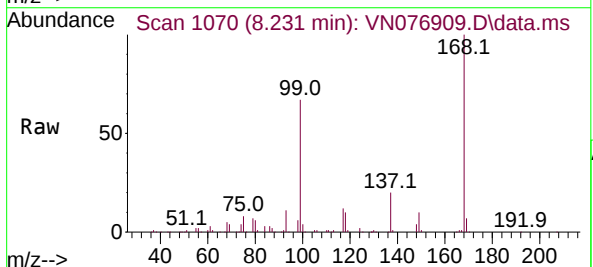



#33

1,2-Dichloroethane-d4

Concen: 48.592 ug/l

RT: 8.584 min Scan# 1130

Delta R.T. 0.001 min

Lab File: VN076909.D

Acq: 09 Mar 2023 18:04

Instrument :

MSVOA_N

ClientSampleId :





PB151321ZHE#02

Tgt Ion: 65 Resp: 306585

Ion Ratio Lower Upper

65 100

67 51.4 0.0 107.2

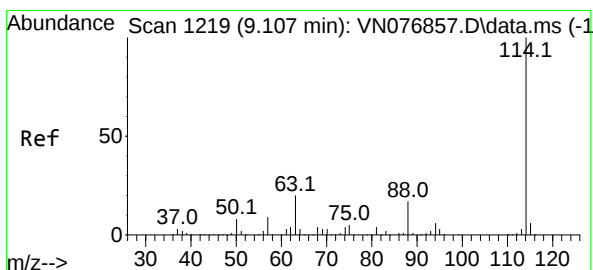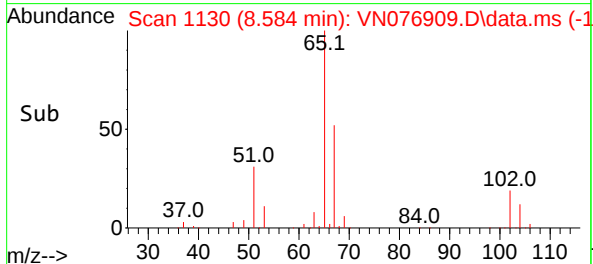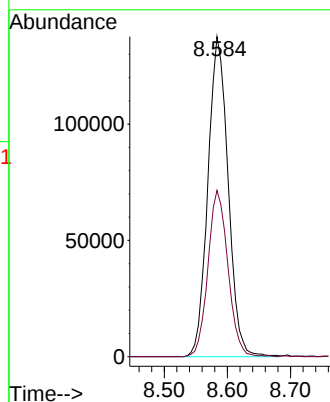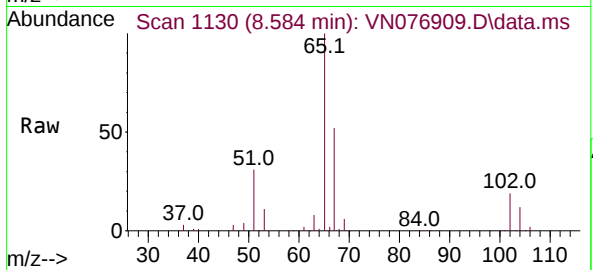

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.107 min Scan# 1219

Delta R.T. 0.000 min

Lab File: VN076909.D

Acq: 09 Mar 2023 18:04




Tgt Ion: 114 Resp: 754094


Ion Ratio Lower Upper

114 100

63 21.1 0.0 36.6

88 16.7 0.0 28.6

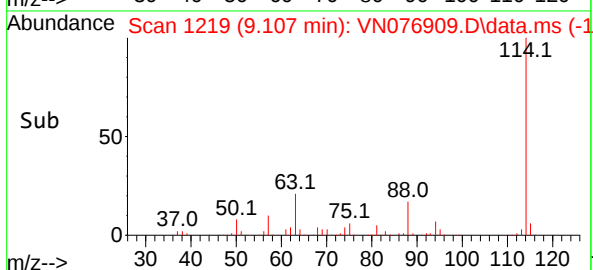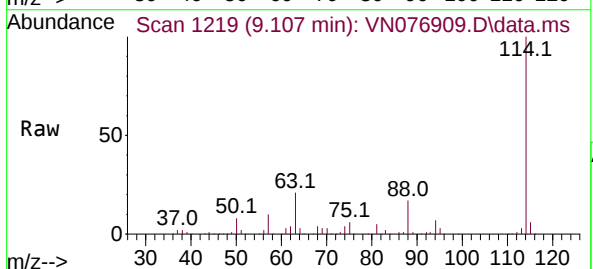

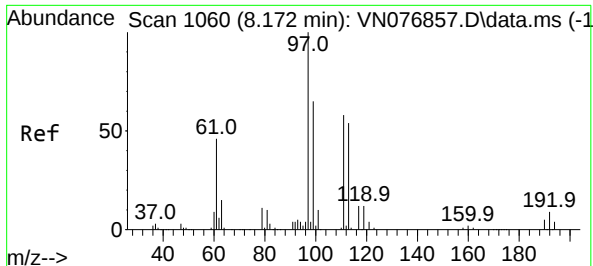

#35

Dibromofluoromethane

Concen: 49.717 ug/l

RT: 8.172 min Scan# 1060

Delta R.T. -0.000 min

Lab File: VN076909.D

Acq: 09 Mar 2023 18:04

Instrument :

MSVOA_N

ClientSampleId :

PB151321ZHE#02





Tgt Ion:113 Resp: 234537

Ion Ratio Lower Upper

113 100

111 102.1 81.8 122.8

192 17.8 13.9 20.9

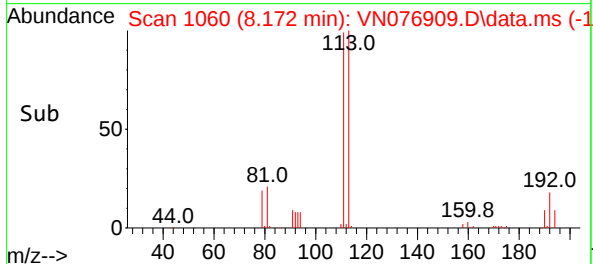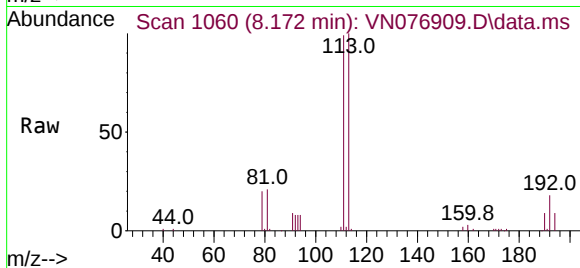

#36

1,1-Dichloropropene

Concen: 5.129 ug/l

RT: 8.237 min Scan# 1071

Delta R.T. -0.141 min

Lab File: VN076909.D

Acq: 09 Mar 2023 18:04




Tgt Ion: 75 Resp: 38891


Ion Ratio Lower Upper

75 100

110 9.7 18.9 56.9#

77 0.0 24.9 37.3#

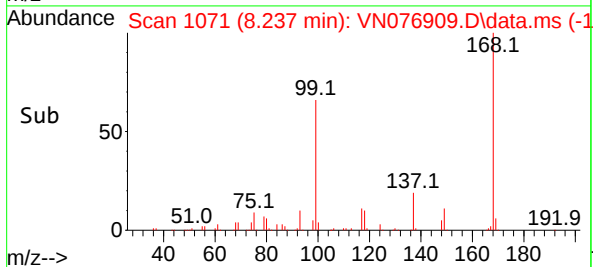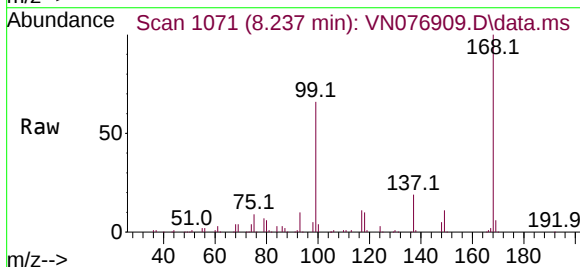

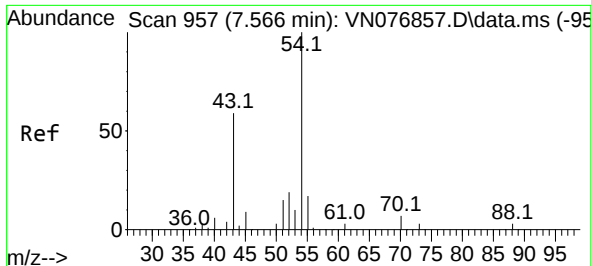

#37

Ethyl Acetate

Concen: 10.496 ug/l

RT: 7.572 min Scan# 91

Delta R.T. 0.006 min

Lab File: VN076909.D

Acq: 09 Mar 2023 18:04

Instrument :

MSVOA_N

ClientSampleId :

PB151321ZHE#02





Tgt Ion: 43 Resp: 81689

Ion Ratio Lower Upper

43 100

61 14.9 13.5 20.3

70 12.9 11.0 16.6

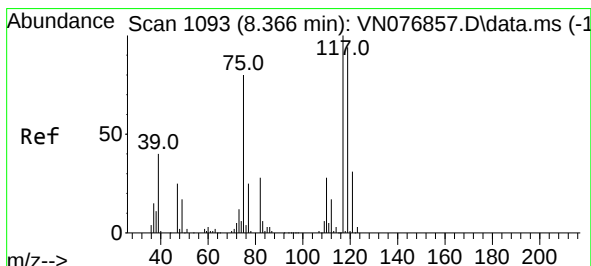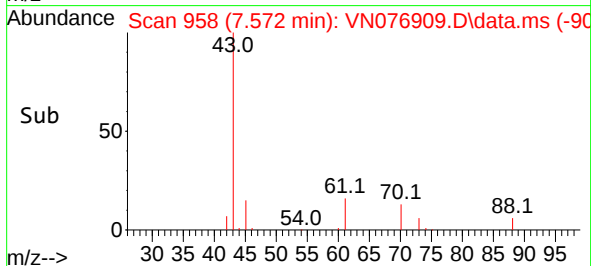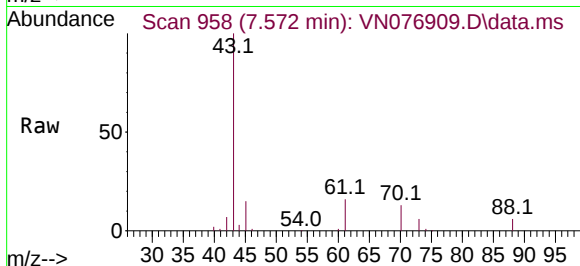

#38

Carbon Tetrachloride

Concen: 6.549 ug/l

RT: 8.231 min Scan# 1070

Delta R.T. -0.135 min

Lab File: VN076909.D

Acq: 09 Mar 2023 18:04




Tgt Ion: 117 Resp: 50443


Ion Ratio Lower Upper

117 100

119 5.5 76.9 115.3#

121 0.0 23.2 34.8#


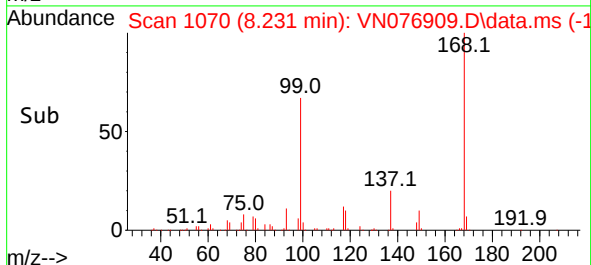
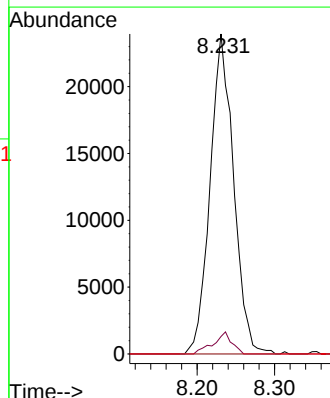
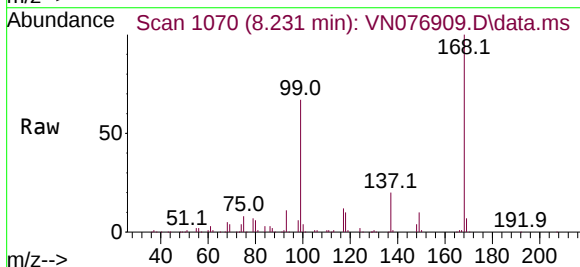


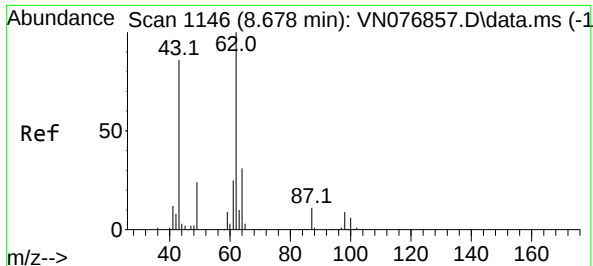

#42
1,2-Dichloroethane
Concen: 0.362 ug/l
RT: 8.695 min Scan# 1149
Delta R.T. 0.017 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
PB151321ZHE#02


Tgt Ion: 62 Resp: 2911
Ion Ratio Lower Upper
62 100
98 0.0 0.0 21.8

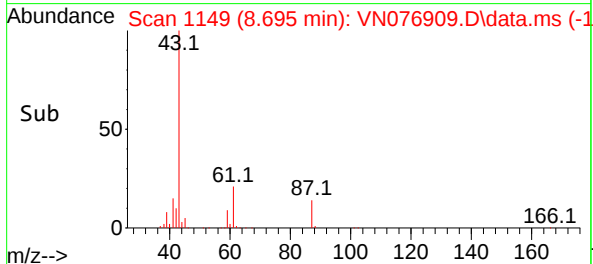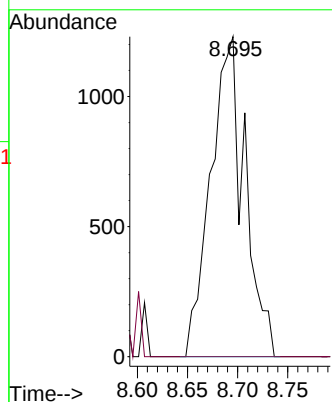

#43
Isopropyl Acetate
Concen: 32.072 ug/l
RT: 8.695 min Scan# 1149
Delta R.T. 0.000 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04

Tgt Ion: 43 Resp: 382116
Ion Ratio Lower Upper
43 100
61 20.4 26.2 39.2#
87 13.6 14.8 22.2#

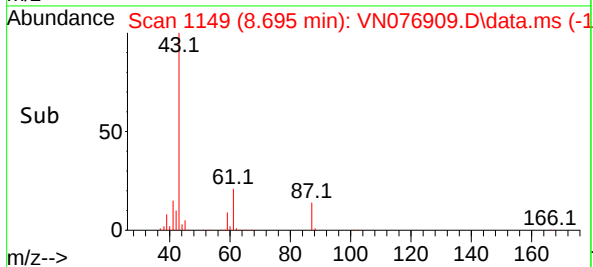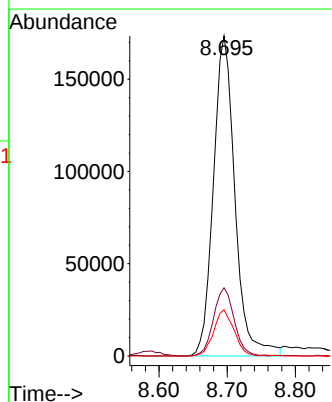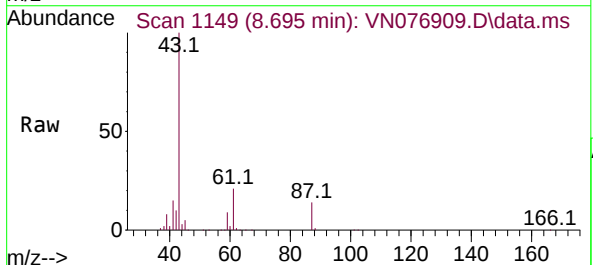

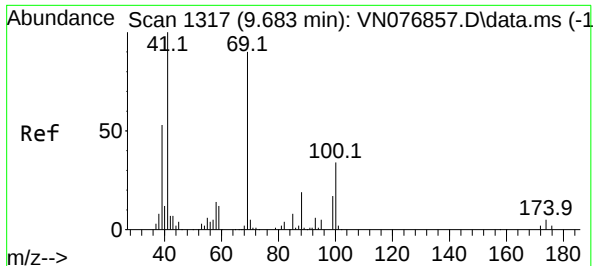

#48

Methyl methacrylate

Concen: 1.641 ug/l

RT: 9.672 min Scan# 1315

Delta R.T. -0.011 min

Lab File: VN076909.D

Acq: 09 Mar 2023 18:04

Instrument :

MSVOA_N

ClientSampleId :

PB151321ZHE#02





Tgt Ion: 41 Resp: 9500

Ion Ratio Lower Upper

41 100

69 0.7 92.6 139.0#

39 52.5 51.4 77.0

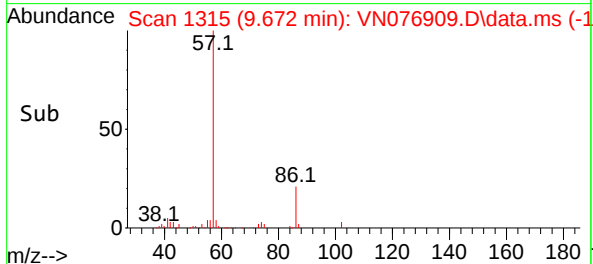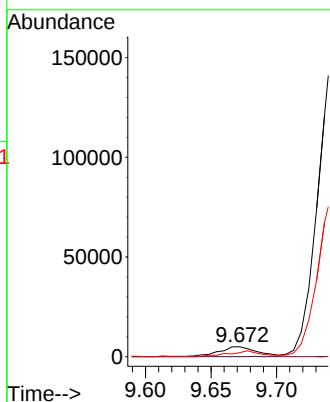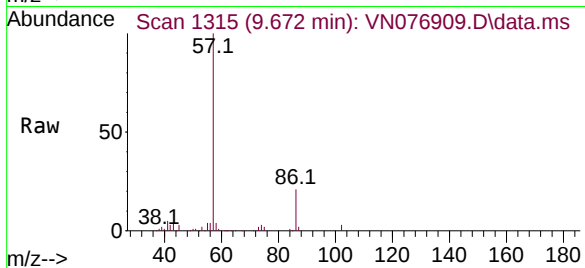

#49

1,4-Dioxane

Concen: 0.547 ug/l

RT: 9.689 min Scan# 1318

Delta R.T. -0.012 min

Lab File: VN076909.D

Acq: 09 Mar 2023 18:04




Tgt Ion: 88 Resp: 58


Ion Ratio Lower Upper

88 100

43 0.0 15.3 22.9#

58 14058.6 47.6 71.4#




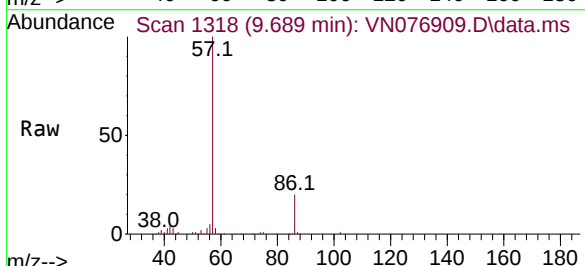




#50
Toluene-d8
Concen: 50.015 ug/l
RT: 10.572 min Scan# 1468
Delta R.T. -0.000 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
PB151321ZHE#02


Tgt Ion: 98 Resp: 909023
Ion Ratio Lower Upper
98 100
100 66.0 52.8 79.2

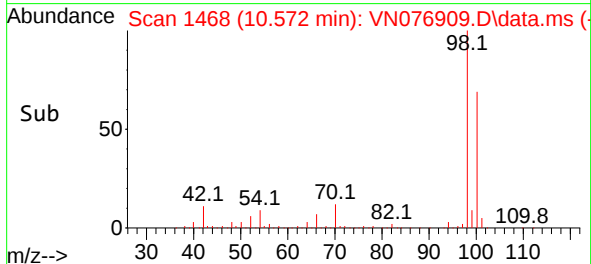

#51
4-Methyl-2-Pentanone
Concen: 2.051 ug/l
RT: 10.448 min Scan# 1447
Delta R.T. 0.000 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04

Tgt Ion: 43 Resp: 15417
Ion Ratio Lower Upper
43 100
58 42.0 37.4 56.0


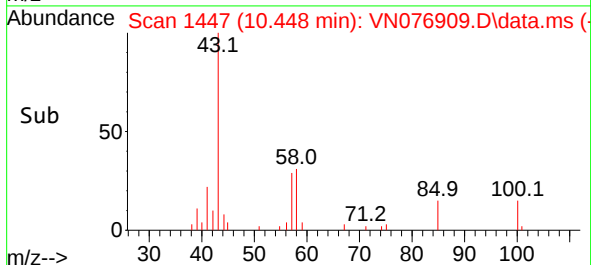

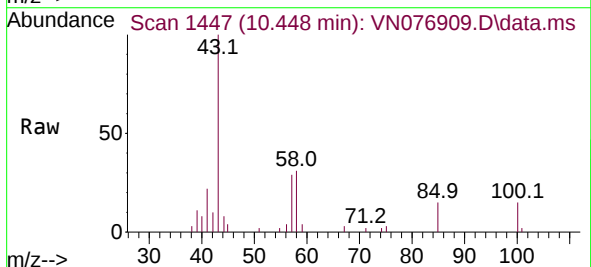


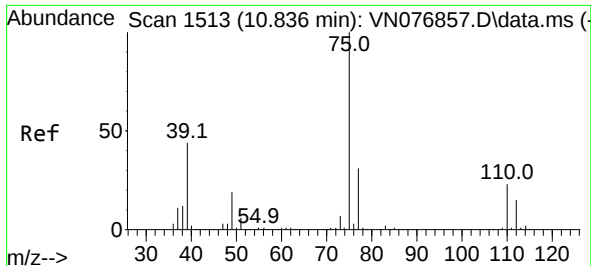

#53
t-1,3-Dichloropropene
Concen: 0.375 ug/l
RT: 10.736 min Scan# 1496
Delta R.T. -0.100 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
PB151321ZHE#02


Tgt Ion: 75 Resp: 2831
Ion Ratio Lower Upper
75 100
77 9.7 25.0 37.6#

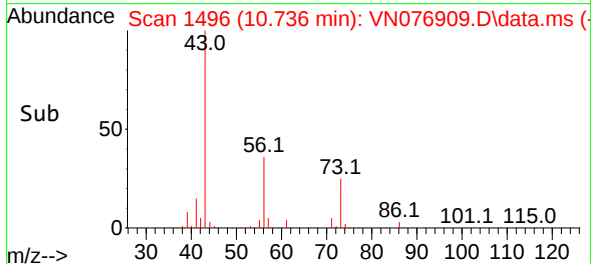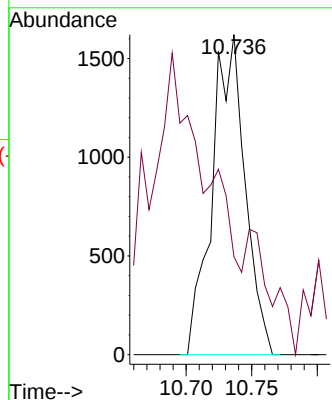

#54
cis-1,3-Dichloropropene
Concen: 16.650 ug/l
RT: 10.360 min Scan# 1432
Delta R.T. 0.047 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04

Tgt Ion: 75 Resp: 144476
Ion Ratio Lower Upper
75 100
77 0.5 25.7 38.5#
39 27.3 29.7 44.5#


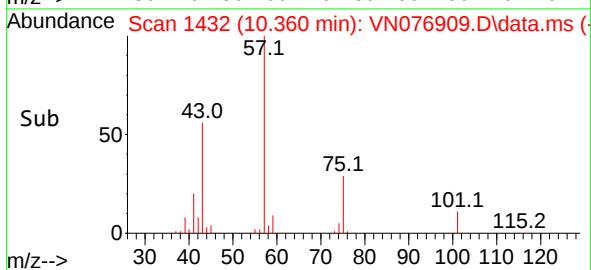
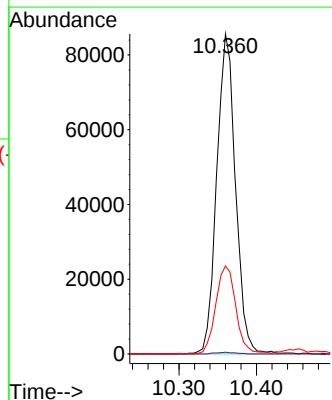
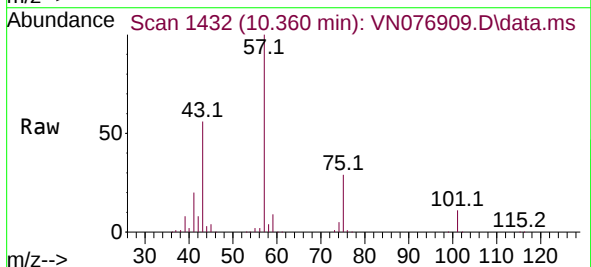


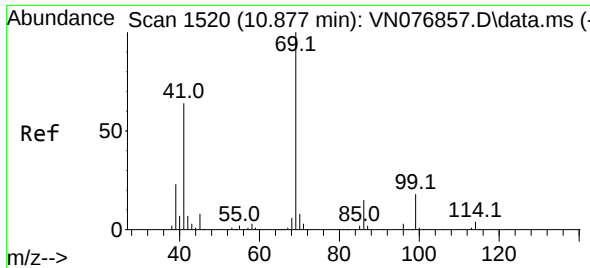

#56
Ethyl methacrylate
Concen: 0.443 ug/l
RT: 10.995 min Scan# 1540
Delta R.T. 0.118 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
PB151321ZHE#02


Tgt Ion: 69 Resp: 3611
Ion Ratio Lower Upper
69 100
41 5134.2 38.0 57.0#
39 2078.9 22.4 33.6#

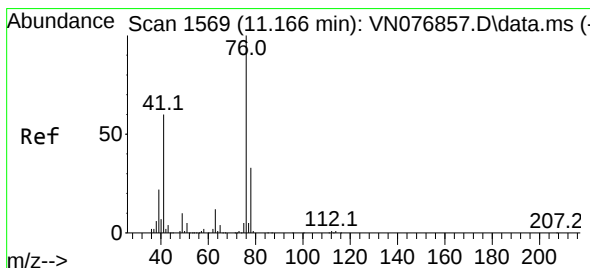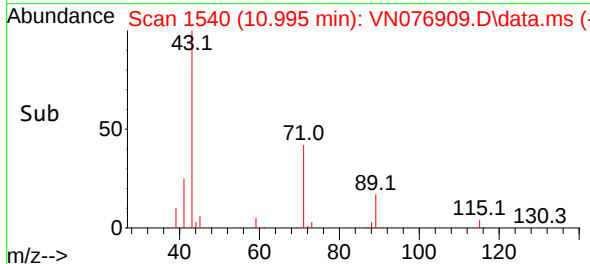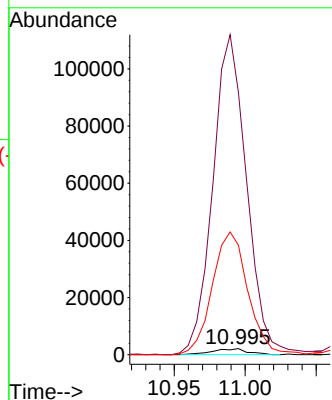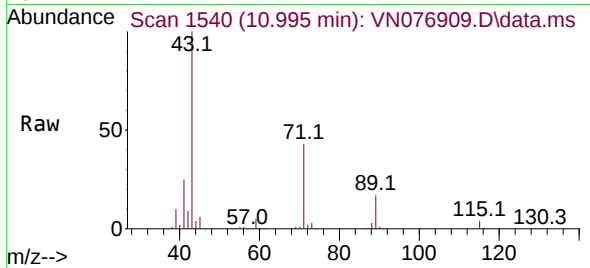

#57
1,3-Dichloropropane
Concen: 2.053 ug/l
RT: 11.201 min Scan# 1575
Delta R.T. 0.035 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04

Tgt Ion: 76 Resp: 19505
Ion Ratio Lower Upper
76 100
78 0.0 26.1 39.1#


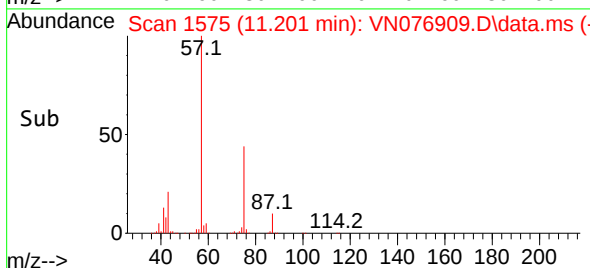
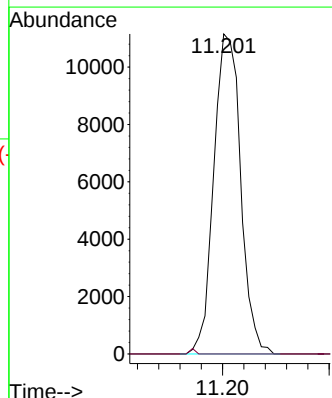
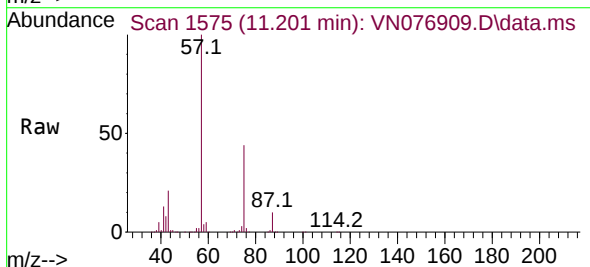




#59
2-Hexanone
Concen: 58.885 ug/l
RT: 11.172 min Scan# 11
Delta R.T. -0.023 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
PB151321ZHE#02


Tgt Ion: 43 Resp: 320661
Ion Ratio Lower Upper
43 100
58 0.0 32.6 98.0#

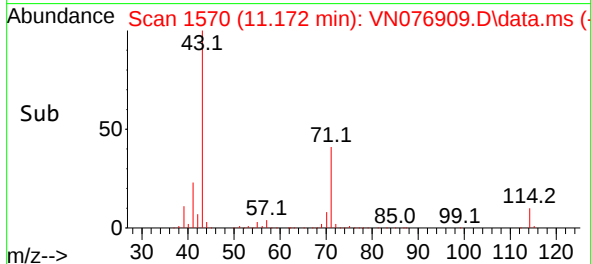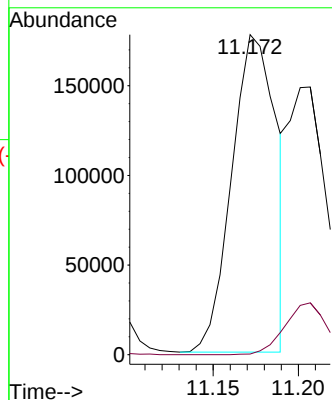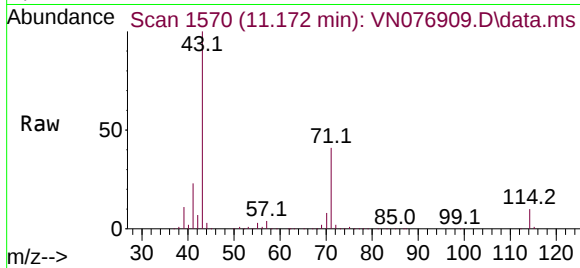

#62
4-Bromofluorobenzene
Concen: 50.902 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. -0.000 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04

Tgt Ion: 95 Resp: 320571
Ion Ratio Lower Upper
95 100
174 72.1 0.0 162.4
176 69.6 0.0 157.4


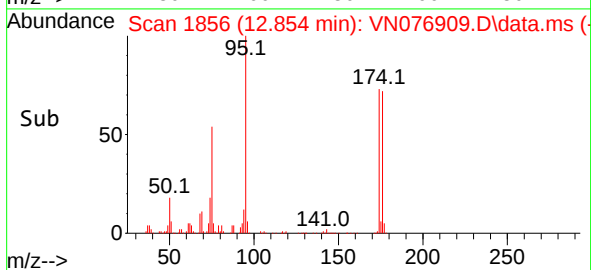
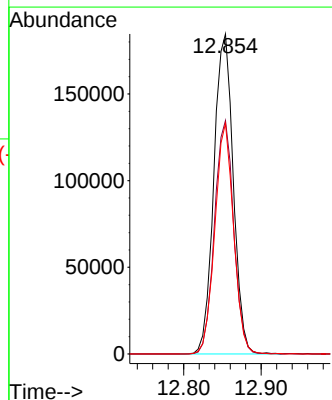
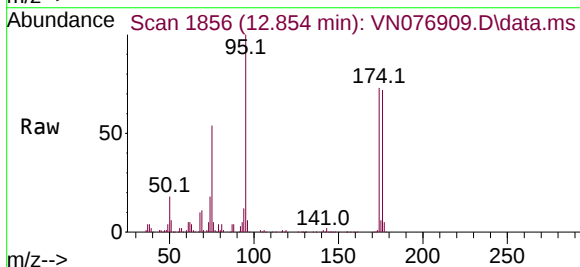


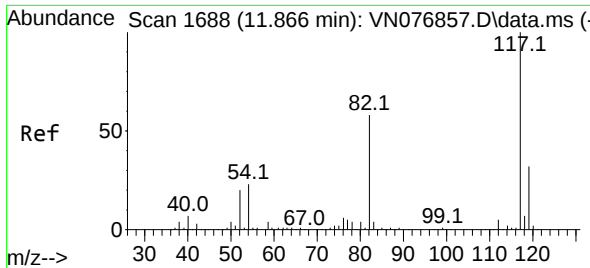

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.866 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
PB151321ZHE#02


Tgt Ion:117 Resp: 671057
Ion Ratio Lower Upper
117 100
82 58.7 43.5 65.3
119 31.0 25.5 38.3

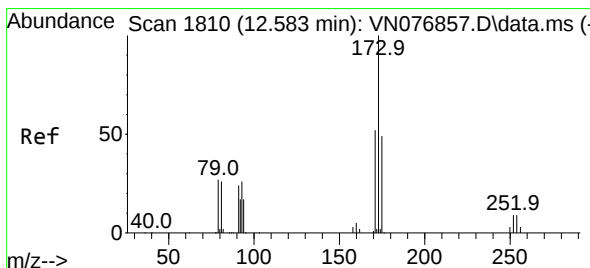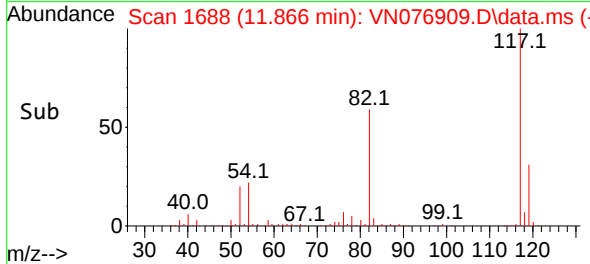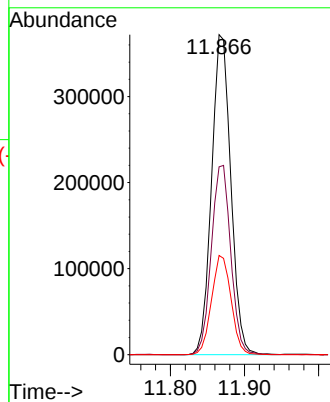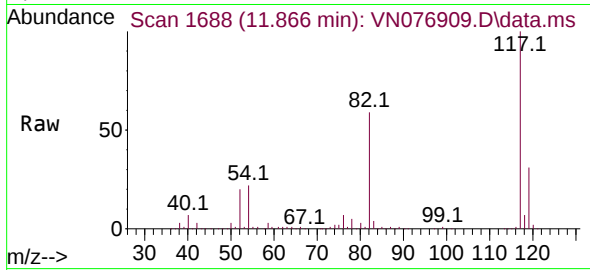

#71
Bromoform
Concen: 0.362 ug/l
RT: 12.848 min Scan# 1855
Delta R.T. 0.265 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04

Tgt Ion:173 Resp: 1293
Ion Ratio Lower Upper
173 100
175 1172.2 24.9 74.6#
254 0.0 0.0 0.0

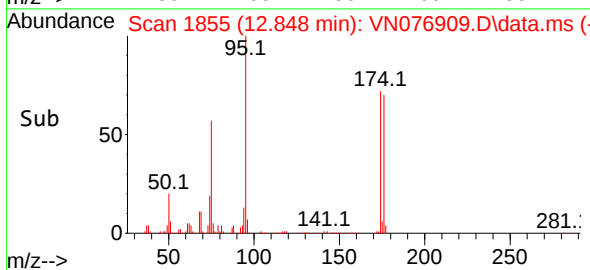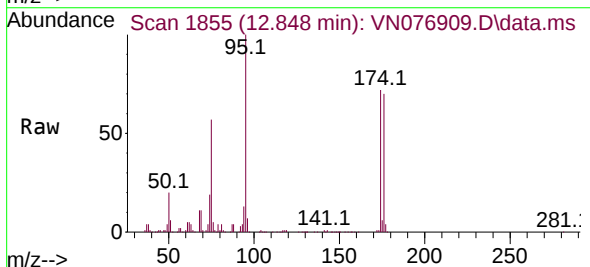



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.795 min Scan# 2016

Delta R.T. 0.000 min

Lab File: VN076909.D

Acq: 09 Mar 2023 18:04

Instrument :

MSVOA_N

ClientSampleId :

PB151321ZHE#02





Tgt Ion:152 Resp: 273298

Ion Ratio Lower Upper

152 100

115 65.1 30.3 90.9

150 158.6 0.0 353.6

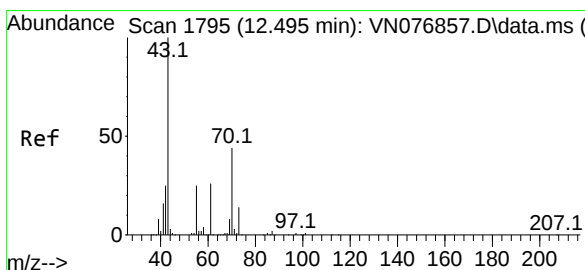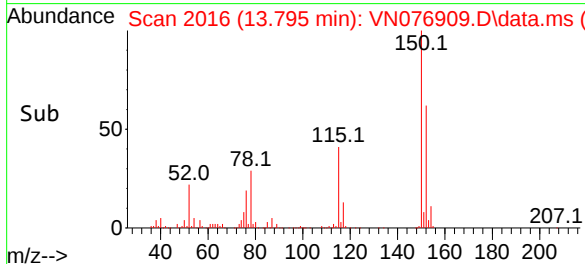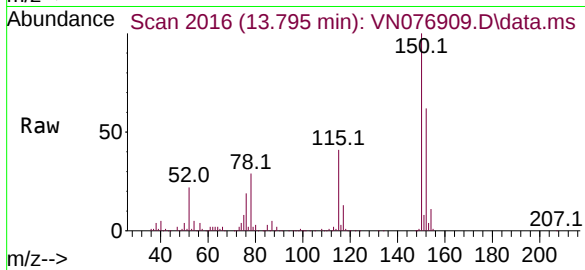

#74

N-ethyl acetate

Concen: 0.349 ug/l

RT: 12.495 min Scan# 1795

Delta R.T. 0.000 min

Lab File: VN076909.D

Acq: 09 Mar 2023 18:04

Tgt Ion: 43 Resp: 3255




Ion Ratio Lower Upper


43 100

70 12.6 46.8 70.2#

55 11.1 23.4 35.2#

61 0.0 23.8 35.8#


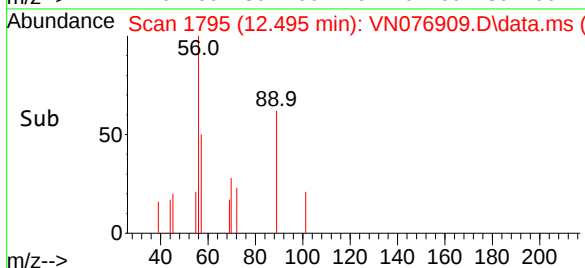
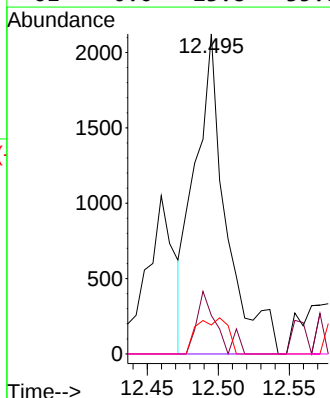
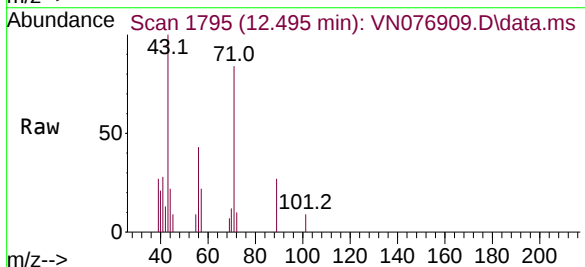


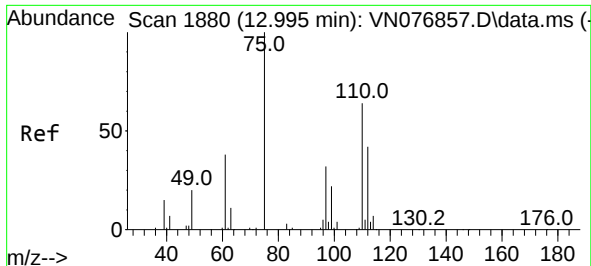

#76
1,2,3-Trichloropropane
Concen: 25.348 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. -0.141 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
PB151321ZHE#02


Tgt Ion: 75 Resp: 174713
Ion Ratio Lower Upper
75 100
77 1.2 93.8 281.4#

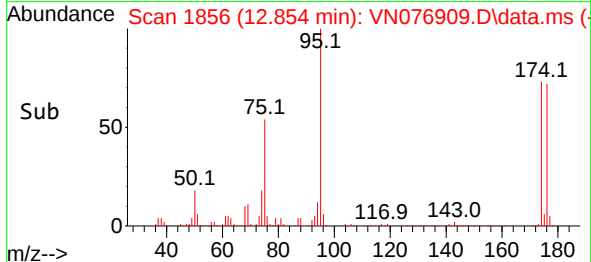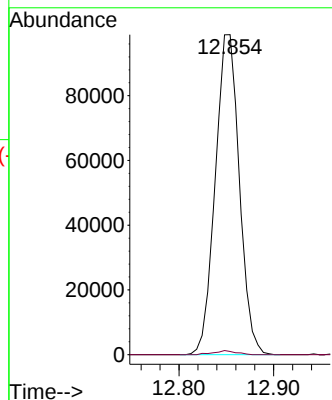

#81
trans-1,4-Dichloro-2-butene
Concen: 83.599 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. 0.112 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04

Tgt Ion: 75 Resp: 174713
Ion Ratio Lower Upper
75 100
53 0.0 67.4 101.0#
89 0.0 39.5 59.3#


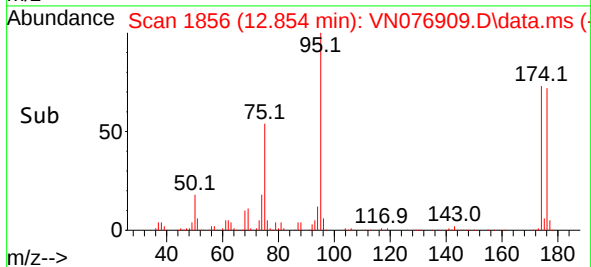
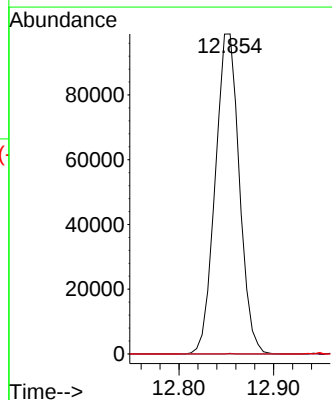
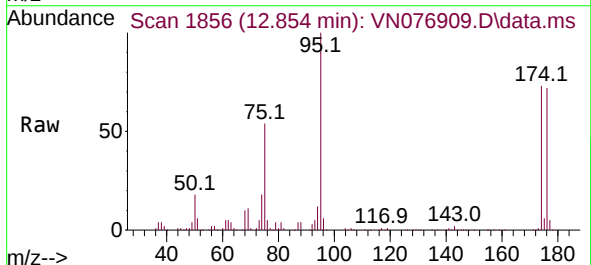


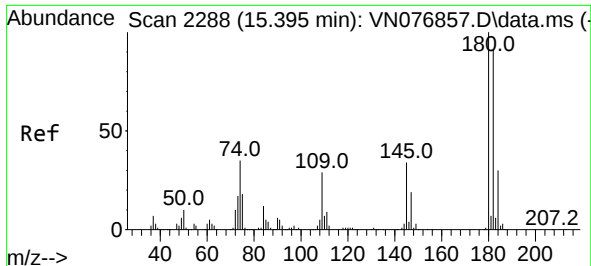

#93
1,2,4-Trichlorobenzene
Concen: 0.353 ug/l
RT: 15.401 min Scan# 21
Delta R.T. 0.006 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
PB151321ZHE#02


Tgt Ion:180 Resp: 1722
Ion Ratio Lower Upper
180 100
182 78.8 47.4 142.2
145 20.8 15.8 47.3

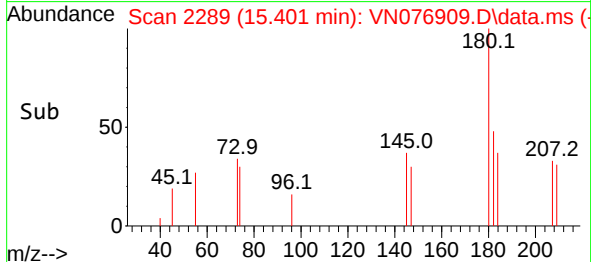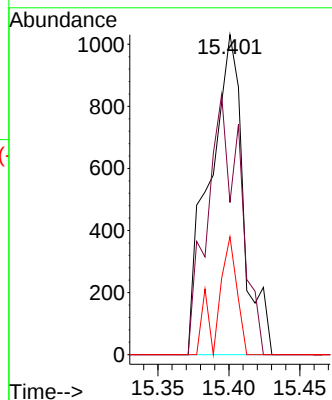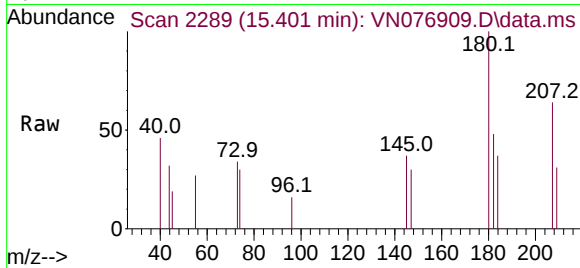

#95
Naphthalene
Concen: 0.354 ug/l
RT: 15.648 min Scan# 2331
Delta R.T. 0.006 min
Lab File: VN076909.D
Acq: 09 Mar 2023 18:04

Tgt Ion:128 Resp: 5532
Ion Ratio Lower Upper
128 100
127 11.8 10.2 15.4
129 6.8 8.9 13.3#

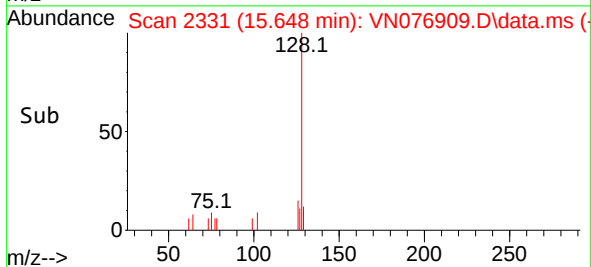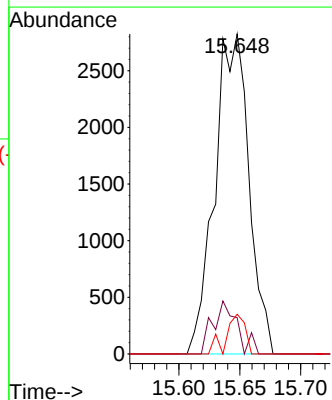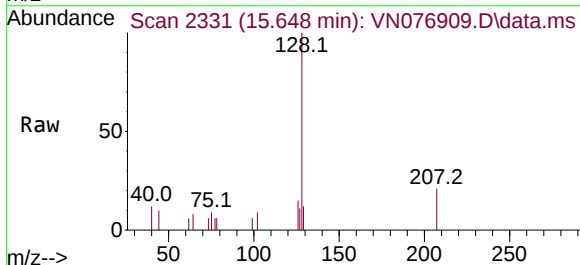

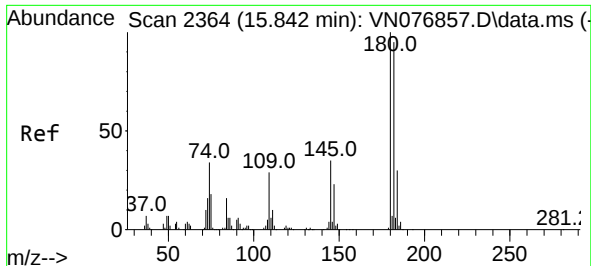

#96
 1,2,3-Trichlorobenzene
 Concen: 0.279 ug/l
 RT: 15.842 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN076909.D
 Acq: 09 Mar 2023 18:04

Instrument :
 MSVOA_N
 ClientSampleId :
 PB151321ZHE#02

Tgt Ion:180 Resp: 1337
 Ion Ratio Lower Upper
 180 100
 182 107.0 47.7 143.1
 145 44.0 17.0 51.0

