
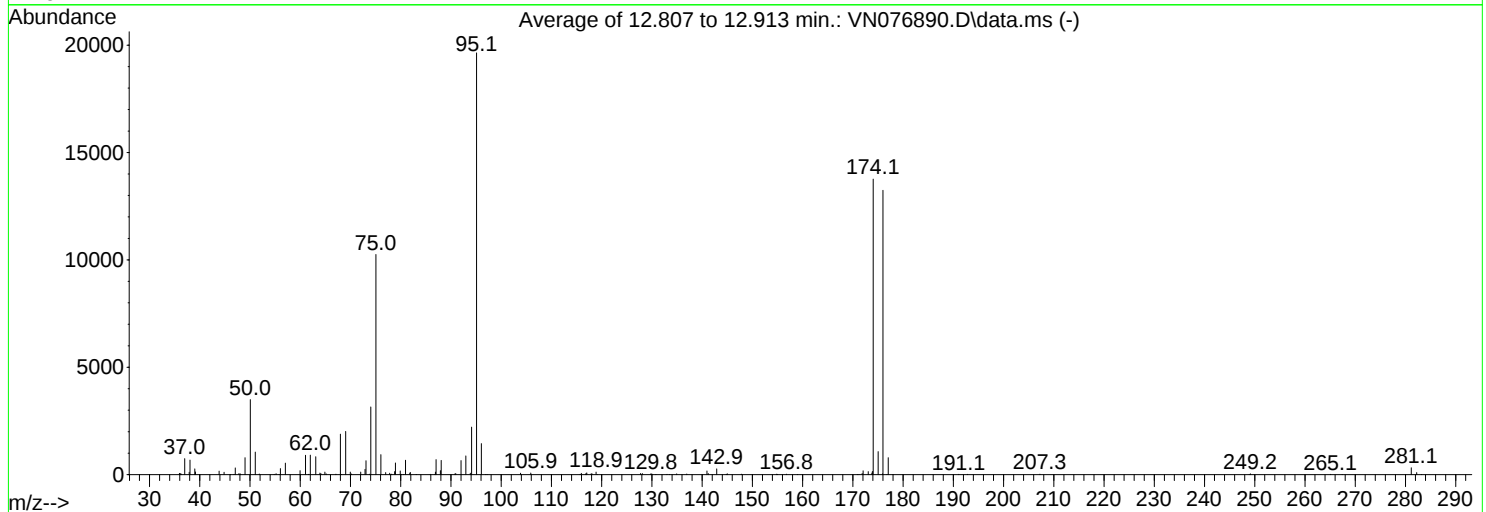


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030923\
Data File : VN076890.D
Acq On : 09 Mar 2023 08:25
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N030823W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Mar 09 04:16:54 2023

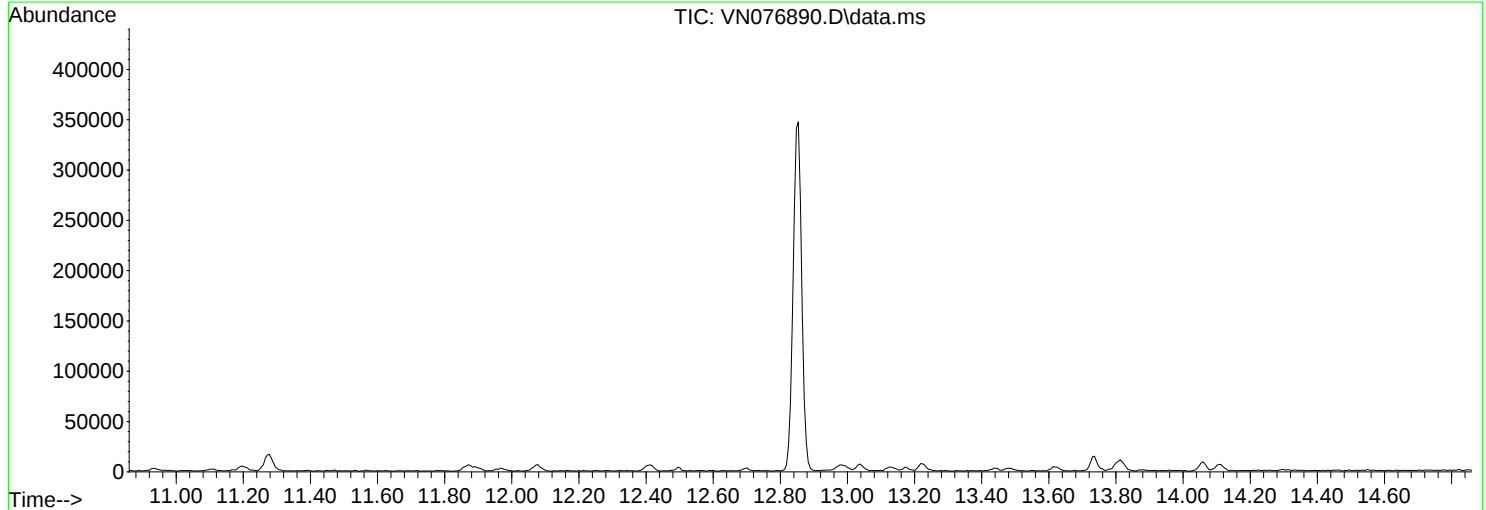

AutoFind: Averaged scan 1848 to 1866; Bkg corrected with scan 1847

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.8	3494	PASS
75	95	30	60	52.2	10250	PASS
95	95	100	100	100.0	19641	PASS
96	95	5	9	7.4	1446	PASS
173	174	0.00	2	1.0	139	PASS
174	95	50	100	70.1	13762	PASS
175	174	5	9	7.8	1073	PASS
176	174	95	101	96.2	13237	PASS
177	176	5	9	6.0	791	PASS