
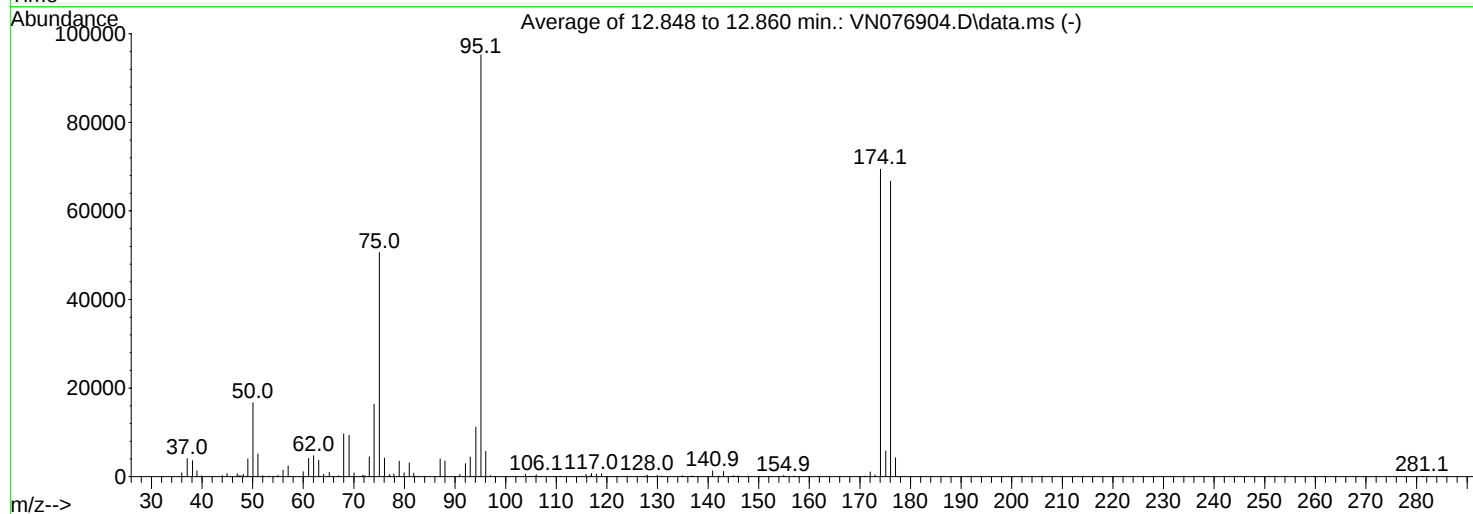


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030923\
Data File : VN076904.D
Acq On : 09 Mar 2023 15:42
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030623W.M
Title : SW846 8260
Last Update : Tue Mar 07 08:45:33 2023

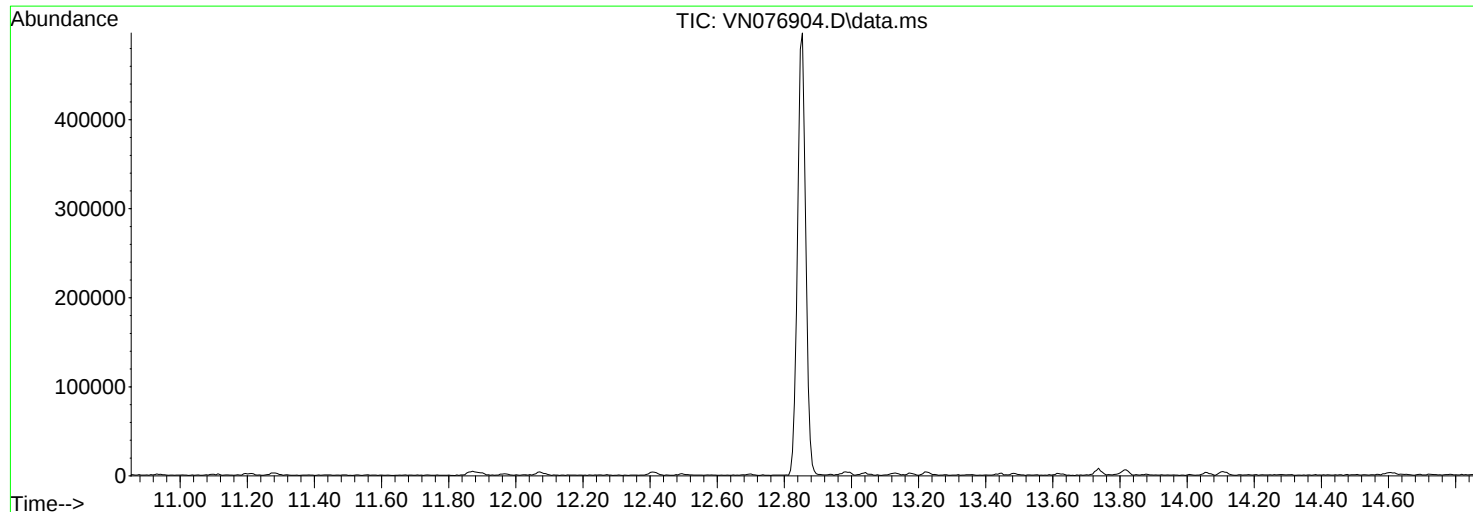

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1847

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	16689	PASS
75	95	30	60	53.2	50637	PASS
95	95	100	100	100.0	95253	PASS
96	95	5	9	6.0	5707	PASS
173	174	0.00	2	0.6	390	PASS
174	95	50	100	72.9	69419	PASS
175	174	5	9	8.3	5784	PASS
176	174	95	101	96.1	66688	PASS
177	176	5	9	6.4	4265	PASS

Average of 12.848 to 12.860 min.: VN076904.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	856	49.05	3996	62.05	4731	72.20	151
37.05	4068	50.05	16689	63.05	3737	73.05	447
38.10	3624	51.05	5127	64.05	525	74.00	1635
39.00	1294	51.95	191	65.15	964	75.05	5063
39.95	174	52.20	92	65.80	80	76.05	4204
44.00	282	53.15	128	67.00	167	76.90	112
44.95	700	55.00	278	68.00	9645	77.10	493
46.95	653	56.00	1448	69.05	9312	77.90	621
47.30	254	57.00	2424	70.05	865	78.95	3488
47.70	229	60.00	1119	71.75	318	79.95	874
48.15	506	61.05	4133	72.00	195	80.95	3092

Average of 12.848 to 12.860 min.: VN076904.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.85	799	103.90	542	116.95	712	137.00	94
82.80	112	104.95	118	117.95	585	140.90	1317
87.05	4030	105.80	183	118.95	694	142.15	143
88.00	3553	106.05	418	127.70	145	143.05	1188
90.95	526	107.00	81	127.95	364	144.80	117
92.05	2934	109.90	60	128.70	71	145.10	240
93.00	4433	110.80	57	129.95	328	145.80	133
94.10	11179	114.80	86	130.80	130	146.10	121
95.10	95253	115.20	51	131.10	51	147.60	51
96.05	5707	115.90	500	134.90	261	147.90	149
97.00	250	116.70	190	136.75	155	148.10	78

Average of 12.848 to 12.860 min.: VN076904.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
149.90	63	177.05	4265				
154.90	241	281.10	92				
155.10	92	281.30	57				
156.90	88						
157.10	103						
171.00	136						
172.05	1033						
173.00	390						
174.05	69419						
175.10	5784						
176.05	66688						

Instrument :

MSVOA_N

ClientSampleId :

BFB