

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN031020\
 Data File : VN060424.D
 Acq On : 10 Mar 2020 18:02
 Operator : JC/MD
 Sample : PB127392ZHE#19
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB127392ZHE#19

Quant Time: Mar 11 07:36:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
 Quant Title : SW846 8260
 QLast Update : Thu Feb 27 13:52:50 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.64	168	205744	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.57	114	336721	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.40	117	319859	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	148381	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.00	65	132440	50.17	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.34%	
35) Dibromofluoromethane	7.57	113	98954	63.31	ug/l	0.00
Spiked Amount 50.000			Recovery	=	126.62%	
50) Toluene-d8	10.08	98	420307	53.13	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.26%	
62) 4-Bromofluorobenzene	12.40	95	156800	52.29	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.58%	
Target Compounds						
16) Acetone	3.79	43	6666	7.820	ug/l	99
20) Methylene Chloride	4.53	84	7445	3.180	ug/l	97
43) Isopropyl Acetate	8.14	43	56352	10.593	ug/l #	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN031020\
Data File : VN060424.D
Acq On : 10 Mar 2020 18:02
Operator : JC/MD
Sample : PB127392ZHE#19
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB127392ZHE#19

Quant Time: Mar 11 07:36:44 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
Quant Title : SW846 8260
QLast Update : Thu Feb 27 13:52:50 2020
Response via : Initial Calibration

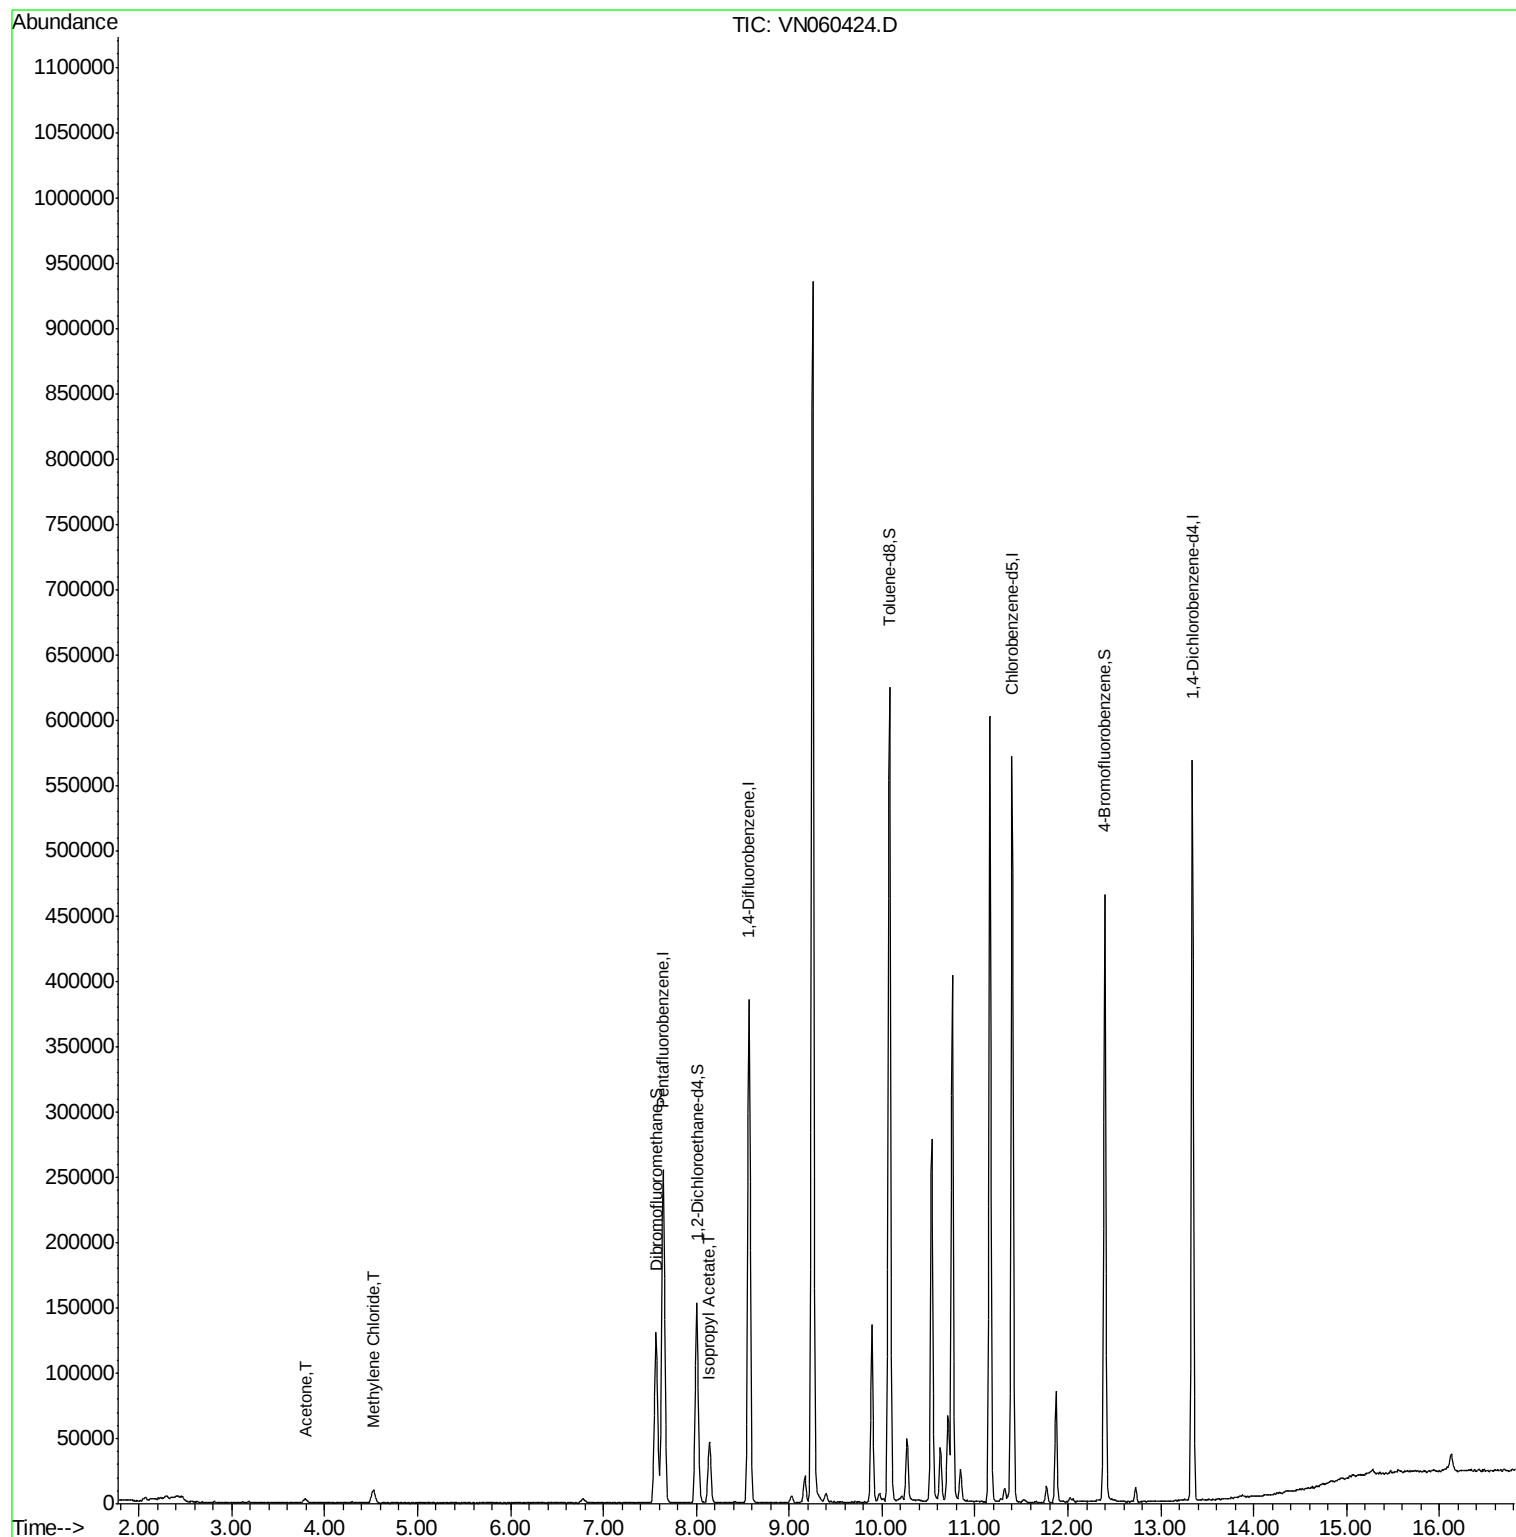



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.64 min Scan# 1826

Delta R.T. 0.00 min

Lab File: VN060424.D

Acq: 10 Mar 2020 18:02

Instrument :

MSVOA_N

ClientSampleId :


PB127392ZHE#19

Tot Ion:168 Resp: 205744

Ion Ratio Lower Upper




168 100

99 56.9 44.7 67.1

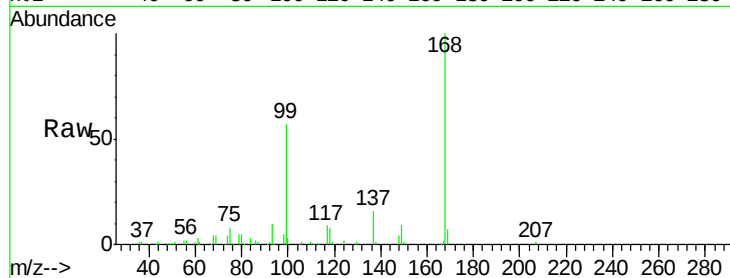

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

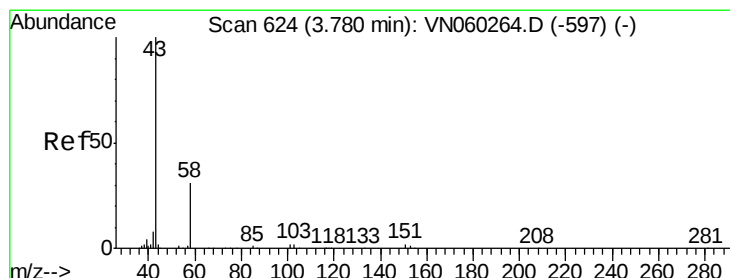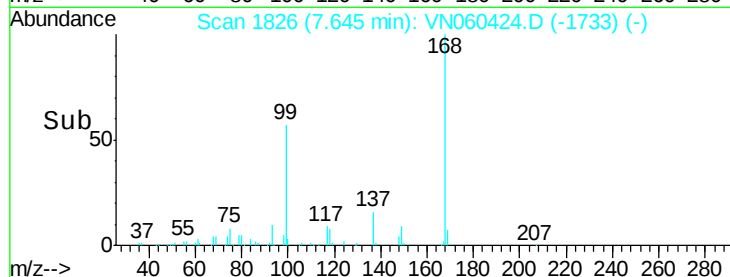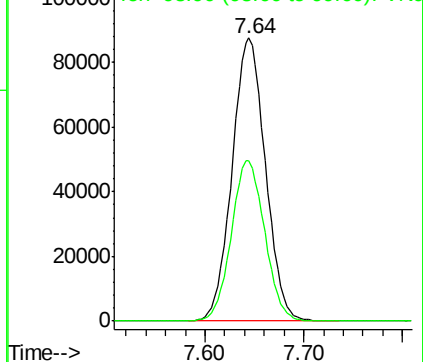

#16

Acetone

Concen: 7.820 ug/l

RT: 3.79 min Scan# 627

Delta R.T. 0.01 min

Lab File: VN060424.D


Acq: 10 Mar 2020 18:02

Tgt Ion: 43 Resp: 6666

Ion Ratio Lower Upper



43 100




58 30.2 24.6 36.8

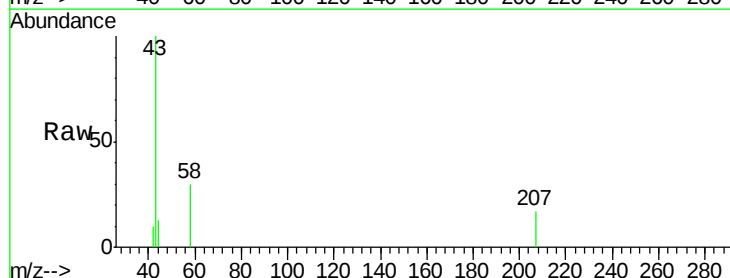

Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 58.00 (57.70 to 58.70): VNO



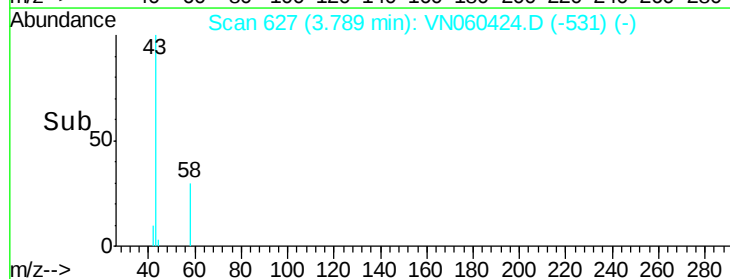
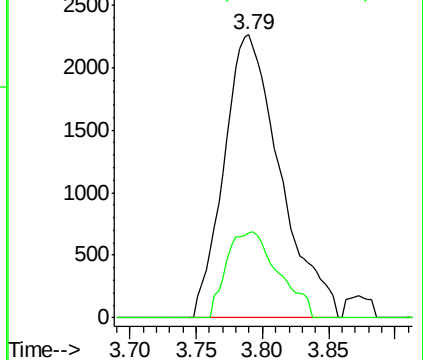


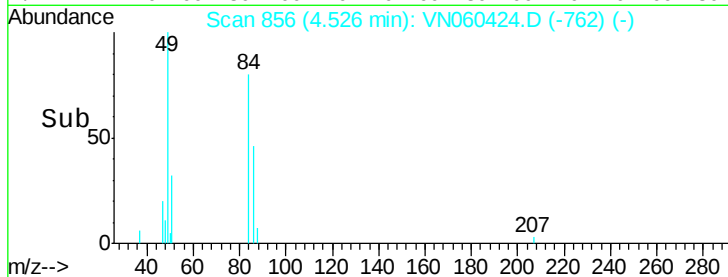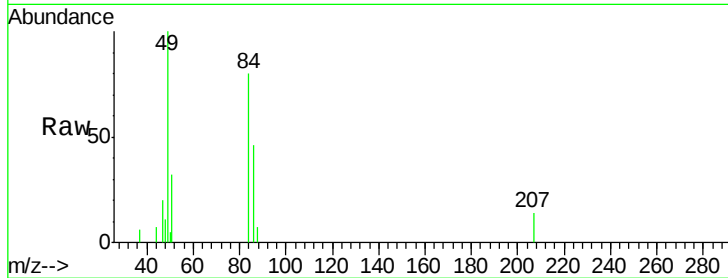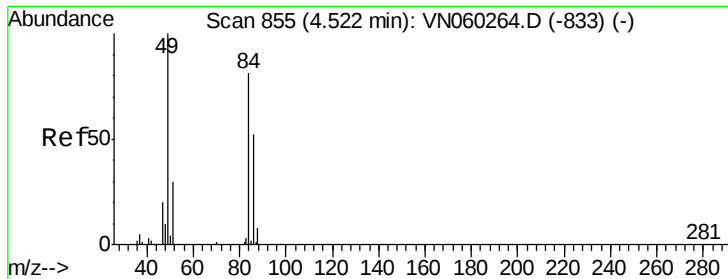

#20
Methylene Chloride
Concen: 3.180 ug/l
RT: 4.53 min Scan# 856
Delta R.T. 0.00 min
Lab File: VN060424.D
Acq: 10 Mar 2020 18:02


Instrument :
MSVOA_N
ClientSampleId :
PB127392ZHE#19


Tot Ion:	84	Resp:	7445
Ion	Ratio	Lower	Upper
84	100		
49	124.8	99.3	148.9
51	40.1	30.1	45.1
86	57.6	51.1	76.7

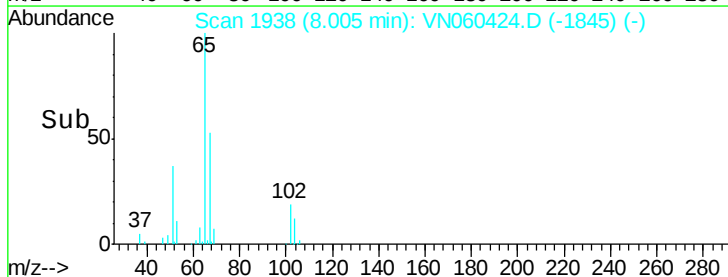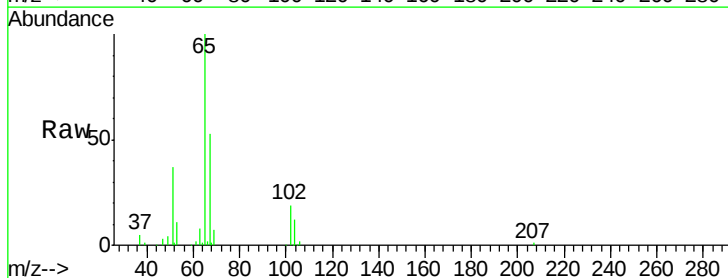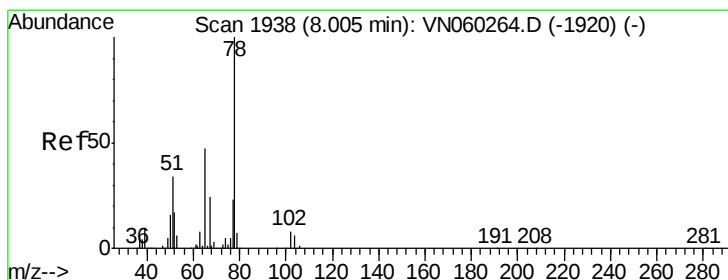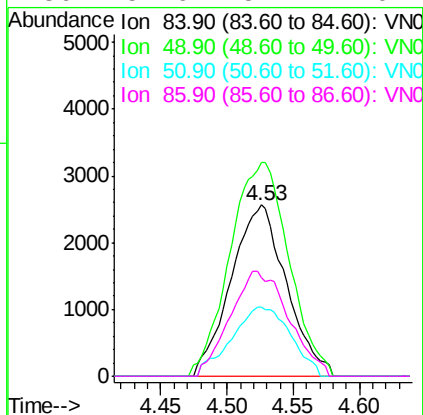

#33
1,2-Dichloroethane-d4
Concen: 50.172 ug/l
RT: 8.00 min Scan# 1938
Delta R.T. 0.00 min
Lab File: VN060424.D
Acq: 10 Mar 2020 18:02

Tgt Ion:	65	Resp:	132440
Ion	Ratio	Lower	Upper
65	100		
67	52.4	0.0	103.8

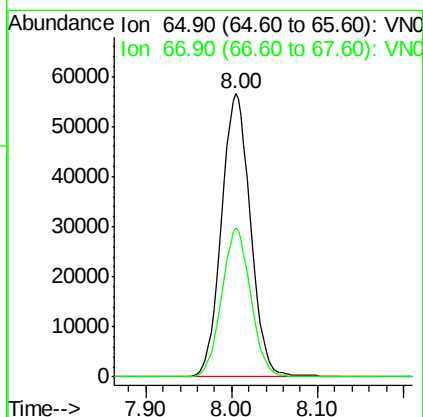

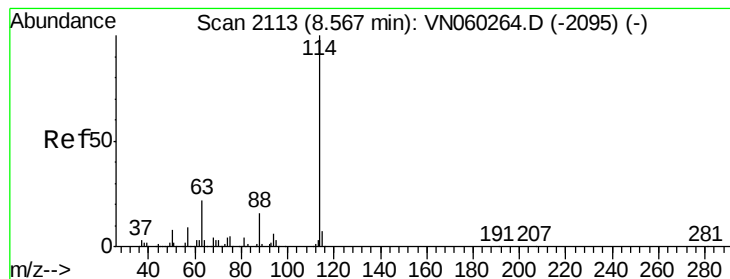

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.57 min Scan# 2113

Delta R.T. 0.00 min

Lab File: VN060424.D

Acq: 10 Mar 2020 18:02

Instrument :

MSVOA_N

ClientSampleId :

PB127392ZHE#19


Tot Ion:114 Resp: 336721

Ion Ratio Lower Upper

114 100

63 21.5 0.0 43.2




88 15.8 0.0 31.6

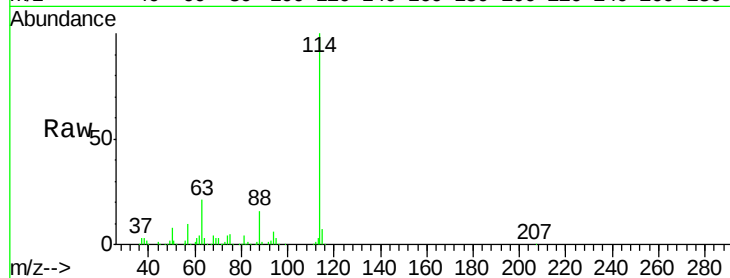

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

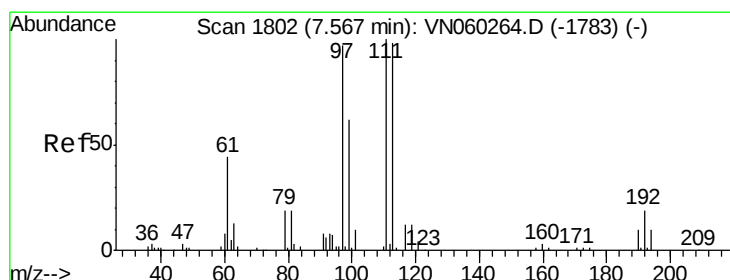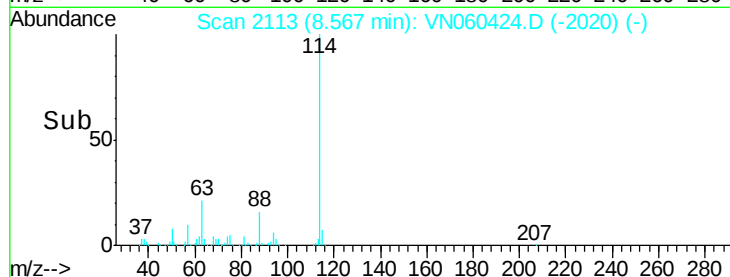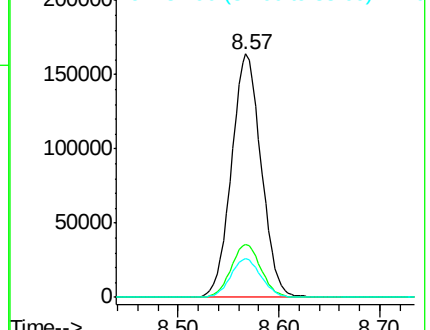

#35

Dibromofluoromethane

Concen: 63.312 ug/l

RT: 7.57 min Scan# 1802

Delta R.T. 0.00 min

Lab File: VN060424.D

Acq: 10 Mar 2020 18:02


Tgt Ion:113 Resp: 98954

Ion Ratio Lower Upper

113 100

111 104.2 82.4 123.6



192 20.0 16.2 24.2

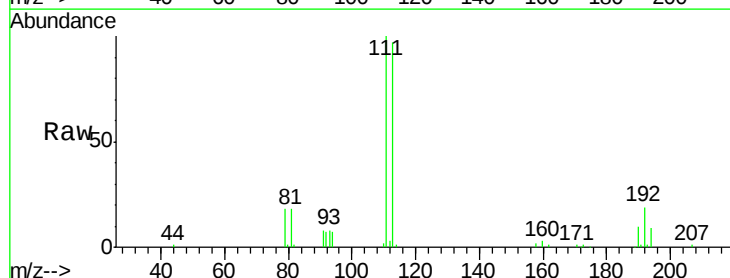


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

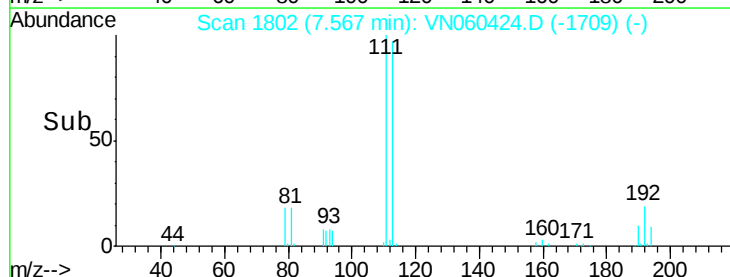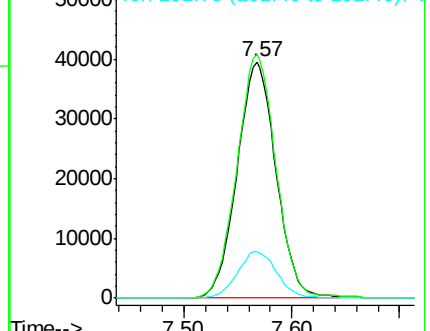

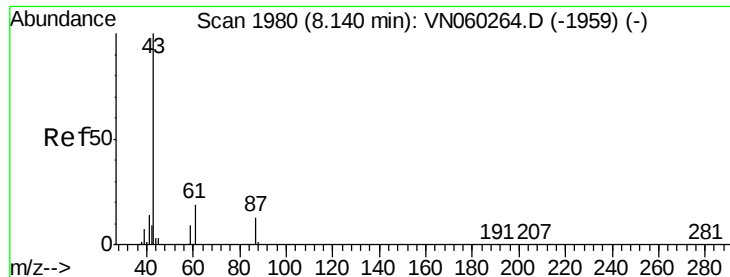

#43

Isopropyl Acetate

Concen: 10.593 ug/l

RT: 8.14 min Scan# 1980

Delta R.T. 0.00 min

Lab File: VN060424.D

Acq: 10 Mar 2020 18:02

Instrument :





MSVOA_N

ClientSampleId :

PB127392ZHE#19

Tot Ion: 43 Resp: 56352

Ion	Ratio	Lower	Upper
43	100		
61	19.4	20.9	31.3#
87	12.5	10.6	16.0

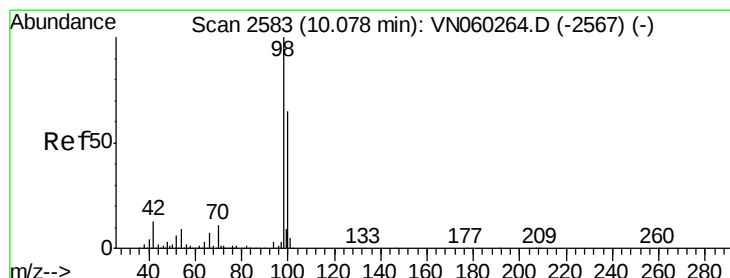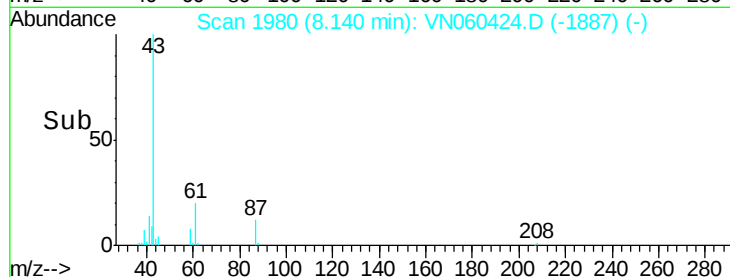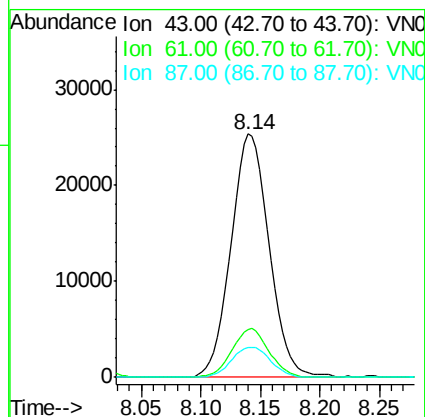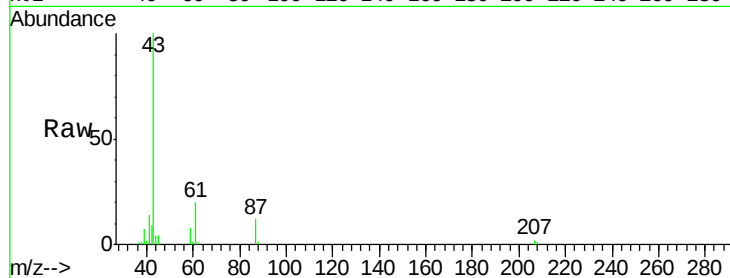

#50

Toluene-d8

Concen: 53.134 ug/l

RT: 10.08 min Scan# 2583




Delta R.T. 0.00 min


Lab File: VN060424.D

Acq: 10 Mar 2020 18:02

Tgt Ion: 98 Resp: 420307

Ion	Ratio	Lower	Upper
98	100		
100	64.6	52.2	78.2

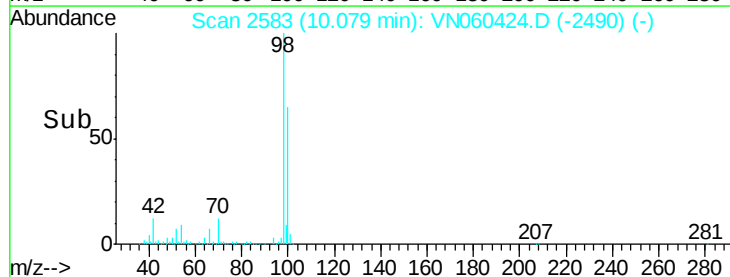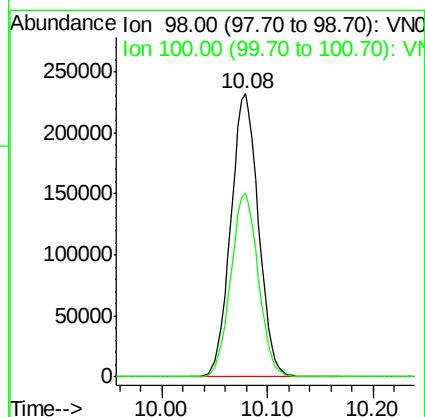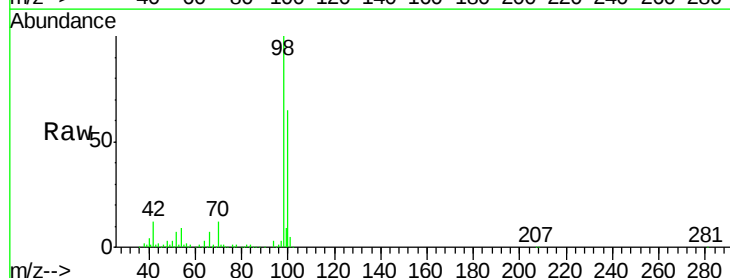

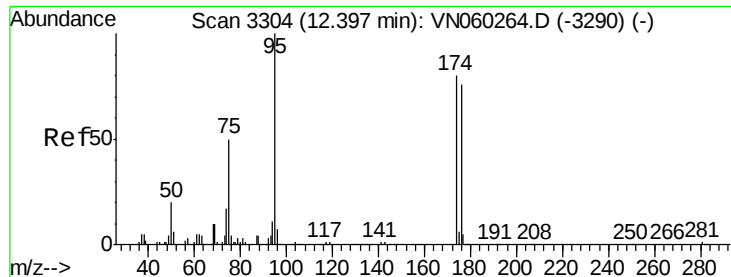

#62

4-Bromofluorobenzene

Concen: 52.291 ug/l

RT: 12.40 min Scan# 3304

Delta R.T. 0.00 min

Lab File: VN060424.D

Acq: 10 Mar 2020 18:02

Instrument :

MSVOA_N

ClientSampleId :

PB127392ZHE#19


Tot Ion: 95 Resp: 156800

Ion Ratio Lower Upper

95 100

174 79.4 0.0 159.2




176 77.3 0.0 153.8

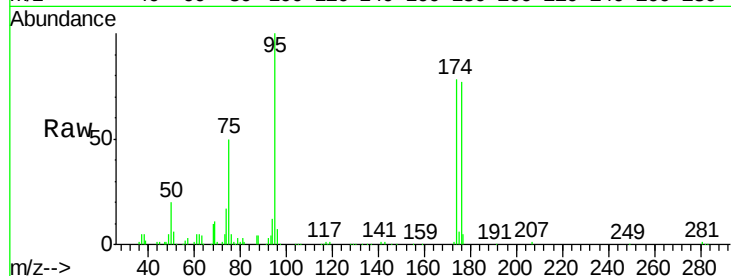

Abundance Ion 94.90 (94.60 to 95.60): VN060424.D (-3290) (-)

Ion 173.80 (173.50 to 174.50): VN060424.D (-3290) (-)

Ion 175.80 (175.50 to 176.50): VN060424.D (-3290) (-)

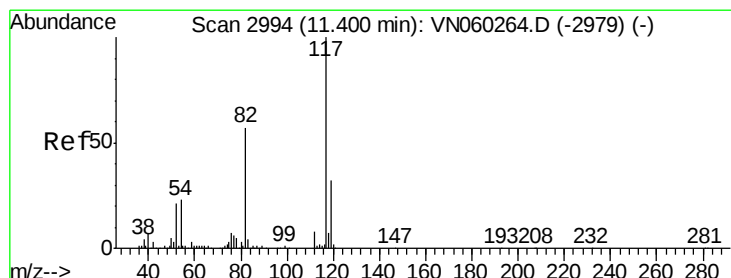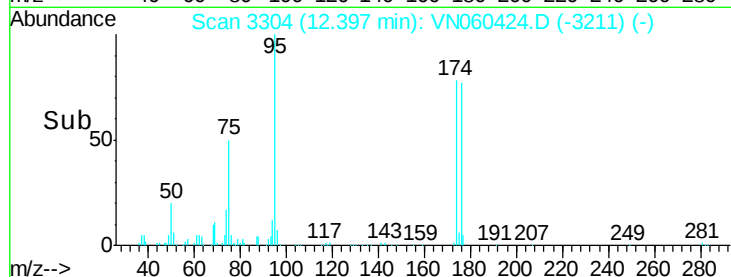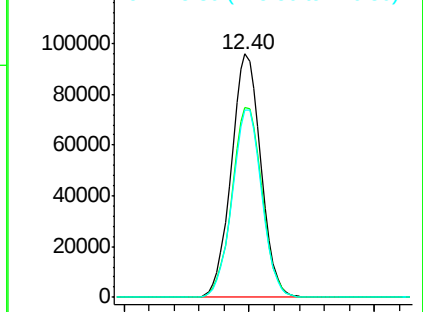

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.40 min Scan# 2994

Delta R.T. 0.00 min

Lab File: VN060424.D

Acq: 10 Mar 2020 18:02


Tgt Ion: 117 Resp: 319859

Ion Ratio Lower Upper

117 100

82 57.4 45.8 68.6



119 32.0 25.8 38.8

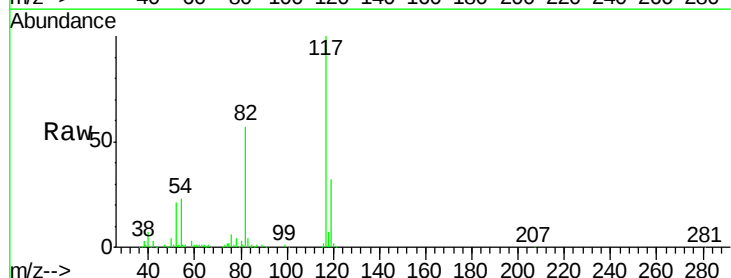


Abundance Ion 116.90 (116.60 to 117.60): VN060424.D (-2979) (-)

Ion 82.00 (81.70 to 82.70): VN060424.D (-2979) (-)

Ion 118.90 (118.60 to 119.60): VN060424.D (-2979) (-)

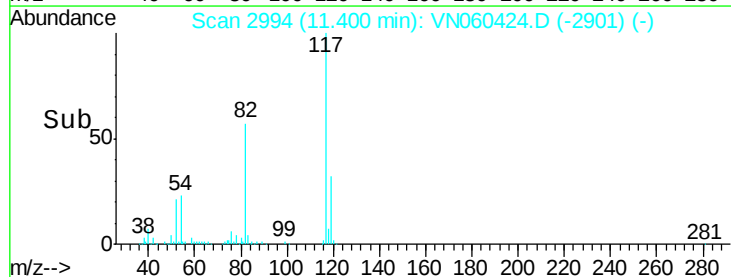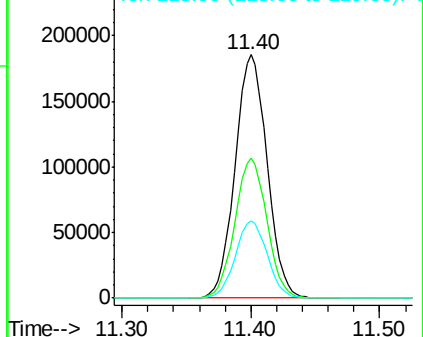

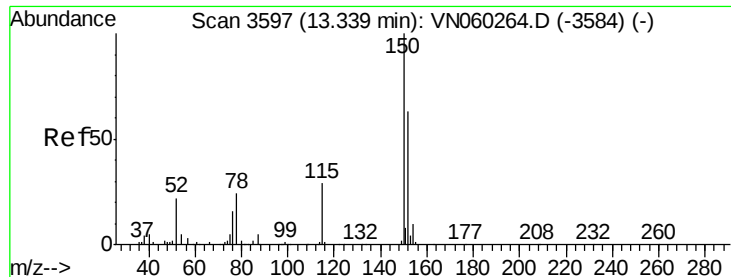

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.34 min Scan# 3597

Delta R.T. 0.00 min

Lab File: VN060424.D

Acq: 10 Mar 2020 18:02

Instrument :

MSVOA_N

ClientSampleId :

PB127392ZHE#19


Tot Ion:152 Resp: 148381

Ion Ratio Lower Upper

152 100

115 59.5 30.0 90.0

150 158.4 0.0 349.6

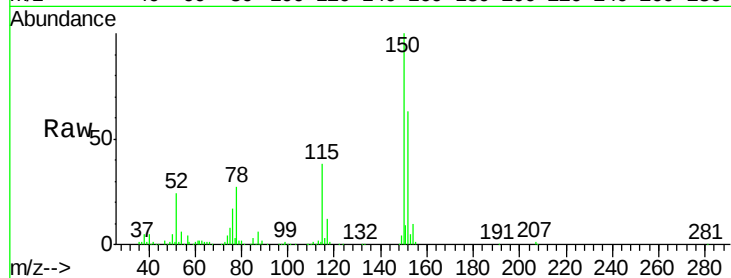

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

