

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031021\
 Data File : VN066166.D
 Acq On : 10 Mar 2021 15:14
 Operator : JC/MD
 Sample : MDL01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Mar 10 17:43:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030921W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 09 14:48:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.582	168	171744	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.512	114	290218	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.347	117	249371	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.286	152	98631	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.947	65	177446	54.75	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 109.50%			
35) Dibromofluoromethane	7.509	113	109037	55.07	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 110.14%			
50) Toluene-d8	10.028	98	407487	52.31	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 104.62%			
62) 4-Bromofluorobenzene	12.345	95	127002	43.80	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 87.60%			
Target Compounds						Qvalue
3) Chloromethane	2.017	50	1549	0.40	ug/l #	81
4) Vinyl Chloride	2.145	62	673	0.22	ug/l #	43
5) Bromomethane	2.529	94	479	0.29	ug/l #	54
10) Methyl Iodide	3.873	142	25	2.69	ug/l #	43
11) Tert butyl alcohol	4.715	59	133	0.24	ug/l #	73
13) Acrolein	3.532	56	5784	3.46	ug/l #	59
16) Acetone	3.744	43	4534	2.77	ug/l #	75
20) Methylene Chloride	4.444	84	689	0.29	ug/l	94
23) Vinyl Acetate	5.793	43	6827	0.73	ug/l #	71
28) Bromochloromethane	7.102	49	1245	0.44	ug/l #	23
29) Tetrahydrofuran	7.129	42	767	0.44	ug/l #	52
31) Cyclohexane	7.582	56	5369	1.15	ug/l #	37
36) 1,1-Dichloropropene	7.584	75	16241	4.92	ug/l #	49
38) Carbon Tetrachloride	7.584	117	17824	6.20	ug/l #	16
43) Isopropyl Acetate	8.086	43	1761	0.22	ug/l #	53
49) 1,4-Dioxane	9.135	88	158	4.30	ug/l #	56
51) 4-Methyl-2-Pentanone	9.918	43	4195	0.85	ug/l #	84
58) 2-Chloroethyl Vinyl ether	9.628	63	1989	13.39	ug/l #	64
59) 2-Hexanone	10.693	43	1544	0.44	ug/l	93
64) Tetrachloroethene	10.572	164	517	0.25	ug/l #	81
68) m/p-Xylenes	11.567	106	1240	0.35	ug/l	75
74) N-amyl acetate	12.031	43	276	3.02	ug/l #	42
76) 1,2,3-Trichloropropane	12.345	75	70429	23.83	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.345	75	70429	74.39	ug/l #	12
82) 4-Chlorotoluene	12.720	91	1420	0.25	ug/l #	54
83) tert-Butylbenzene	12.940	119	1170	0.21	ug/l	89
85) sec-Butylbenzene	13.120	105	1456	0.20	ug/l #	77
87) 1,3-Dichlorobenzene	13.230	146	718	0.22	ug/l	88
88) 1,4-Dichlorobenzene	13.230	146	718	0.22	ug/l	90
92) 1,2-Dibromo-3-Chloropr...	14.214	75	230	0.33	ug/l #	1
93) 1,2,4-Trichlorobenzene	14.855	180	336	2.36	ug/l #	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031021\
Data File : VN066166.D
Acq On : 10 Mar 2021 15:14
Operator : JC/MD
Sample : MDL01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Mar 10 17:43:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030921W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 09 14:48:21 2021
Response via : Initial Calibration




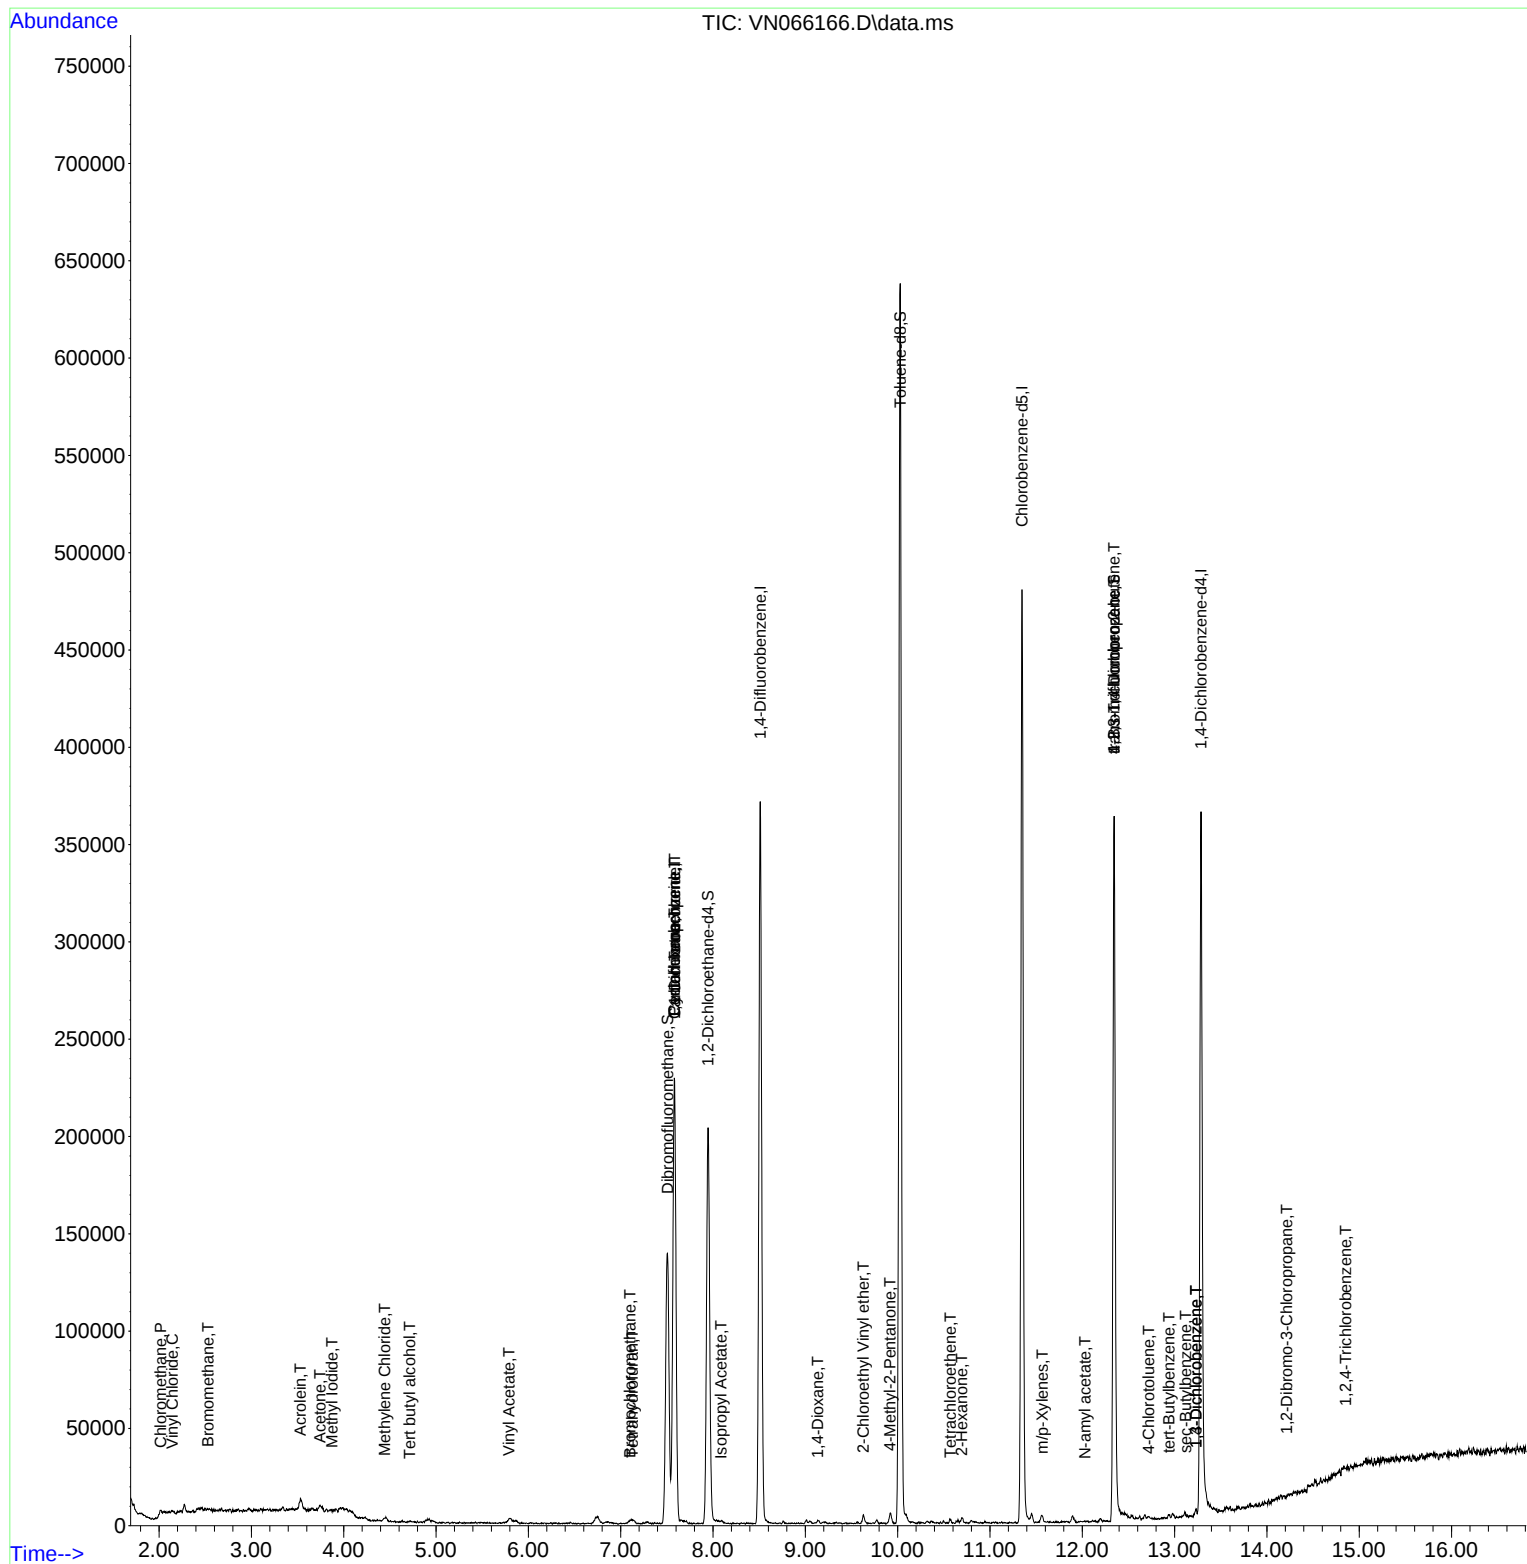




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.582 min Scan# 2197
Delta R.T. -0.008 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 171744
Ion Ratio Lower Upper
168 100
99 63.1 42.6 63.8

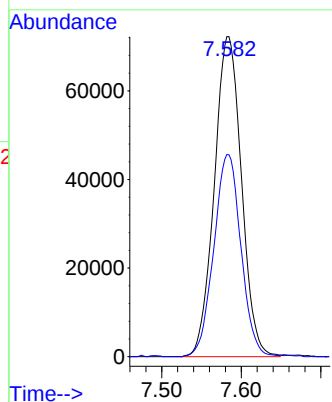

#3
Chloromethane
Concen: 0.40 ug/l
RT: 2.017 min Scan# 122
Delta R.T. -0.000 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14

Tgt Ion: 50 Resp: 1549
Ion Ratio Lower Upper
50 100
52 42.8 25.8 38.8#









#4
 Vinyl Chloride
 Concen: 0.22 ug/l
 RT: 2.145 min Scan# 170
 Delta R.T. -0.006 min
 Lab File: VN066166.D
 Acq: 10 Mar 2021 15:14




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion: 62 Resp: 673
 Ion Ratio Lower Upper
 62 100
 64 0.0 25.1 37.7#

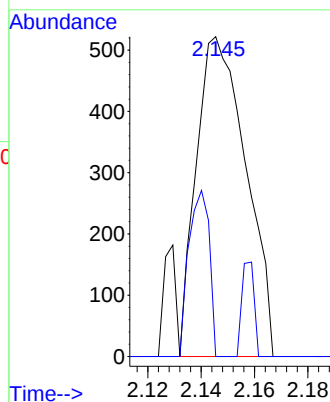

#5
 Bromomethane
 Concen: 0.29 ug/l
 RT: 2.529 min Scan# 313
 Delta R.T. 0.005 min
 Lab File: VN066166.D
 Acq: 10 Mar 2021 15:14

Tgt Ion: 94 Resp: 479
 Ion Ratio Lower Upper
 94 100
 96 134.5 73.0 109.4#

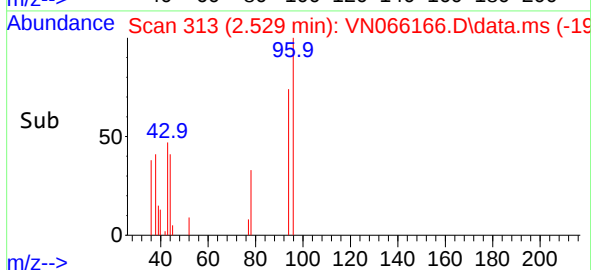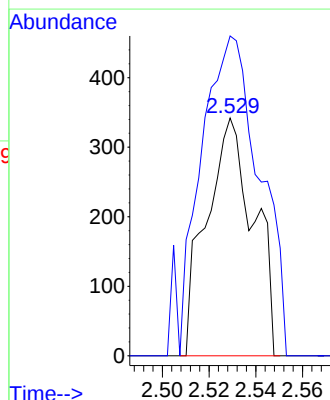



#10

Methyl Iodide

Concen: 2.69 ug/l


RT: 3.873 min Scan# 814

Delta R.T. -0.002 min




Lab File: VN066166.D

Acq: 10 Mar 2021 15:14

Instrument :
MSVOA_N
ClientSampled :

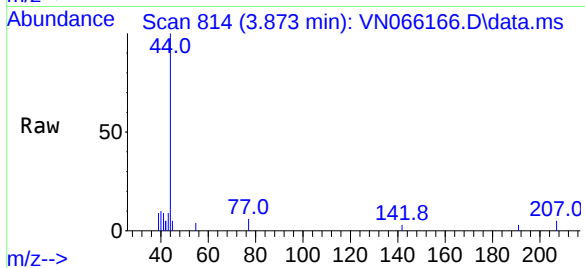

Tgt Ion:	142	Resp:	25
Ion	Ratio	Lower	Upper
142	100		
127	0.0	31.7	47.5#
141	0.0	10.9	16.3#

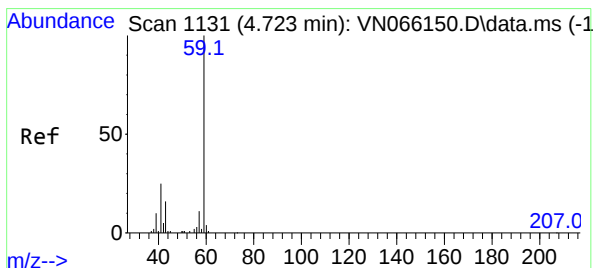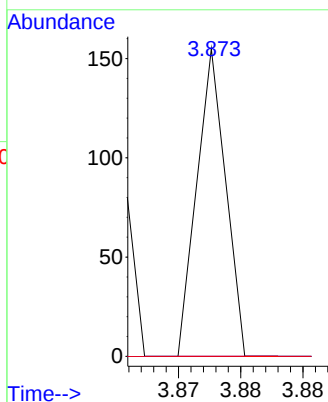

#11

Tert butyl alcohol

Concen: 0.24 ug/l




RT: 4.715 min Scan# 1128


Delta R.T. -0.008 min

Lab File: VN066166.D

Acq: 10 Mar 2021 15:14

Tgt Ion:	59	Resp:	133
Ion	Ratio	Lower	Upper
59	100		
57	0.0	8.0	12.0#


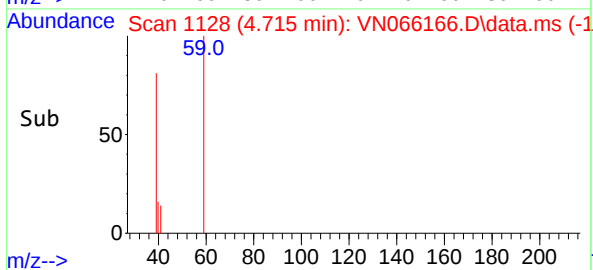
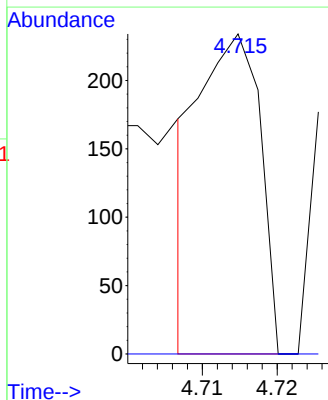
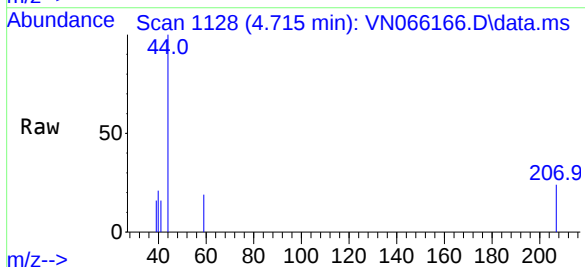




#13
Acrolein
Concen: 3.46 ug/l
RT: 3.532 min Scan# 687
Delta R.T. -0.005 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 5784
Ion Ratio Lower Upper
56 100
55 36.7 56.0 84.0#

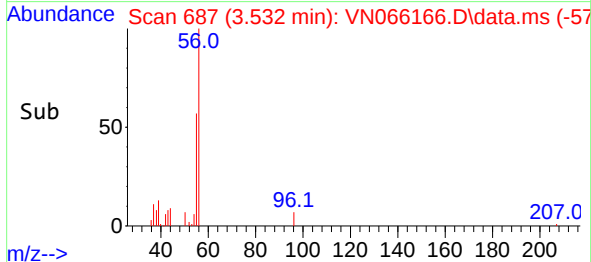

#16
Acetone
Concen: 2.77 ug/l
RT: 3.744 min Scan# 766
Delta R.T. -0.005 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14


Tgt Ion: 43 Resp: 4534
Ion Ratio Lower Upper
43 100
58 19.4 27.0 40.6#

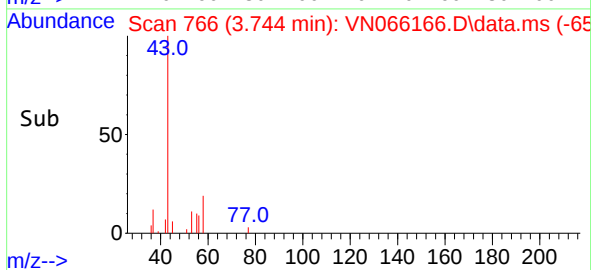

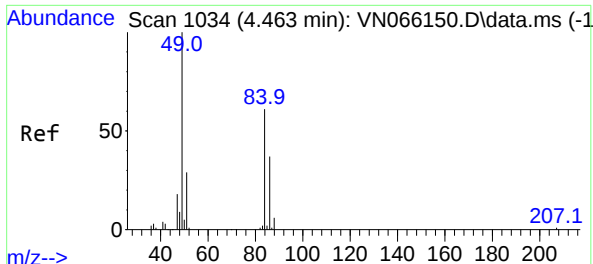




#20
Methylene Chloride
Concen: 0.29 ug/l
RT: 4.444 min Scan# 1027
Delta R.T. -0.019 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14

Instrument :
MSVOA_N
ClientSampled :

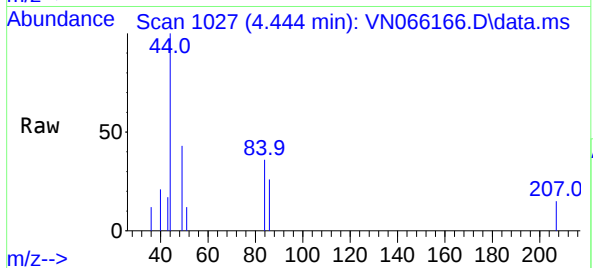

Tgt Ion: 84 Resp: 689




Ion	Ratio	Lower	Upper
84	100		
49	121.6	94.6	141.8
51	34.8	29.9	44.9
86	73.8	51.4	77.2

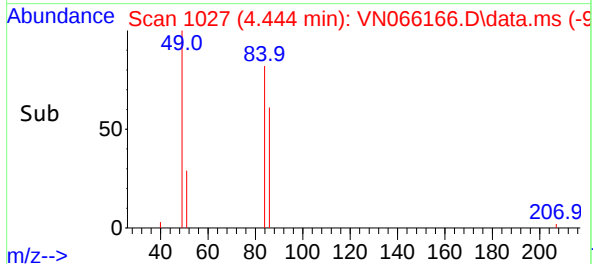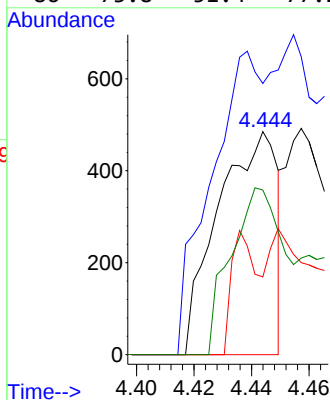


#23
Vinyl Acetate
Concen: 0.73 ug/l
RT: 5.793 min Scan# 1530
Delta R.T. -0.011 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14

Tgt Ion: 43 Resp: 6827

Ion	Ratio	Lower	Upper
43	100		
86	0.0	8.6	13.0#


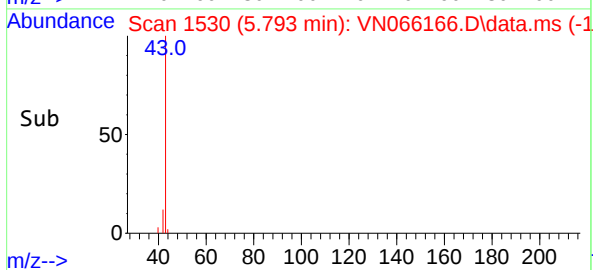
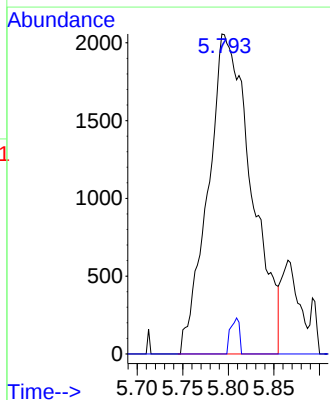
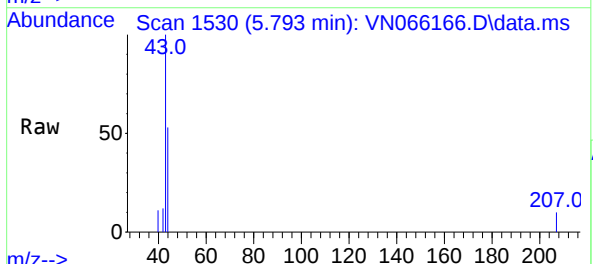




#28
Bromochloromethane
Concen: 0.44 ug/l
RT: 7.102 min Scan# 2018
Delta R.T. -0.008 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 49 Resp: 1245
Ion Ratio Lower Upper
49 100
129 0.0 0.0 3.6
130 12.9 67.8 101.6#

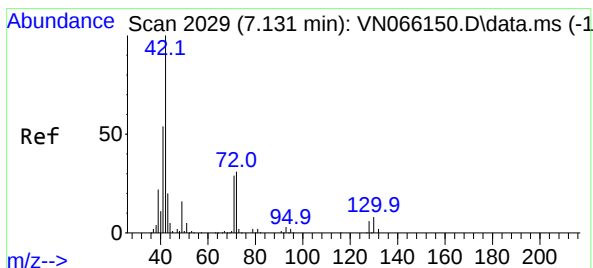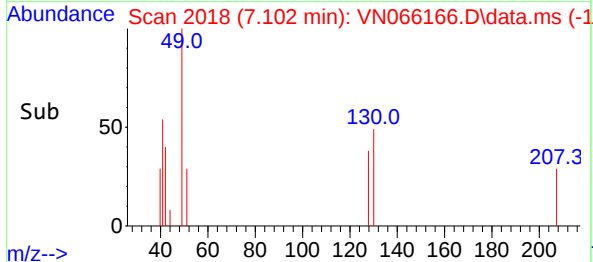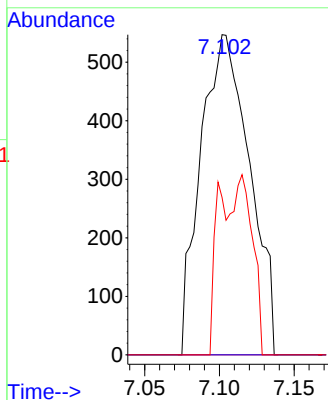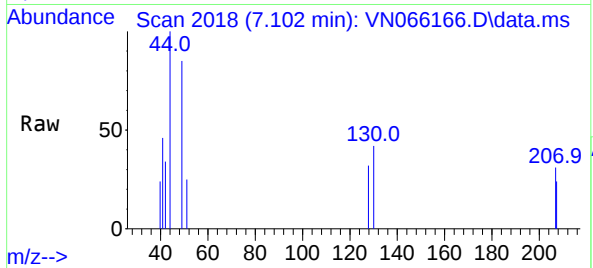

#29
Tetrahydrofuran
Concen: 0.44 ug/l
RT: 7.129 min Scan# 2028
Delta R.T. -0.002 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14


Tgt Ion: 42 Resp: 767
Ion Ratio Lower Upper
42 100
72 19.3 36.6 55.0#
71 6.5 34.3 51.5#

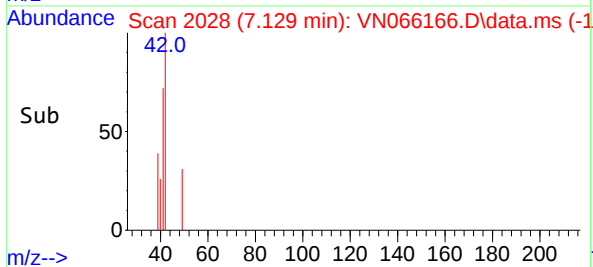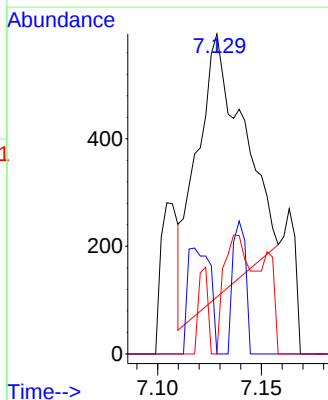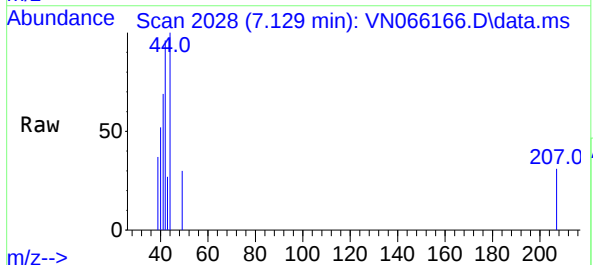






#31
Cyclohexane
Concen: 1.15 ug/l
RT: 7.582 min Scan# 2197
Delta R.T. 0.006 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion: 56 Resp: 5369
Ion Ratio Lower Upper
56 100
69 158.8 26.6 39.8#
84 90.6 70.4 105.6

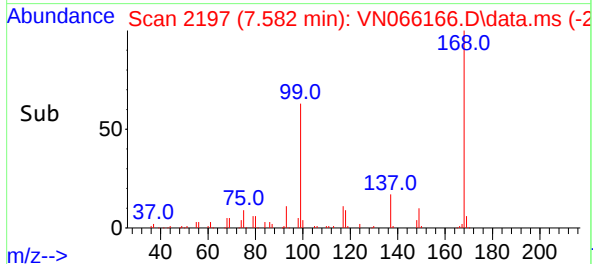


#33
1,2-Dichloroethane-d4
Concen: 54.75 ug/l
RT: 7.947 min Scan# 2333
Delta R.T. -0.005 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14

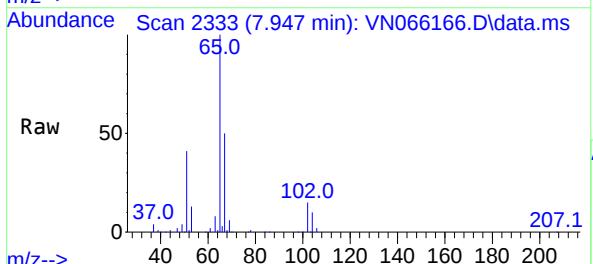

Tgt Ion: 65 Resp: 177446
Ion Ratio Lower Upper
65 100
67 51.5 0.0 107.2

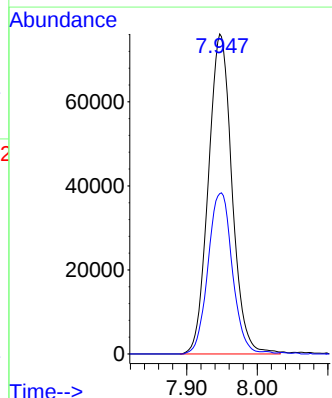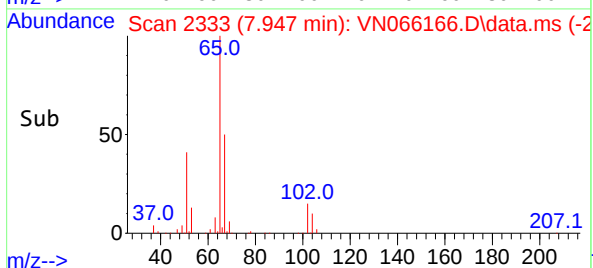




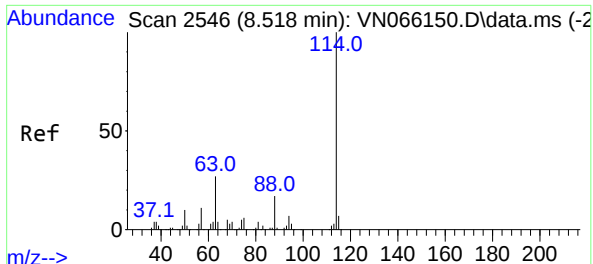


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.512 min Scan# 2544
Delta R.T. -0.006 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion:114 Resp: 290218
Ion Ratio Lower Upper
114 100
63 26.0 0.0 38.6
88 17.4 0.0 30.6

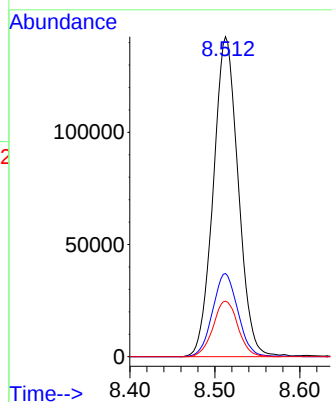


#35

Dibromofluoromethane
Concen: 55.07 ug/l
RT: 7.509 min Scan# 2170
Delta R.T. 0.000 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14

Tgt Ion:113 Resp: 109037
Ion Ratio Lower Upper
113 100
111 102.4 82.2 123.2
192 18.4 15.4 23.0


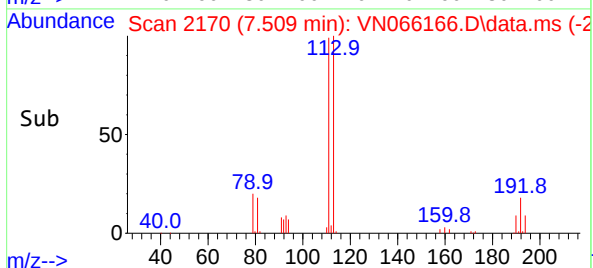

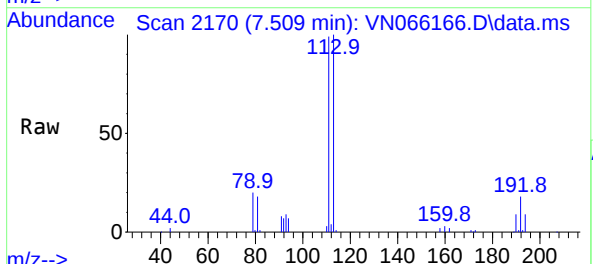




#36
1,1-Dichloropropene
Concen: 4.92 ug/l
RT: 7.584 min Scan# 2198
Delta R.T. -0.132 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 16241
Ion Ratio Lower Upper
75 100
110 9.3 18.2 54.6#
77 0.0 24.9 37.3#

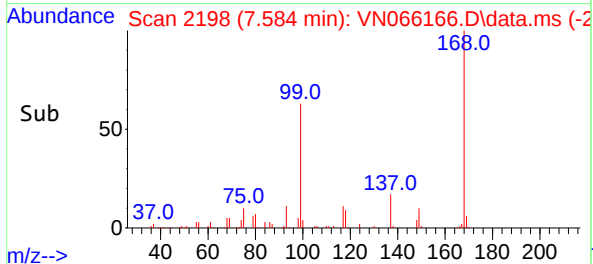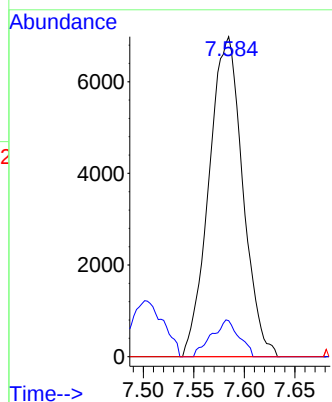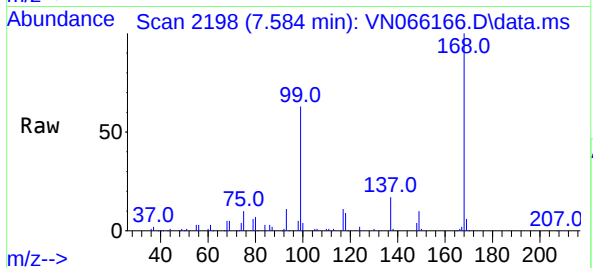

#38
Carbon Tetrachloride
Concen: 6.20 ug/l
RT: 7.584 min Scan# 2198
Delta R.T. -0.113 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14


Tgt Ion:117 Resp: 17824
Ion Ratio Lower Upper
117 100
119 4.5 76.0 114.0#
121 0.0 24.5 36.7#

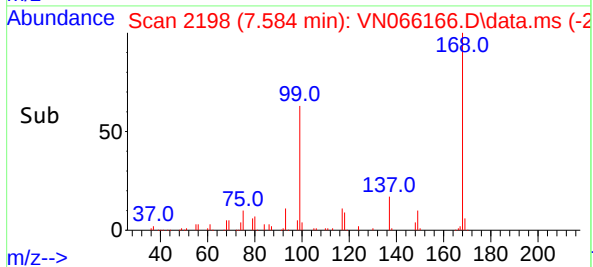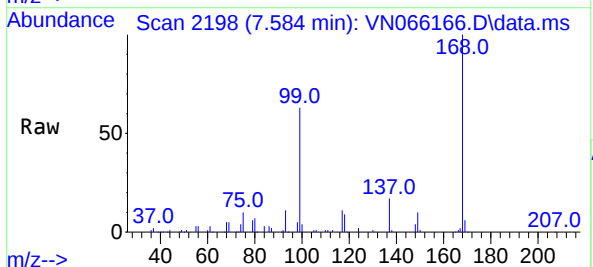






#43
Isopropyl Acetate
Concen: 0.22 ug/l
RT: 8.086 min Scan# 2385
Delta R.T. -0.011 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 43 Resp: 1761
Ion Ratio Lower Upper
43 100
61 0.0 22.5 33.7#
87 0.0 11.1 16.7#

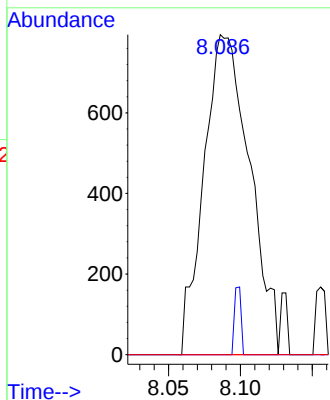


#49
1,4-Dioxane
Concen: 4.30 ug/l
RT: 9.135 min Scan# 2776
Delta R.T. -0.008 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14

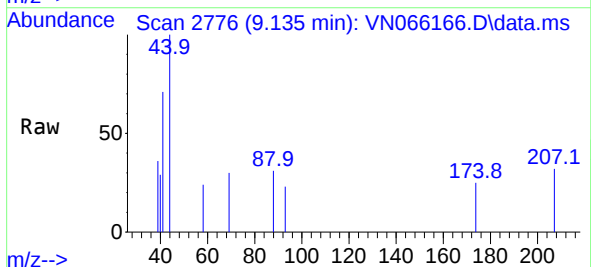

Tgt Ion: 88 Resp: 158
Ion Ratio Lower Upper
88 100
43 0.0 24.7 37.1#
58 34.8 52.6 78.8#



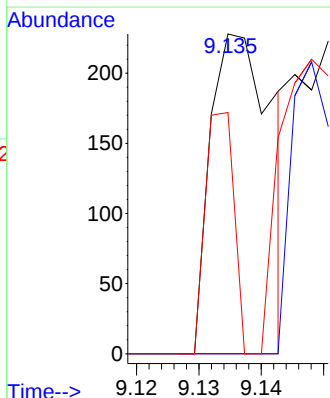





#50
Toluene-d8
Concen: 52.31 ug/l
RT: 10.028 min Scan# 3109
Delta R.T. -0.002 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 98 Resp: 407487
Ion Ratio Lower Upper
98 100
100 63.7 50.5 75.7

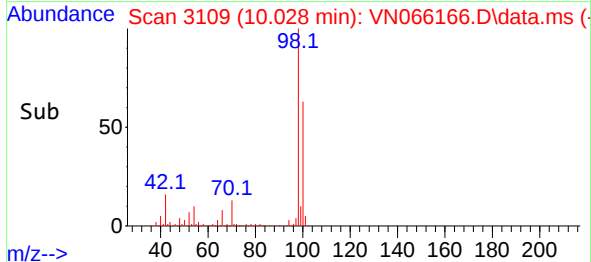

#51
4-Methyl-2-Pentanone
Concen: 0.85 ug/l
RT: 9.918 min Scan# 3068
Delta R.T. -0.005 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14

Tgt Ion: 43 Resp: 4195
Ion Ratio Lower Upper
43 100
58 30.8 32.5 48.7#



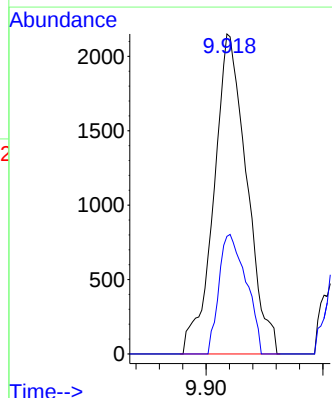





#58
2-Chloroethyl Vinyl ether
Concen: 13.39 ug/l
RT: 9.628 min Scan# 2960
Delta R.T. -0.005 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 63 Resp: 1989
Ion Ratio Lower Upper
63 100
106 9.4 22.6 33.8#

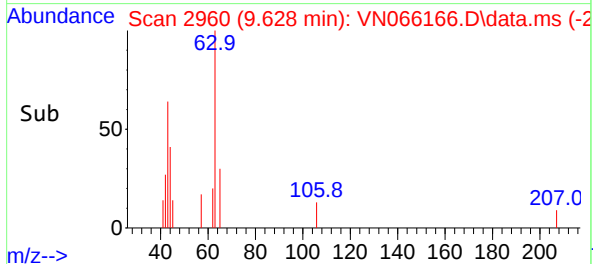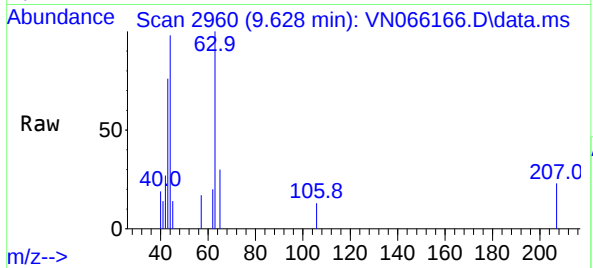

#59
2-Hexanone
Concen: 0.44 ug/l
RT: 10.693 min Scan# 3357
Delta R.T. -0.000 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14

Tgt Ion: 43 Resp: 1544
Ion Ratio Lower Upper
43 100
58 61.2 28.1 84.3


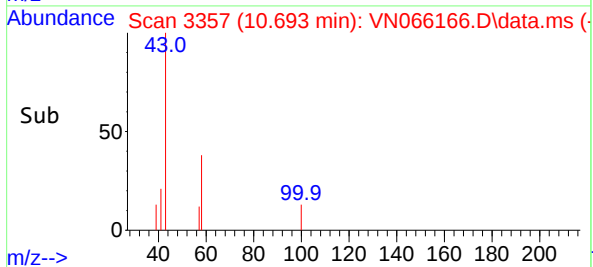

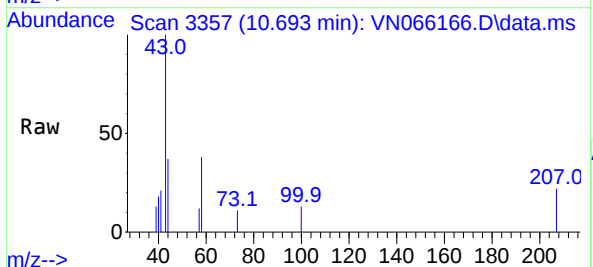




#62
4-Bromofluorobenzene
Concen: 43.80 ug/l
RT: 12.345 min Scan# 3973
Delta R.T. -0.003 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 127002
Ion Ratio Lower Upper
95 100
174 72.2 0.0 169.0
176 70.0 0.0 162.4

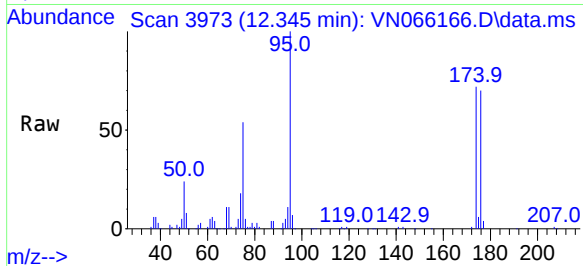

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.347 min Scan# 3601
Delta R.T. -0.003 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14


Tgt Ion: 117 Resp: 249371
Ion Ratio Lower Upper
117 100
82 63.3 43.7 65.5
119 31.1 26.1 39.1

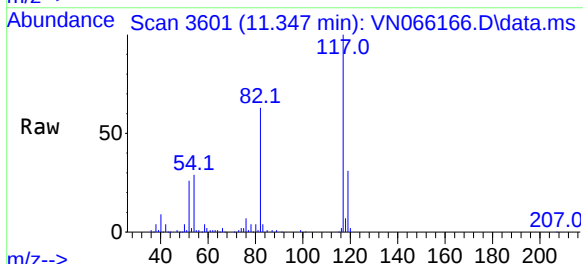






#64
Tetrachloroethene
Concen: 0.25 ug/l
RT: 10.572 min Scan# 3312
Delta R.T. 0.000 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion:164 Resp: 517
Ion Ratio Lower Upper
164 100
166 127.4 102.6 154.0
129 52.8 76.2 114.4#
131 72.4 73.4 110.2#

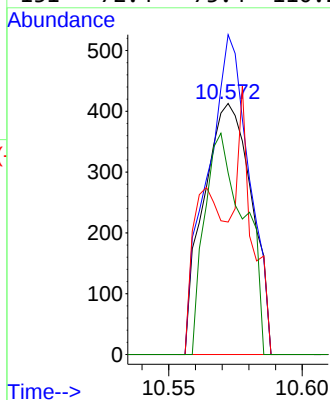


#68
m/p-Xylenes
Concen: 0.35 ug/l
RT: 11.567 min Scan# 3683
Delta R.T. 0.003 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14

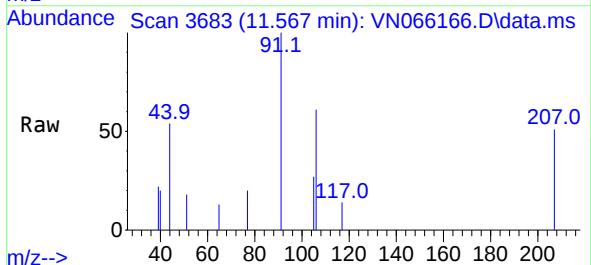

Tgt Ion:106 Resp: 1240
Ion Ratio Lower Upper
106 100
91 239.6 161.4 242.0



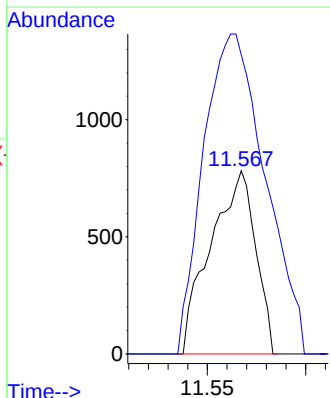
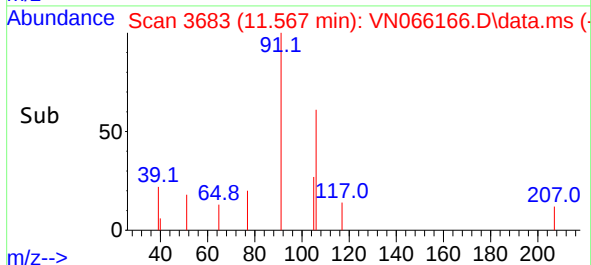




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.286 min Scan# 4324
Delta R.T. -0.003 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:152 Resp: 98631
Ion Ratio Lower Upper
152 100
115 60.5 28.5 85.6
150 158.5 0.0 347.6

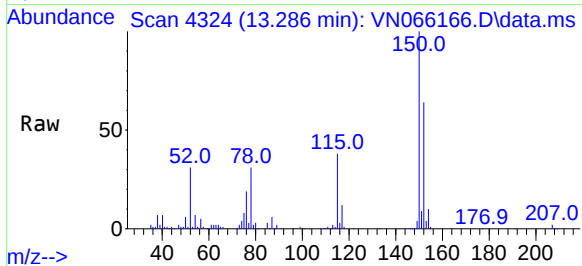

#74
N-ethyl acetate
Concen: 3.02 ug/l
RT: 12.031 min Scan# 3856
Delta R.T. 0.016 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14

Tgt Ion: 43 Resp: 276
Ion Ratio Lower Upper
43 100
70 0.0 34.4 51.6#
55 0.0 20.7 31.1#
61 0.0 19.1 28.7#


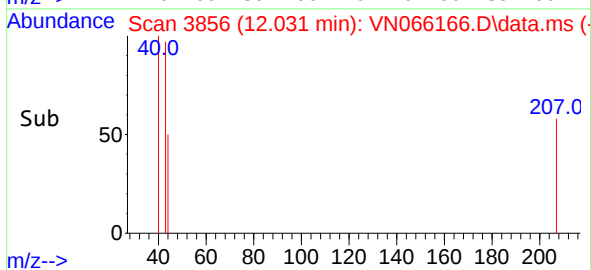
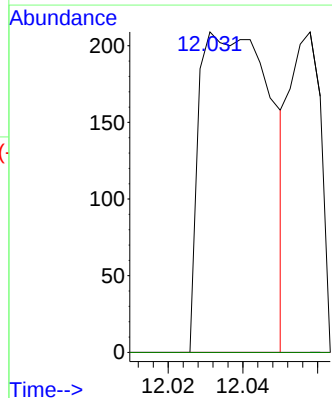
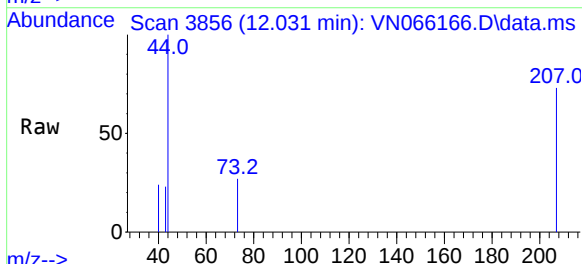




#76
1,2,3-Trichloropropane
Concen: 23.83 ug/l
RT: 12.345 min Scan# 3973
Delta R.T. -0.153 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 70429
Ion Ratio Lower Upper
75 100
77 1.2 0.0 0.0#

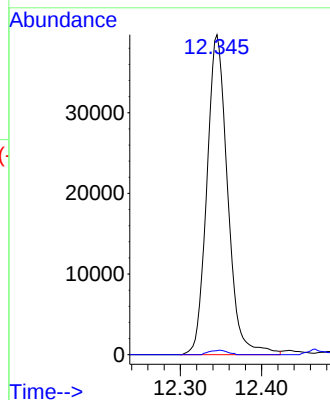

#81
trans-1,4-Dichloro-2-butene
Concen: 74.39 ug/l
RT: 12.345 min Scan# 3973
Delta R.T. 0.099 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14

Tgt Ion: 75 Resp: 70429
Ion Ratio Lower Upper
75 100
53 0.0 74.6 111.8#
89 0.0 35.8 53.8#



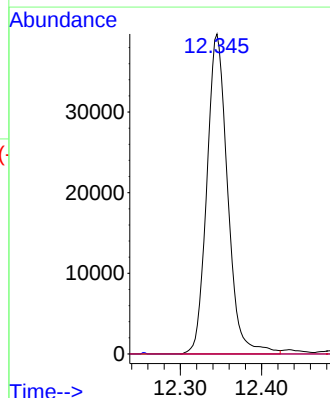





#82
4-Chlorotoluene
Concen: 0.25 ug/l
RT: 12.720 min Scan# 4113
Delta R.T. 0.002 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 1420
Ion Ratio Lower Upper
91 100
126 8.2 17.2 51.6#

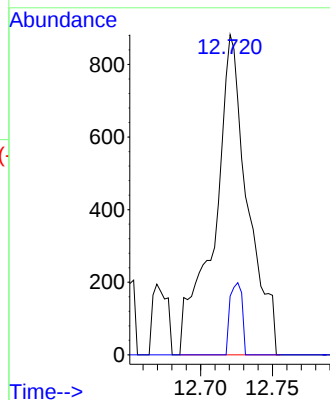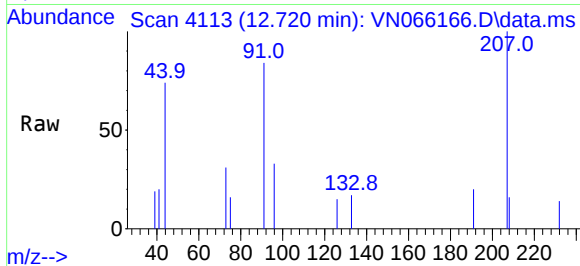

#83
tert-Butylbenzene
Concen: 0.21 ug/l
RT: 12.940 min Scan# 4195
Delta R.T. 0.002 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14

Tgt Ion: 119 Resp: 1170
Ion Ratio Lower Upper
119 100
91 54.2 33.0 98.9
134 26.7 12.7 38.1


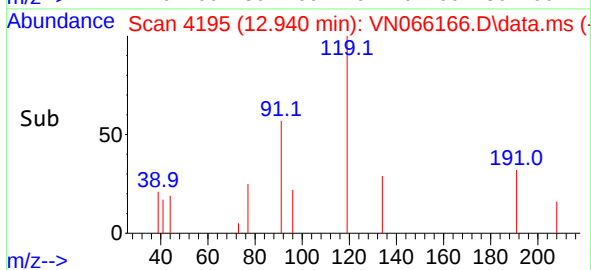
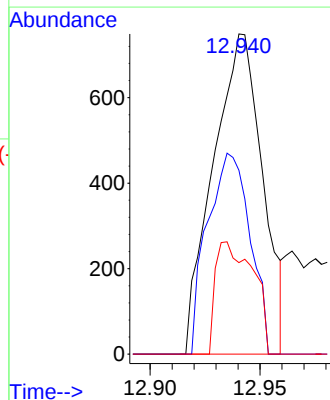
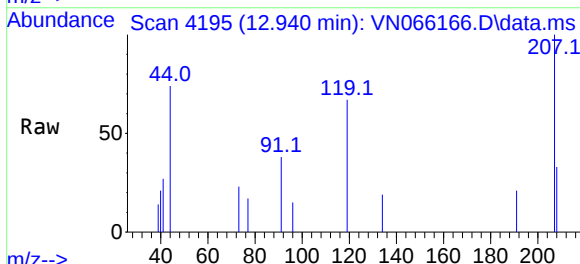




#85
sec-Butylbenzene
Concen: 0.20 ug/l
RT: 13.120 min Scan# 4262
Delta R.T. 0.005 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:105 Resp: 1456
Ion Ratio Lower Upper
105 100
134 9.5 10.0 30.0#

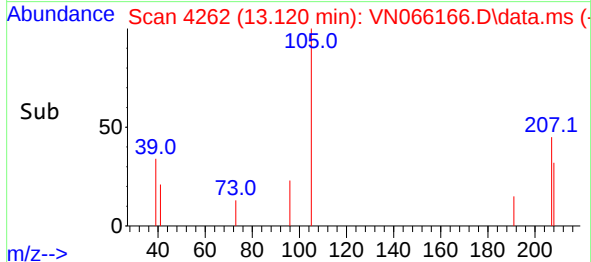

#87
1,3-Dichlorobenzene
Concen: 0.22 ug/l
RT: 13.230 min Scan# 4303
Delta R.T. 0.003 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14


Tgt Ion:146 Resp: 718
Ion Ratio Lower Upper
146 100
111 25.2 19.5 58.5
148 60.6 32.3 96.9

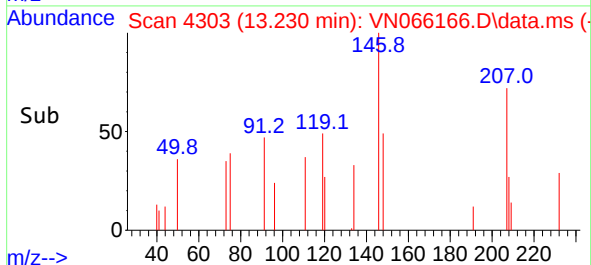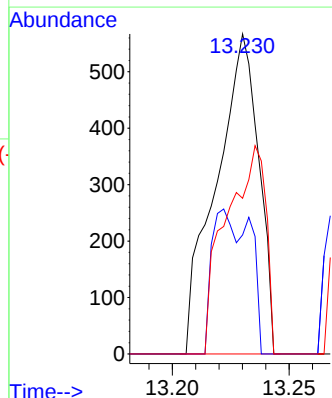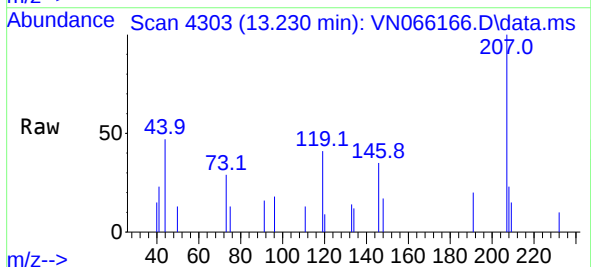






#88
1,4-Dichlorobenzene
Concen: 0.22 ug/l
RT: 13.230 min Scan# 4303
Delta R.T. -0.078 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion:146 Resp: 718
Ion Ratio Lower Upper
146 100
111 25.2 19.0 57.0
148 60.6 31.8 95.3

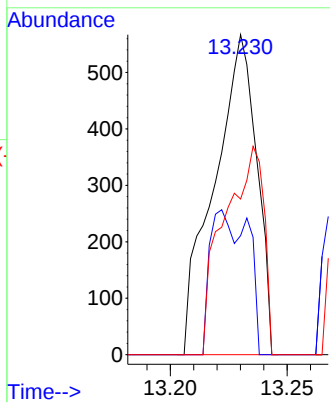


#92
1,2-Dibromo-3-Chloropropane
Concen: 0.33 ug/l
RT: 14.214 min Scan# 4670
Delta R.T. 0.000 min
Lab File: VN066166.D
Acq: 10 Mar 2021 15:14

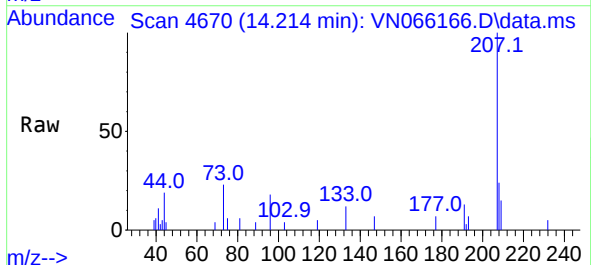


Tgt Ion: 75 Resp: 230
Ion Ratio Lower Upper
75 100
155 0.0 44.1 132.4#
157 0.0 56.0 168.2#

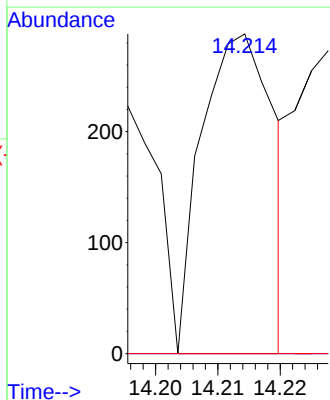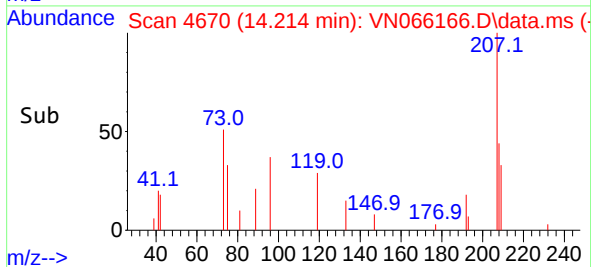



#93
 1,2,4-Trichlorobenzene
 Concen: 2.36 ug/l
 RT: 14.855 min Scan# 4909
 Delta R.T. 0.005 min
 Lab File: VN066166.D
 Acq: 10 Mar 2021 15:14

Instrument :
 MSVOA_N
 ClientSampleId :

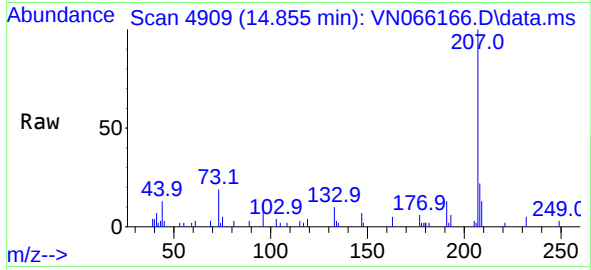

Tgt Ion:	180	Resp:	336
Ion	Ratio	Lower	Upper
180	100		
182	61.9	47.3	142.0
145	0.0	15.6	46.8#

