


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031021\
Data File : VN066162.D
Acq On : 10 Mar 2021 8:35
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030921W.M
Title : SW846 8260
Last Update : Tue Mar 09 14:48:21 2021

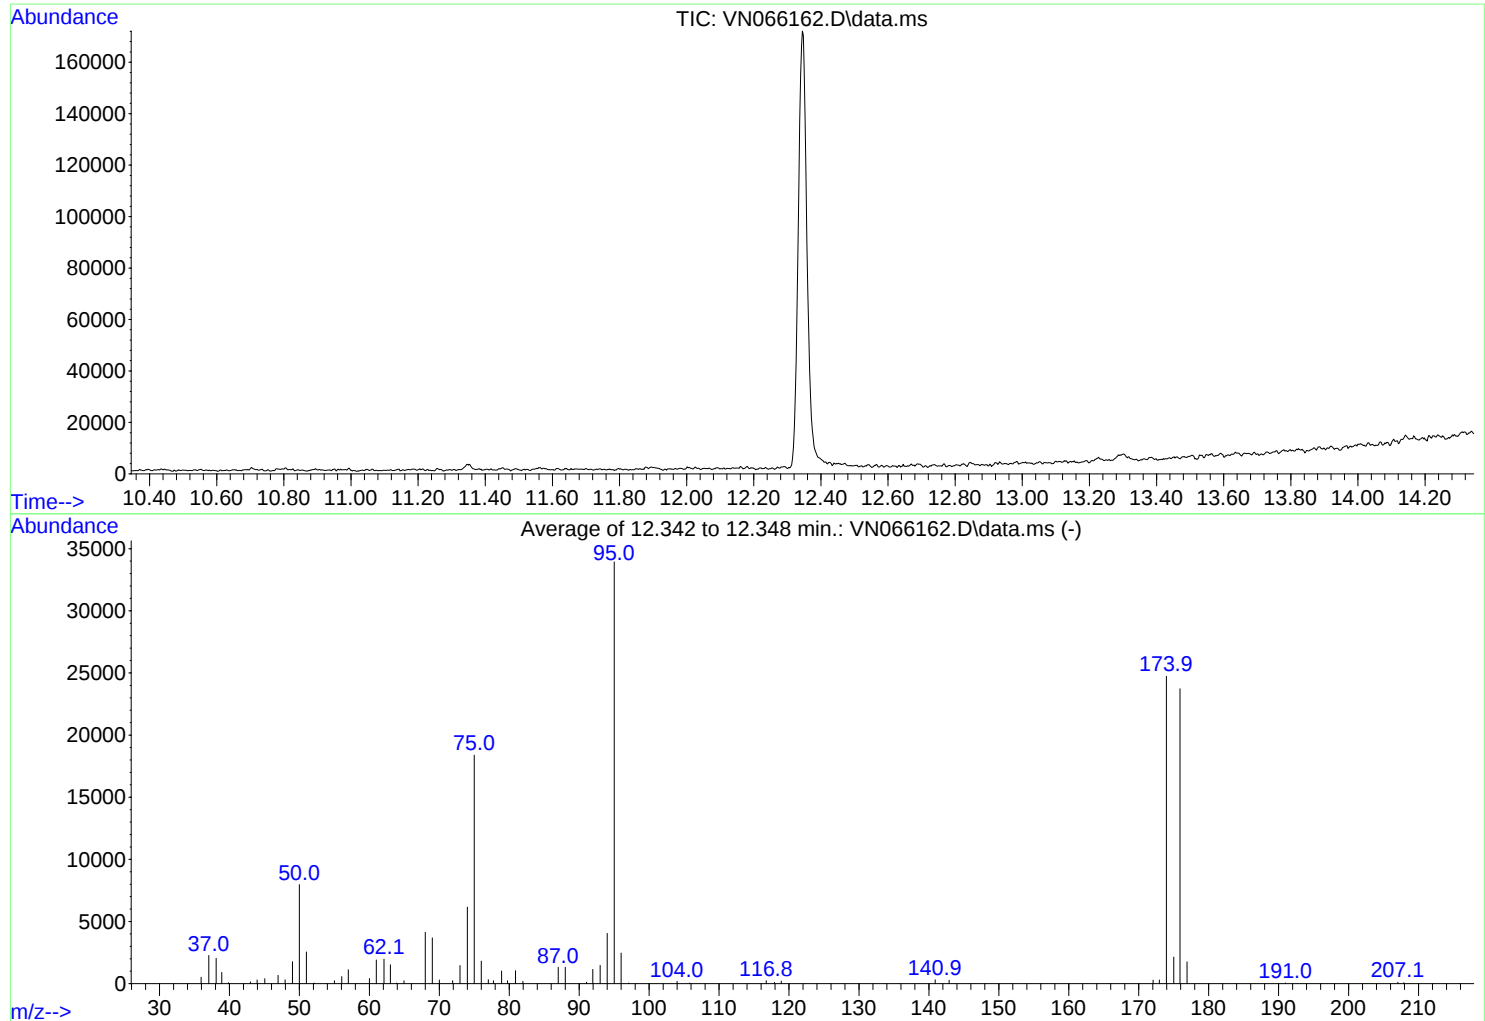

AutoFind: Scans 3972, 3973, 3974; Background Corrected with Scan 3957

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	7969	PASS
75	95	30	60	54.2	18392	PASS
95	95	100	100	100.0	33941	PASS
96	95	5	9	7.3	2461	PASS
173	174	0.00	2	1.2	296	PASS
174	95	50	100	72.9	24731	PASS
175	174	5	9	8.7	2144	PASS
176	174	95	101	95.9	23725	PASS
177	176	5	9	7.4	1756	PASS