

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031023\
 Data File : VN076939.D
 Acq On : 10 Mar 2023 21:14
 Operator : JC\MD
 Sample : 01870-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 RAW-WATER

Quant Time: Mar 13 01:25:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031023W.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 10 13:47:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.231	168	426439	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.107	114	702250	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.866	117	624466	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.795	152	261577	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.584	65	310559	48.802	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	97.600%
35) Dibromofluoromethane	8.172	113	223941	47.848	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.700%
50) Toluene-d8	10.572	98	838635	48.619	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	97.240%
62) 4-Bromofluorobenzene	12.854	95	296802	47.043	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	94.080%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031023\
Data File : VN076939.D
Acq On : 10 Mar 2023 21:14
Operator : JC\MD
Sample : 01870-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
RAW-WATER

Quant Time: Mar 13 01:25:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031023W.M
Quant Title : SW846 8260
QLast Update : Fri Mar 10 13:47:39 2023
Response via : Initial Calibration




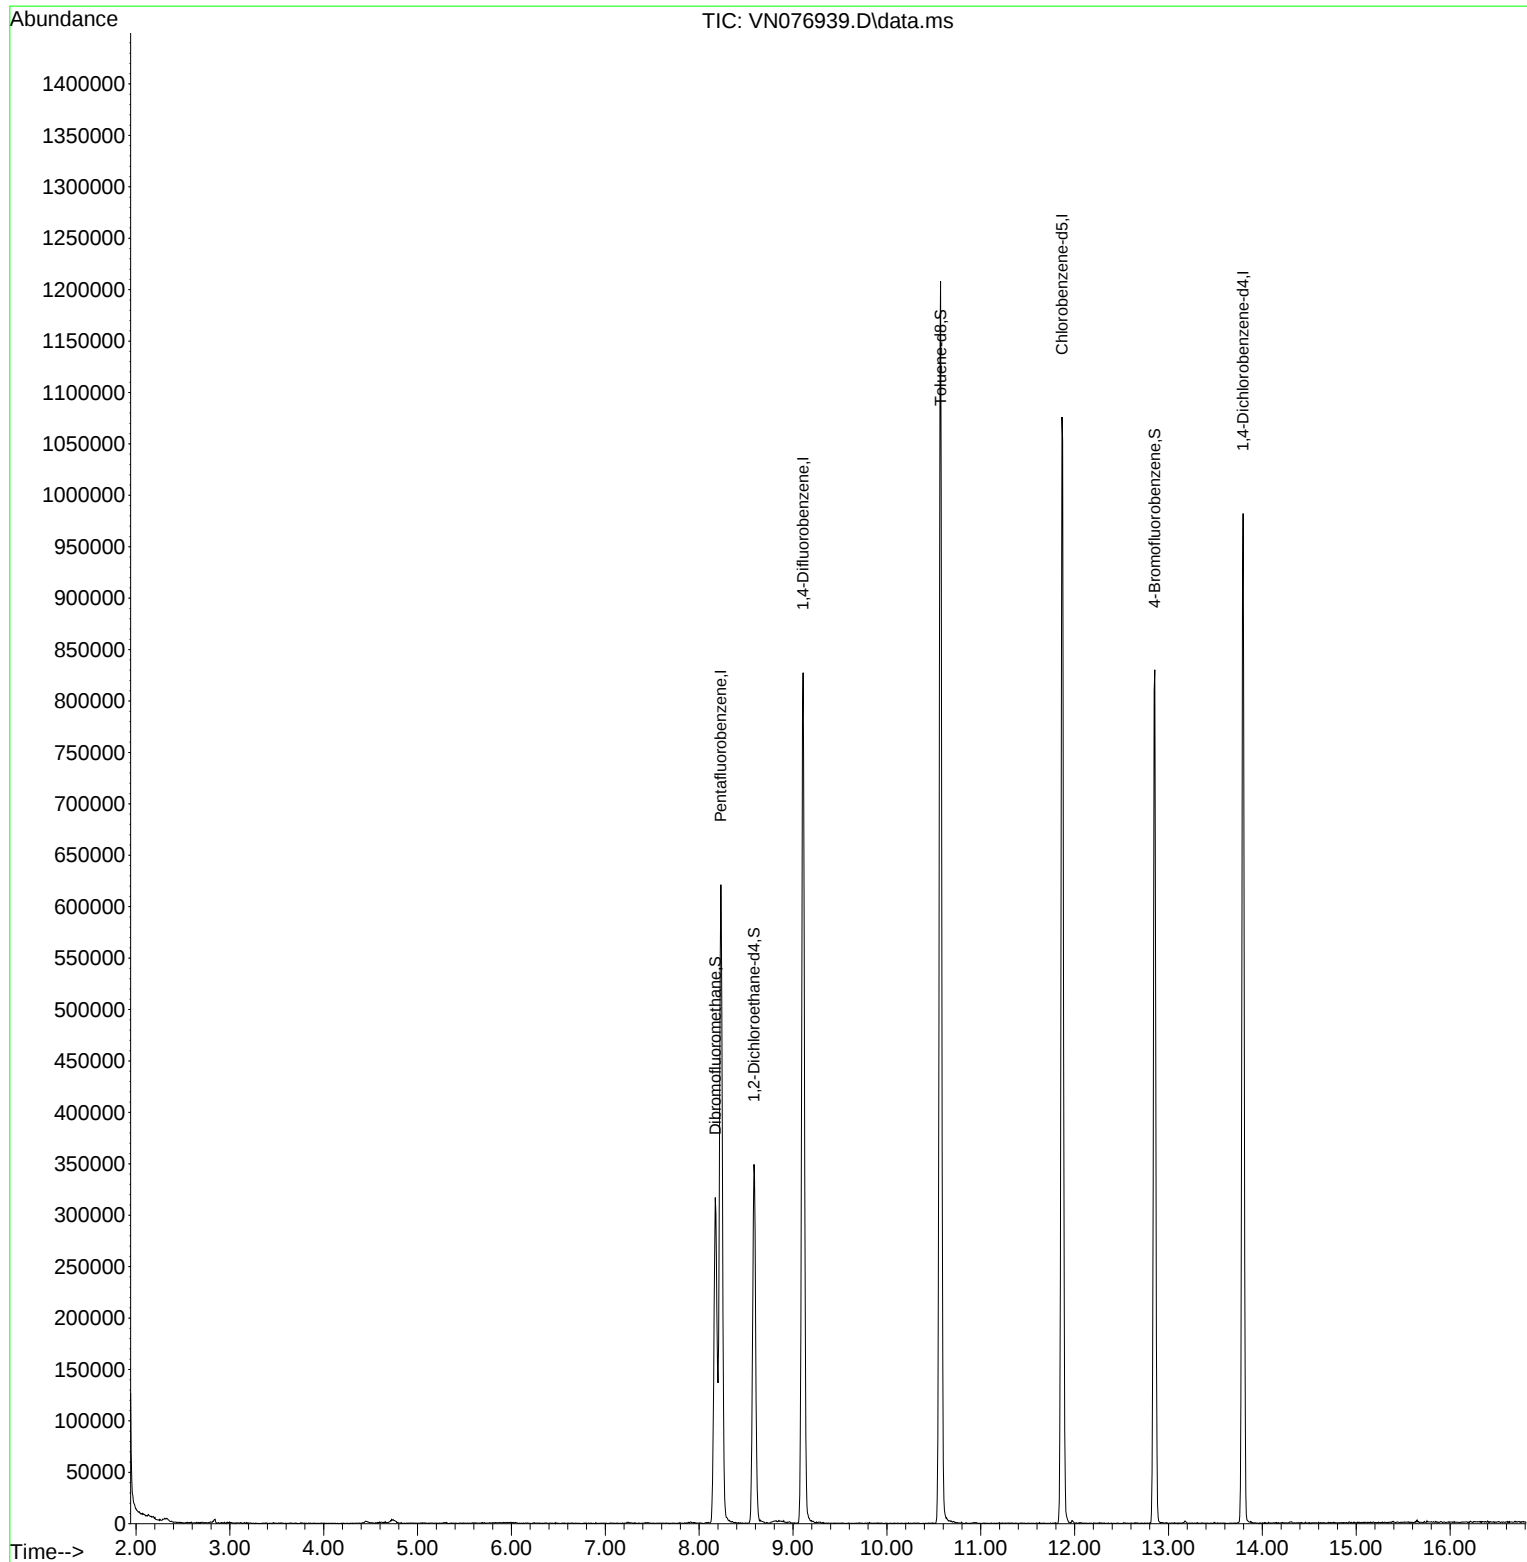


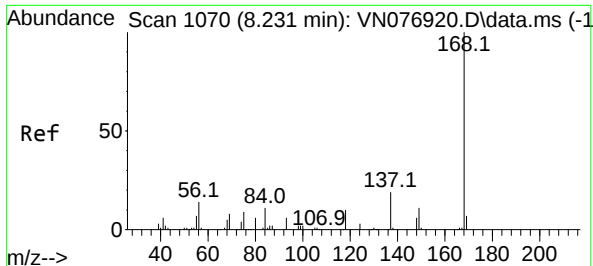

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.231 min Scan# 1070
Delta R.T. -0.000 min
Lab File: VN076939.D
Acq: 10 Mar 2023 21:14




Instrument :
MSVOA_N
ClientSampleId :
RAW-WATER


Tgt Ion:168 Resp: 426439
Ion Ratio Lower Upper
168 100
99 68.4 48.6 73.0

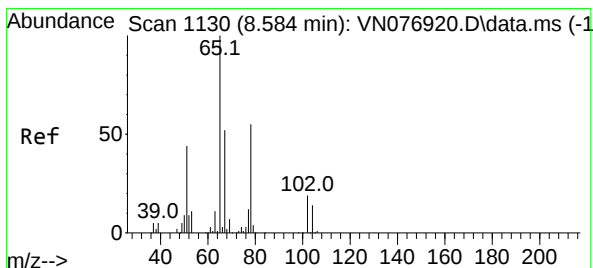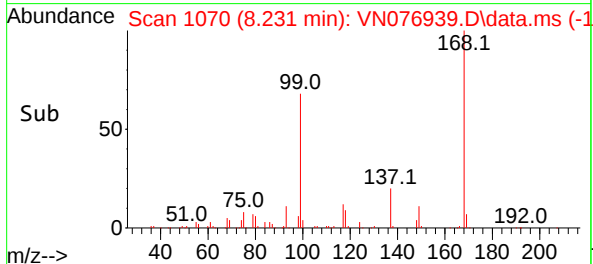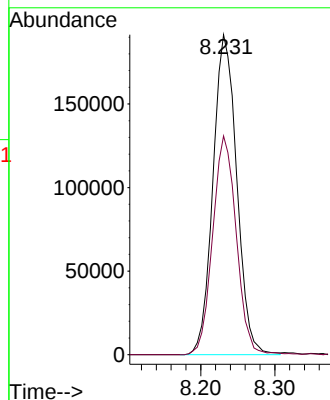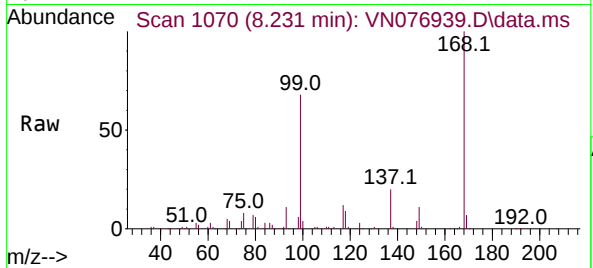

#33
1,2-Dichloroethane-d4
Concen: 48.802 ug/l
RT: 8.584 min Scan# 1130
Delta R.T. 0.000 min
Lab File: VN076939.D
Acq: 10 Mar 2023 21:14

Tgt Ion: 65 Resp: 310559
Ion Ratio Lower Upper
65 100
67 50.2 0.0 107.2

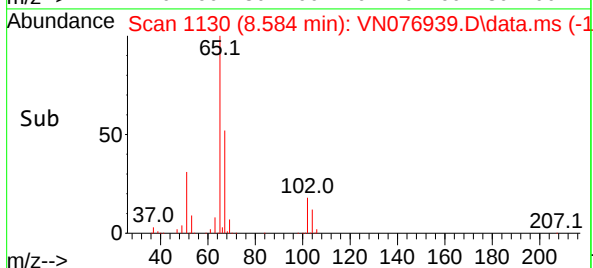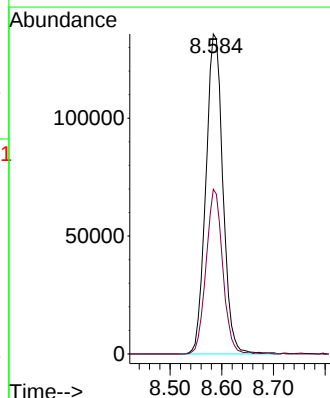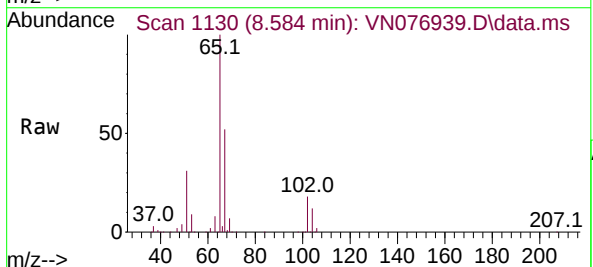

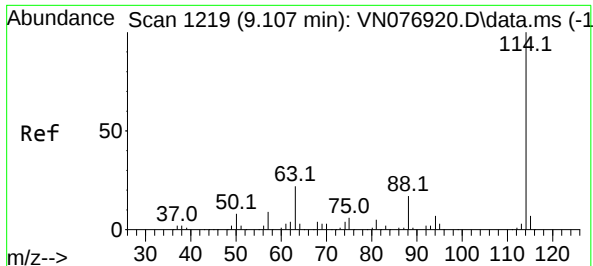

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.107 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN076939.D

Acq: 10 Mar 2023 21:14

Instrument :

MSVOA_N

ClientSampleId :

RAW-WATER





Tgt Ion:114 Resp: 702250

Ion Ratio Lower Upper

114 100

63 21.7 0.0 36.6

88 18.1 0.0 28.6

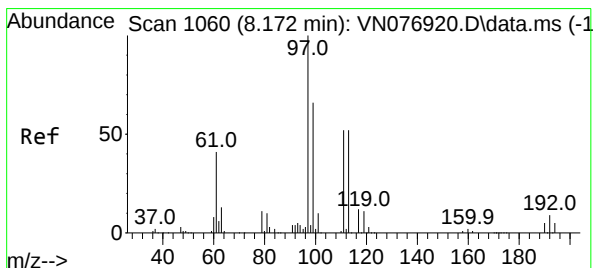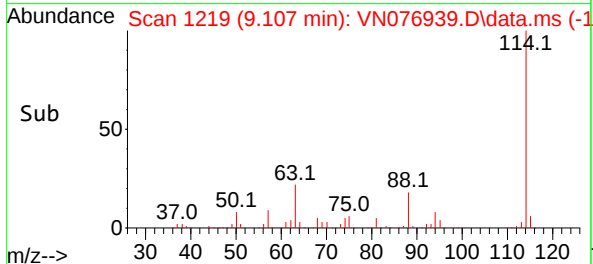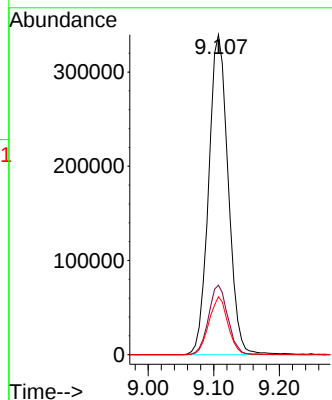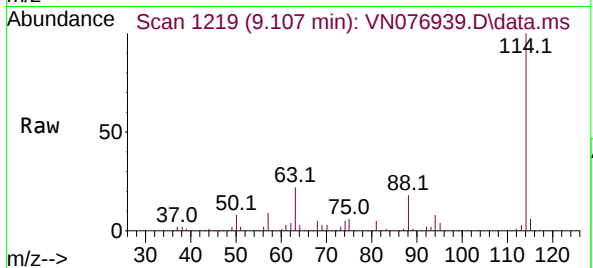

#35

Dibromofluoromethane

Concen: 47.848 ug/l

RT: 8.172 min Scan# 1060

Delta R.T. 0.000 min

Lab File: VN076939.D

Acq: 10 Mar 2023 21:14




Tgt Ion:113 Resp: 223941


Ion Ratio Lower Upper

113 100

111 101.2 81.8 122.8

192 18.1 13.9 20.9

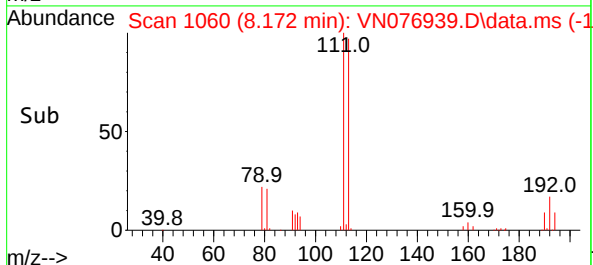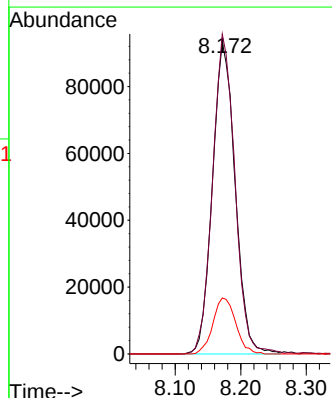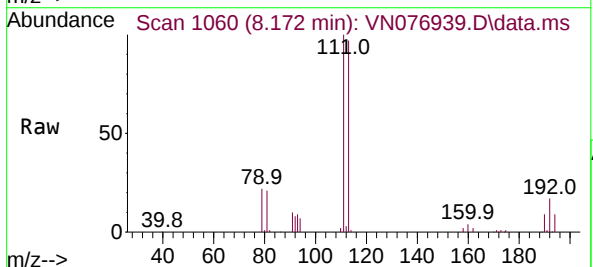

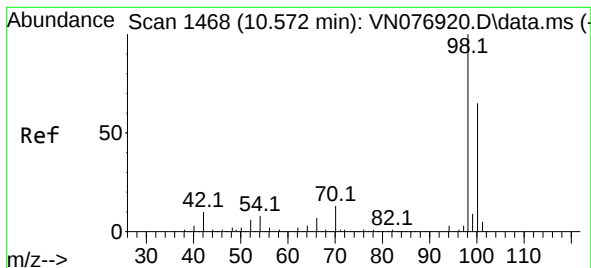

#50

Toluene-d8

Concen: 48.619 ug/l

RT: 10.572 min Scan# 1468

Delta R.T. 0.000 min

Lab File: VN076939.D

Acq: 10 Mar 2023 21:14

Instrument :

MSVOA_N

ClientSampleId :





RAW-WATER

Tgt Ion: 98 Resp: 838635

Ion Ratio Lower Upper

98 100

100 64.9 52.8 79.2

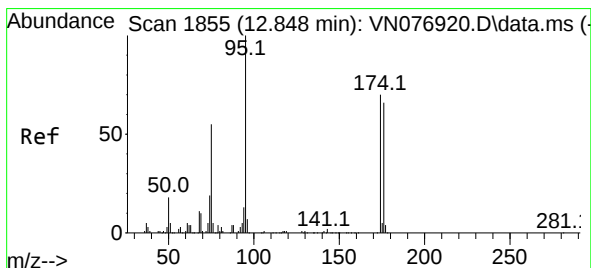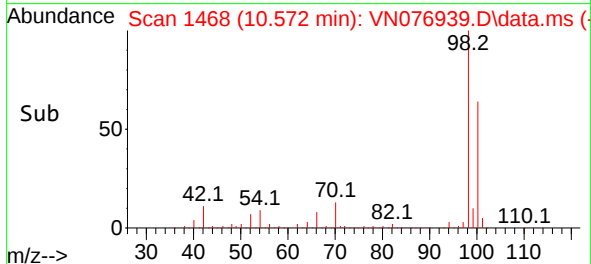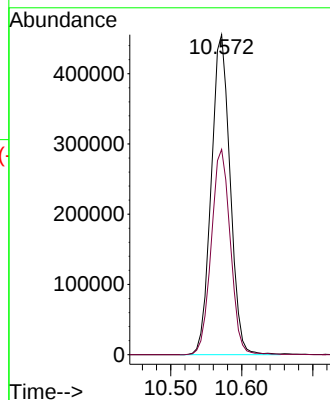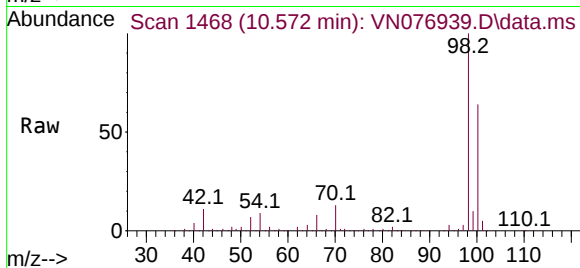

#62

4-Bromofluorobenzene

Concen: 47.043 ug/l

RT: 12.854 min Scan# 1856

Delta R.T. 0.006 min

Lab File: VN076939.D

Acq: 10 Mar 2023 21:14




Tgt Ion: 95 Resp: 296802


Ion Ratio Lower Upper

95 100

174 74.2 0.0 162.4

176 71.5 0.0 157.4


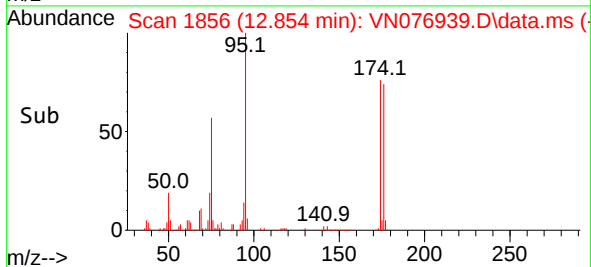
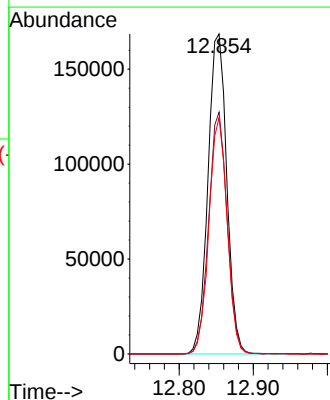
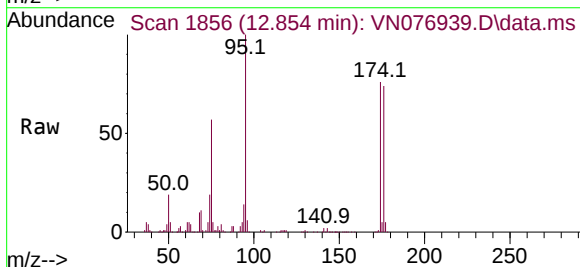


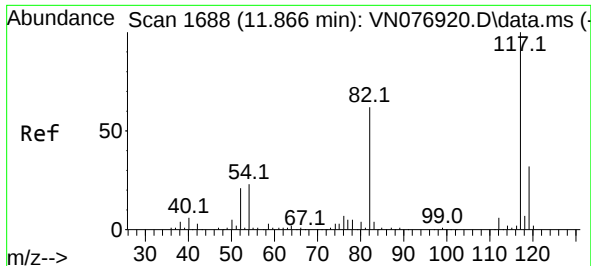

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.866 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN076939.D
Acq: 10 Mar 2023 21:14

Instrument :
MSVOA_N
ClientSampleId :
RAW-WATER

Tgt Ion:117 Resp: 624466
Ion Ratio Lower Upper
117 100
82 58.9 43.5 65.3
119 31.5 25.5 38.3

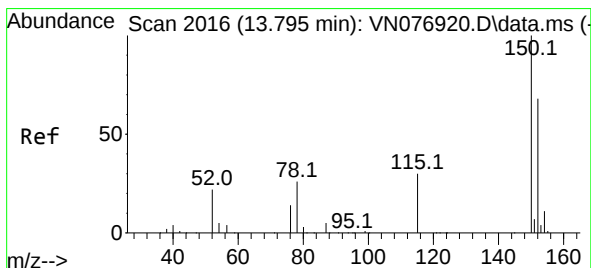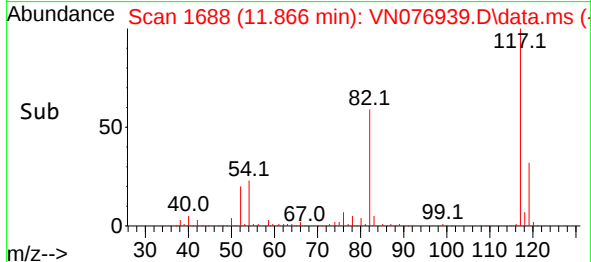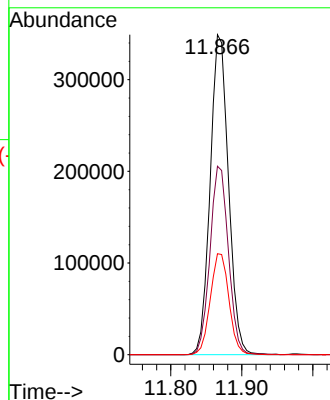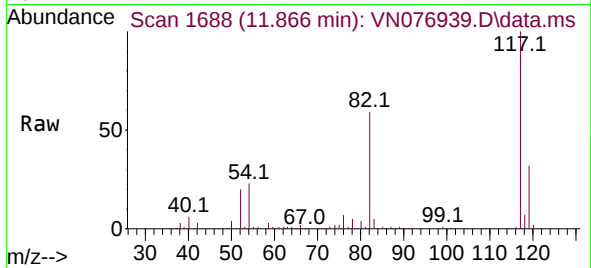

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.795 min Scan# 2016
Delta R.T. 0.000 min
Lab File: VN076939.D
Acq: 10 Mar 2023 21:14

Tgt Ion:152 Resp: 261577
Ion Ratio Lower Upper
152 100
115 65.2 30.3 90.9
150 157.5 0.0 353.6

