
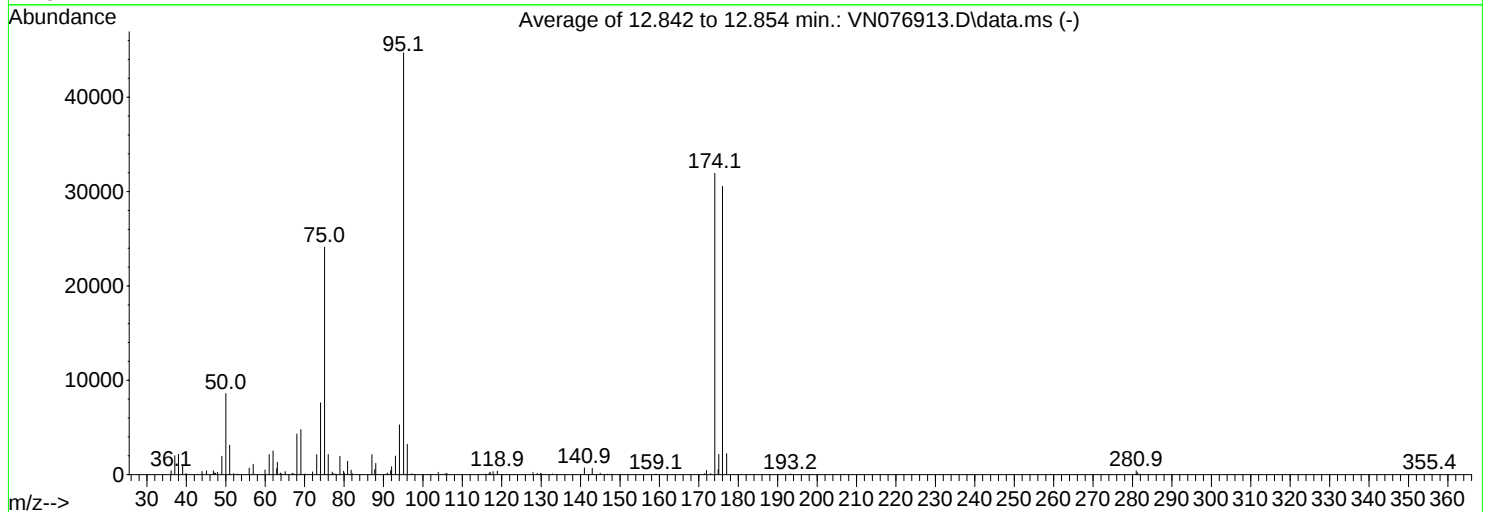


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031023\
Data File : VN076913.D
Acq On : 10 Mar 2023 08:27
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031023W.M
Title : SW846 8260
Last Update : Fri Mar 10 13:47:39 2023

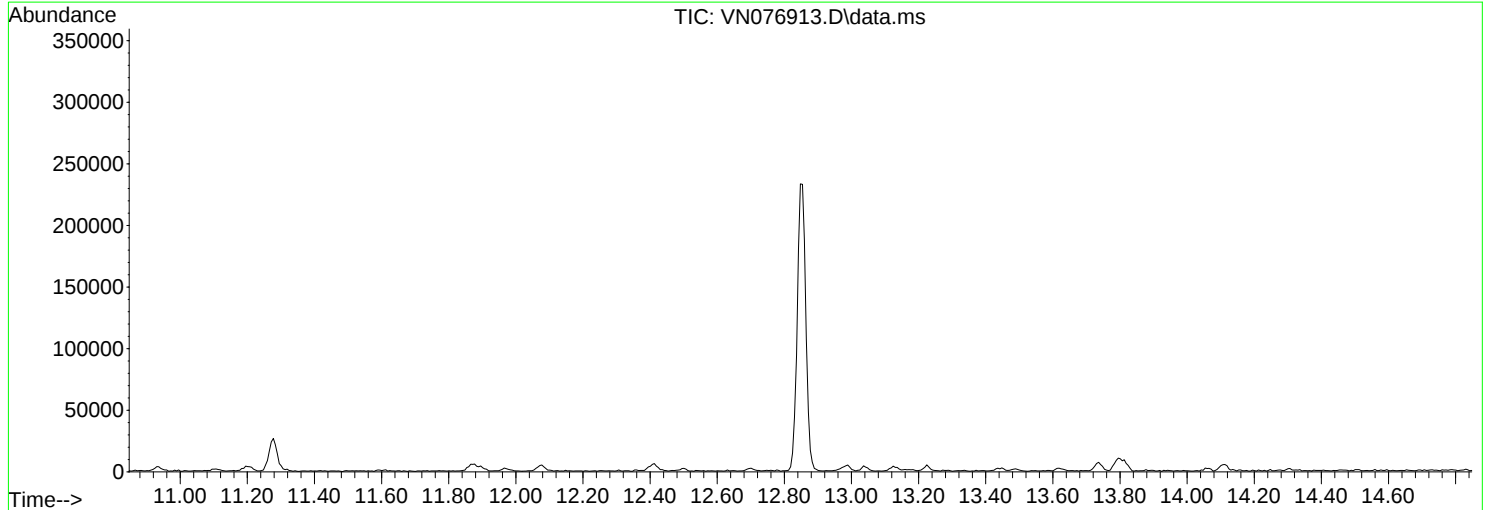

AutoFind: Scans 1854, 1855, 1856; Background Corrected with Scan 1847

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	8598	PASS
75	95	30	60	53.9	24115	PASS
95	95	100	100	100.0	44704	PASS
96	95	5	9	7.2	3199	PASS
173	174	0.00	2	0.3	97	PASS
174	95	50	100	71.4	31939	PASS
175	174	5	9	6.8	2157	PASS
176	174	95	101	95.7	30560	PASS
177	176	5	9	7.3	2234	PASS

Average of 12.842 to 12.854 min.: VN076913.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.15	421	49.00	1927	63.10	1313	73.05	2124
37.05	2002	50.00	8598	63.80	167	74.05	7611
38.00	2157	51.00	3128	64.00	134	75.05	2411
39.05	1038	52.05	117	65.05	316	76.00	2135
39.90	144	53.00	69	66.85	155	77.00	275
43.95	335	55.95	689	67.20	87	77.20	132
45.10	401	56.95	1095	68.05	4315	77.80	75
46.85	402	59.95	484	69.05	4787	78.95	1931
47.20	181	61.00	2126	69.90	52	79.90	358
47.40	135	62.00	2503	70.20	71	80.10	168
47.90	261	62.90	626	72.00	286	80.90	1421

Average of 12.842 to 12.854 min.: VN076913.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.80	468	95.10	44704	118.90	376	159.10	68
82.10	101	96.05	3199	127.95	242	171.50	110
87.05	2126	97.20	102	129.00	133	171.95	444
87.80	546	103.90	230	129.80	135	173.00	97
88.05	1192	105.60	52	130.00	85	174.05	31939
90.70	55	105.80	92	132.90	66	174.90	545
91.05	177	106.05	138	140.95	716	175.05	2157
91.80	416	115.90	65	142.95	675	176.00	30560
92.05	839	116.80	168	145.00	147	177.05	2234
93.05	1969	117.05	257	146.90	55	193.20	61
94.05	5277	117.80	330	147.90	51	206.80	52

Average of 12.842 to 12.854 min.: VN076913.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
280.95	403						
281.30	210						
281.90	52						
355.40	58						

Instrument :

MSVOA_N

ClientSampleId :

BFB