
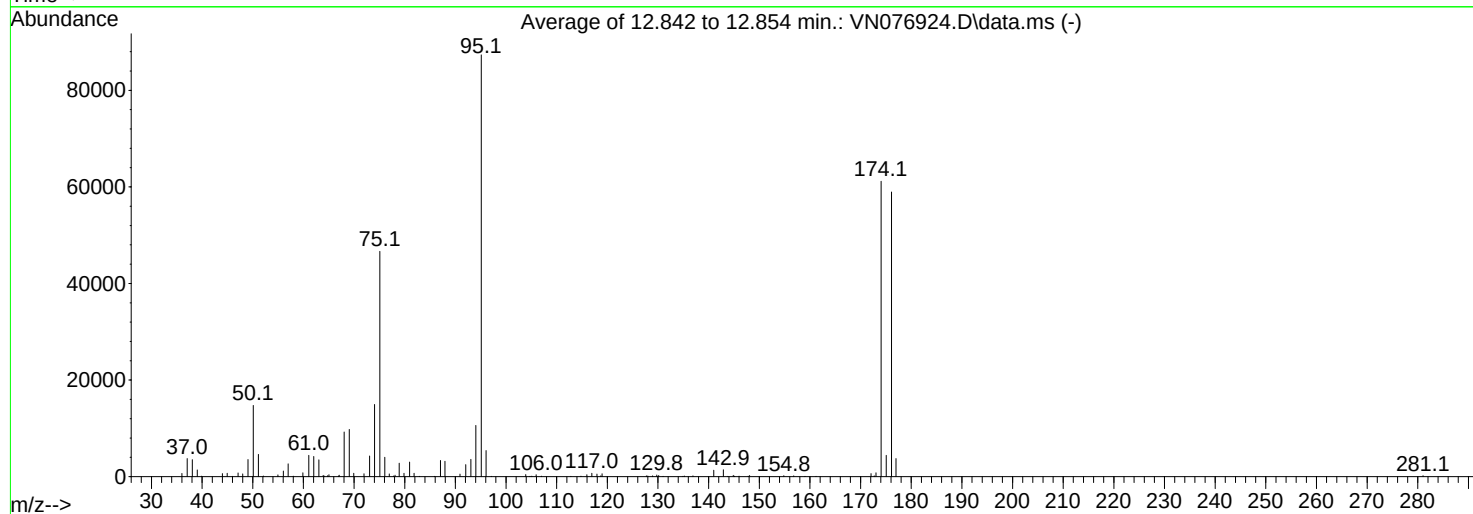


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031023\
Data File : VN076924.D
Acq On : 10 Mar 2023 14:44
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031023W.M
Title : SW846 8260
Last Update : Fri Mar 10 13:47:39 2023

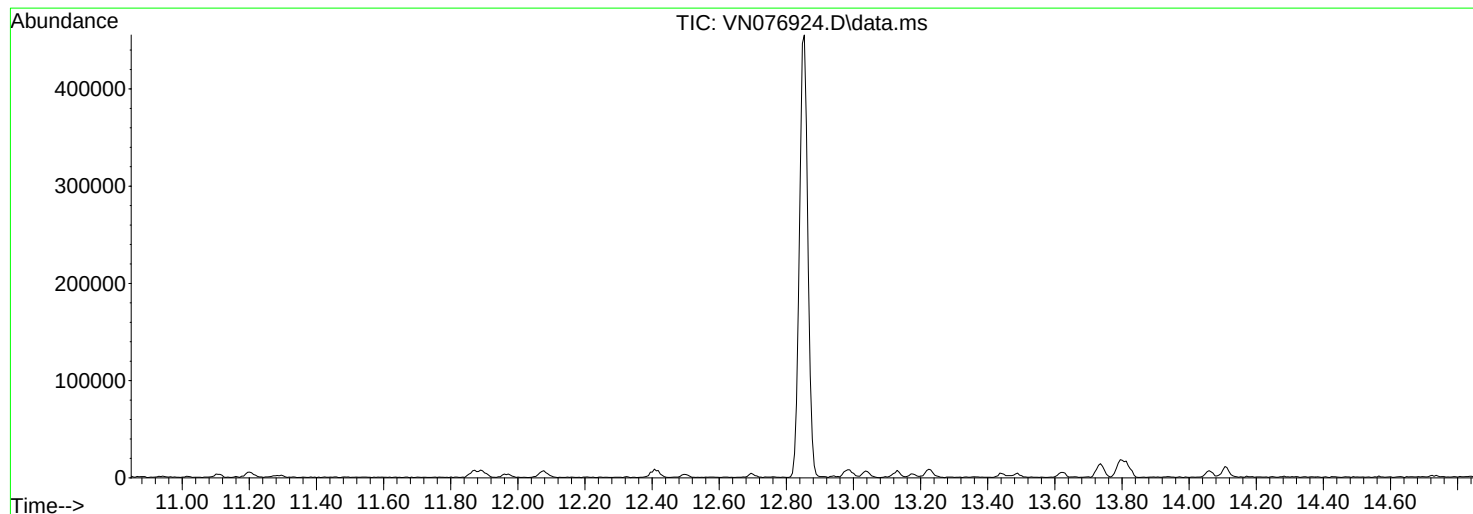

AutoFind: Scans 1854, 1855, 1856; Background Corrected with Scan 1846

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.9	14760	PASS
75	95	30	60	53.4	46675	PASS
95	95	100	100	100.0	87355	PASS
96	95	5	9	6.2	5412	PASS
173	174	0.00	2	1.3	780	PASS
174	95	50	100	70.0	61165	PASS
175	174	5	9	7.2	4419	PASS
176	174	95	101	96.4	58965	PASS
177	176	5	9	6.3	3744	PASS

Average of 12.842 to 12.854 min.: VN076924.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	660	50.10	14760	63.90	257	74.05	1495
37.05	3748	51.10	4612	64.10	134	75.10	4667
38.05	3507	52.10	130	64.80	204	76.05	400
39.05	1401	54.95	352	65.05	393	76.95	57
39.90	85	56.05	1157	66.90	141	77.80	133
44.00	628	57.00	2640	67.05	296	78.10	302
44.95	685	58.00	105	68.05	9254	78.90	2785
46.00	54	59.90	794	69.05	9768	79.85	709
47.10	756	61.05	4416	69.95	693	80.95	3022
48.00	568	62.05	4173	71.95	590	81.85	687
49.05	3562	63.05	3496	73.05	4289	82.90	64

Average of 12.842 to 12.854 min.: VN076924.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
85.90	55	104.70	71	127.70	157	143.80	65
87.05	3342	105.10	84	128.00	149	144.85	254
87.95	3184	105.95	399	128.95	155	145.10	106
90.90	544	107.00	109	129.75	333	146.00	89
92.05	2481	112.80	69	130.15	230	147.80	94
93.05	3589	114.80	103	131.00	72	148.10	236
94.05	10594	115.95	389	134.90	59	154.85	208
95.10	87355	116.95	695	135.20	123	156.80	182
96.05	5412	117.95	518	136.90	155	159.00	58
97.10	77	118.70	163	141.00	1322	161.20	61
103.90	451	118.95	590	142.90	1420	172.05	641

Average of 12.842 to 12.854 min.: VN076924.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.70	159						
173.05	780						
174.05	61165						
175.05	4419						
176.10	58965						
177.00	3744						
281.05	216						

Instrument :

MSVOA_N

ClientSampleId :

BFB