

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031025\
 Data File : VN085916.D
 Acq On : 10 Mar 2025 13:22
 Operator : JC\MD
 Sample : VN0310WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0310WBL01

Quant Time: Mar 11 01:37:14 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 19 03:43:32 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	185188	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	337149	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	297684	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	112686	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	131135	54.619	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	109.240%
35) Dibromofluoromethane	8.165	113	111691	50.627	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	101.260%
50) Toluene-d8	10.565	98	376828	46.947	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	93.900%
62) 4-Bromofluorobenzene	12.847	95	118920	44.967	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	89.940%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031025\
Data File : VN085916.D
Acq On : 10 Mar 2025 13:22
Operator : JC\MD
Sample : VN0310WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0310WBL01

Quant Time: Mar 11 01:37:14 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 19 03:43:32 2025
Response via : Initial Calibration




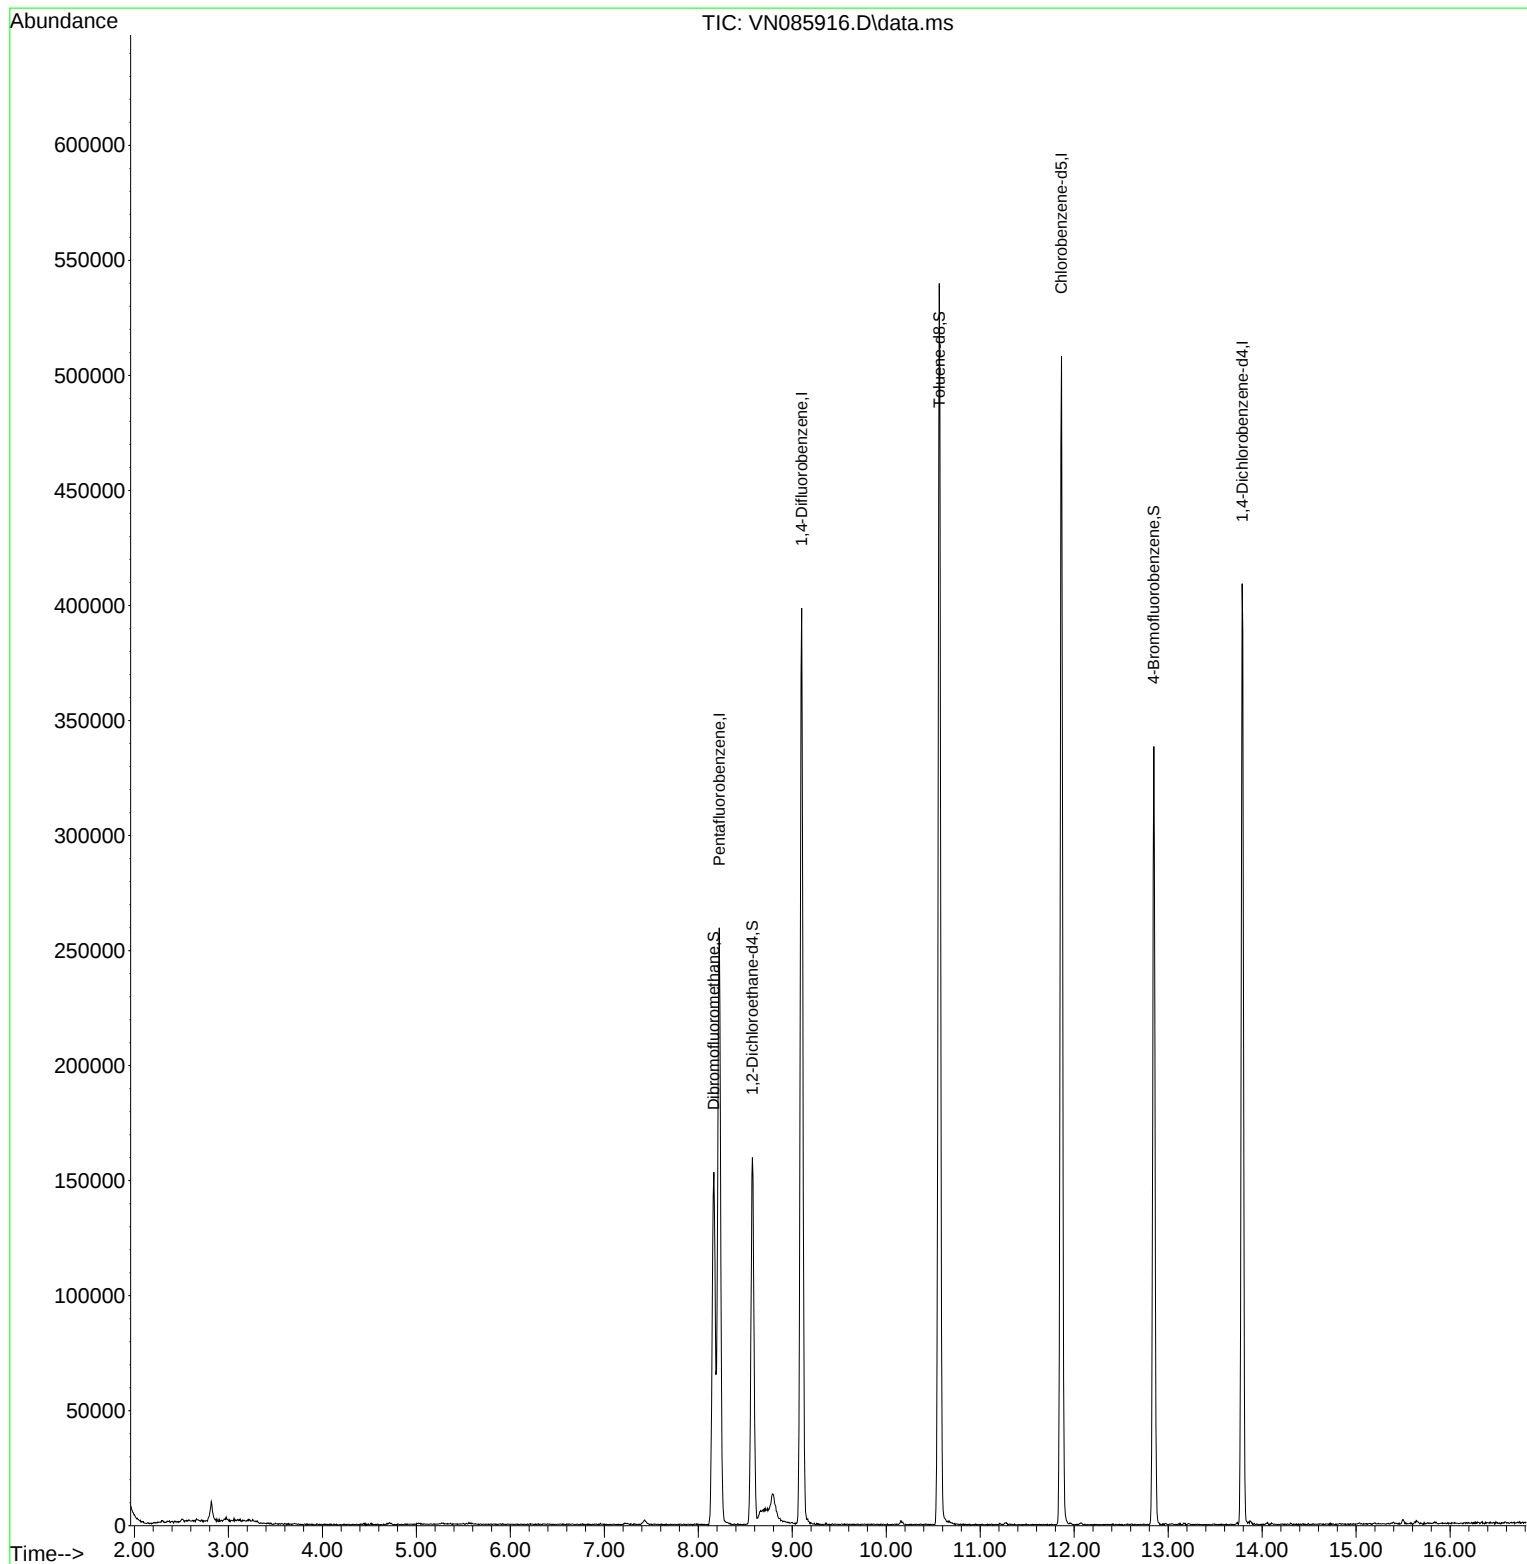


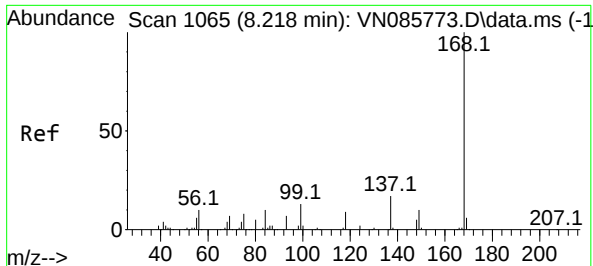

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1106
Delta R.T. 0.006 min
Lab File: VN085916.D
Acq: 10 Mar 2025 13:22




Instrument :
MSVOA_N
ClientSampleId :
VN0310WBL01


Tgt Ion:168 Resp: 185188
Ion Ratio Lower Upper
168 100
99 60.0 47.9 71.9

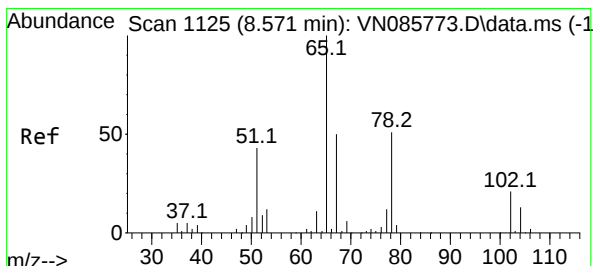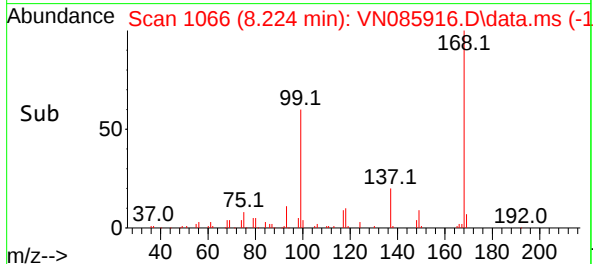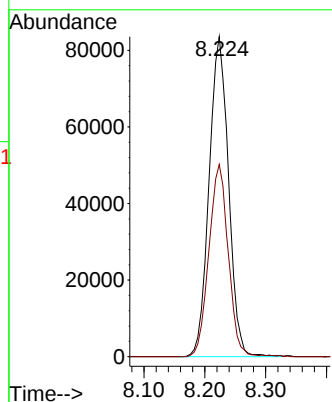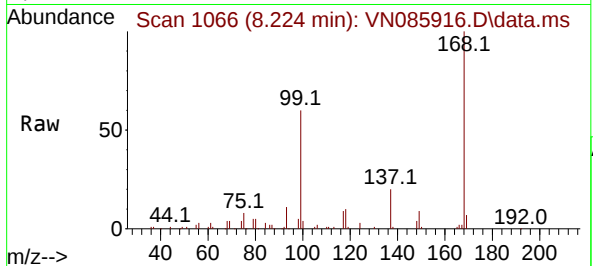

#33
1,2-Dichloroethane-d4
Concen: 54.619 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.006 min
Lab File: VN085916.D
Acq: 10 Mar 2025 13:22

Tgt Ion: 65 Resp: 131135
Ion Ratio Lower Upper
65 100
67 53.7 0.0 106.2

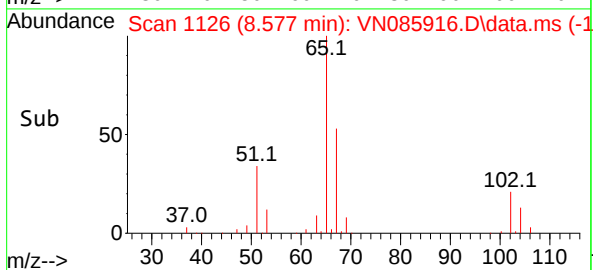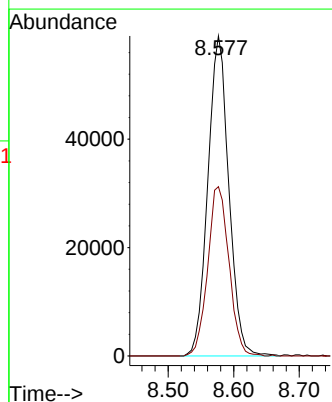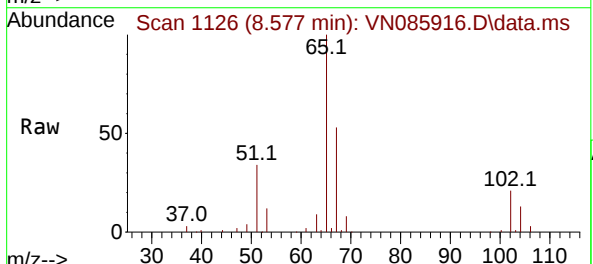

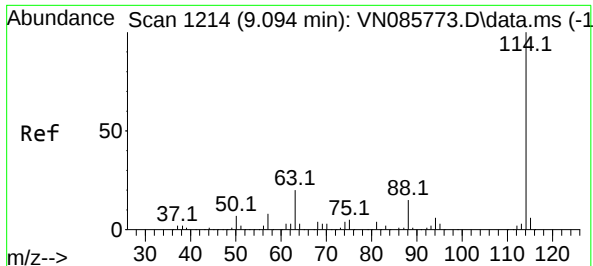

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 11

Delta R.T. 0.006 min

Lab File: VN085916.D

Acq: 10 Mar 2025 13:22

Instrument :

MSVOA_N

ClientSampleId :

VN0310WBL01





Tgt Ion:114 Resp: 337149

Ion Ratio Lower Upper

114 100

63 20.5 0.0 39.2

88 16.7 0.0 30.0

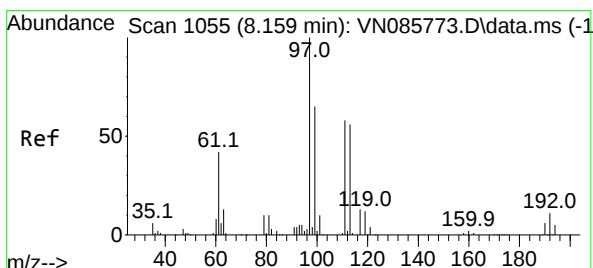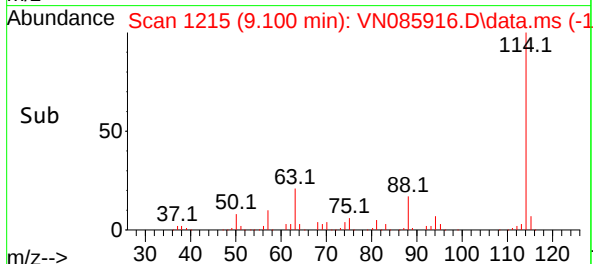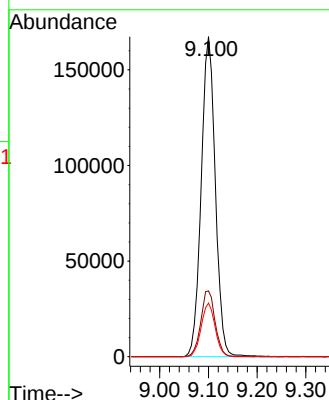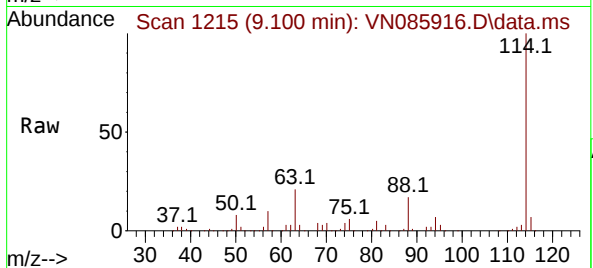

#35

Dibromofluoromethane

Concen: 50.627 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.006 min

Lab File: VN085916.D

Acq: 10 Mar 2025 13:22




Tgt Ion:113 Resp: 111691


Ion Ratio Lower Upper

113 100

111 103.6 82.2 123.4

192 18.7 14.7 22.1


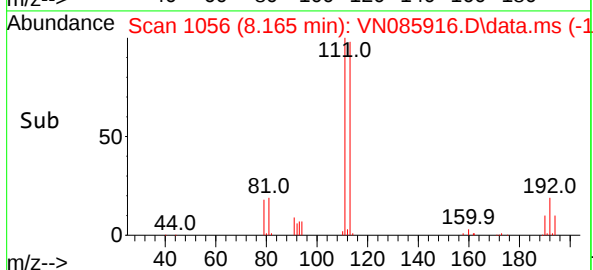
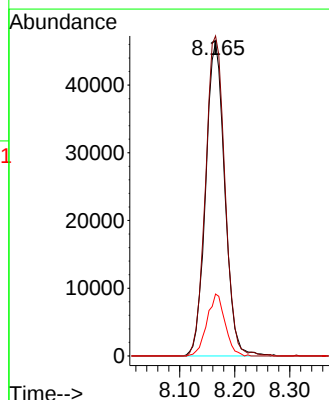
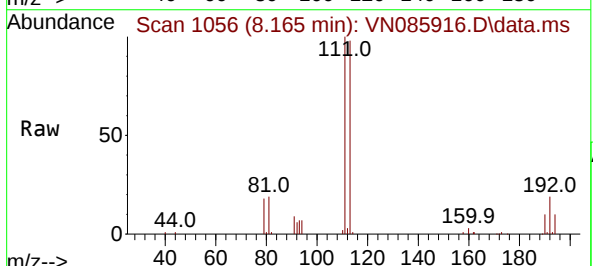


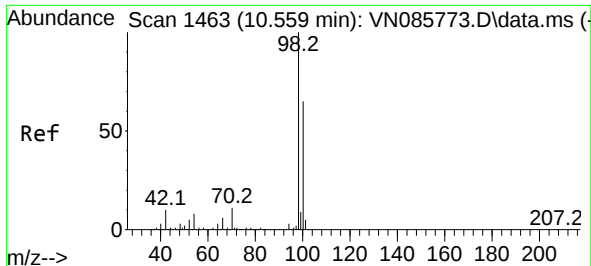

#50
Toluene-d8
Concen: 46.947 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.006 min
Lab File: VN085916.D
Acq: 10 Mar 2025 13:22




Instrument :
MSVOA_N
ClientSampleId :
VN0310WBL01


Tgt Ion: 98 Resp: 376828
Ion Ratio Lower Upper
98 100
100 64.8 52.1 78.1

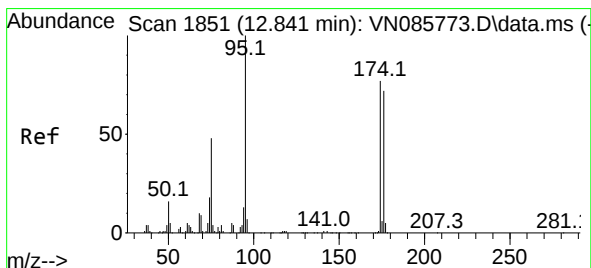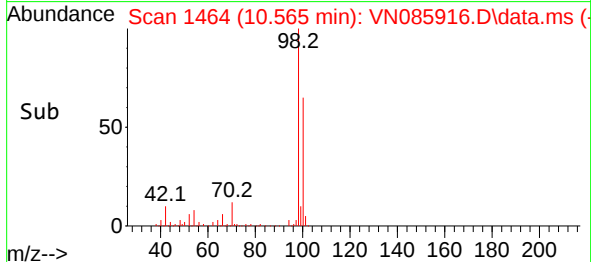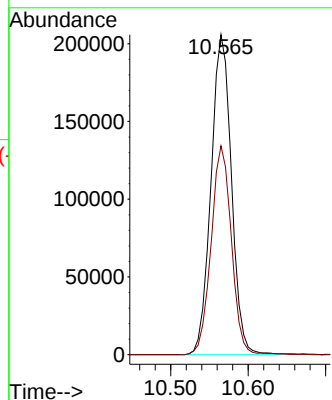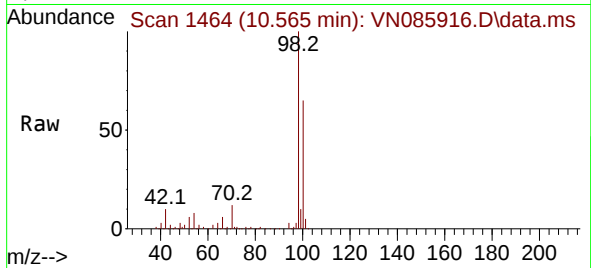

#62
4-Bromofluorobenzene
Concen: 44.967 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.006 min
Lab File: VN085916.D
Acq: 10 Mar 2025 13:22

Tgt Ion: 95 Resp: 118920
Ion Ratio Lower Upper
95 100
174 77.1 0.0 152.4
176 72.7 0.0 146.6


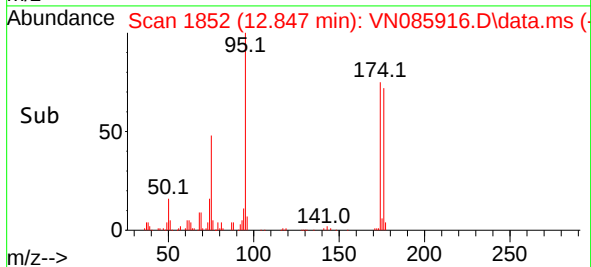
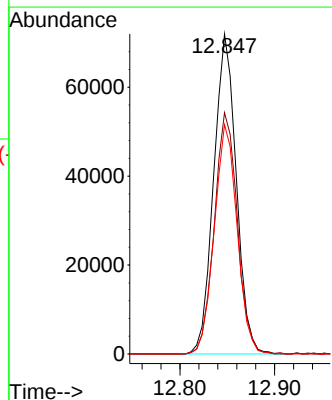
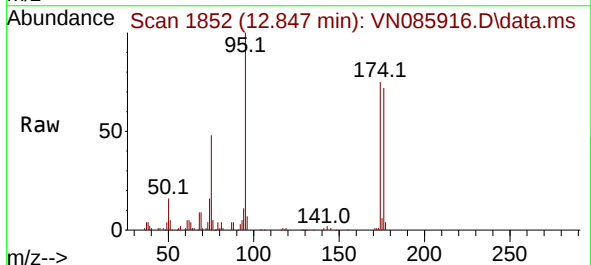


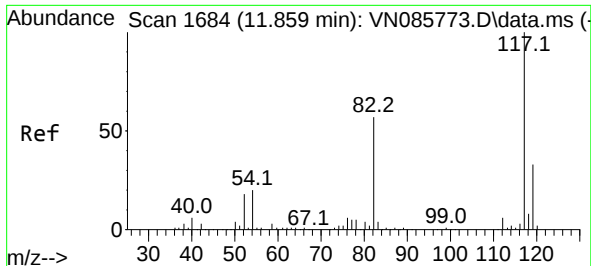

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. 0.006 min
Lab File: VN085916.D
Acq: 10 Mar 2025 13:22

Instrument :
MSVOA_N
ClientSampleId :
VN0310WBL01

Tgt Ion:117 Resp: 297684
Ion Ratio Lower Upper
117 100
82 57.2 45.7 68.5
119 33.0 26.2 39.2

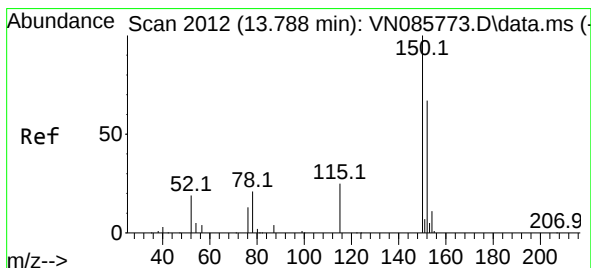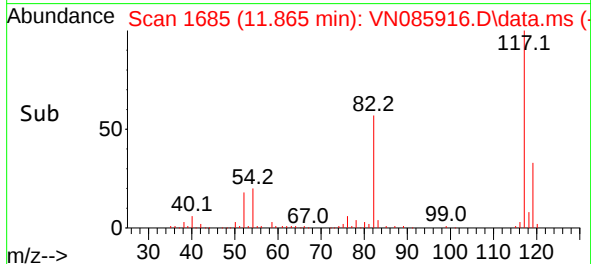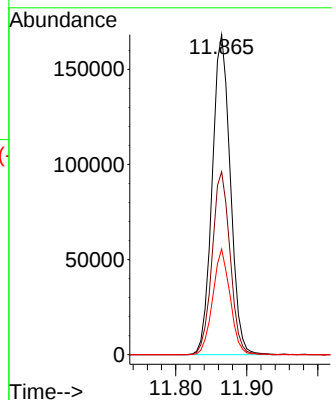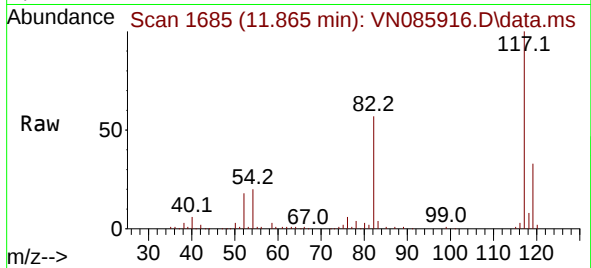

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. 0.000 min
Lab File: VN085916.D
Acq: 10 Mar 2025 13:22

Tgt Ion:152 Resp: 112686
Ion Ratio Lower Upper
152 100
115 64.0 30.4 91.3
150 158.5 0.0 345.4

