

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031124\
 Data File : VN081353.D
 Acq On : 11 Mar 2024 10:55
 Operator : JC\MD
 Sample : VN0311MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0311MBL01

Quant Time: Mar 12 04:48:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030524W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 06 03:12:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	317811	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	557519	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	486072	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	193985	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	224601	48.877	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	97.760%
35) Dibromofluoromethane	8.165	113	175061	51.251	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.500%
50) Toluene-d8	10.565	98	662604	51.892	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	103.780%
62) 4-Bromofluorobenzene	12.853	95	206853	45.835	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	=	91.660%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031124\
Data File : VN081353.D
Acq On : 11 Mar 2024 10:55
Operator : JC\MD
Sample : VN0311MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0311MBL01

Quant Time: Mar 12 04:48:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030524W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 06 03:12:57 2024
Response via : Initial Calibration




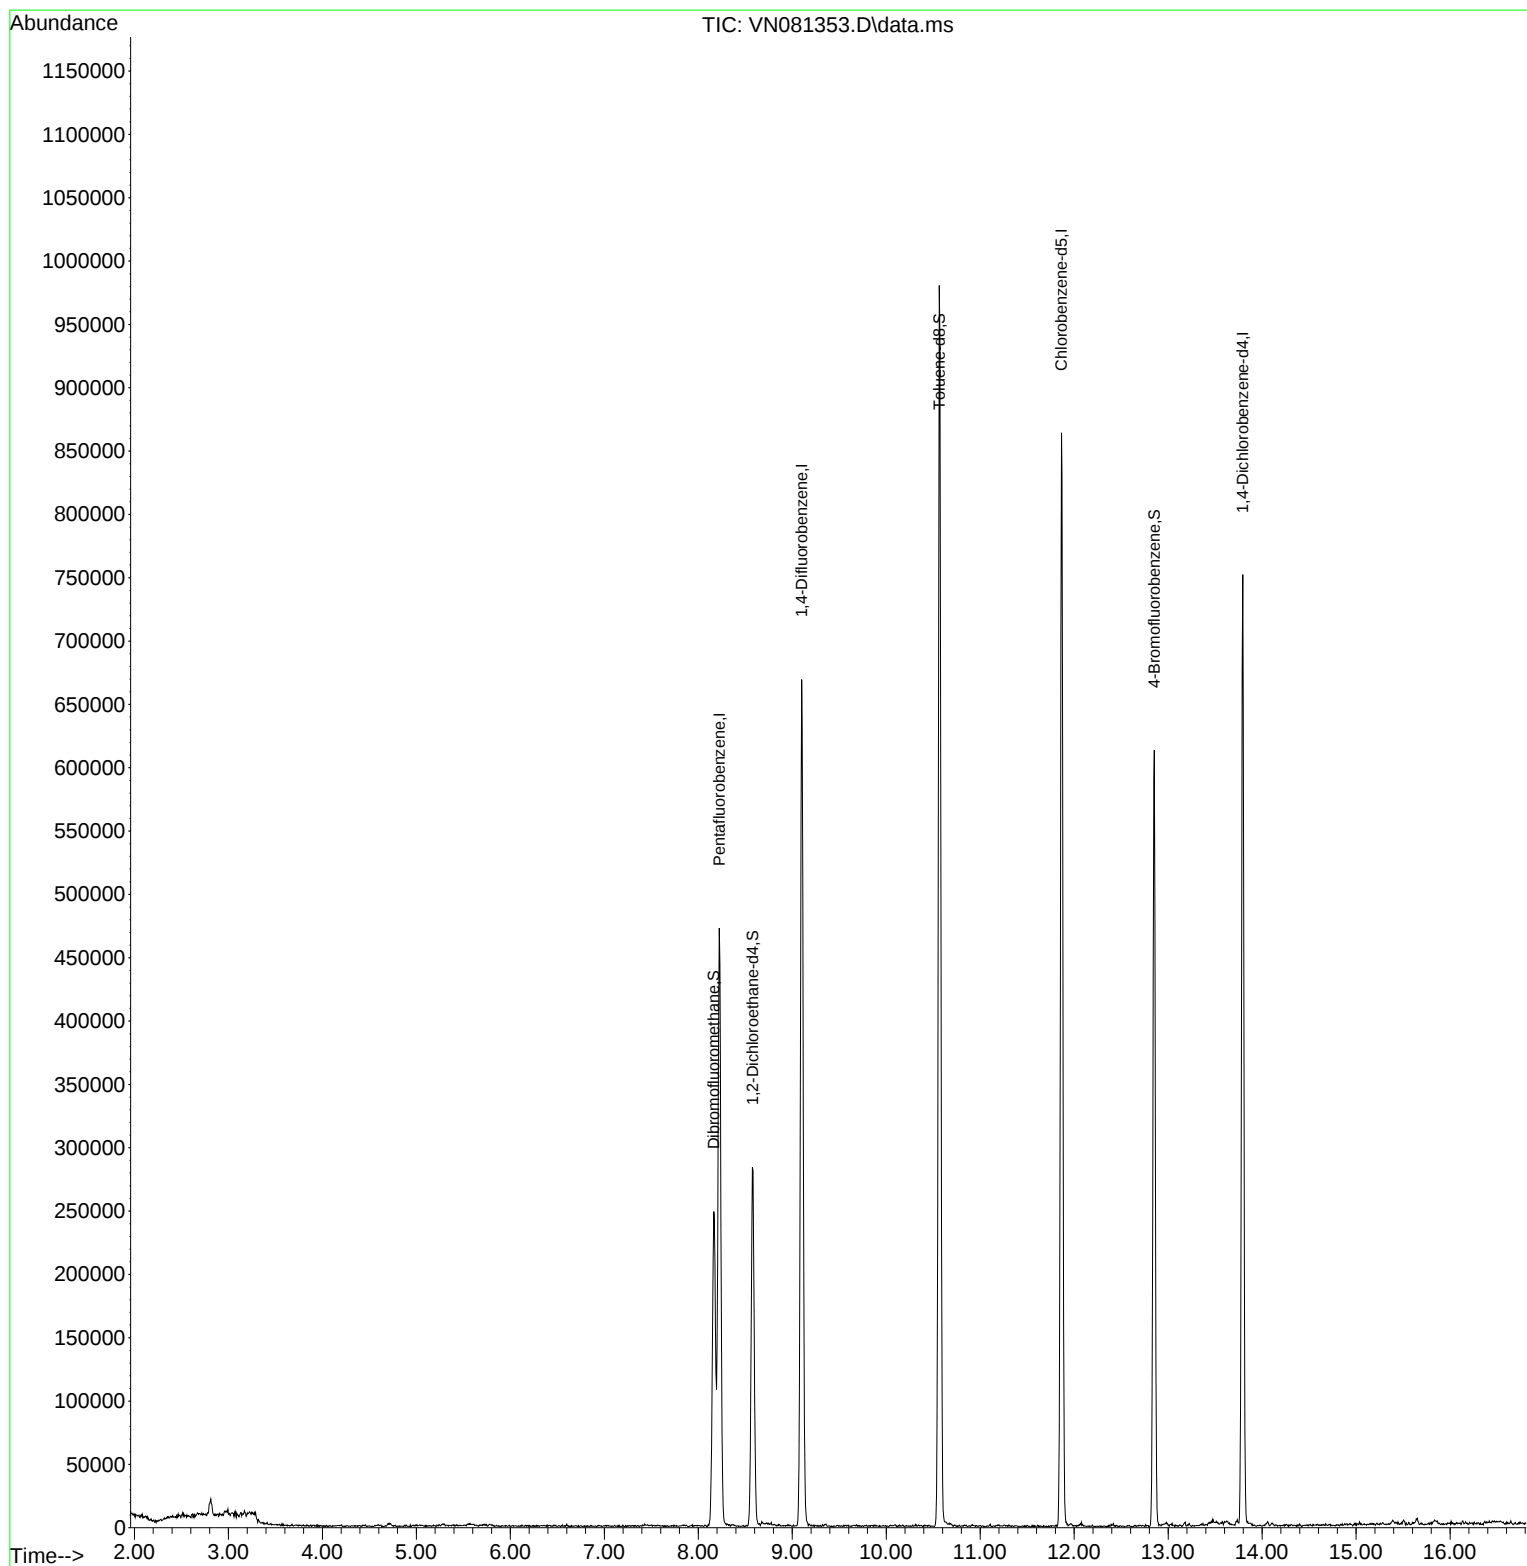


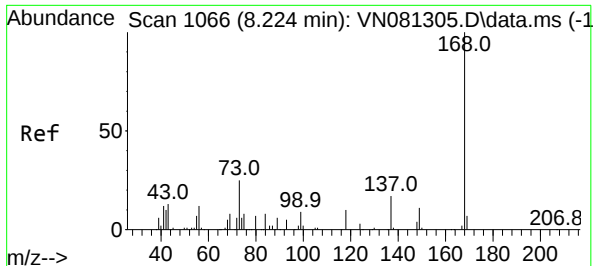

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN081353.D
Acq: 11 Mar 2024 10:55




Instrument :
MSVOA_N
ClientSampleId :
VN0311MBL01


Tgt Ion:168 Resp: 317811
Ion Ratio Lower Upper
168 100
99 62.8 59.9 89.9

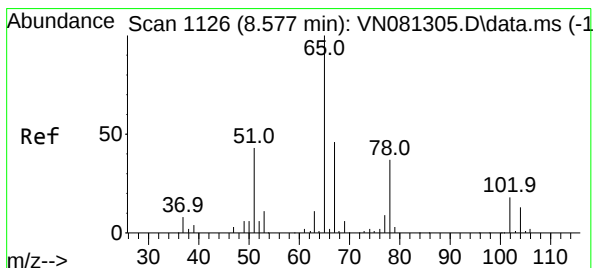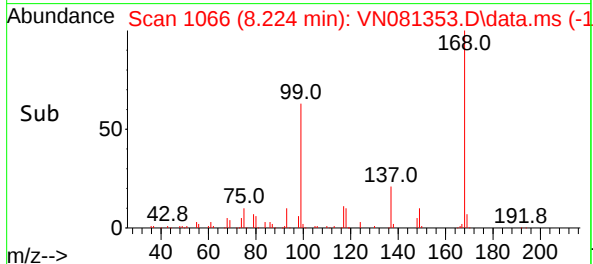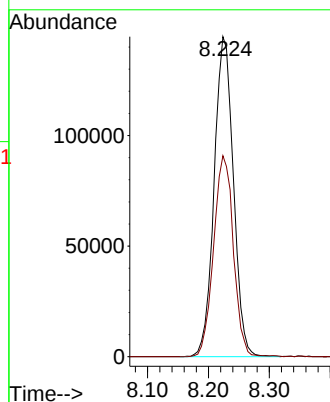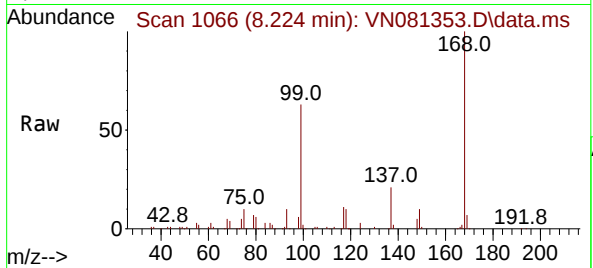

#33
1,2-Dichloroethane-d4
Concen: 48.877 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VN081353.D
Acq: 11 Mar 2024 10:55

Tgt Ion: 65 Resp: 224601
Ion Ratio Lower Upper
65 100
67 52.4 0.0 102.4

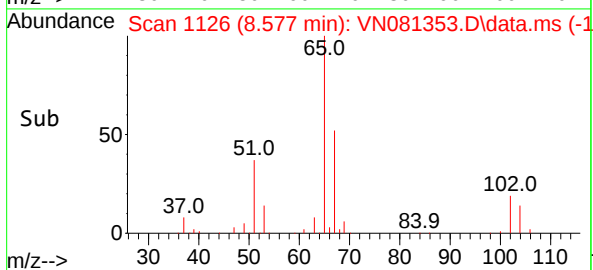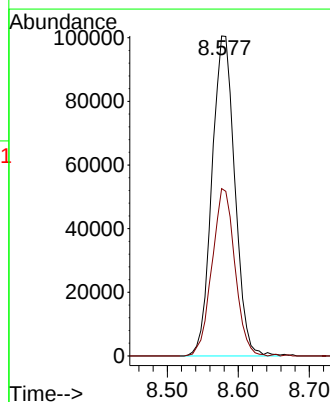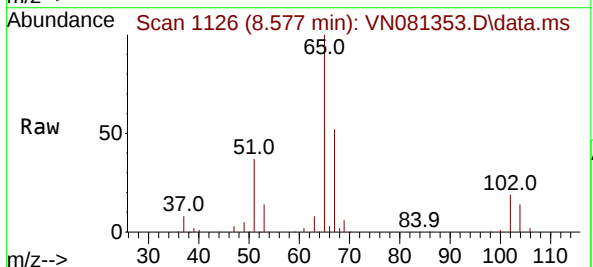

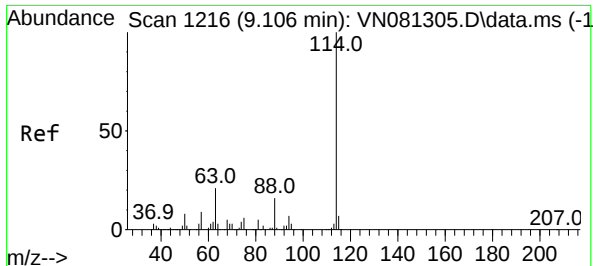

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. -0.006 min

Lab File: VN081353.D

Acq: 11 Mar 2024 10:55

Instrument :

MSVOA_N

ClientSampleId :

VN0311MBL01





Tgt Ion:114 Resp: 557519

Ion Ratio Lower Upper

114 100

63 21.5 0.0 48.0

88 16.1 0.0 34.8

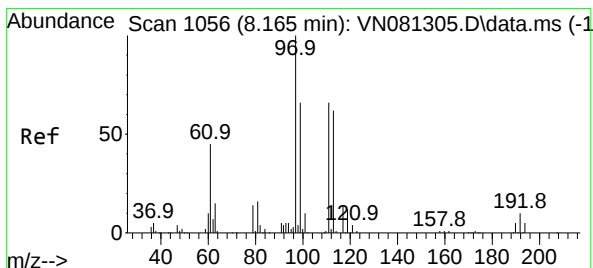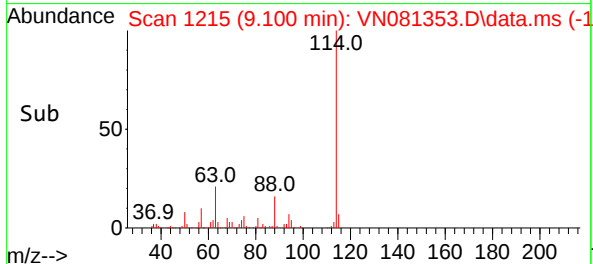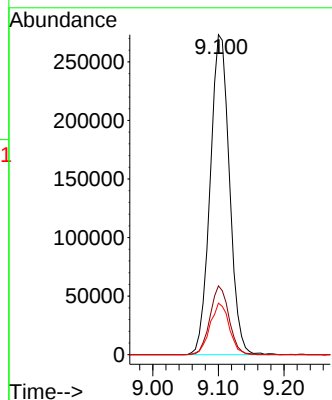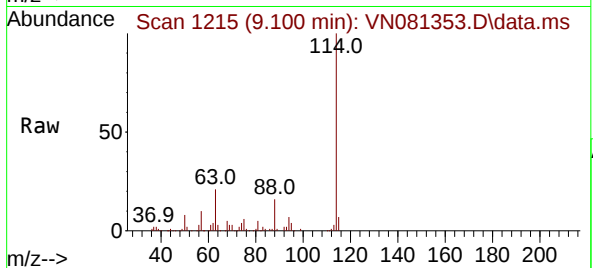

#35

Dibromofluoromethane

Concen: 51.251 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN081353.D

Acq: 11 Mar 2024 10:55




Tgt Ion:113 Resp: 175061


Ion Ratio Lower Upper

113 100

111 103.8 82.2 123.4

192 16.6 12.5 18.7


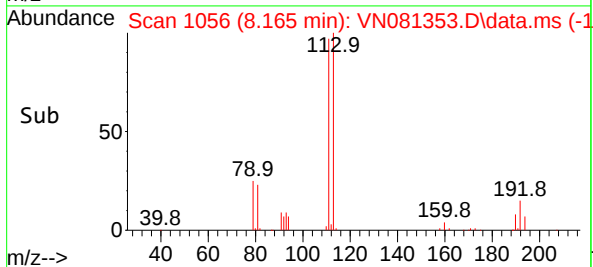
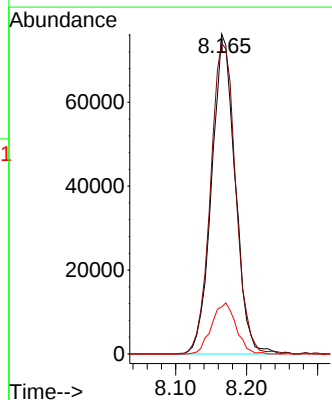
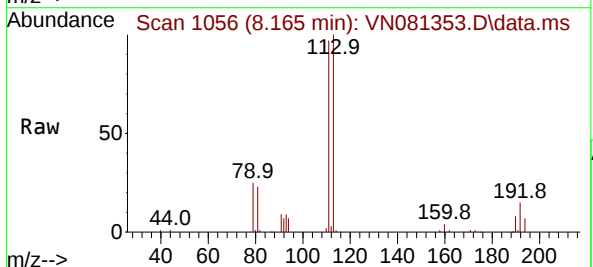


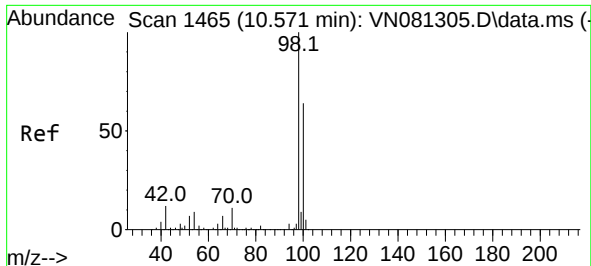

#50
Toluene-d8
Concen: 51.892 ug/l
RT: 10.565 min Scan# 1465
Delta R.T. -0.006 min
Lab File: VN081353.D
Acq: 11 Mar 2024 10:55




Instrument :
MSVOA_N
ClientSampleId :
VN0311MBL01


Tgt Ion: 98 Resp: 662604
Ion Ratio Lower Upper
98 100
100 65.2 51.4 77.0

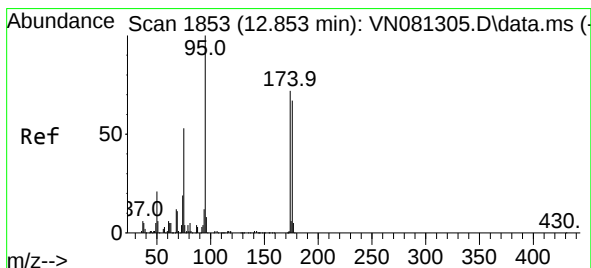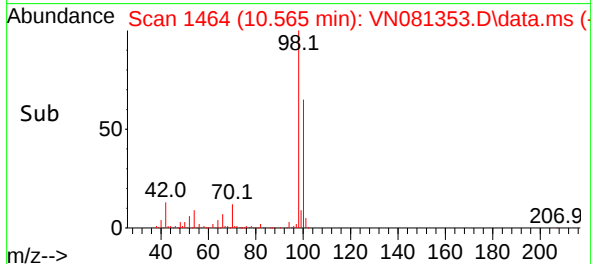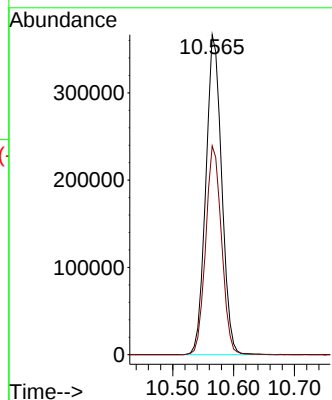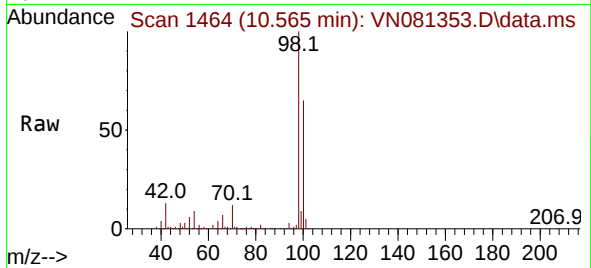

#62
4-Bromofluorobenzene
Concen: 45.835 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN081353.D
Acq: 11 Mar 2024 10:55

Tgt Ion: 95 Resp: 206853
Ion Ratio Lower Upper
95 100
174 71.2 0.0 120.4
176 69.3 0.0 121.0


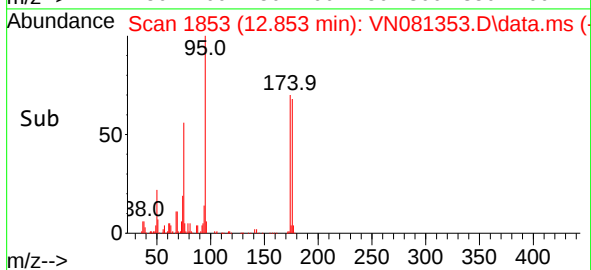
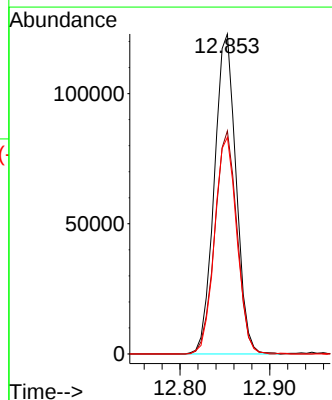
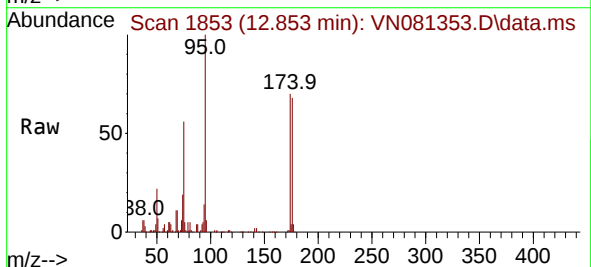


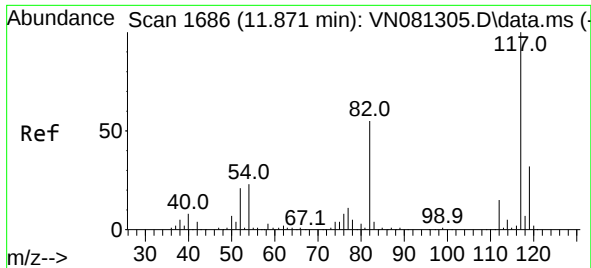

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.006 min
Lab File: VN081353.D
Acq: 11 Mar 2024 10:55

Instrument :
MSVOA_N
ClientSampleId :
VN0311MBL01

Tgt Ion:117 Resp: 486072
Ion Ratio Lower Upper
117 100
82 57.9 52.7 79.1
119 32.1 25.3 37.9

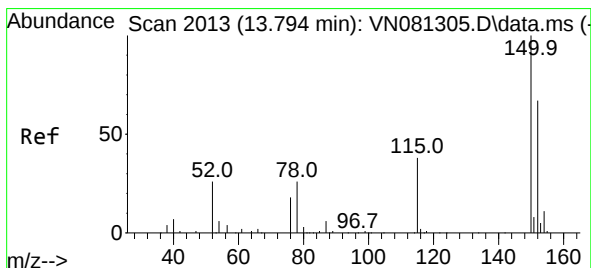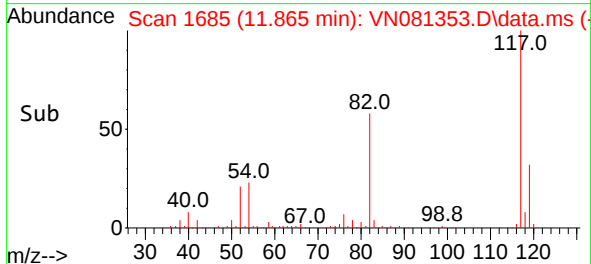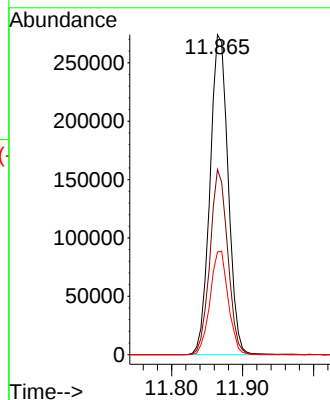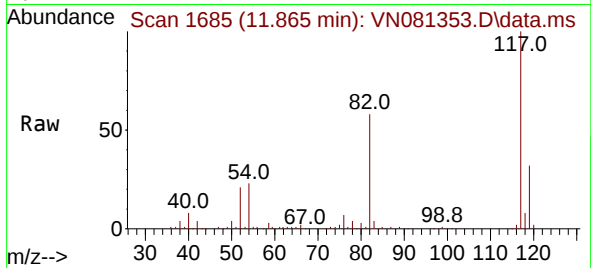

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN081353.D
Acq: 11 Mar 2024 10:55

Tgt Ion:152 Resp: 193985
Ion Ratio Lower Upper
152 100
115 63.4 32.3 96.8
150 156.9 0.0 339.8

