

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031124\
 Data File : VN081358.D
 Acq On : 11 Mar 2024 13:04
 Operator : JC\MD
 Sample : P1724-01
 Misc : 1.06g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 13925

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030524W.M
 Title : SW846 8260

Signal : TIC: VN081358.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.830	136	149	150	rBV5	43284	115011	6.23%	1.133%
2	2.895	153	160	163	rVV9	23159	69050	3.74%	0.680%
3	5.259	552	562	571	rBV5	5625	18811	1.02%	0.185%
4	8.165	1045	1056	1060	rBV2	245383	591393	32.01%	5.826%
5	8.218	1060	1065	1076	rVB	476975	1056242	57.17%	10.406%
6	8.577	1115	1126	1138	rBV	290451	653294	35.36%	6.436%
7	9.100	1205	1215	1229	rBV	694714	1400917	75.83%	13.801%
8	10.012	1363	1370	1380	rVV3	12004	24398	1.32%	0.240%
9	10.147	1383	1393	1406	rBV4	20876	46134	2.50%	0.454%
10	10.488	1444	1451	1456	rBV5	11306	22232	1.20%	0.219%
11	10.565	1456	1464	1473	rBV	1012409	1847415	100.00%	18.200%
12	11.870	1676	1686	1700	rBV	847305	1576019	85.31%	15.526%
13	12.853	1845	1853	1862	rVB	654660	1130160	61.18%	11.134%
14	13.170	1899	1907	1914	rVB7	12566	33214	1.80%	0.327%
15	13.482	1954	1960	1965	rVB3	16067	28023	1.52%	0.276%
16	13.794	2004	2013	2027	rVB	862390	1466124	79.36%	14.444%
17	14.335	2099	2105	2112	rVB5	11582	21873	1.18%	0.215%
18	14.629	2150	2155	2158	rBV5	10049	18758	1.02%	0.185%
19	15.041	2219	2225	2232	rVB9	13025	31671	1.71%	0.312%




Sum of corrected areas: 10150739

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031124\
Data File : VN081358.D
Acq On : 11 Mar 2024 13:04
Operator : JC\MD
Sample : P1724-01
Misc : 1.06g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
13925

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030524W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

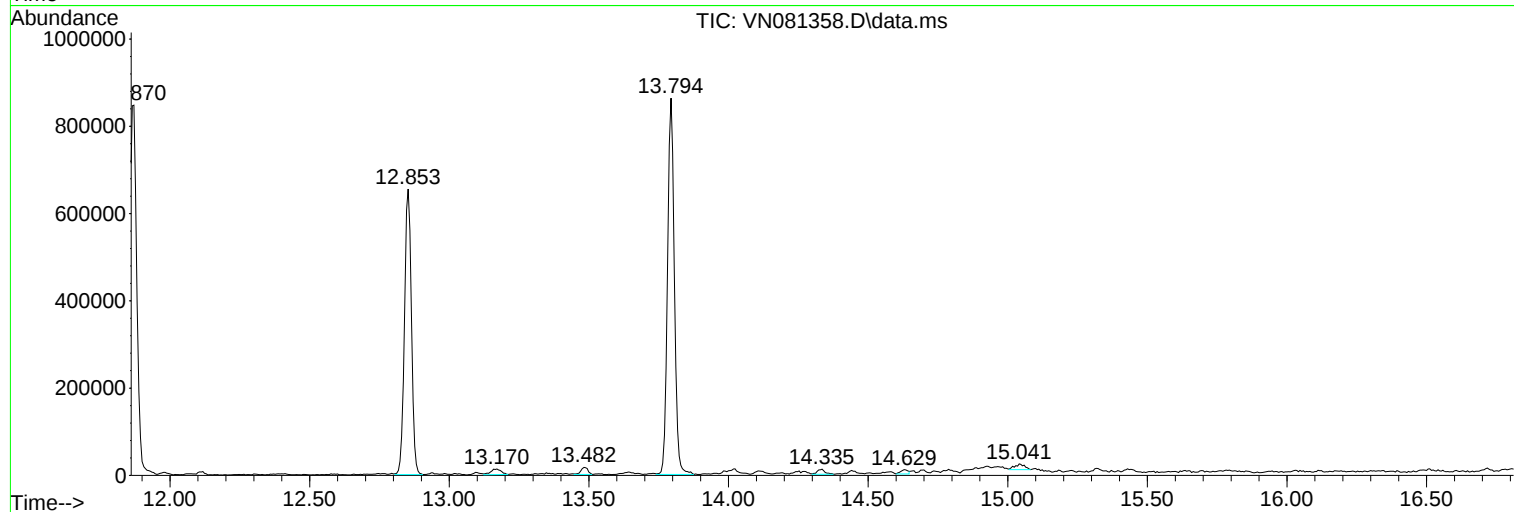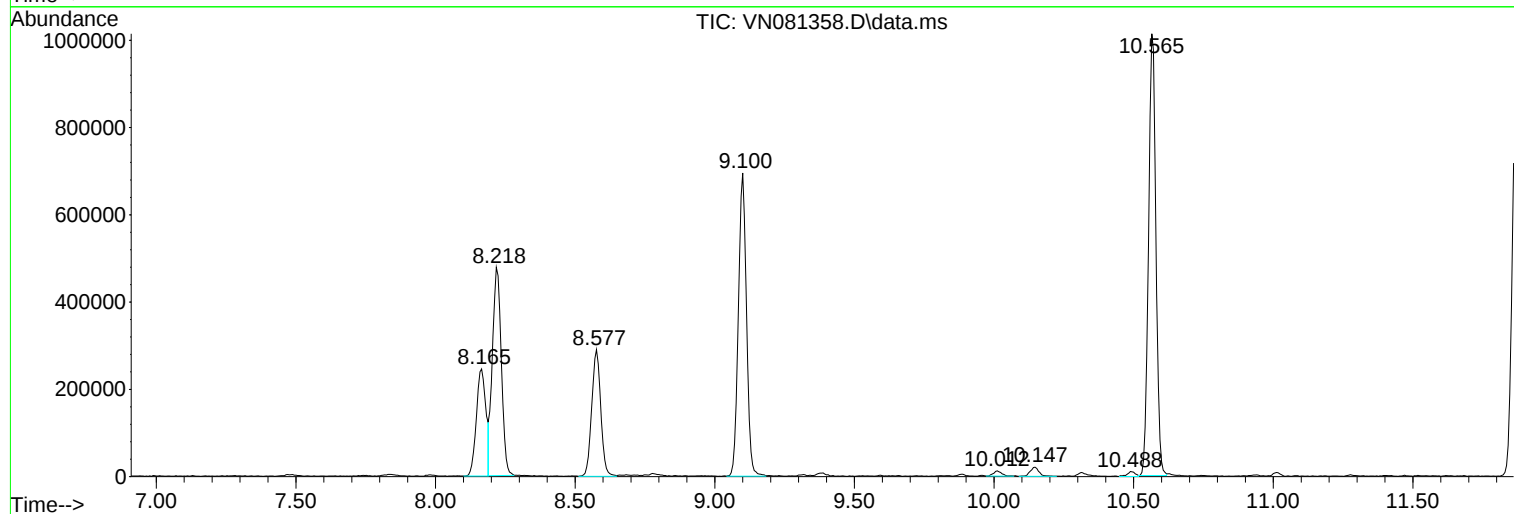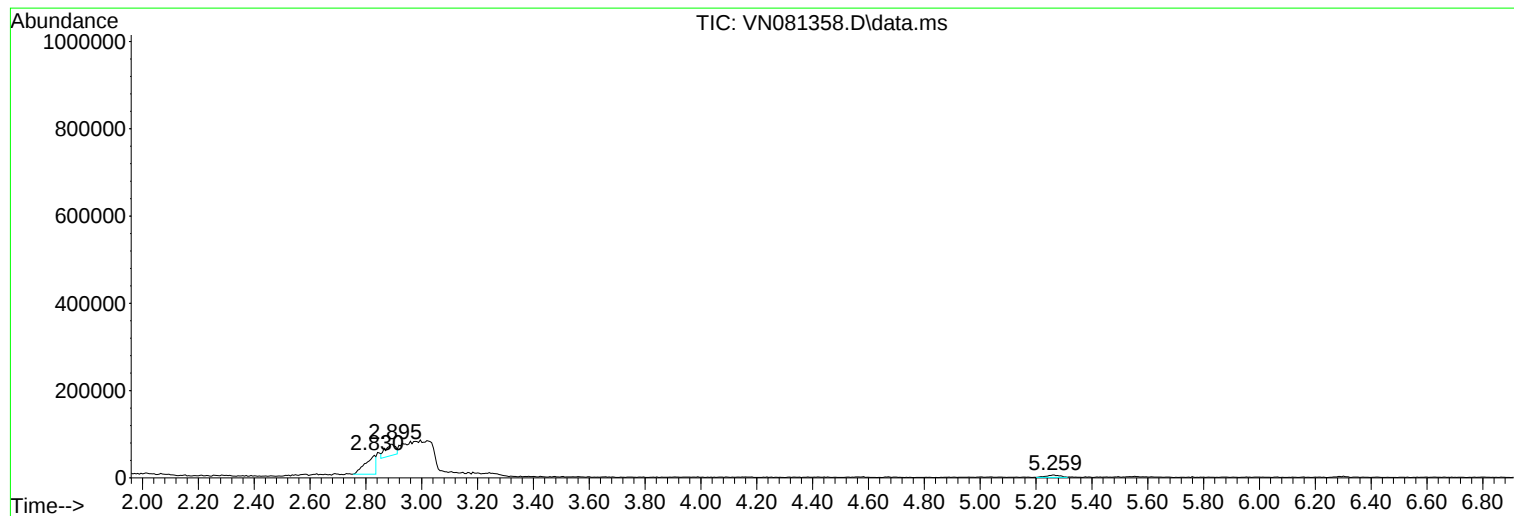

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031124\
Data File : VN081358.D
Acq On : 11 Mar 2024 13:04
Operator : JC\MD
Sample : P1724-01
Misc : 1.06g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 8 Sample Multiplier: 1










Instrument :
MSVOA_N
ClientSampleId :
13925

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030524W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown2.830 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
2.830	5.44 ug/l	115011	Pentafluorobenzene	8.218	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Phosgene	98	CCl2O	000075-44-5	32
2	bis(chloromethyl) carbonate	158	C3H4Cl2O3	1000404-37-0	22
3	2-[2-(2-Chloro-ethoxy)-ethoxy]-p...	216	C10H13ClO3	1000317-46-1	17
4	Ethene, (2-chloroethoxy)-	106	C4H7ClO	000110-75-8	12
5	Bis(.beta.-chloroethyl) sulfoxide	174	C4H8Cl2OS	005819-08-9	12

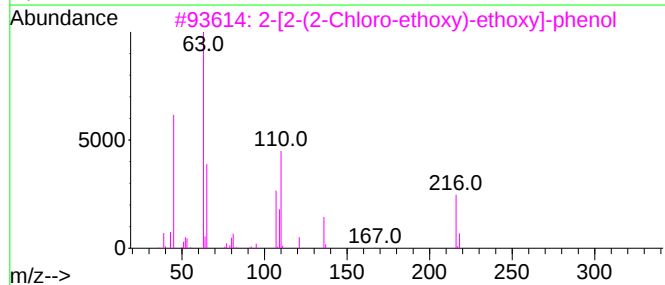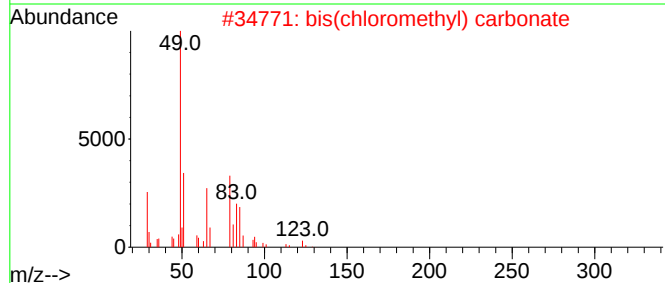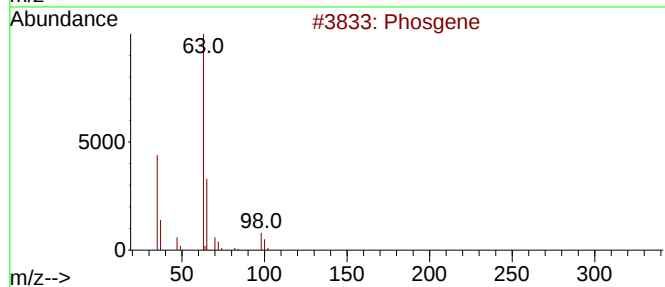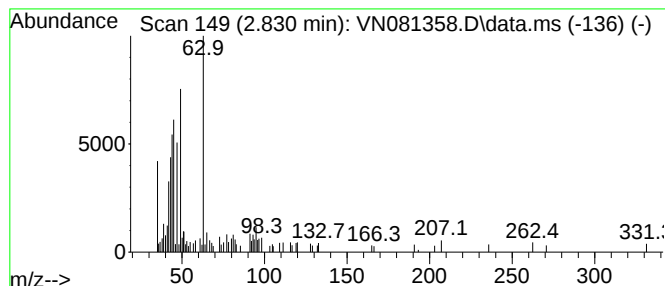

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031124\
Data File : VN081358.D
Acq On : 11 Mar 2024 13:04
Operator : JC\MD
Sample : P1724-01
Misc : 1.06g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
13925

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030524W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown2.830	2.830	5.4	ug/l	115011	1	8.218	1056240	50.0