
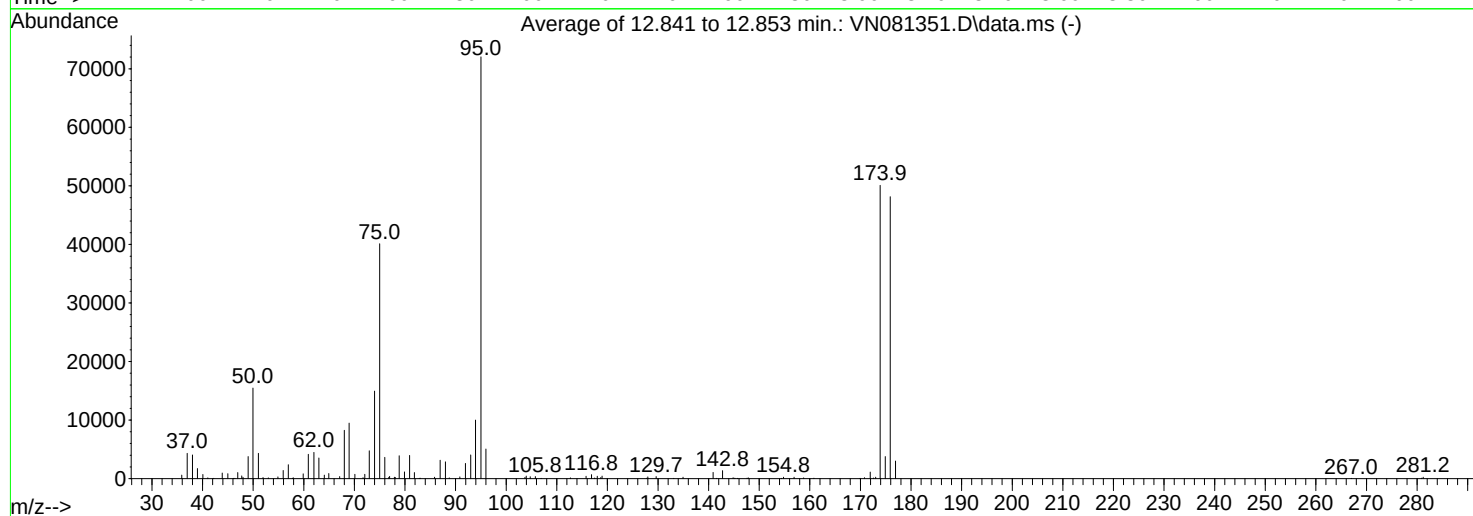


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031124\
Data File : VN081351.D
Acq On : 11 Mar 2024 08:48
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030524W.M
Title : SW846 8260
Last Update : Wed Mar 06 03:12:57 2024

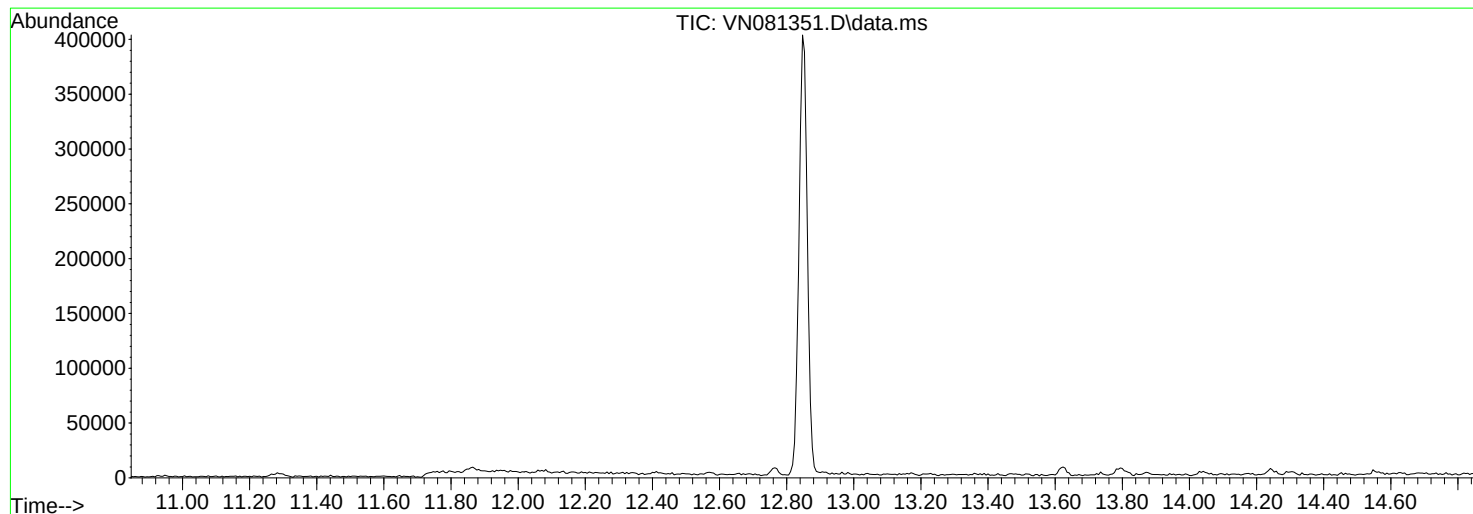

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	15482	PASS
75	95	30	60	55.7	40117	PASS
95	95	100	100	100.0	72043	PASS
96	95	5	9	7.0	5048	PASS
173	174	0.00	2	0.5	251	PASS
174	95	50	100	69.5	50101	PASS
175	174	5	9	7.5	3779	PASS
176	174	95	101	96.1	48147	PASS
177	176	5	9	6.3	3020	PASS

Average of 12.841 to 12.853 min.: VN081351.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	607	46.95	1034	57.80	89	70.10	74
36.95	4323	47.75	472	57.95	136	71.70	16
38.00	4045	48.00	229	59.90	819	72.05	74
39.00	1718	49.00	3776	60.90	4160	72.95	476
40.05	716	49.95	15482	62.00	4494	74.00	14943
41.05	129	51.05	4328	63.00	3525	75.00	40117
42.20	65	51.95	186	64.05	602	76.00	3639
43.90	948	53.00	148	64.95	881	76.80	226
45.00	858	54.90	307	67.10	367	76.95	372
46.10	59	55.95	1399	68.00	8248	77.90	246
46.40	65	56.95	2373	68.95	9494	78.10	192

Average of 12.841 to 12.853 min.: VN081351.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.85	3914	91.95	2591	115.80	407	140.90	1077
79.90	1138	93.00	4046	116.85	685	141.60	50
80.90	3959	93.95	10005	117.50	102	142.75	1381
81.85	1029	95.00	72043	118.00	405	144.85	155
82.80	65	96.00	5048	118.70	191	145.20	85
83.00	75	103.70	223	118.95	447	145.70	67
85.85	243	103.95	438	127.80	87	147.60	85
86.95	3151	104.75	337	128.00	291	147.85	128
88.00	2872	105.75	349	129.65	357	154.40	66
88.75	129	106.90	71	133.10	63	154.80	246
90.85	312	112.70	130	134.95	249	156.90	239

Average of 12.841 to 12.853 min.: VN081351.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
158.80	139	267.00	55				
160.80	77	280.90	84				
169.90	56	281.20	237				
170.80	164						
171.95	1118						
172.60	116						
173.00	251						
173.90	50101						
174.90	3779						
175.90	48147						
176.95	3020						