
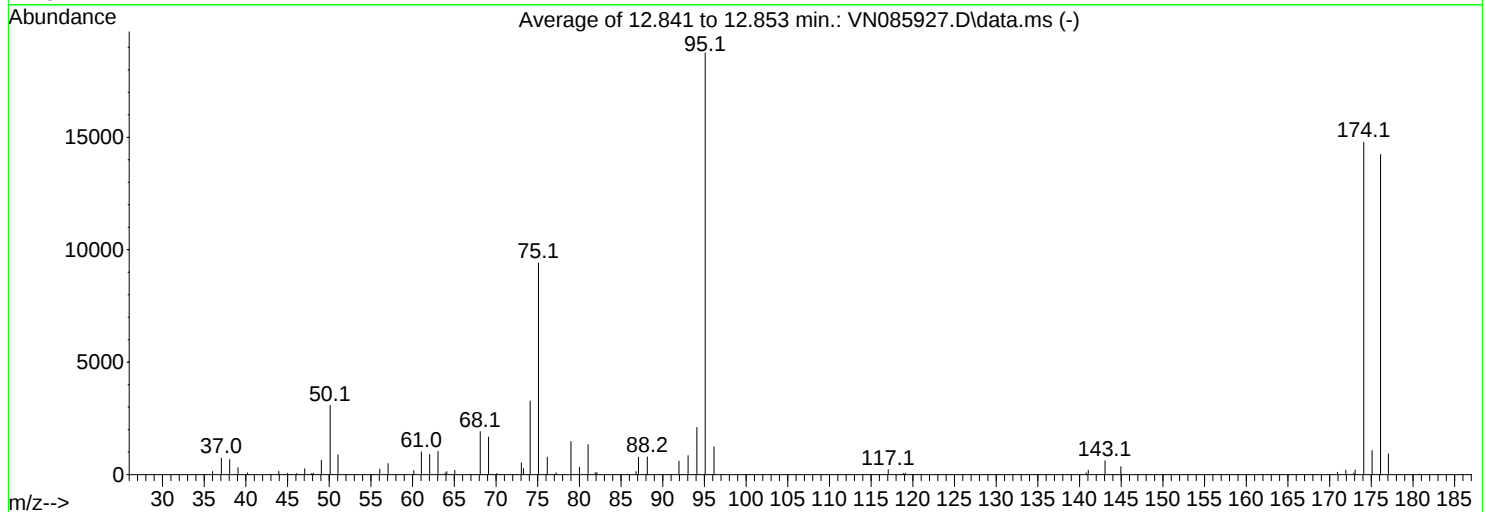


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031125\
Data File : VN085927.D
Acq On : 11 Mar 2025 12:12
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Title : SW846 8260
Last Update : Wed Feb 19 03:43:32 2025

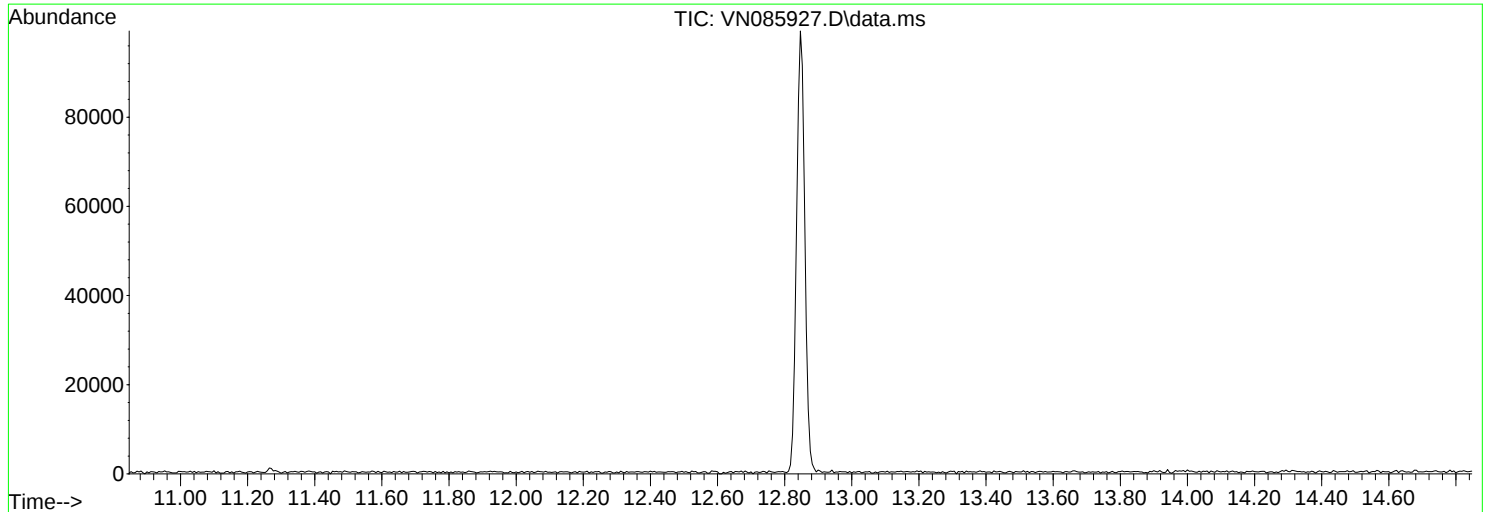

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	3078	PASS
75	95	30	60	50.2	9414	PASS
95	95	100	100	100.0	18755	PASS
96	95	5	9	6.6	1247	PASS
173	174	0.00	2	1.4	214	PASS
174	95	50	100	78.8	14780	PASS
175	174	5	9	7.3	1076	PASS
176	174	95	101	96.3	14234	PASS
177	176	5	9	6.5	923	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	136	49.05	643	65.05	193	80.00	321
37.05	733	50.10	3078	68.10	1917	81.05	1338
38.05	671	51.05	888	69.10	1669	81.90	81
39.05	309	56.05	249	70.10	57	82.10	91
40.20	75	57.05	488	73.05	525	86.80	136
43.95	149	60.15	182	73.30	268	87.10	777
45.00	66	61.05	1010	74.10	3275	88.15	787
46.10	53	62.05	899	75.10	9414	91.95	607
47.05	266	63.05	1037	76.15	779	93.05	850
47.90	50	63.90	76	77.20	79	94.10	2096
48.10	62	64.10	138	79.00	1472	95.10	18755

Average of 12.841 to 12.853 min.: VN085927.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
96.15	1247	173.05	214				
117.05	223	174.10	14780				
118.90	57	175.10	1076				
119.10	64	176.10	14234				
140.80	78	177.05	923				
141.05	199						
143.05	616						
144.95	358						
170.95	108						
171.95	200						
172.90	72						

Instrument :

MSVOA_N

ClientSampleId :

BFB