



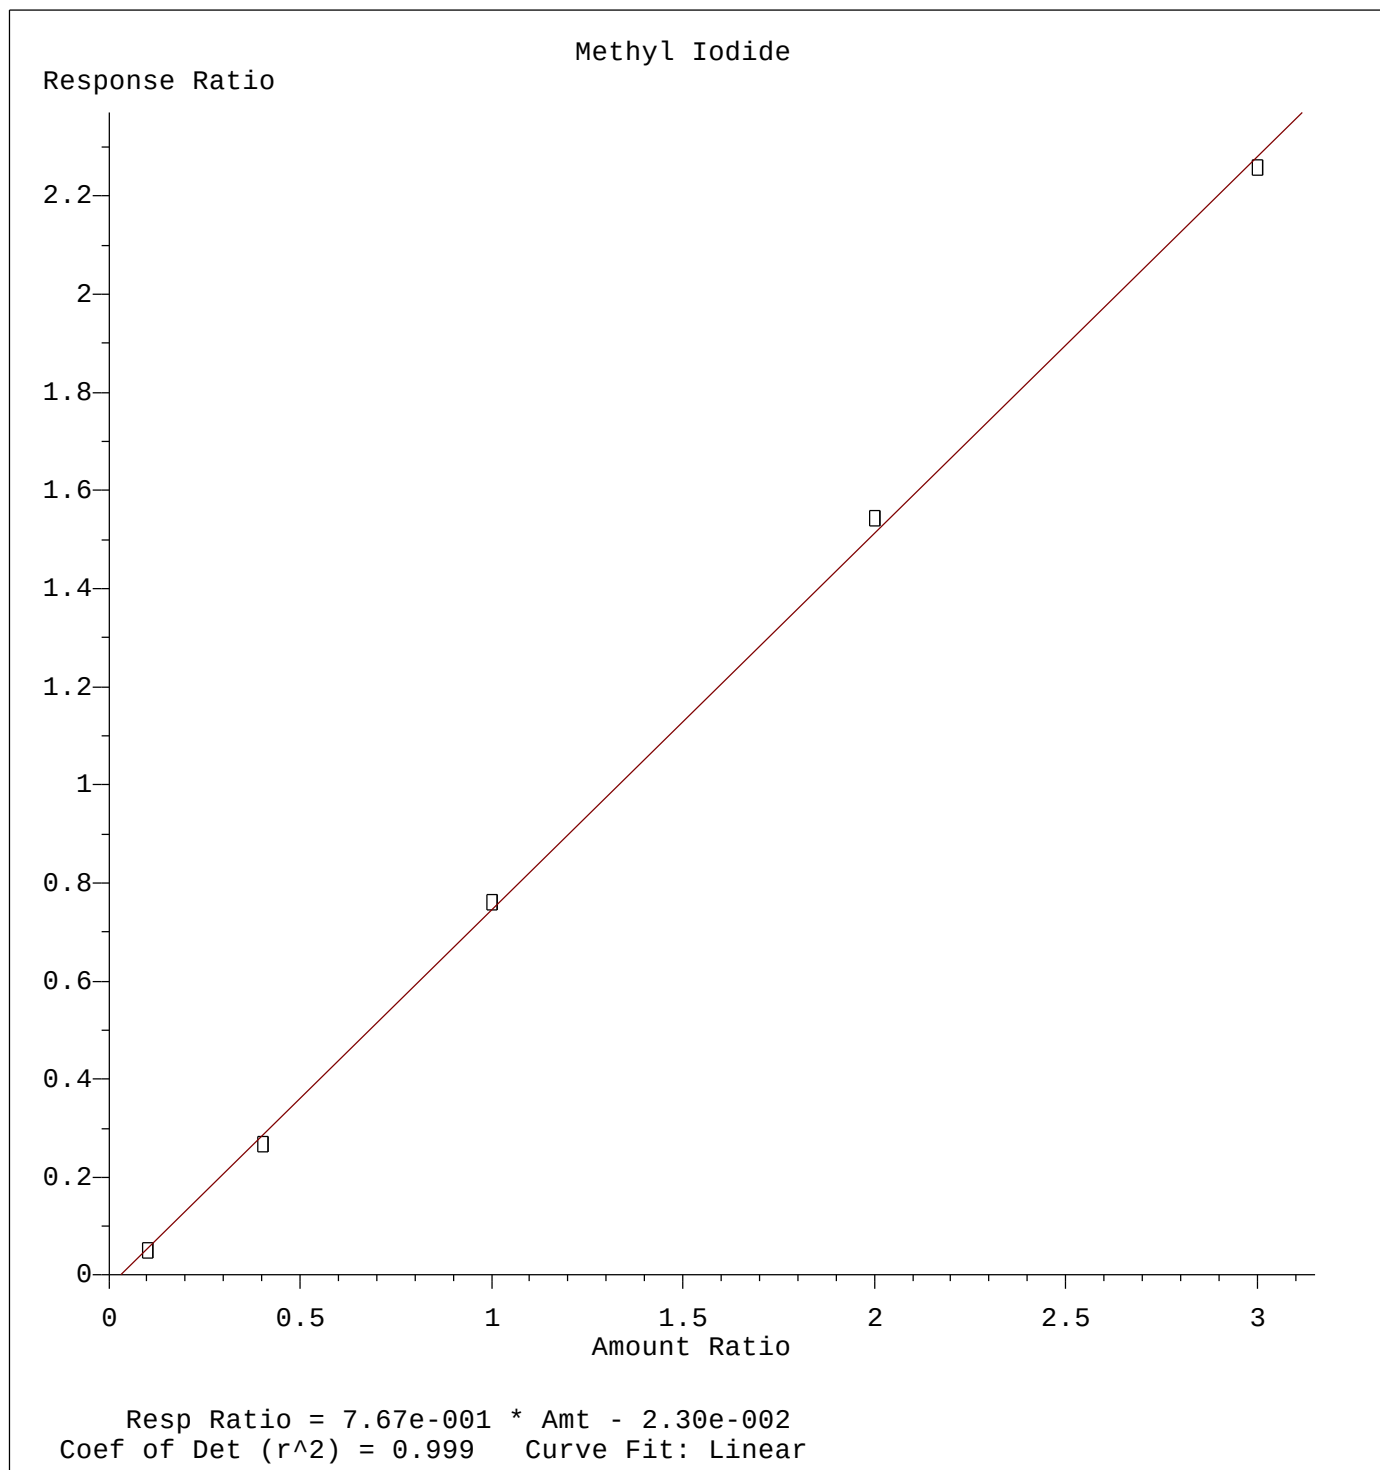

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
Calibration Table Last Updated: Wed Mar 13 03:33:31 2019

Naphthalene

Response Ratio

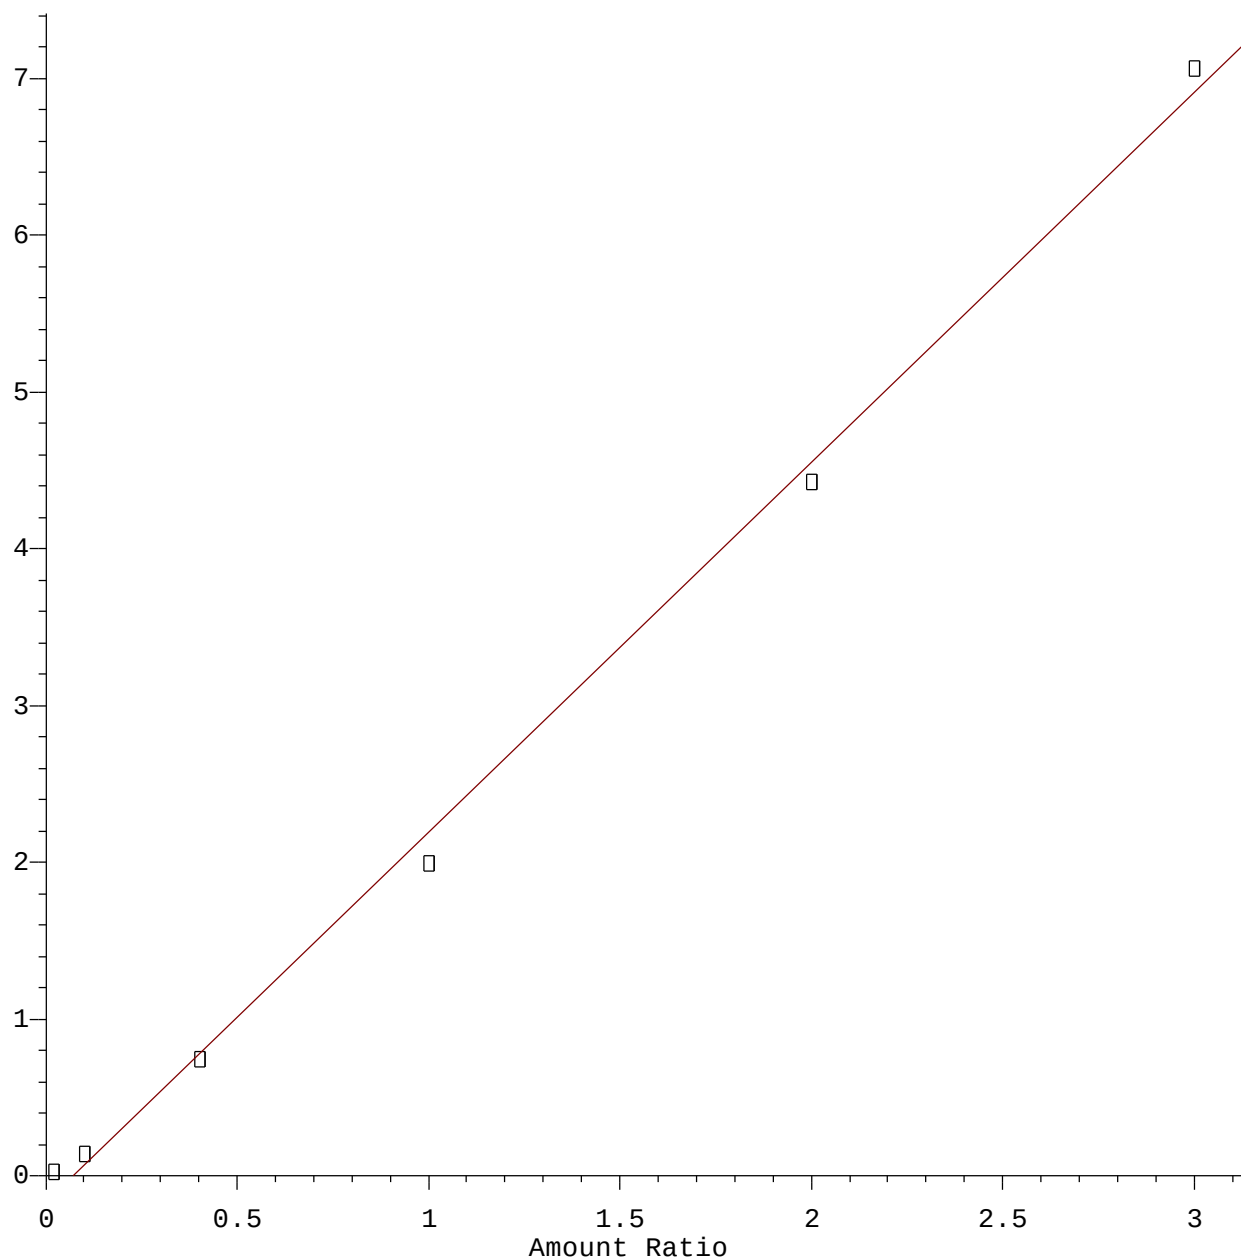


Resp Ratio = 2.36×10^0 * Amt - 1.64×10^{-1}
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
Calibration Table Last Updated: Wed Mar 13 03:33:31 2019


1,2,4-Trichlorobenzene

Response Ratio

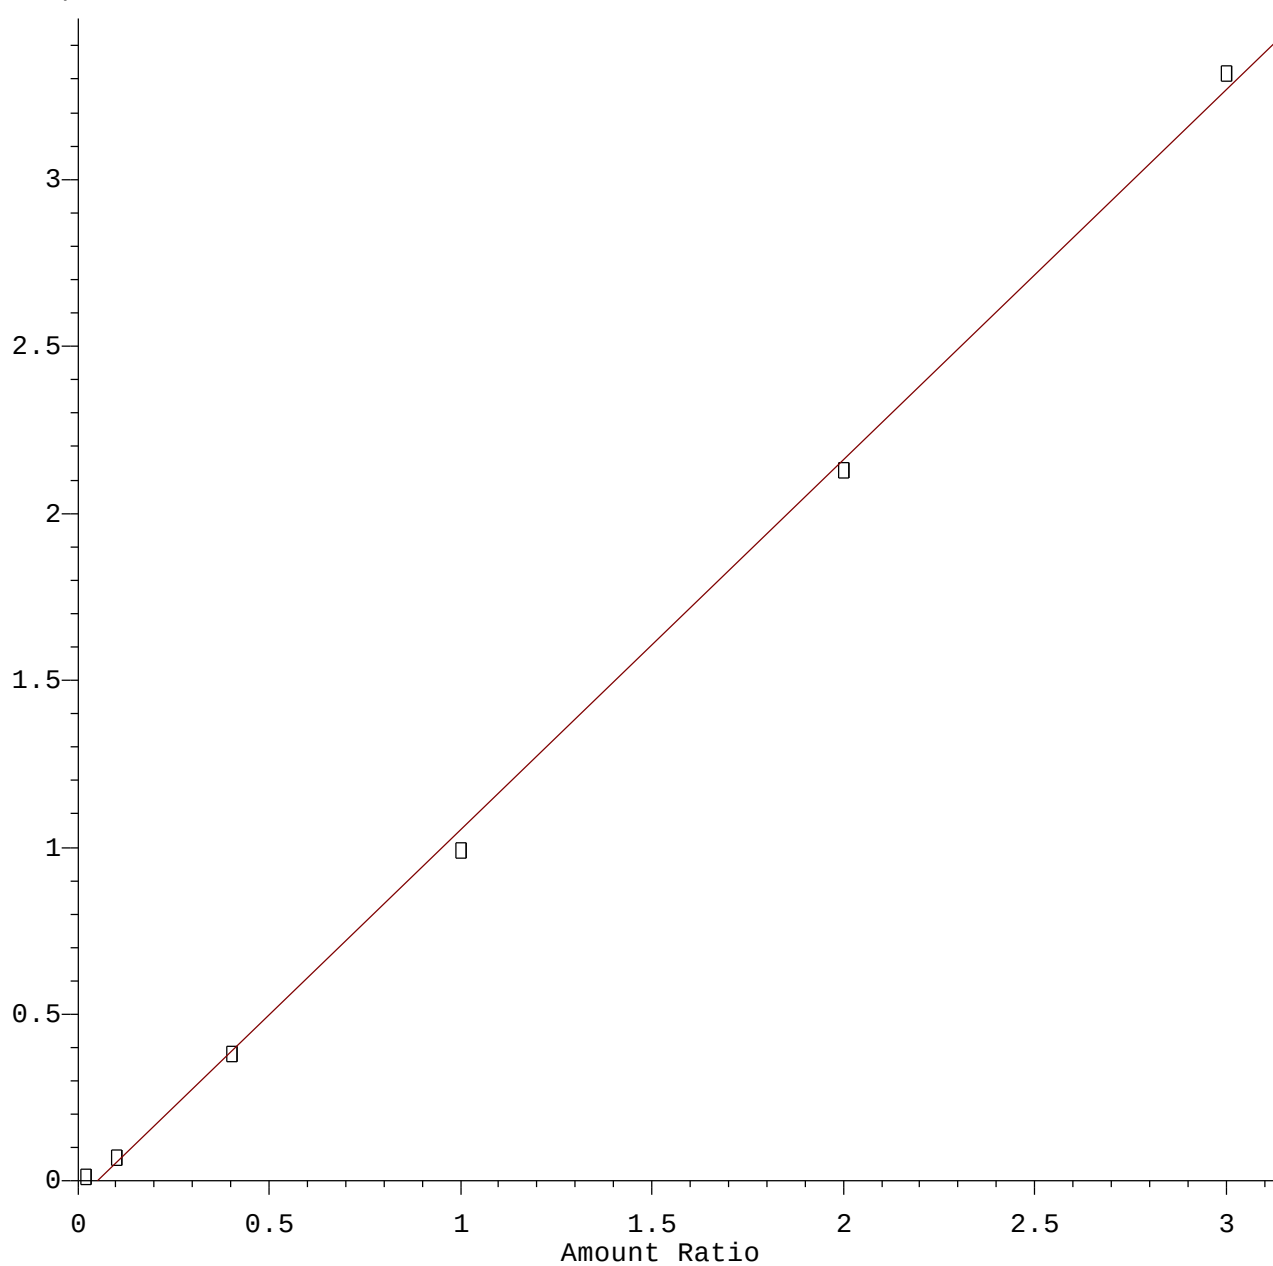

Resp Ratio = 1.11e+000 * Amt - 5.58e-002
Coef of Det (r²) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
Calibration Table Last Updated: Wed Mar 13 03:33:31 2019

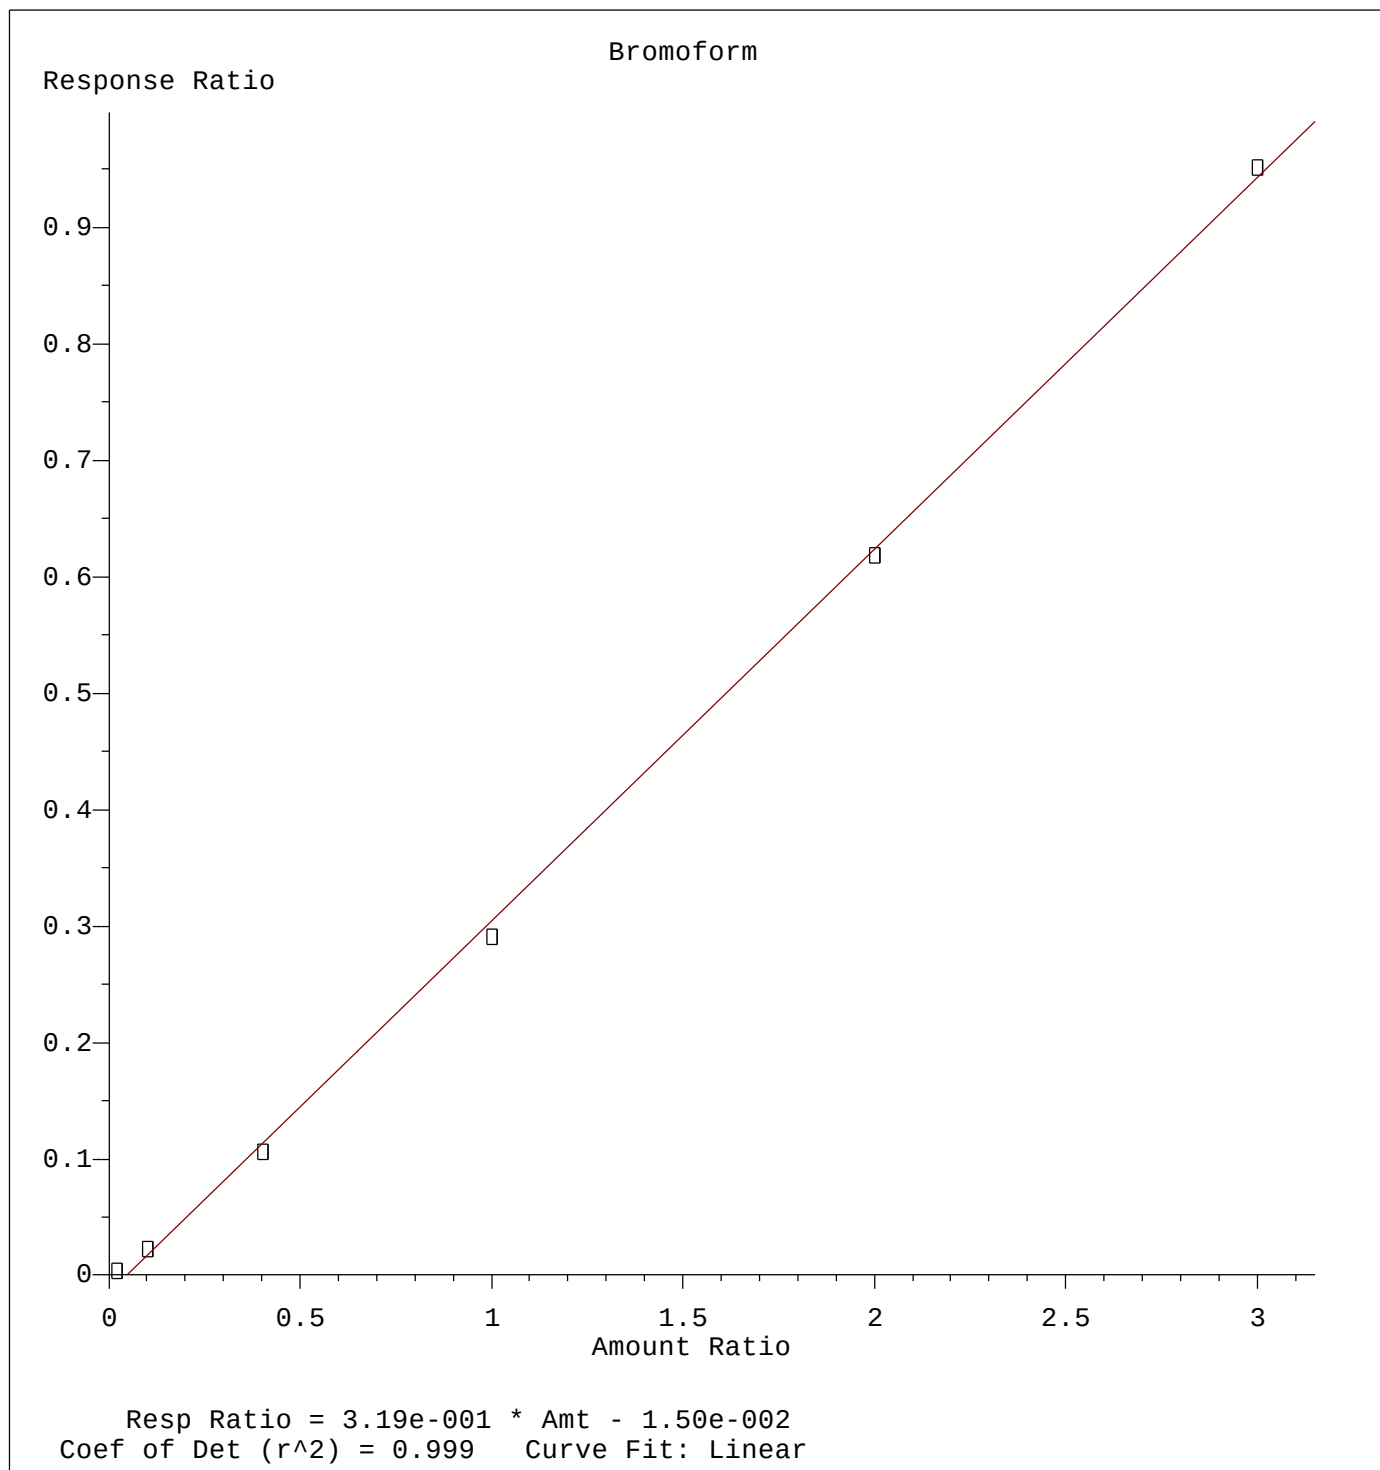

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
Calibration Table Last Updated: Wed Mar 13 03:33:31 2019

2-Chloroethyl Vinyl ether

Response Ratio

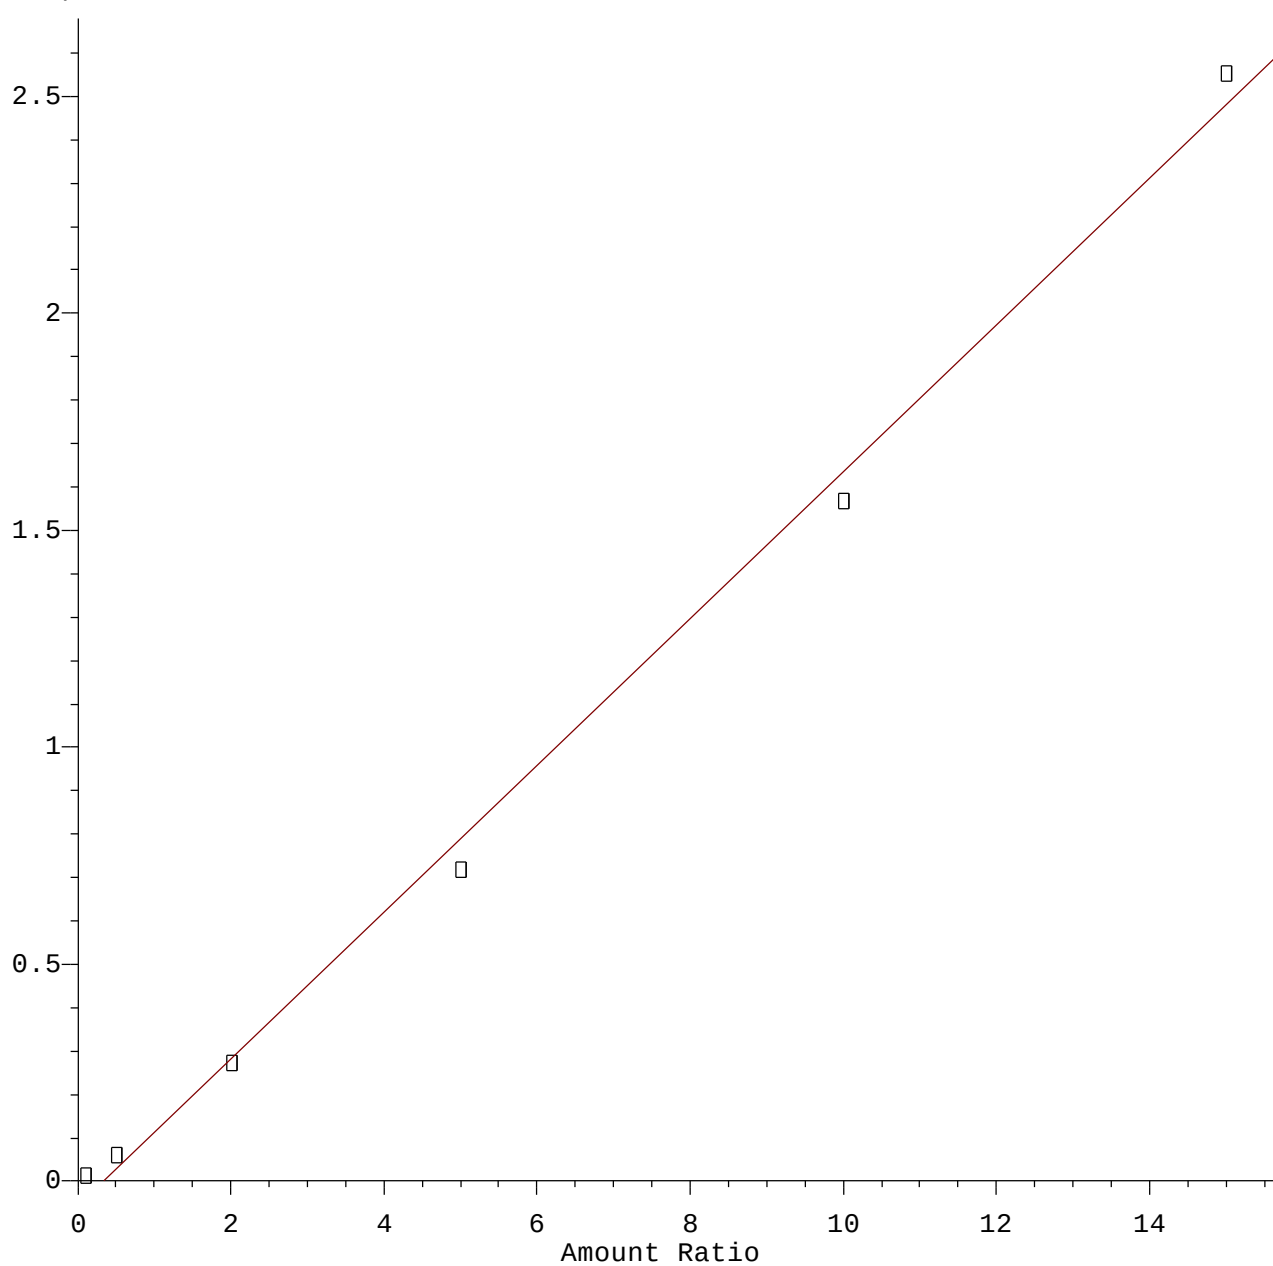


Resp Ratio = $1.69 \times 10^{-1} \times \text{Amt} - 5.69 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
Calibration Table Last Updated: Wed Mar 13 03:33:31 2019


t-1,3-Dichloropropene

Response Ratio

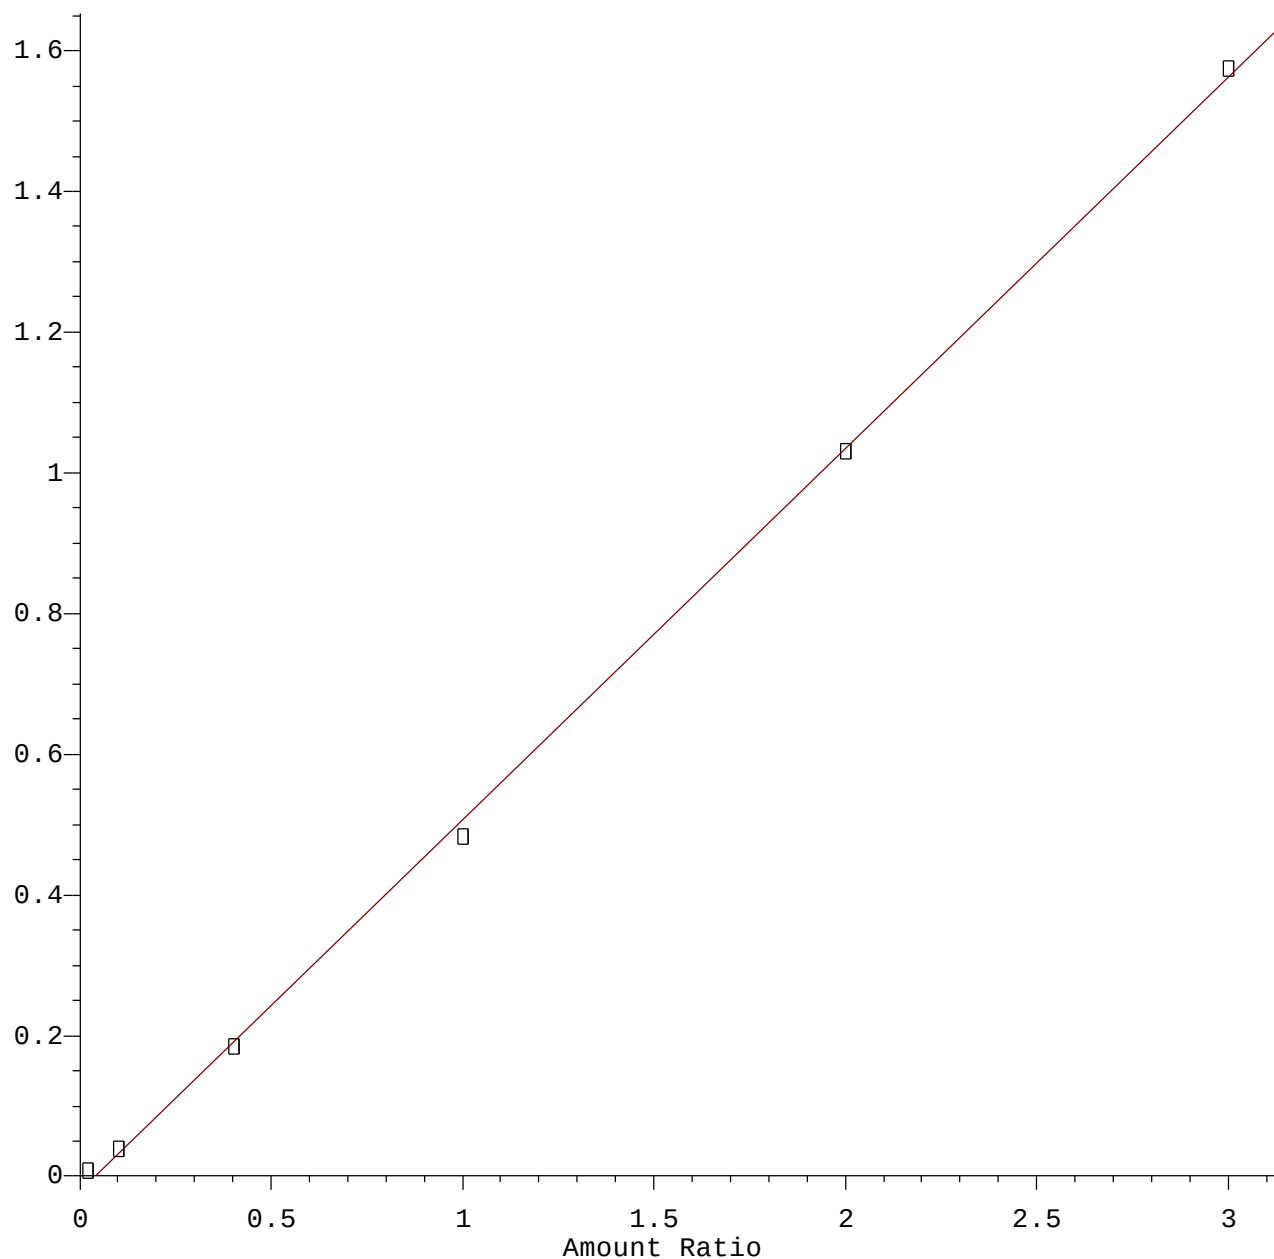

Resp Ratio = $5.28 \times 10^{-1} \times \text{Amt} - 2.10 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
Calibration Table Last Updated: Wed Mar 13 03:33:31 2019

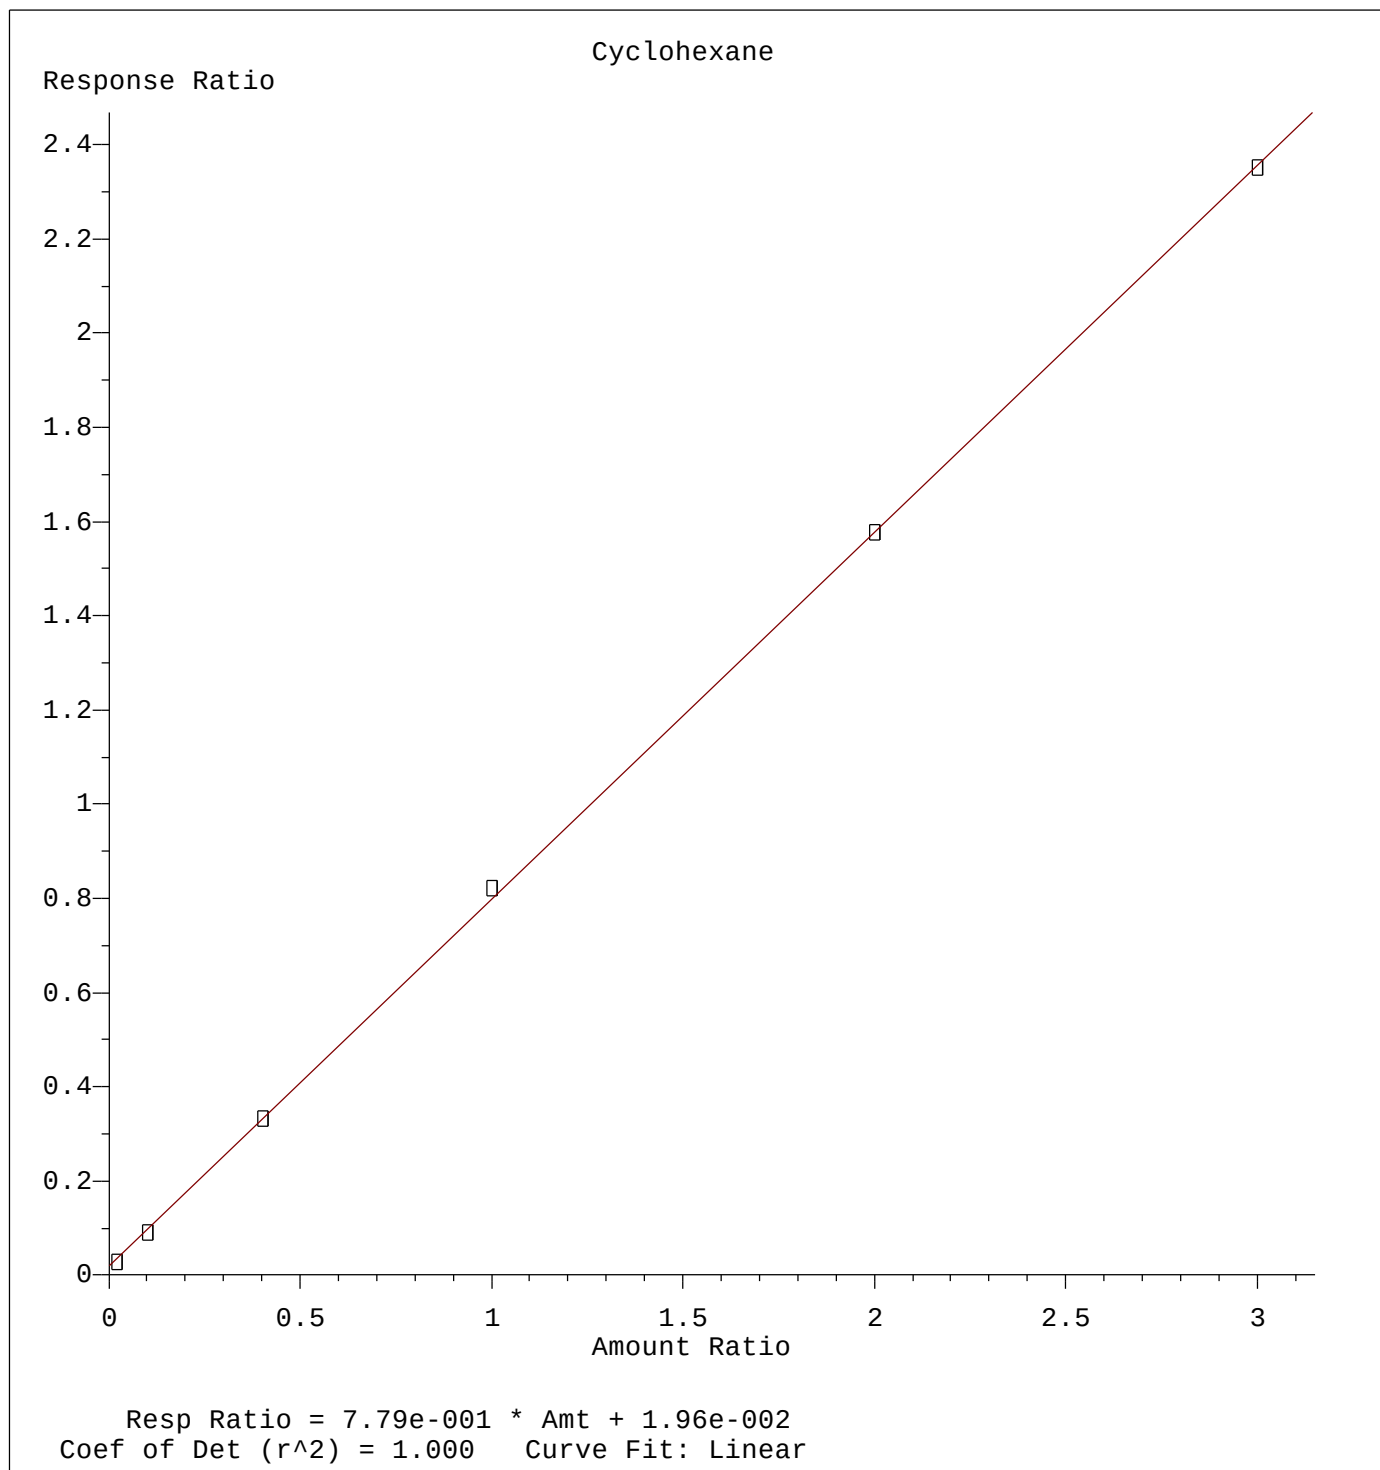

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
Calibration Table Last Updated: Wed Mar 13 03:33:31 2019