


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN031219\
Data File : VN054156.D
Acq On : 12 Mar 2019 8:43
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
Title : SW846 8260
Last Update : Wed Mar 13 03:33:31 2019

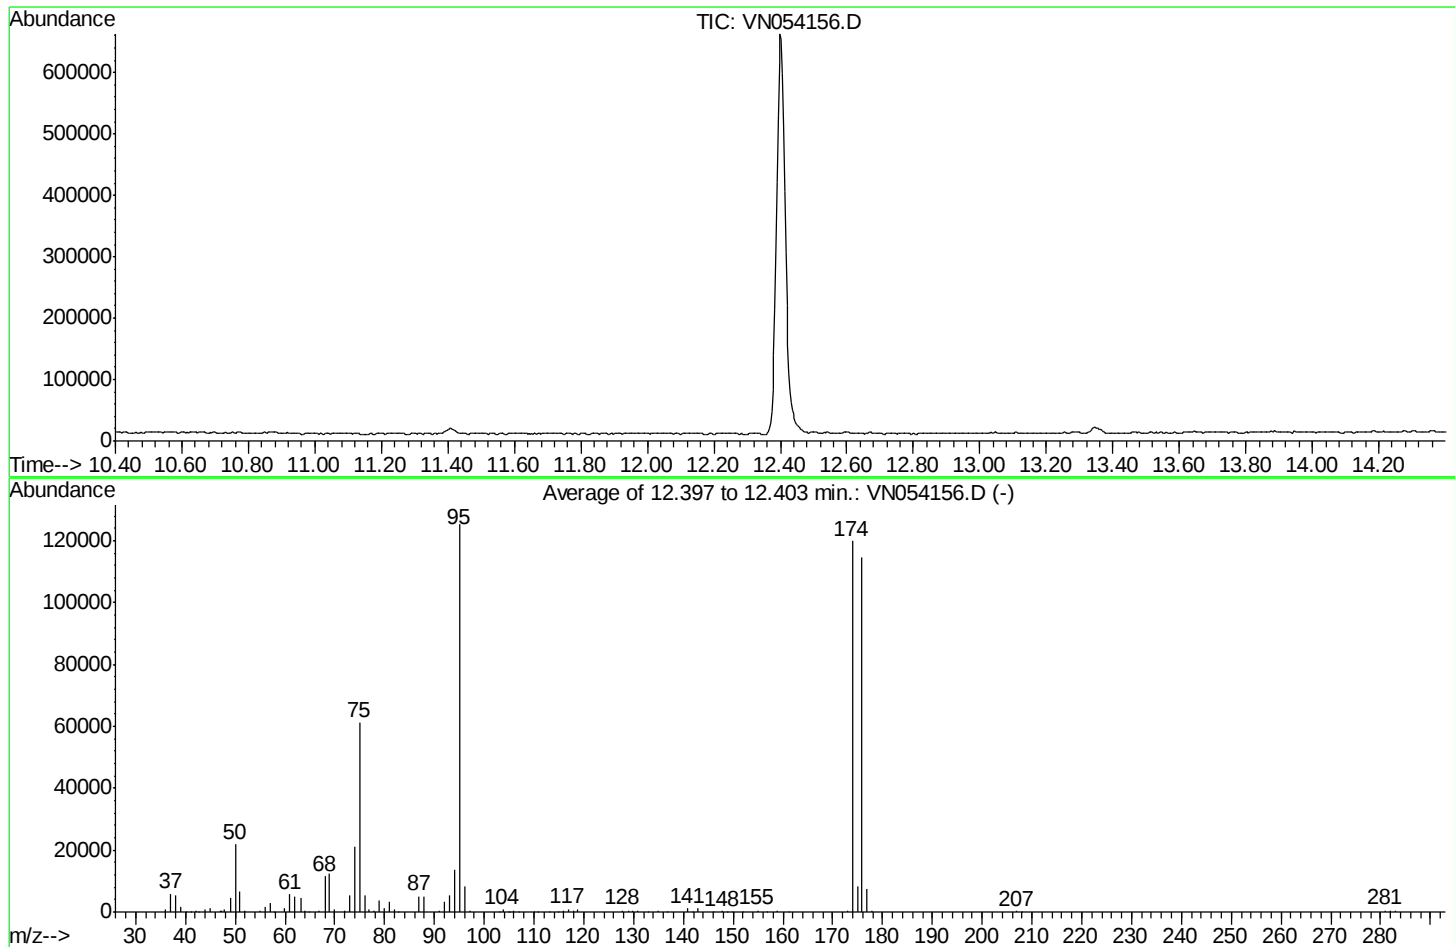

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	21864	PASS
75	95	30	60	48.7	61096	PASS
95	95	100	100	100.0	125346	PASS
96	95	5	9	6.7	8361	PASS
173	174	0.00	2	0.5	610	PASS
174	95	50	100	95.6	119834	PASS
175	174	5	9	6.9	8279	PASS
176	174	95	101	95.7	114680	PASS
177	176	5	9	6.5	7459	PASS