


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN031219\
Data File : VN054176.D
Acq On : 12 Mar 2019 21:19
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
Title : SW846 8260
Last Update : Wed Mar 13 03:33:31 2019

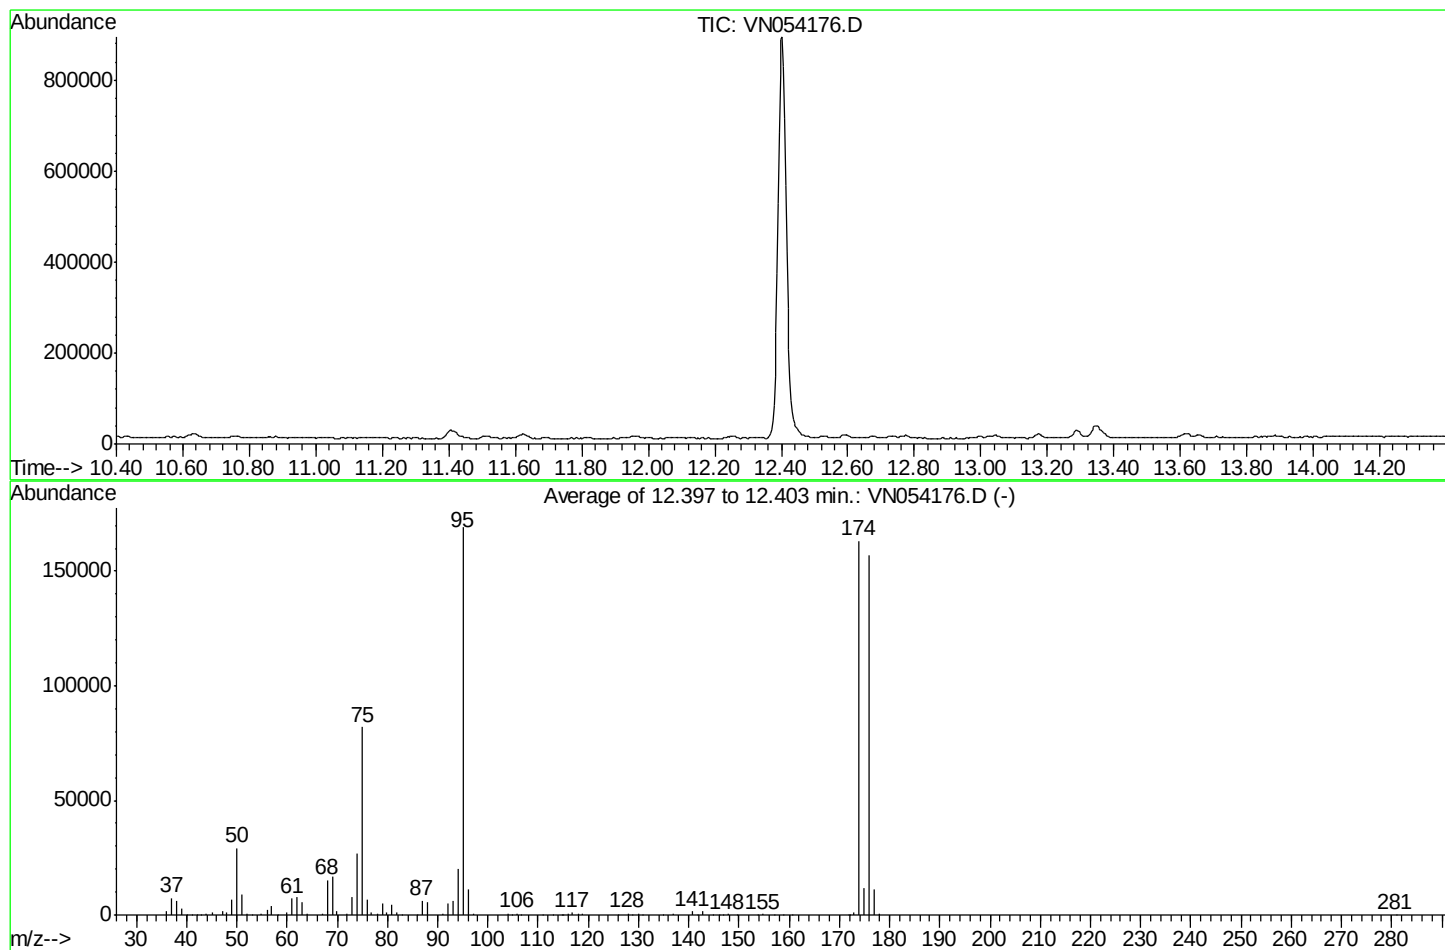

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3289

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	29200	PASS
75	95	30	60	48.5	82072	PASS
95	95	100	100	100.0	169152	PASS
96	95	5	9	6.5	11040	PASS
173	174	0.00	2	0.8	1252	PASS
174	95	50	100	96.5	163178	PASS
175	174	5	9	7.3	11986	PASS
176	174	95	101	96.4	157226	PASS
177	176	5	9	7.0	11006	PASS