


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN031220\
 Data File : VN060463.D
 Acq On : 12 Mar 2020 8:26
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
 Title : SW846 8260
 Last Update : Thu Feb 27 13:52:50 2020

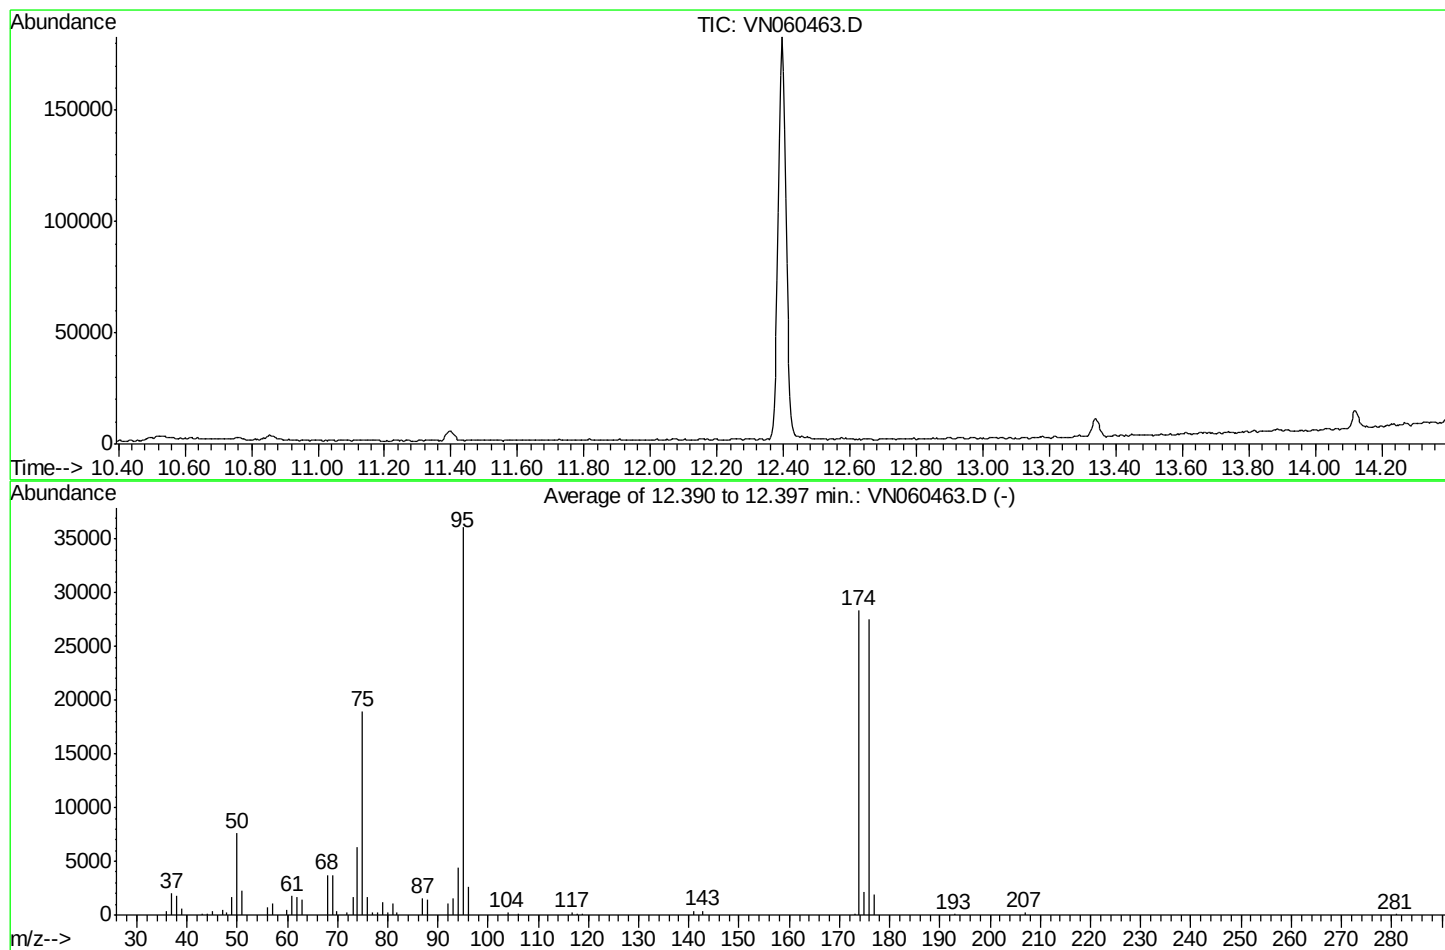

AutoFind: Scans 3302, 3303, 3304; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	7584	PASS
75	95	30	60	52.4	18904	PASS
95	95	100	100	100.0	36093	PASS
96	95	5	9	7.4	2672	PASS
173	174	0.00	2	0.4	123	PASS
174	95	50	100	78.5	28344	PASS
175	174	5	9	7.6	2143	PASS
176	174	95	101	97.1	27512	PASS
177	176	5	9	6.8	1882	PASS