


Chloromethane

Response Ratio

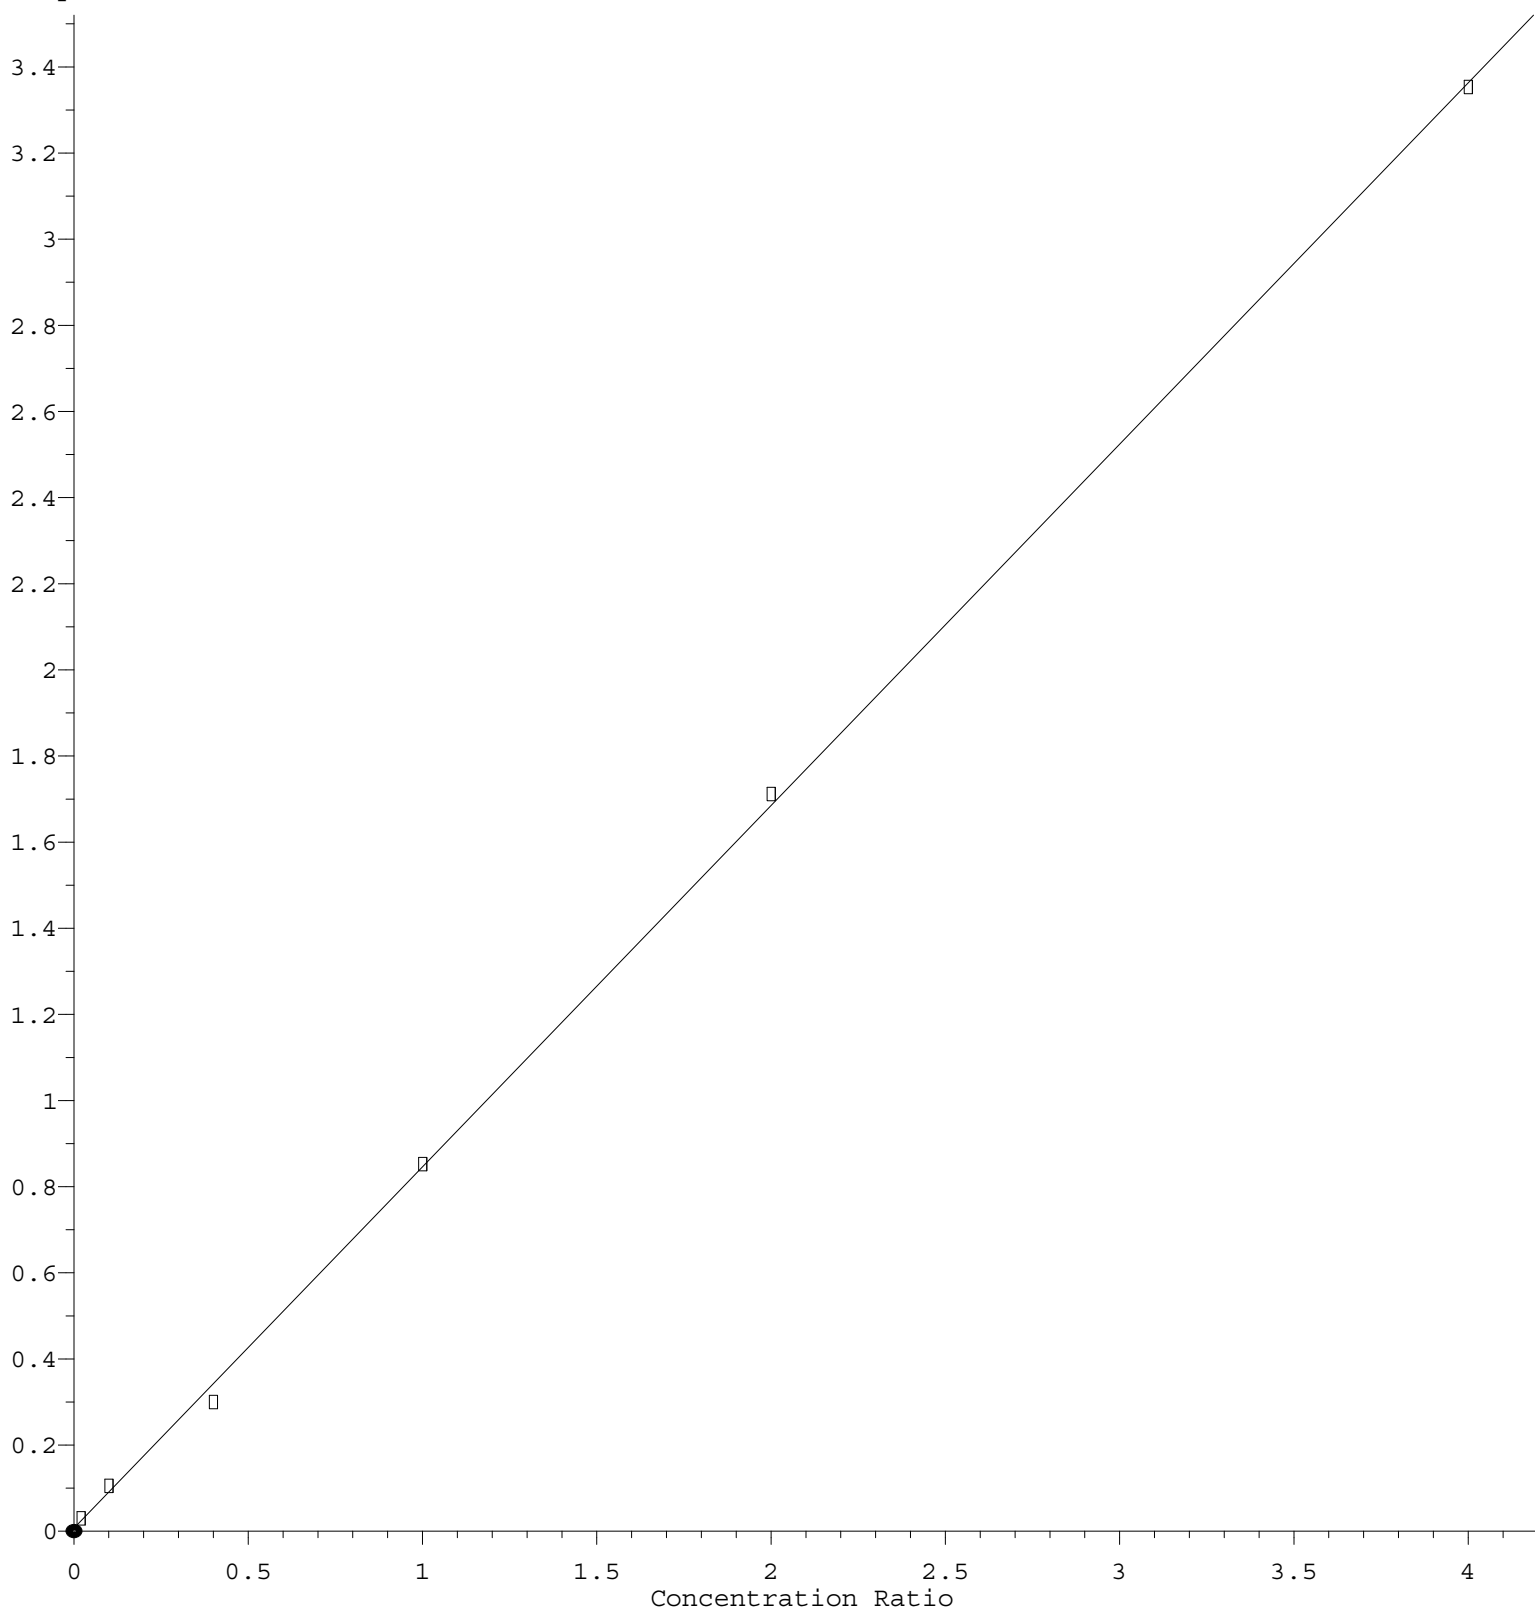

$$\text{Response} = 8.394\text{e-}001 * \text{Amt} + 6.542\text{e-}003$$


Coef of Det (r^2) = 0.999648 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031221W.M

Calibration Table Last Updated: Fri Mar 12 13:00:23 2021

Acrolein


Response Ratio

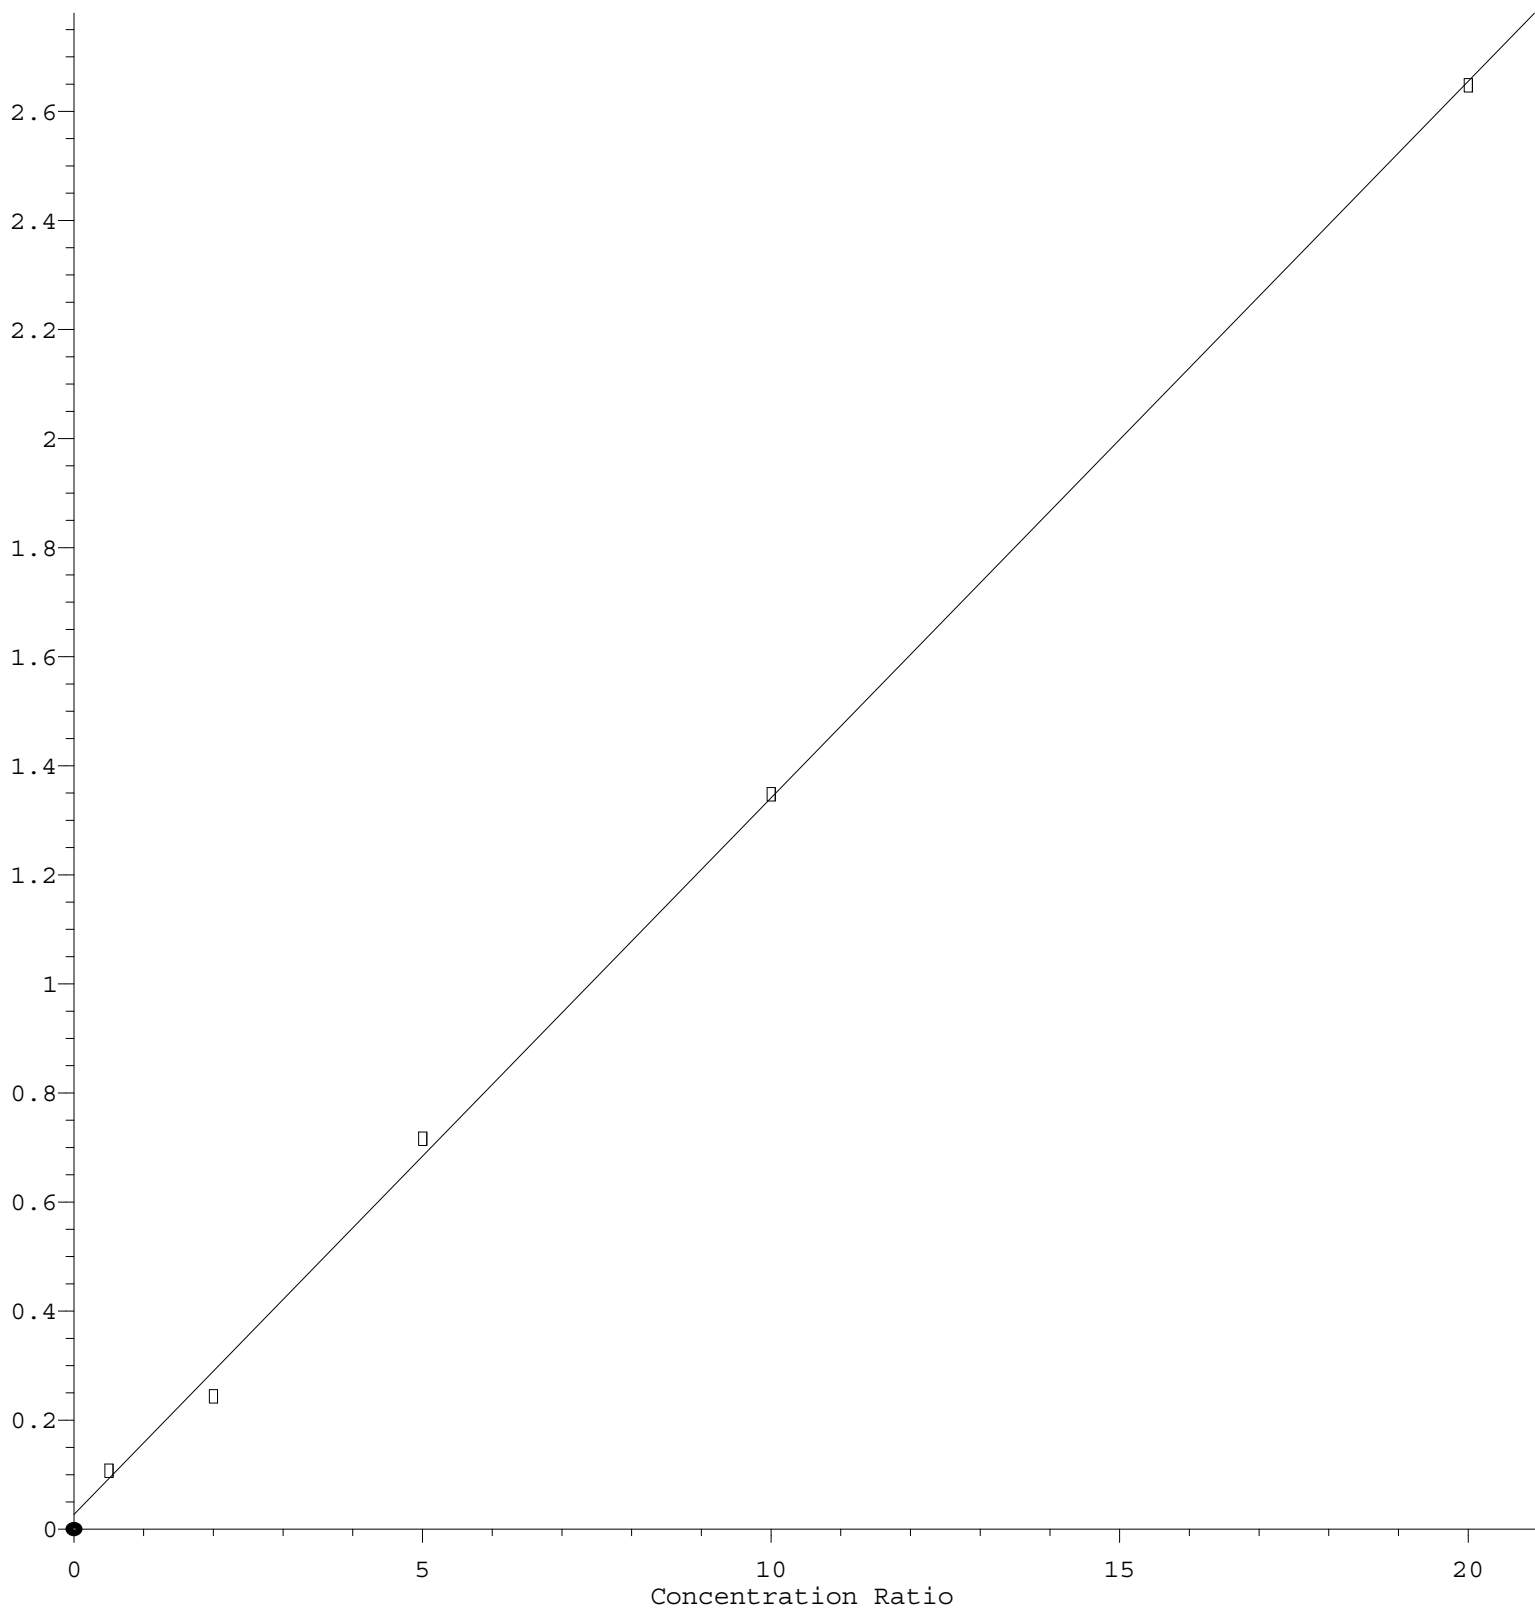

Response = 1.314e-001 * Amt + 2.691e-002
 Coef of Det (r^2) = 0.999190 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031221W.M
 Calibration Table Last Updated: Fri Mar 12 13:00:23 2021

Acetone

Response Ratio

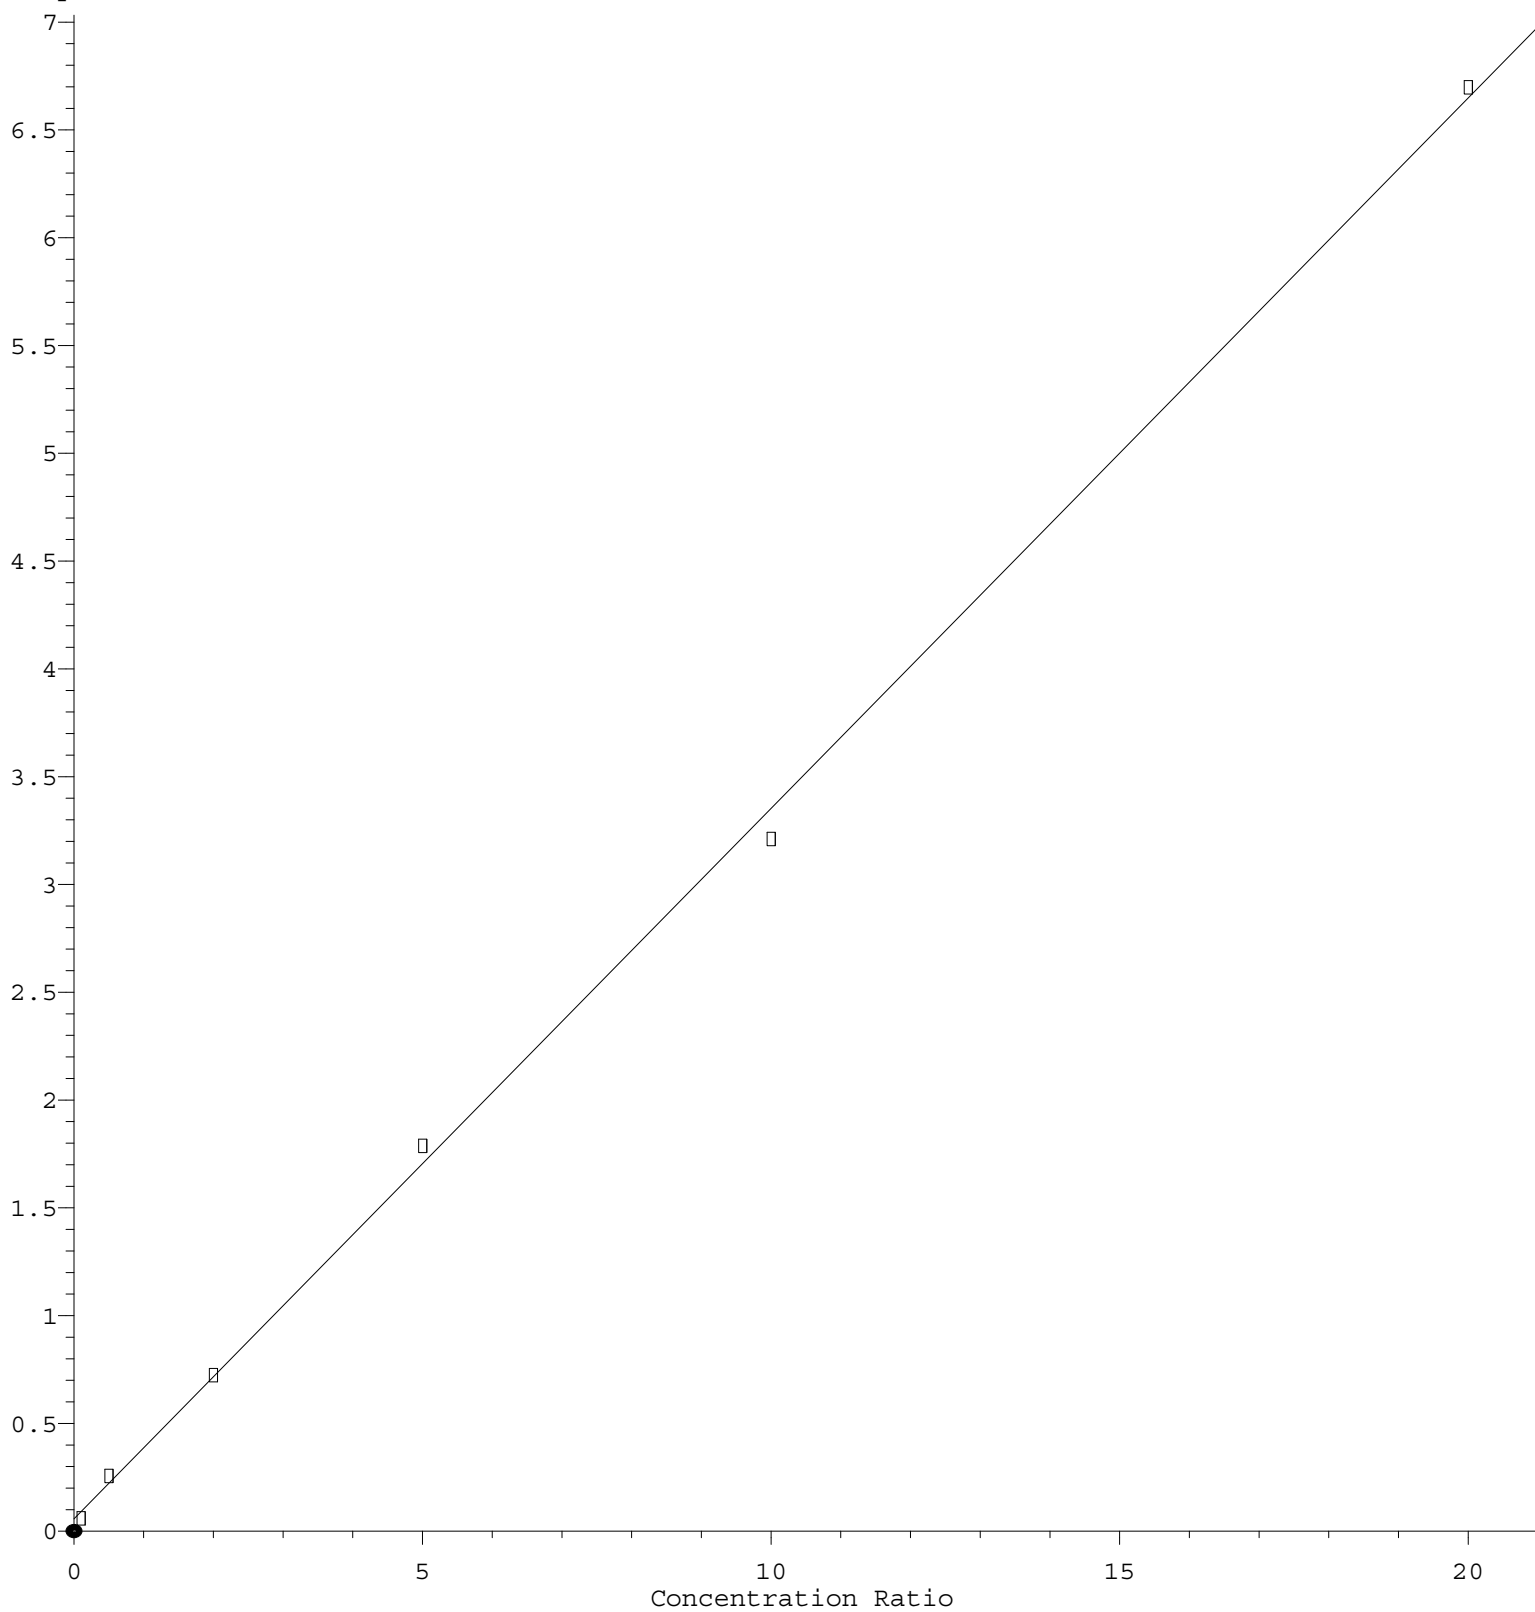

$$\text{Response} = 3.296\text{e-}001 * \text{Amt} + 5.713\text{e-}002$$


Coef of Det (r^2) = 0.999014 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031221W.M

Calibration Table Last Updated: Fri Mar 12 13:00:23 2021

Ethyl methacrylate

Response Ratio

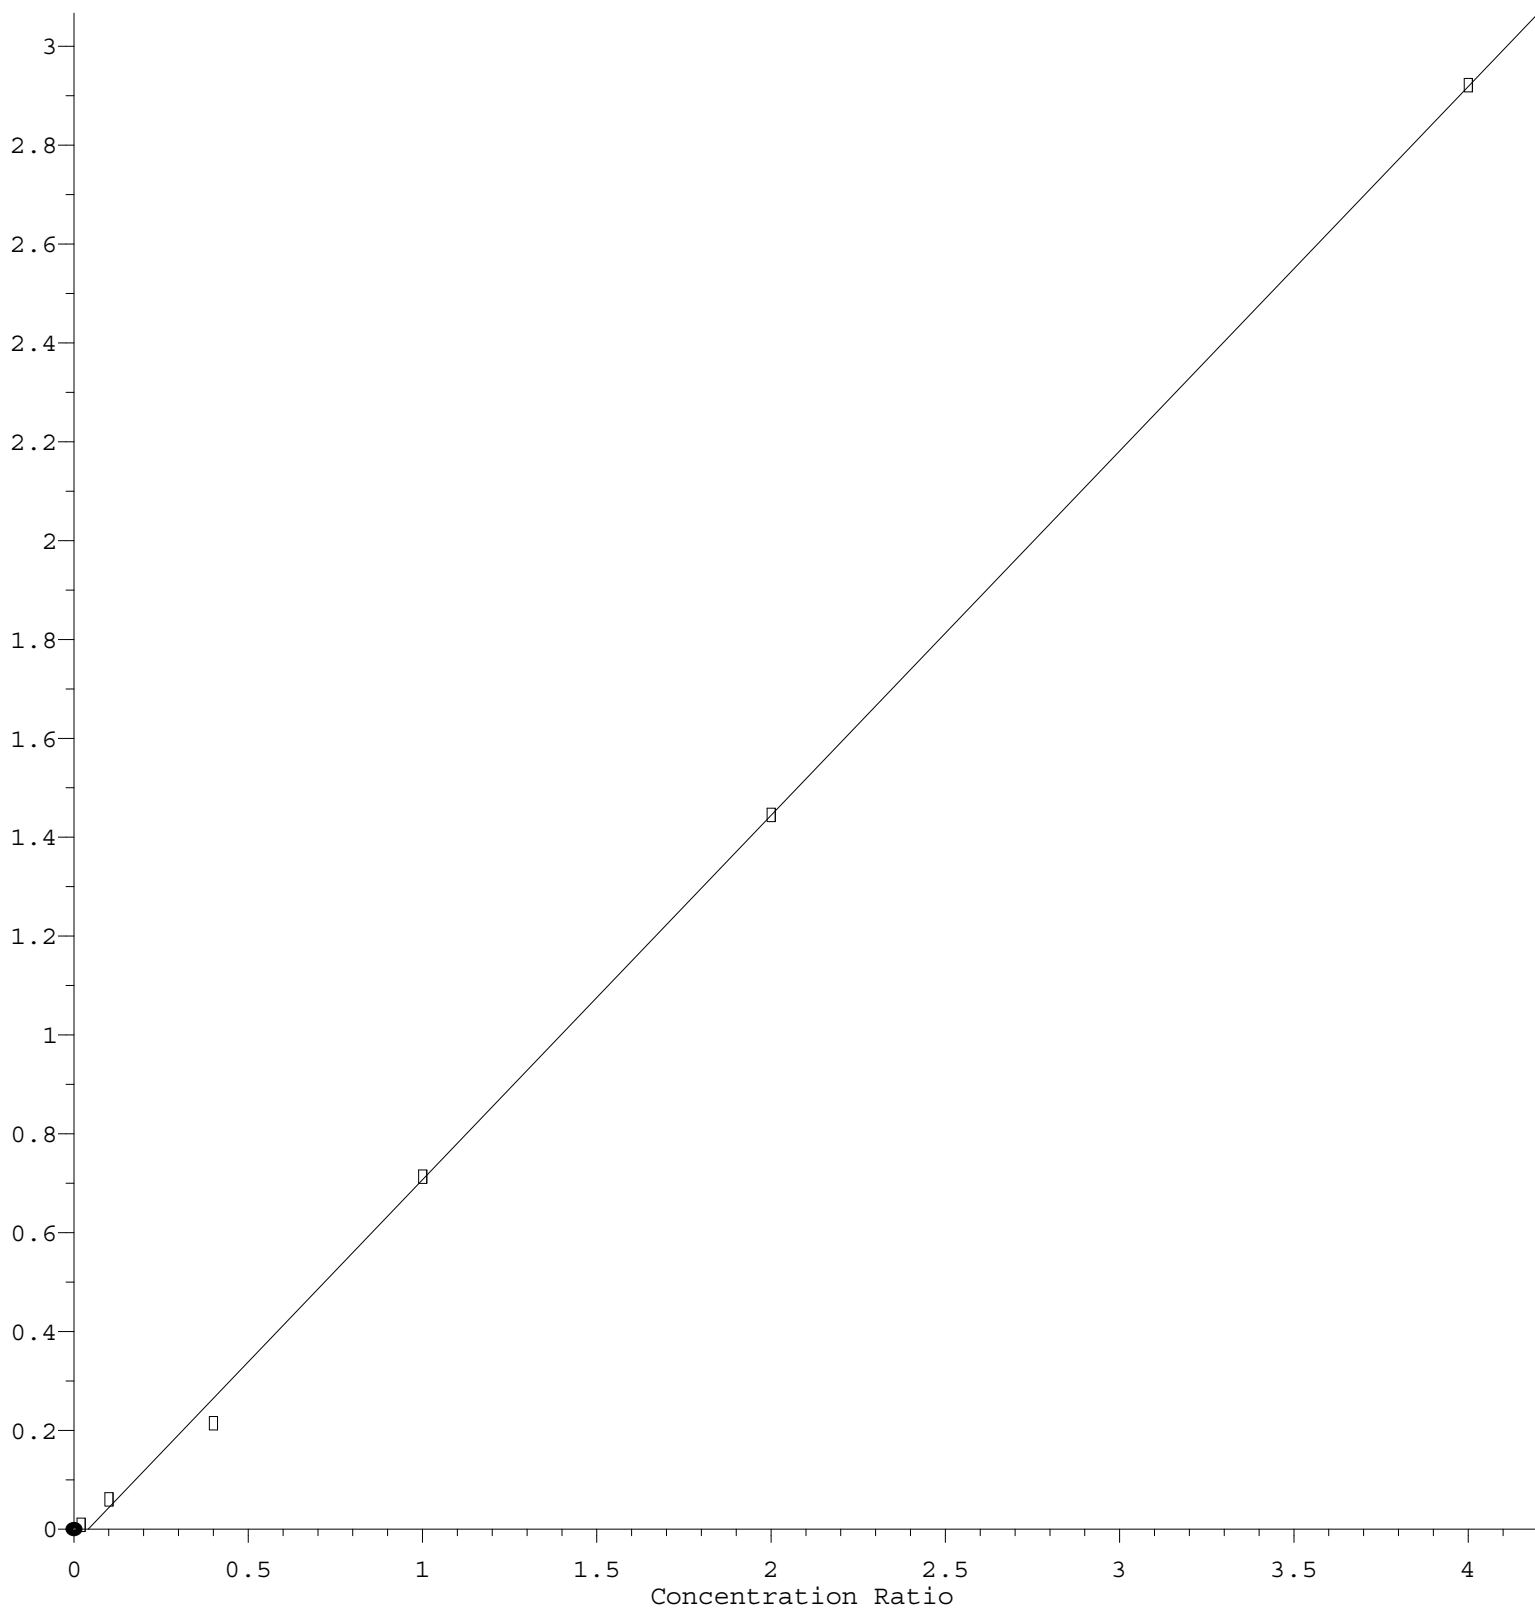

$$\text{Response} = 7.373\text{e-}001 * \text{Amt} - 3.030\text{e-}002$$


Coef of Det (r^2) = 0.999459 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031221W.M

Calibration Table Last Updated: Fri Mar 12 13:00:23 2021

2-Chloroethyl Vinyl ether

Response Ratio

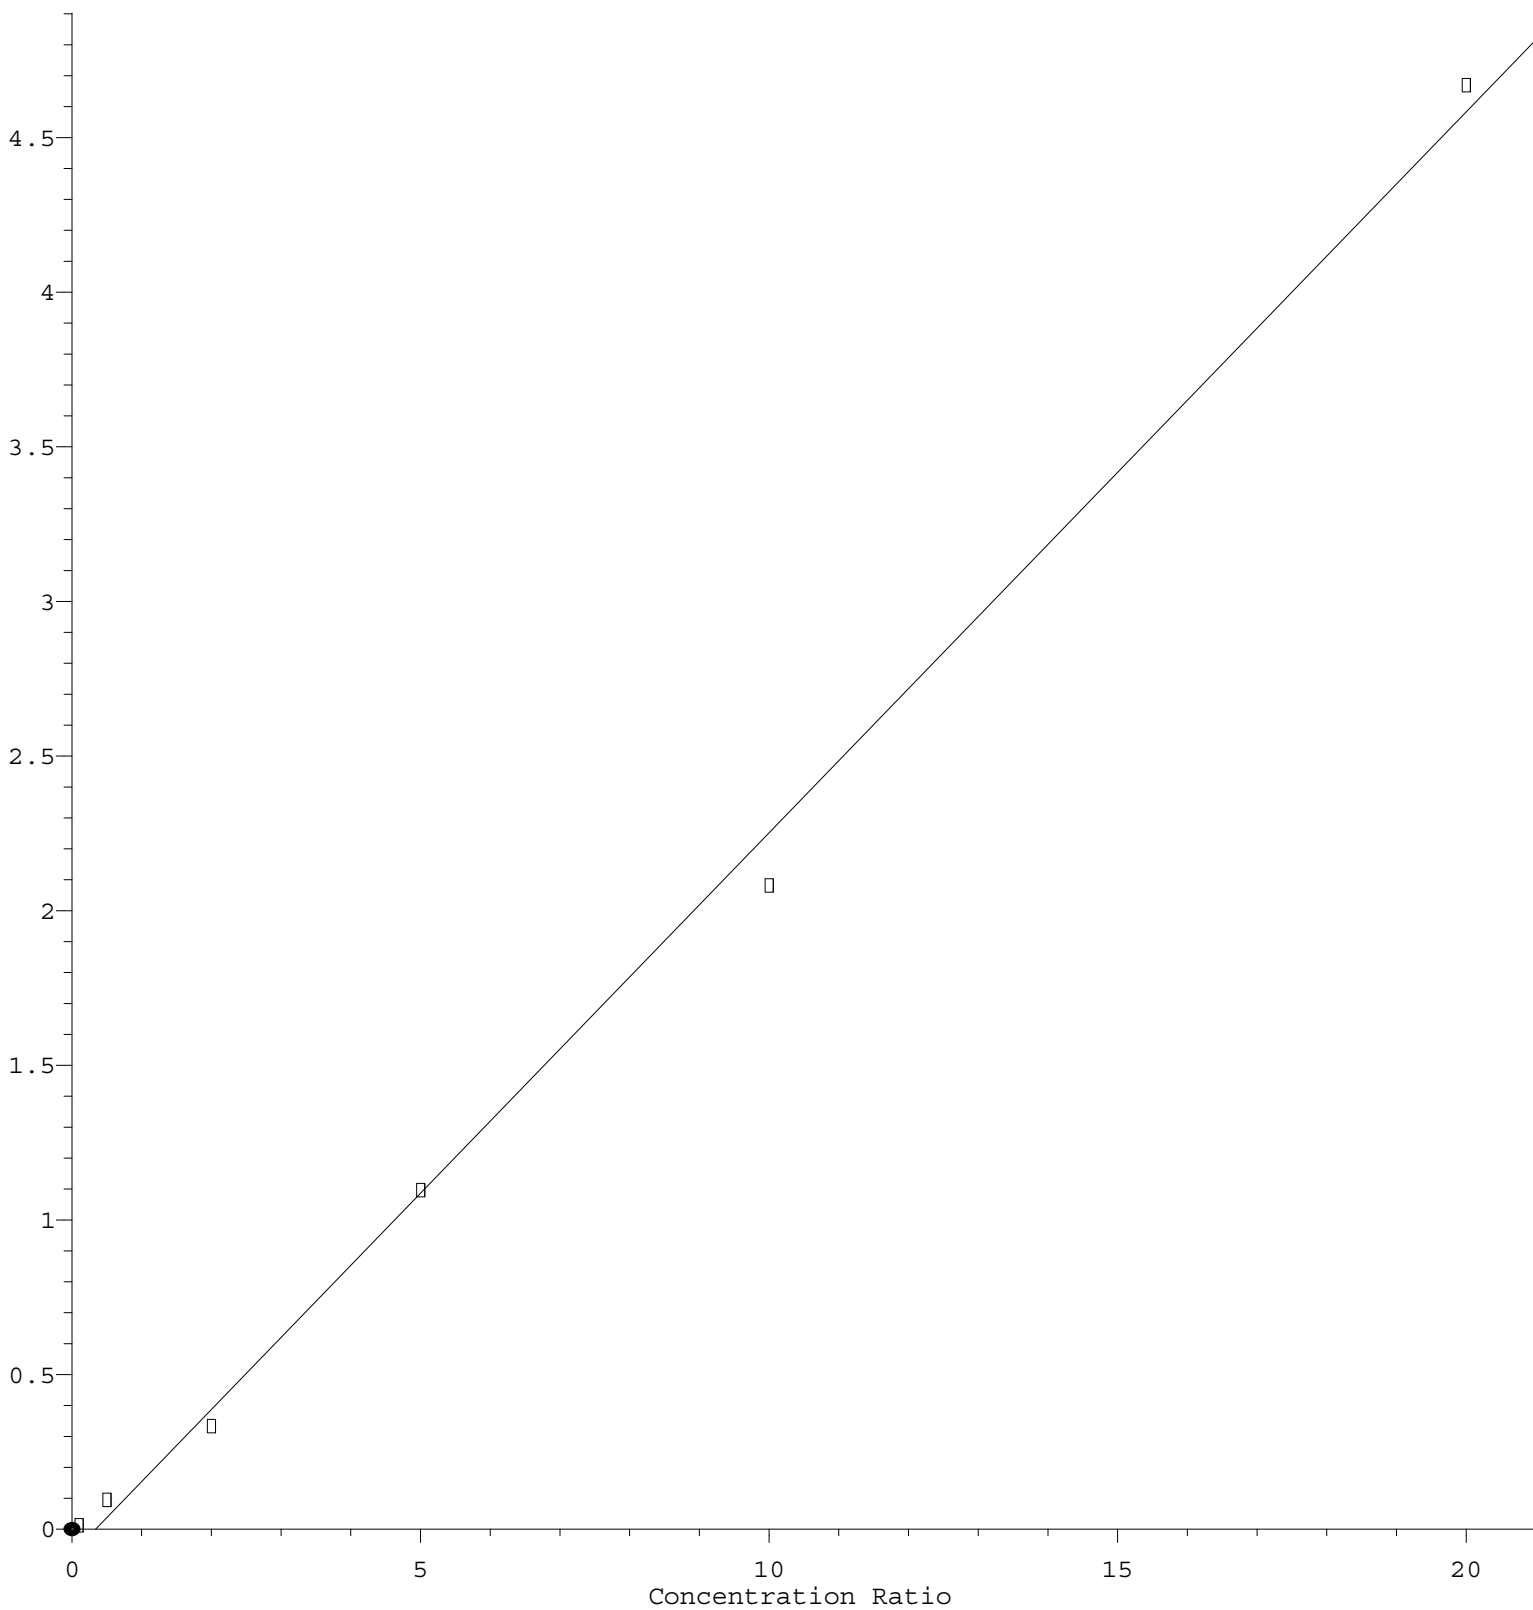

$$\text{Response} = 2.332\text{e-}001 * \text{Amt} - 7.992\text{e-}002$$


Coef of Det (r^2) = 0.997034 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031221W.M

Calibration Table Last Updated: Fri Mar 12 13:00:23 2021

2-Hexanone

Response Ratio

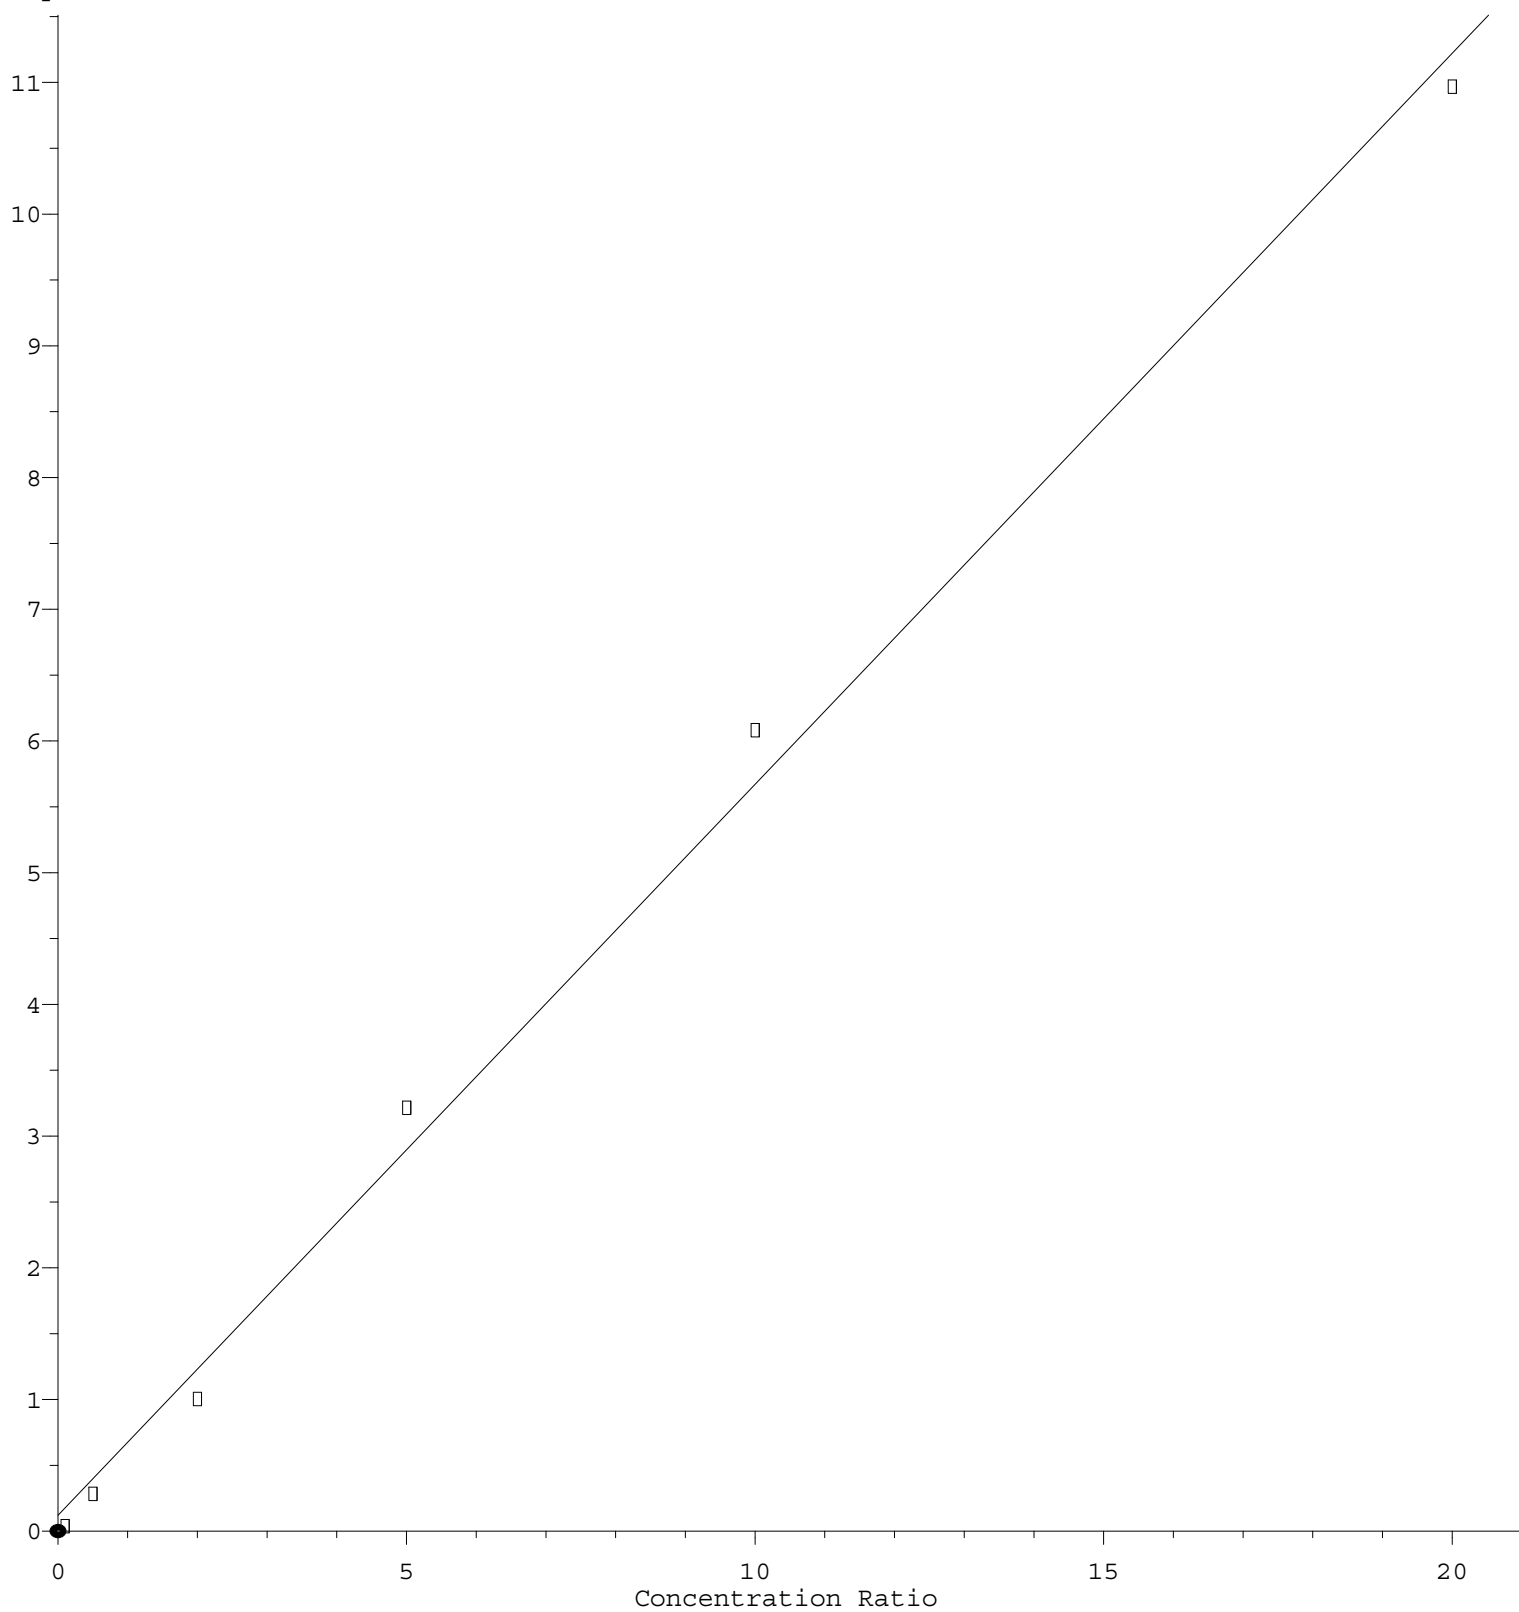

$$\text{Response} = 5.554\text{e-}001 * \text{Amt} + 1.169\text{e-}001$$


Coef of Det (r^2) = 0.995406 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031221W.M

Calibration Table Last Updated: Fri Mar 12 13:00:23 2021

Styrene

Response Ratio

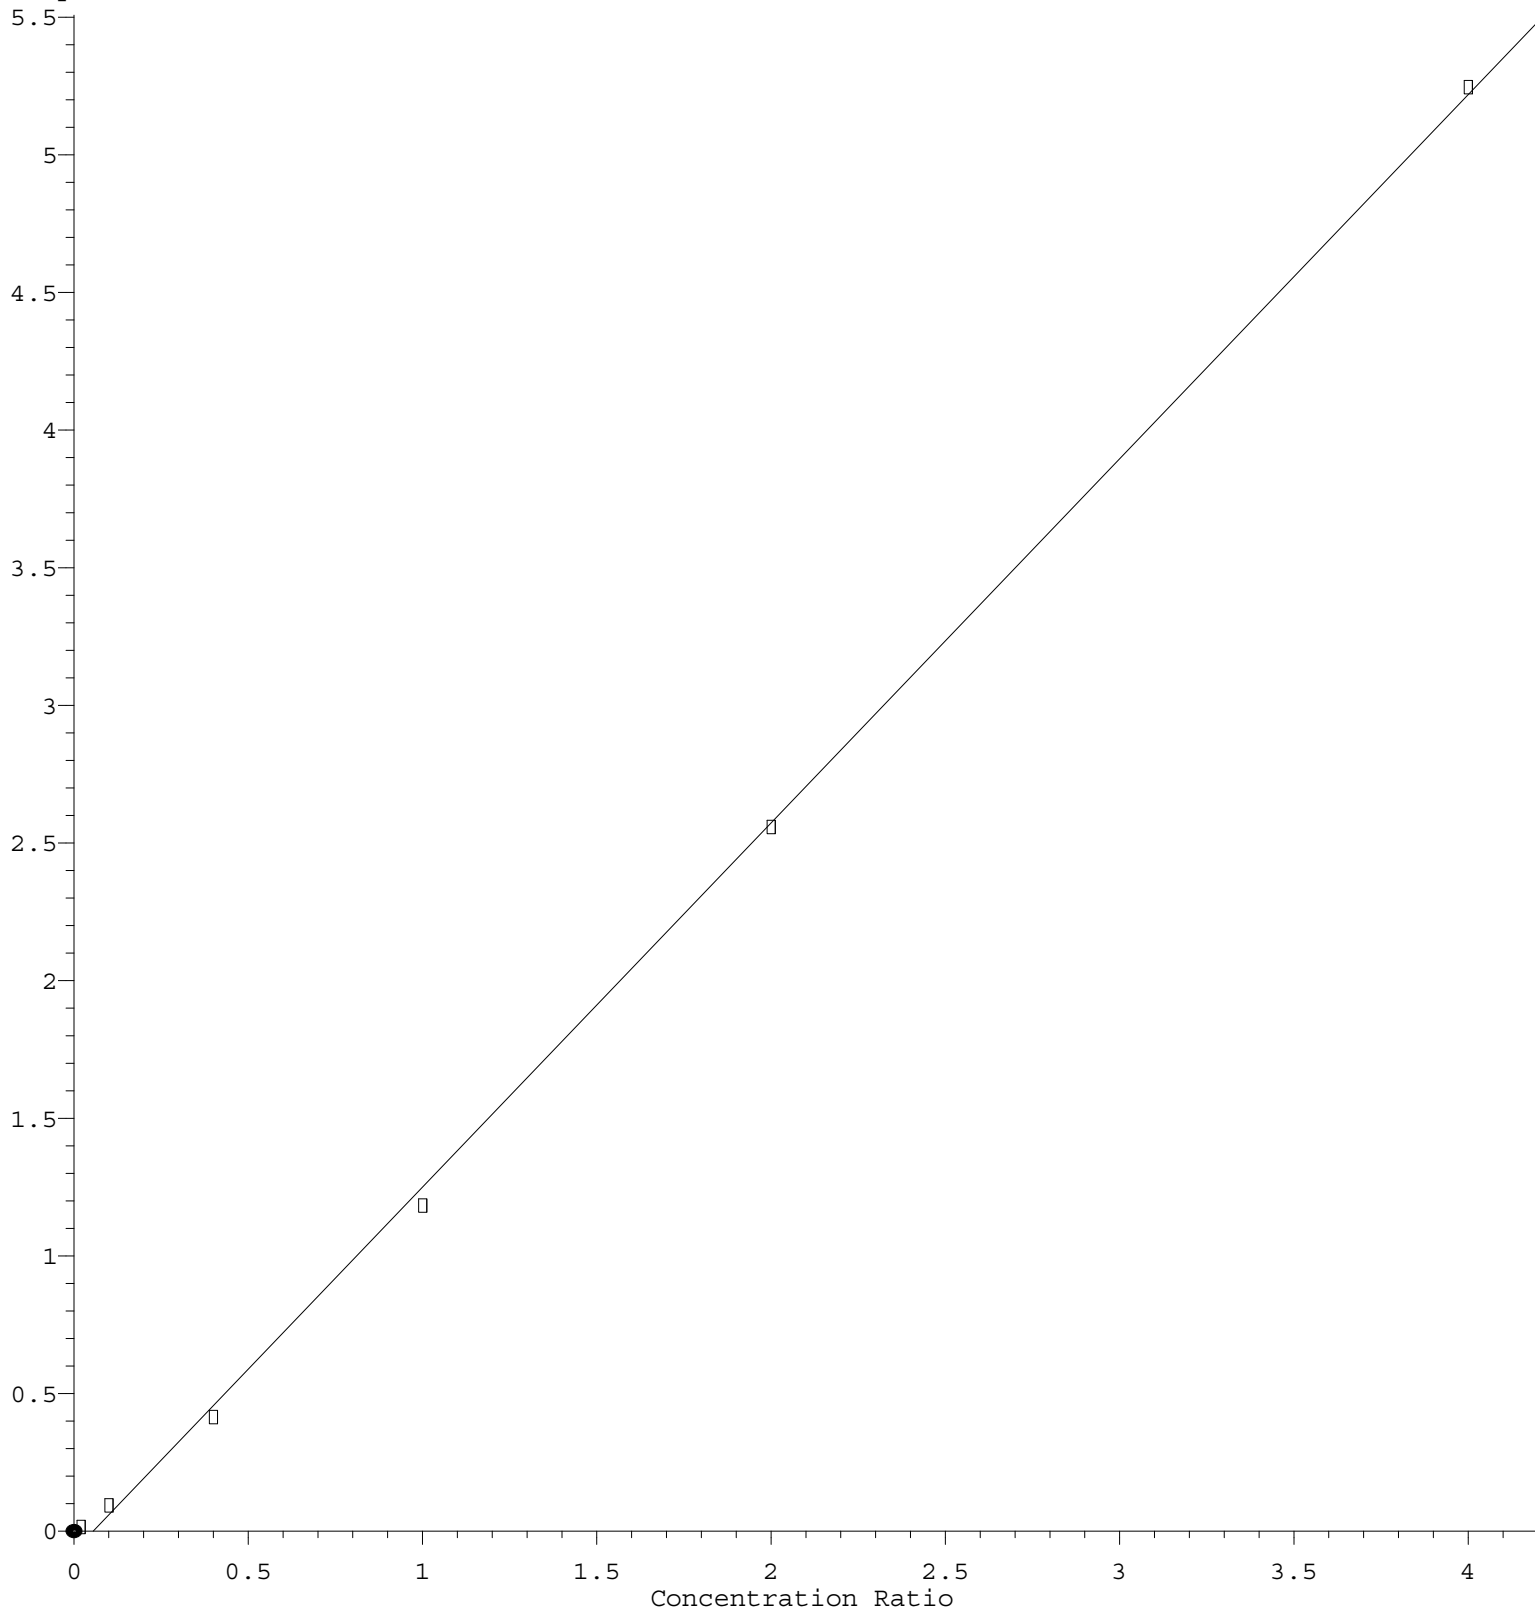

$$\text{Response} = 1.323\text{e}+000 * \text{Amt} - 7.311\text{e}-002$$


Coef of Det (r^2) = 0.999409 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031221W.M

Calibration Table Last Updated: Fri Mar 12 13:00:23 2021

Bromoform

Response Ratio

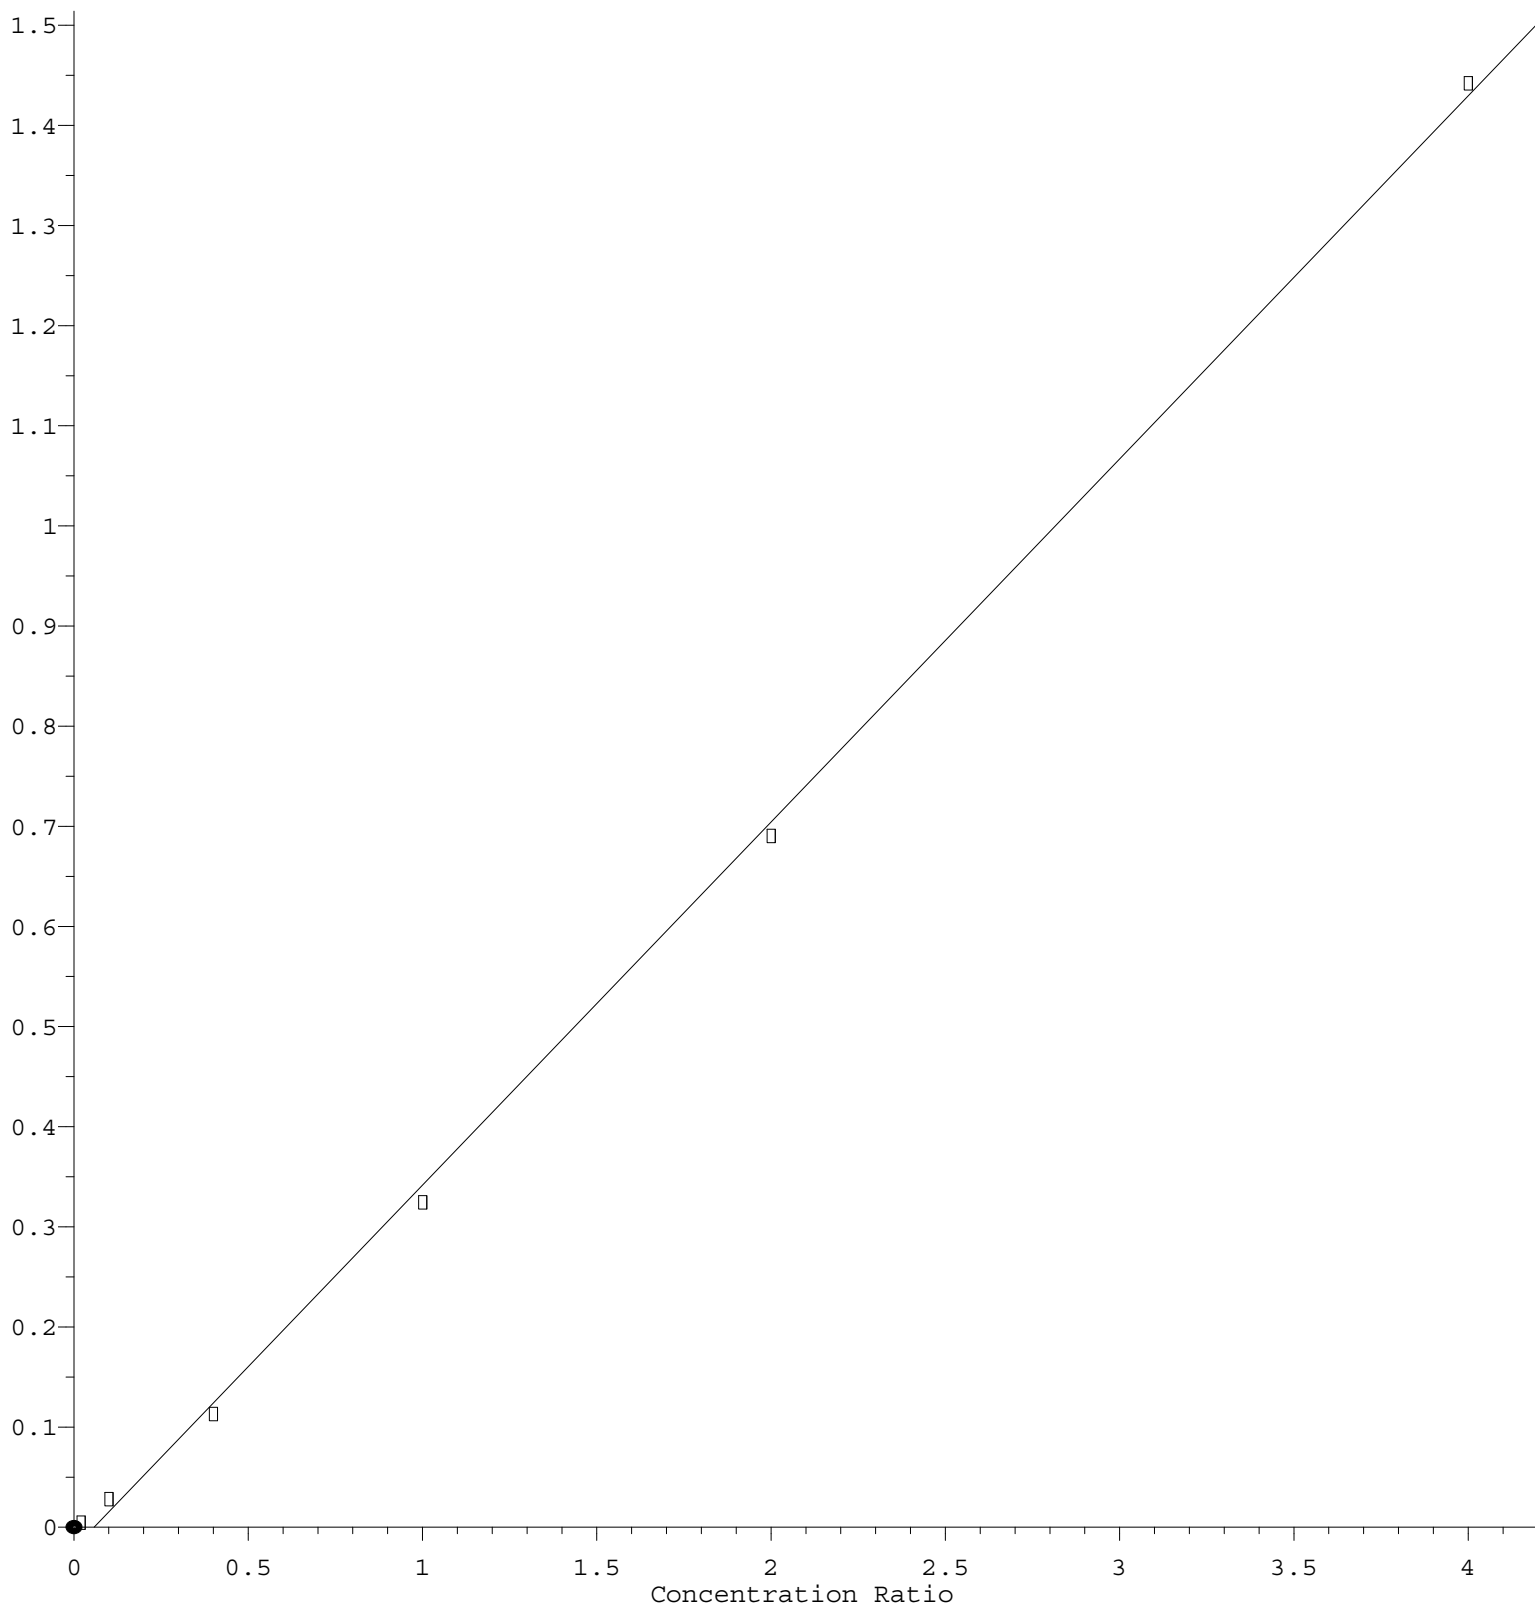

$$\text{Response} = 3.627 \times 10^{-1} \times \text{Amt} - 2.087 \times 10^{-2}$$


Coef of Det (r^2) = 0.999183 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031221W.M

Calibration Table Last Updated: Fri Mar 12 13:00:23 2021

N-amyl acetate

Response Ratio

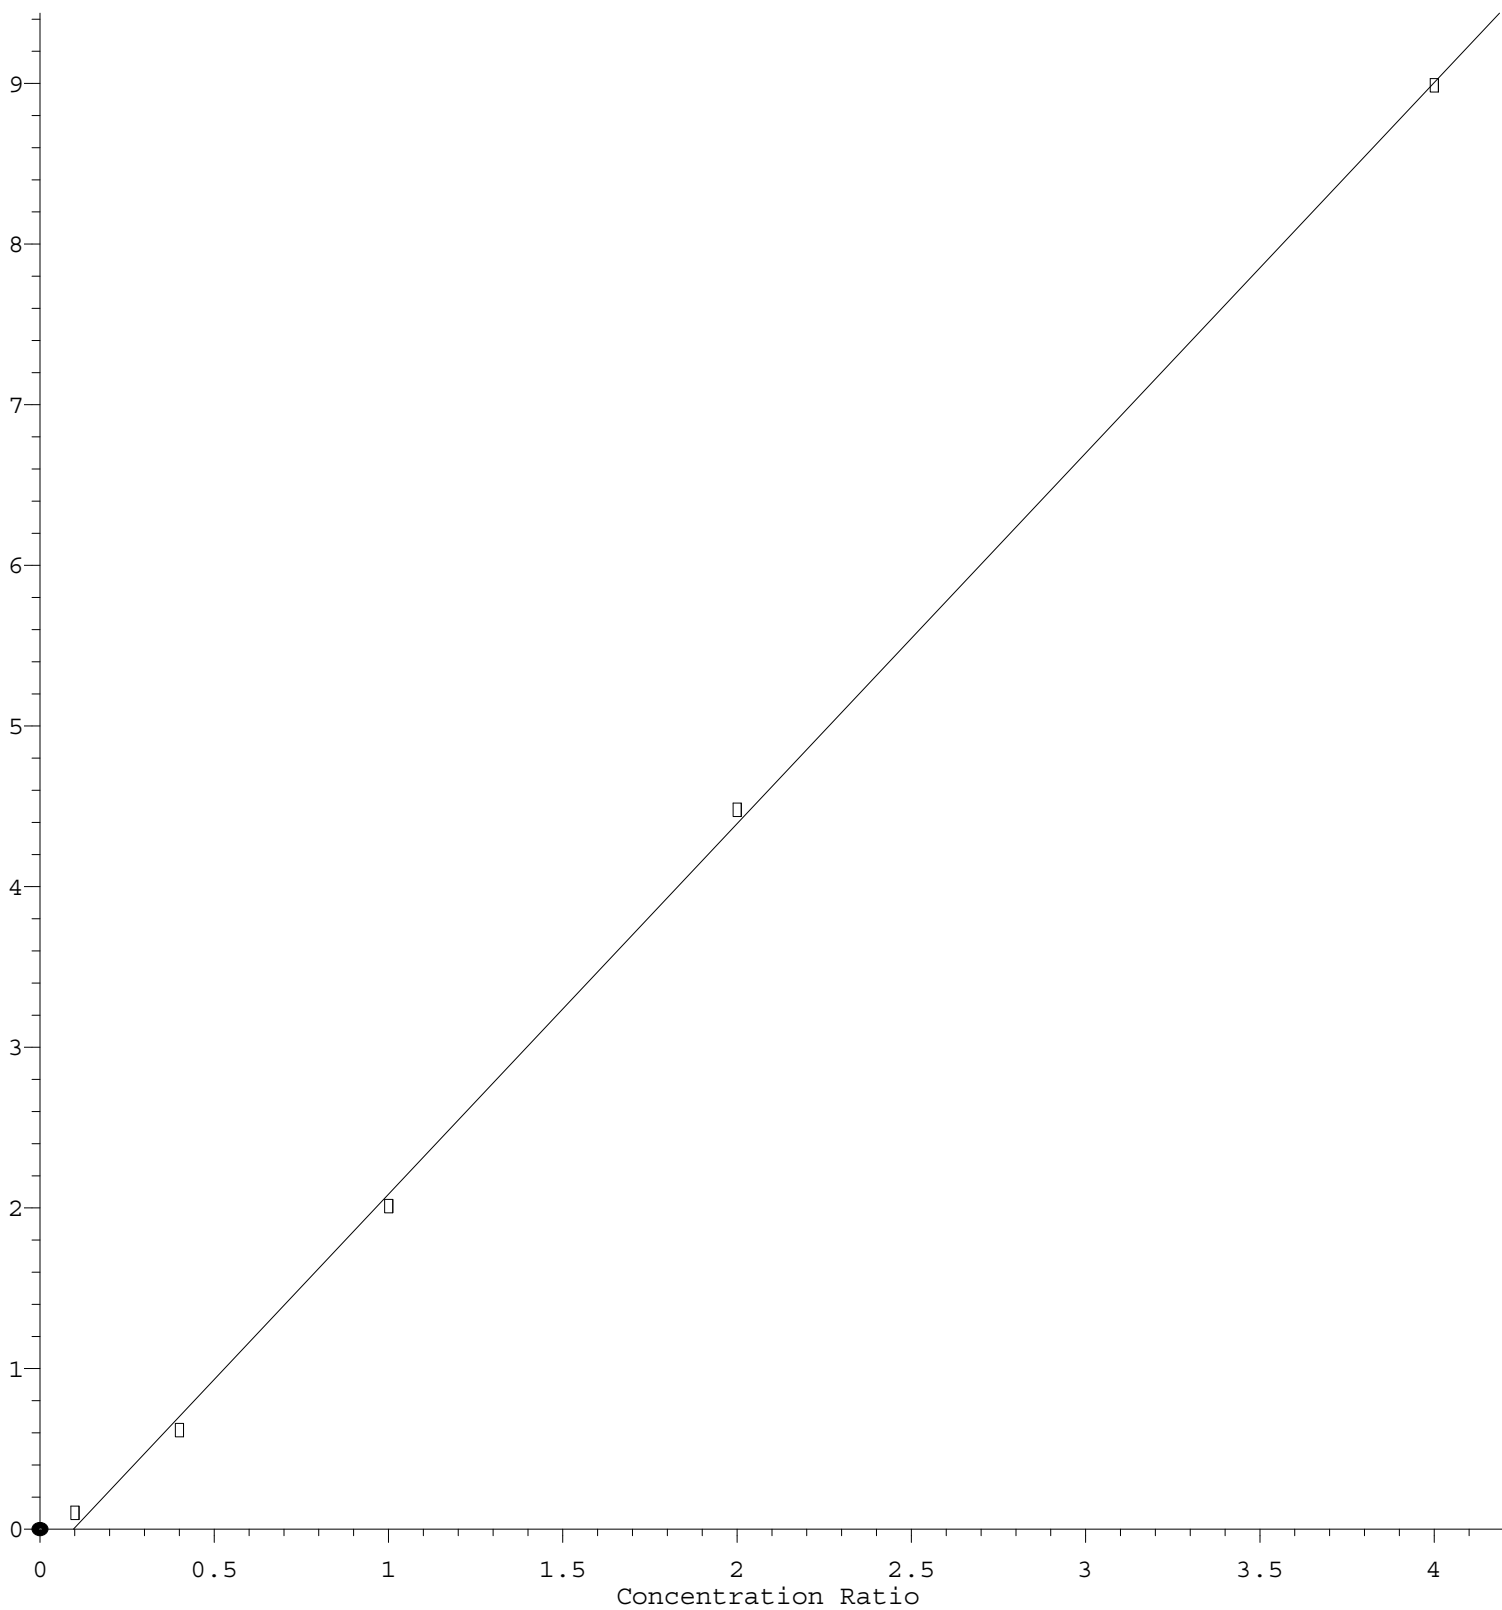

$$\text{Response} = 2.307\text{e}+000 * \text{Amt} - 2.212\text{e}-001$$


Coef of Det (r^2) = 0.999455 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031221W.M

Calibration Table Last Updated: Fri Mar 12 13:00:23 2021

1,2,4-Trichlorobenzene

Response Ratio

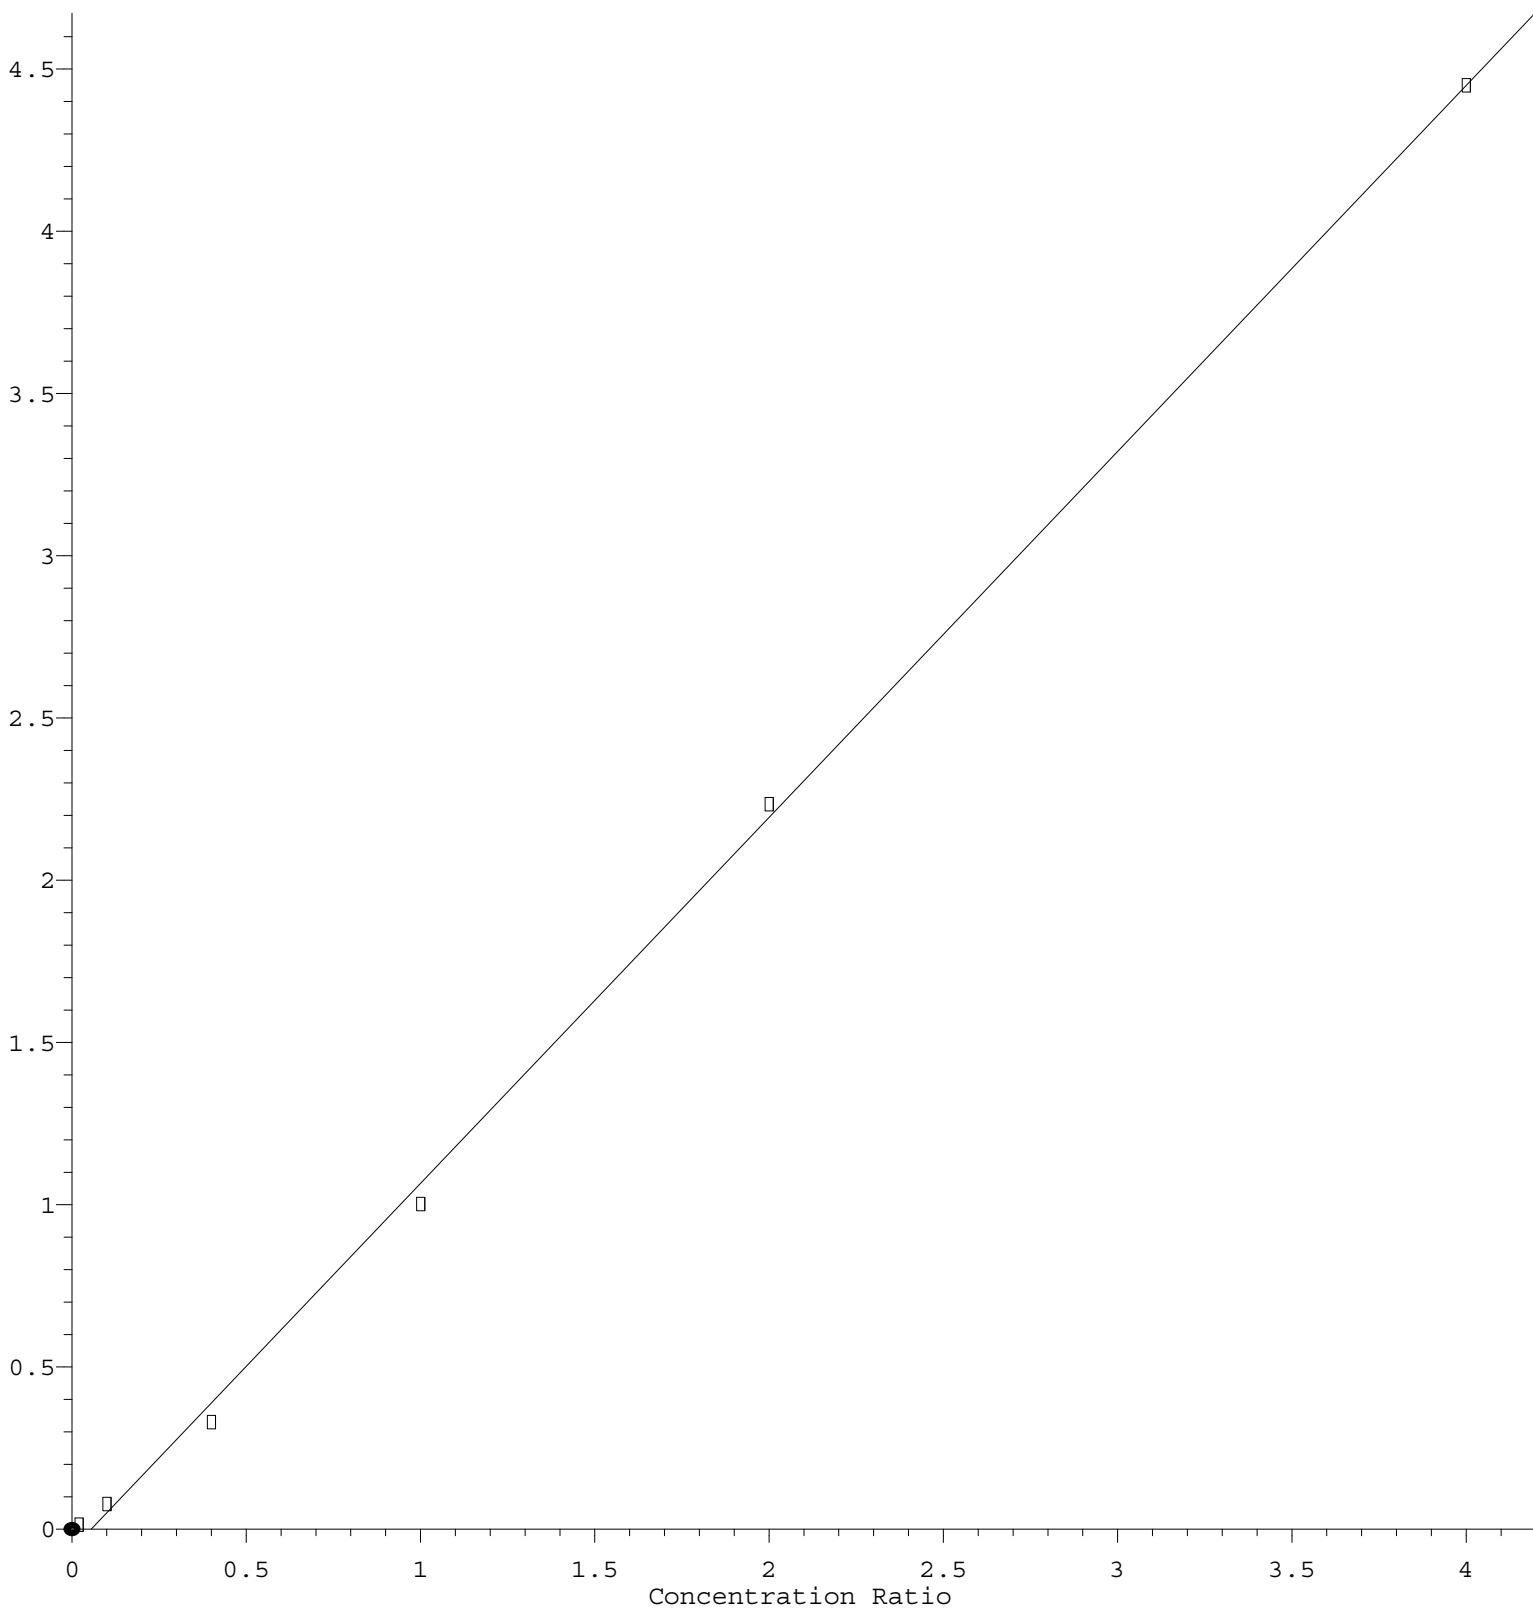

$$\text{Response} = 1.128\text{e}+000 * \text{Amt} - 6.255\text{e}-002$$


Coef of Det (r^2) = 0.999149 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031221W.M

Calibration Table Last Updated: Fri Mar 12 13:00:23 2021

Naphthalene

Response Ratio

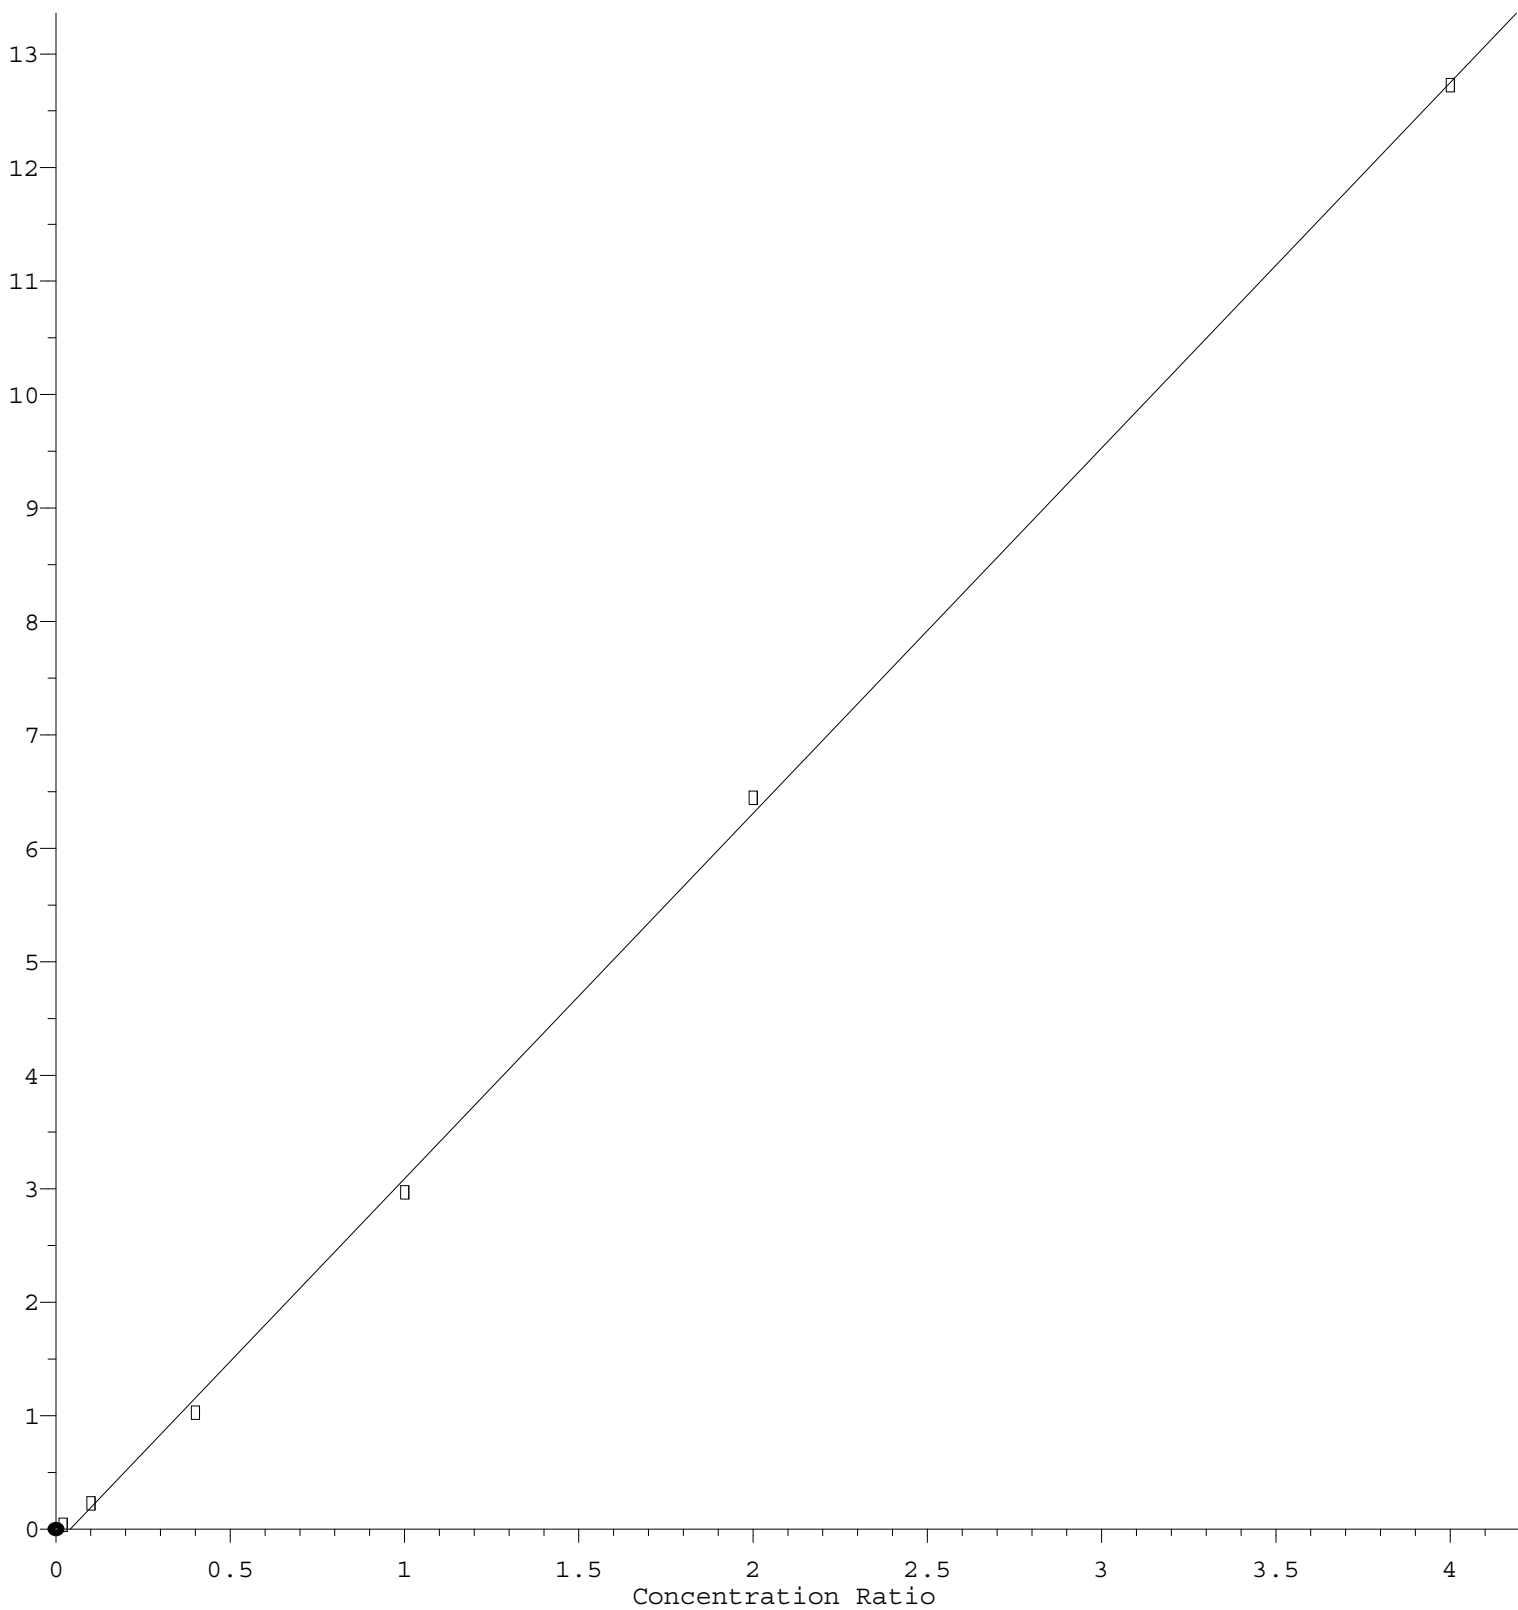

$$\text{Response} = 3.221\text{e}+000 * \text{Amt} - 1.315\text{e}-001$$


Coef of Det (r^2) = 0.999483 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031221W.M

Calibration Table Last Updated: Fri Mar 12 13:00:23 2021

1,2,3-Trichlorobenzene

Response Ratio

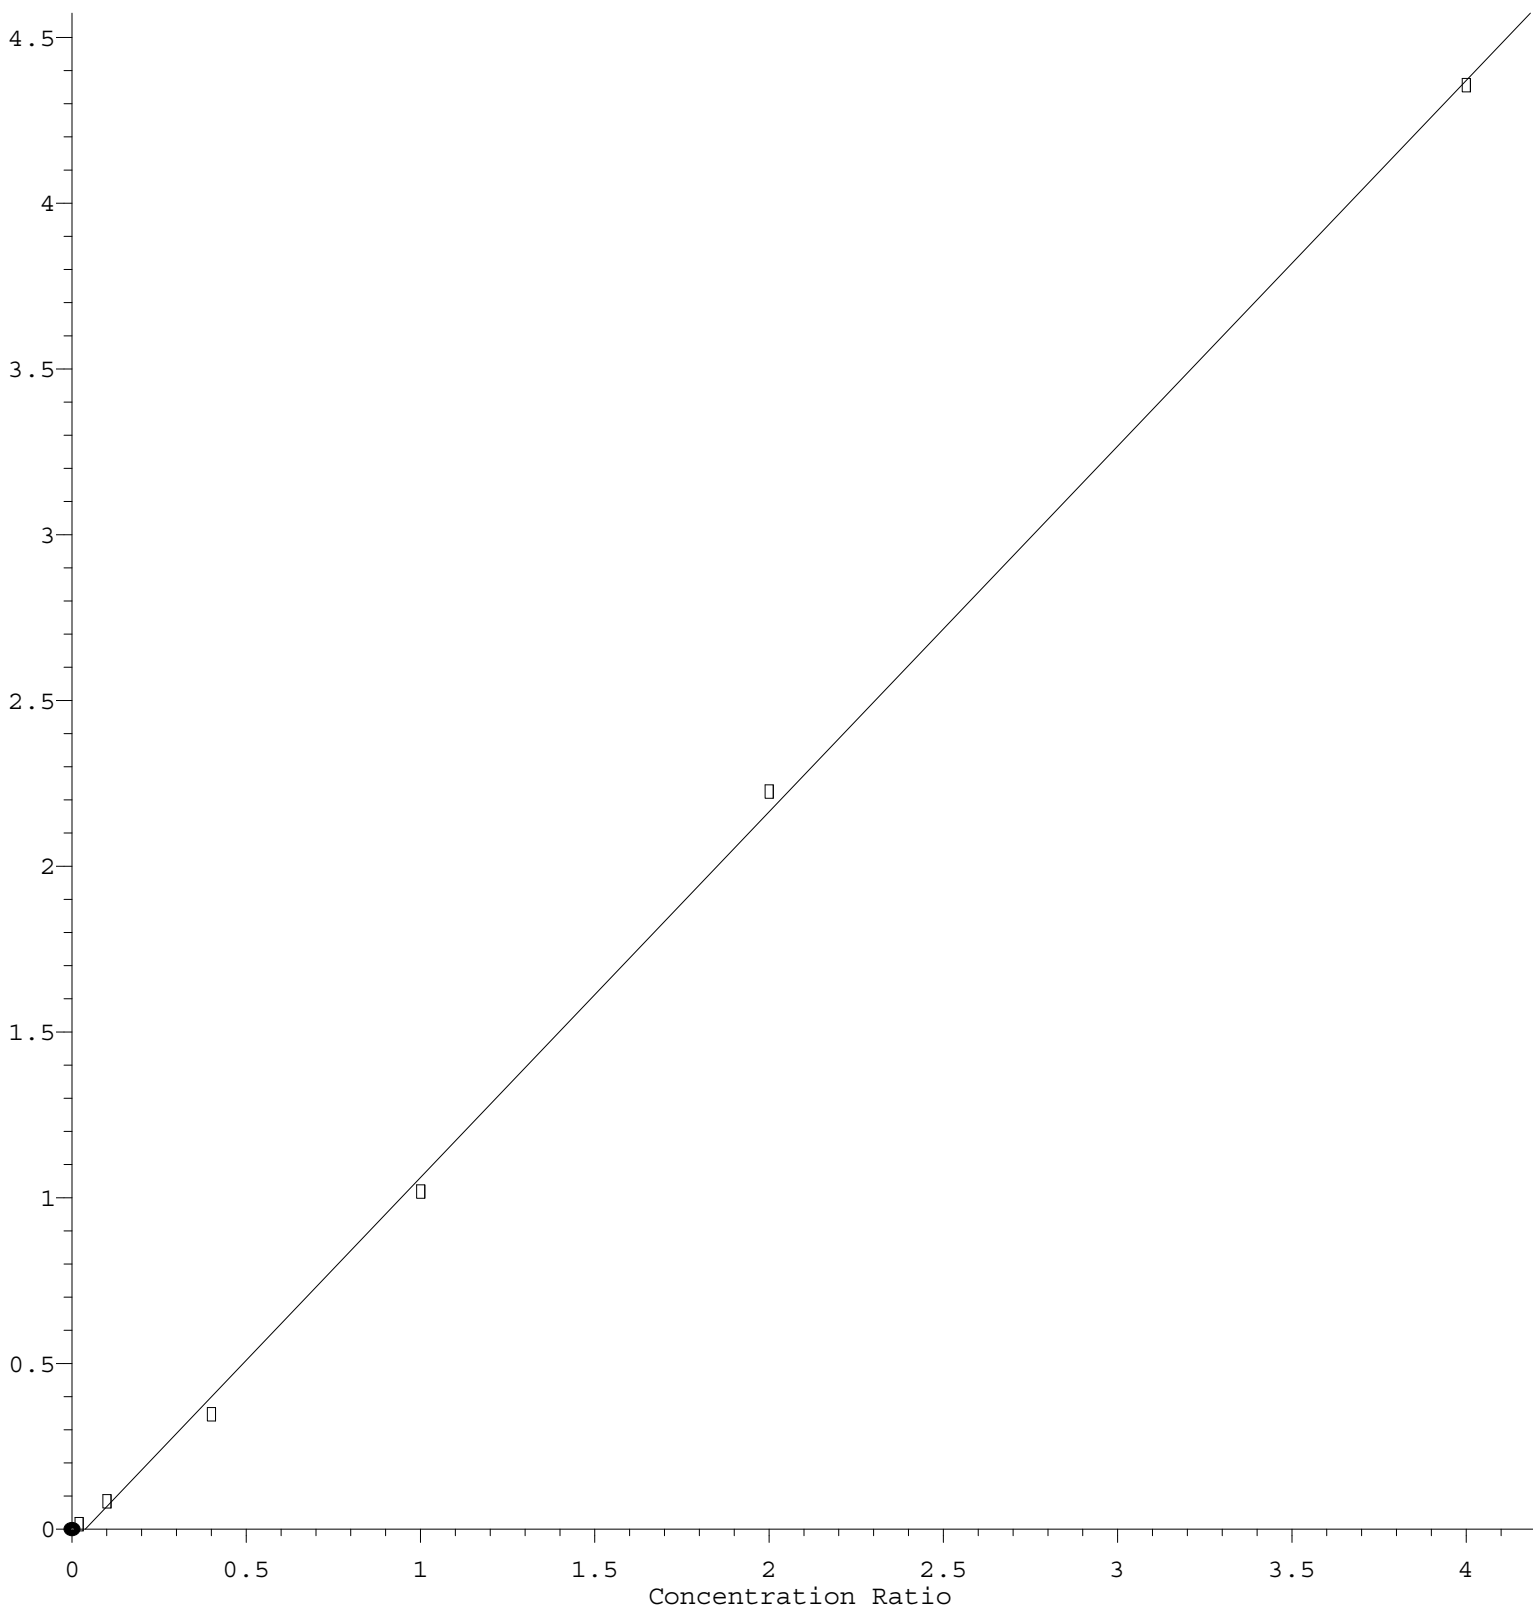

$$\text{Response} = 1.103e+000 * \text{Amt} - 4.176e-002$$

Coef of Det (r^2) = 0.999304 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031221W.M

Calibration Table Last Updated: Fri Mar 12 13:00:23 2021