


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031221\
Data File : VN066174.D
Acq On : 12 Mar 2021 8:45
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031221W.M
Title : SW846 8260
Last Update : Fri Mar 12 13:00:23 2021

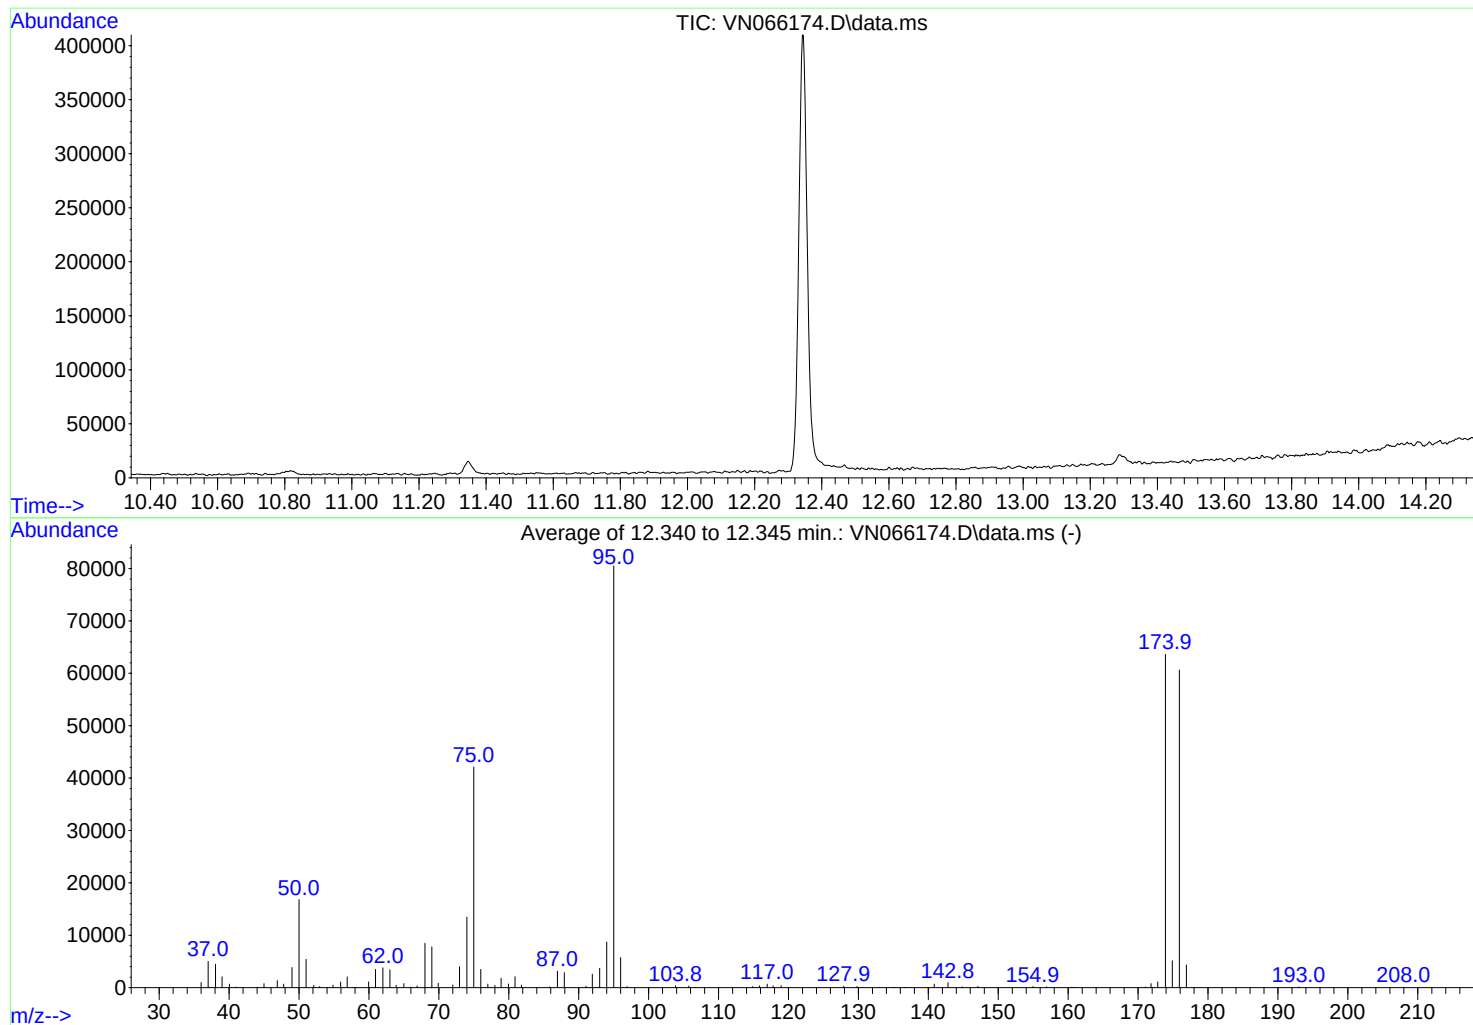

AutoFind: Scans 3971, 3972, 3973; Background Corrected with Scan 3955

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	16784	PASS
75	95	30	60	52.3	42115	PASS
95	95	100	100	100.0	80512	PASS
96	95	5	9	7.1	5751	PASS
173	174	0.00	2	1.7	1090	PASS
174	95	50	100	79.0	63632	PASS
175	174	5	9	8.1	5134	PASS
176	174	95	101	95.3	60635	PASS
177	176	5	9	7.1	4333	PASS