
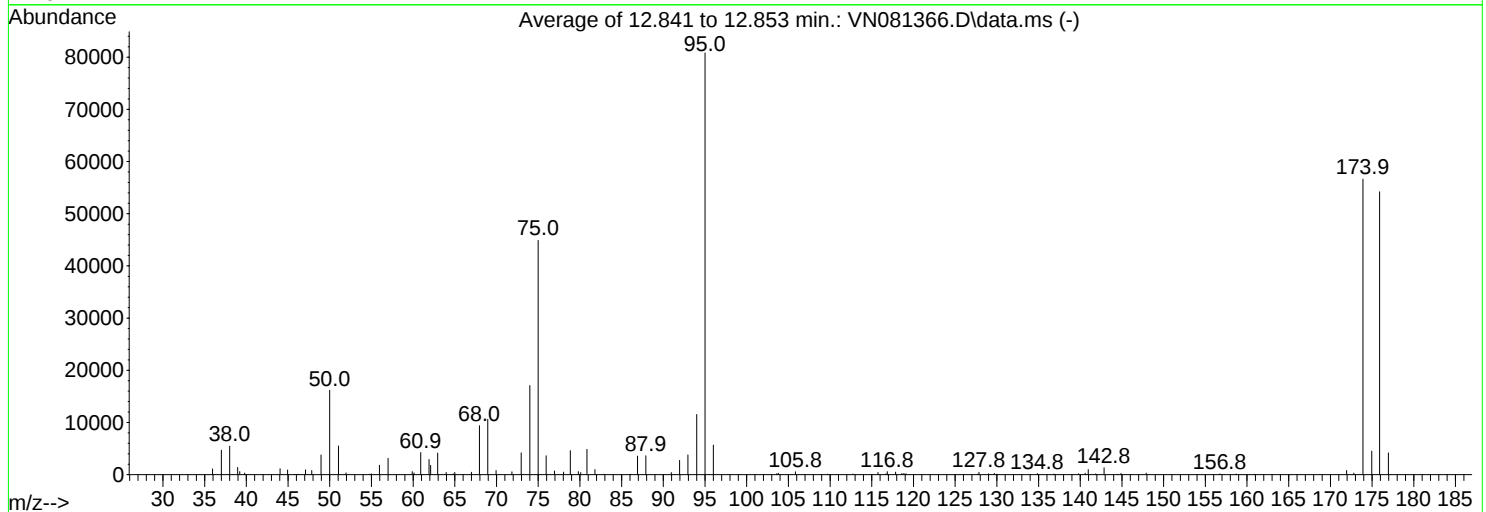


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031224\
Data File : VN081366.D
Acq On : 12 Mar 2024 08:46
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030524W.M
Title : SW846 8260
Last Update : Wed Mar 06 03:12:57 2024

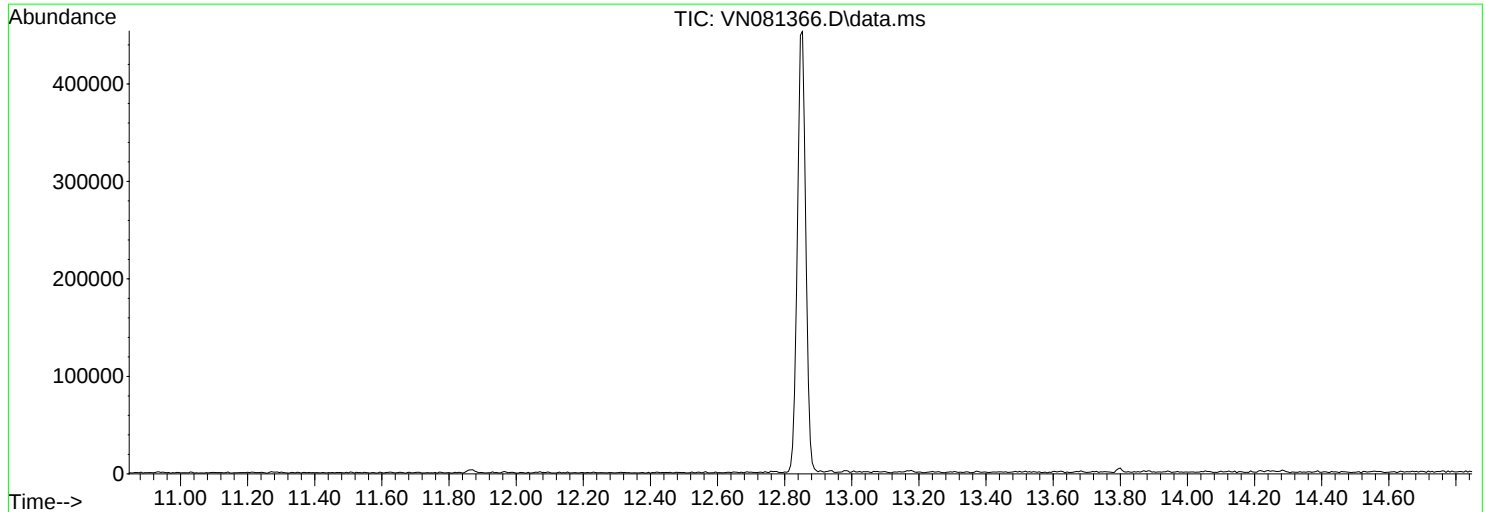

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	16149	PASS
75	95	30	60	55.5	44901	PASS
95	95	100	100	100.0	80832	PASS
96	95	5	9	7.0	5684	PASS
173	174	0.00	2	0.6	314	PASS
174	95	50	100	70.1	56643	PASS
175	174	5	9	8.0	4510	PASS
176	174	95	101	95.7	54203	PASS
177	176	5	9	7.7	4173	PASS

Average of 12.841 to 12.853 min.: VN081366.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	1107	47.85	812	60.90	4223	71.85	541
37.00	4691	48.95	3770	61.90	2911	72.95	418
38.00	5451	50.00	16149	62.10	1795	74.00	1707
38.95	1379	51.05	5504	62.95	4142	75.00	4490
39.20	580	51.95	328	63.95	440	75.95	3624
39.80	317	54.80	96	64.80	144	76.95	711
44.05	1141	55.00	144	65.00	434	78.05	490
44.95	904	55.95	1820	67.00	454	78.85	4610
45.80	52	57.00	3137	67.95	9378	79.80	582
46.20	54	59.90	575	68.95	10605	80.10	390
47.10	916	60.10	345	69.95	803	80.85	4841

Average of 12.841 to 12.853 min.: VN081366.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.80	993	103.60	177	118.85	256	140.95	988
82.90	101	103.80	276	119.10	200	141.85	161
86.10	85	105.85	552	127.70	106	142.85	1330
86.90	3570	106.90	62	127.85	465	144.50	57
87.90	3618	109.70	85	129.00	170	144.90	256
90.95	393	112.75	128	129.70	247	147.90	304
91.95	2718	115.75	435	130.00	92	156.75	141
92.95	3783	116.70	141	134.85	218	158.70	122
94.00	11532	116.85	578	136.85	129	160.90	58
95.00	80832	117.85	489	139.80	177	171.95	798
96.00	5684	118.60	222	140.60	278	172.80	314

Average of 12.841 to 12.853 min.: VN081366.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
173.90	56643						
174.95	4510						
175.90	54203						
176.95	4173						

Instrument :
MSVOA_N
ClientSampleId :
BFB