
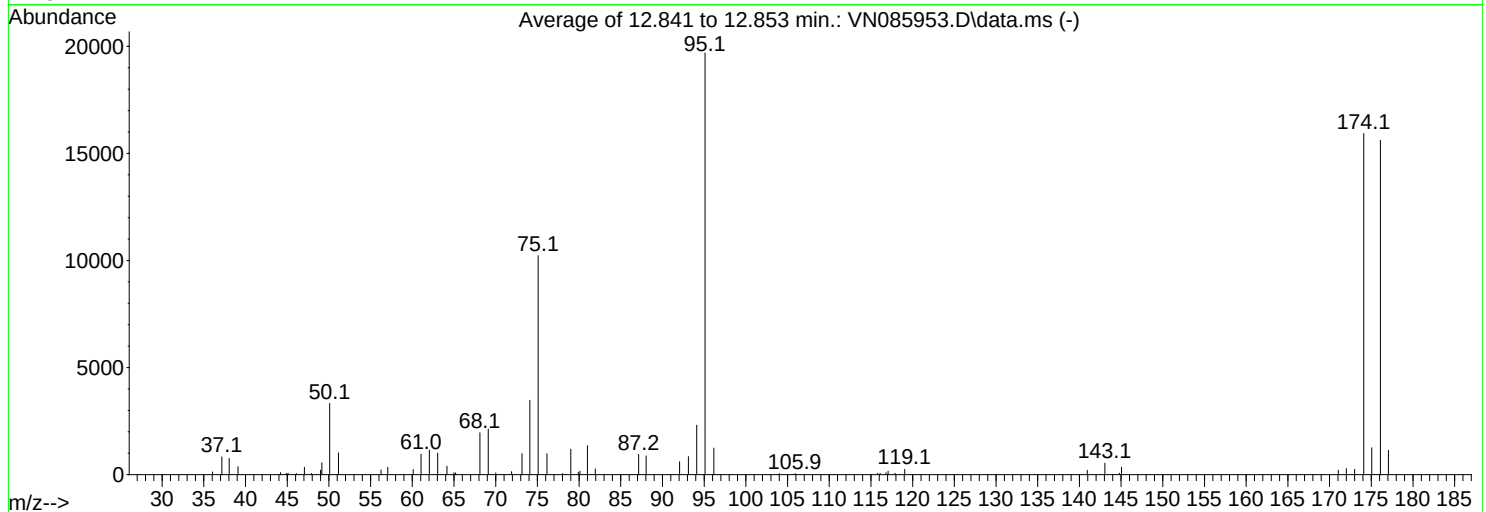


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031225\
Data File : VN085953.D
Acq On : 12 Mar 2025 11:20
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Title : SW846 8260
Last Update : Wed Feb 19 03:43:32 2025

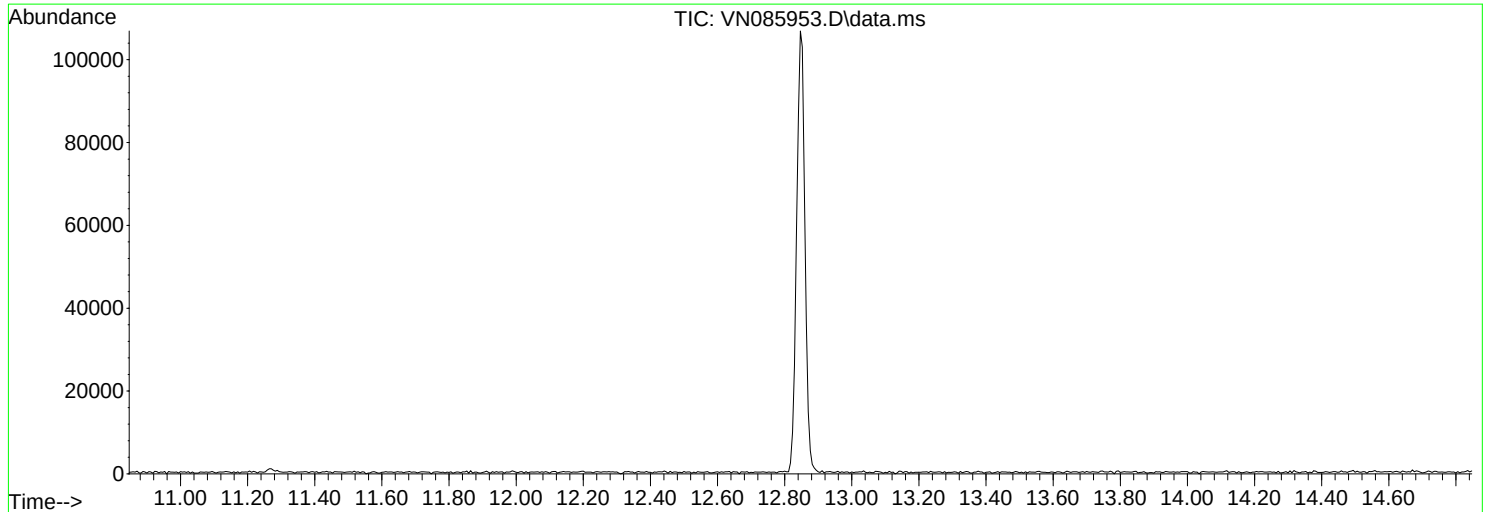

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	3323	PASS
75	95	30	60	51.9	10225	PASS
95	95	100	100	100.0	19696	PASS
96	95	5	9	6.3	1239	PASS
173	174	0.00	2	1.6	248	PASS
174	95	50	100	80.9	15933	PASS
175	174	5	9	7.9	1257	PASS
176	174	95	101	98.0	15619	PASS
177	176	5	9	7.3	1137	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	127	49.15	554	65.20	81	79.90	111
37.15	831	50.10	3323	68.10	1959	80.10	167
38.05	756	51.15	1018	69.10	2128	81.00	135
39.10	372	56.25	225	70.00	80	81.95	26
44.20	96	57.05	342	71.90	140	87.15	944
44.90	57	60.10	238	73.15	984	88.05	873
45.10	64	61.05	960	74.10	3469	92.05	608
46.10	52	62.05	1151	75.10	10225	93.10	843
47.05	346	63.05	1006	76.15	977	94.10	2307
47.90	54	64.15	393	78.00	52	95.10	19696
49.00	212	65.00	87	79.00	1188	96.15	1239

Average of 12.841 to 12.853 min.: VN085953.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
104.00	51	145.05	344				
105.90	52	171.05	208				
115.80	59	172.00	287				
116.10	56	173.00	248				
116.80	87	174.10	15933				
117.05	164	175.05	1257				
117.90	61	176.10	15619				
119.05	250	177.05	1137				
140.95	199						
143.05	538						
144.80	68						

Instrument :

MSVOA_N

ClientSampleId :

BFB