

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN031319\
 Data File : VN054219.D
 Acq On : 13 Mar 2019 18:18
 Operator : JC/SP
 Sample : K1842-11
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PR-MW-04_030819

Quant Time: Mar 14 07:38:18 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 13 03:33:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	1375228	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	2229193	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	2408832	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	1093265	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.03	65	731622	50.09	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.18%	
35) Dibromofluoromethane	7.59	113	681938	47.43	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.86%	
50) Toluene-d8	10.09	98	2824389	53.19	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.38%	
62) 4-Bromofluorobenzene	12.40	95	1118524	60.20	ug/l	0.00
Spiked Amount 50.000			Recovery	=	120.40%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN031319\
Data File : VN054219.D
Acq On : 13 Mar 2019 18:18
Operator : JC/SP
Sample : K1842-11
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PR-MW-04_030819

Quant Time: Mar 14 07:38:18 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 13 03:33:31 2019
Response via : Initial Calibration

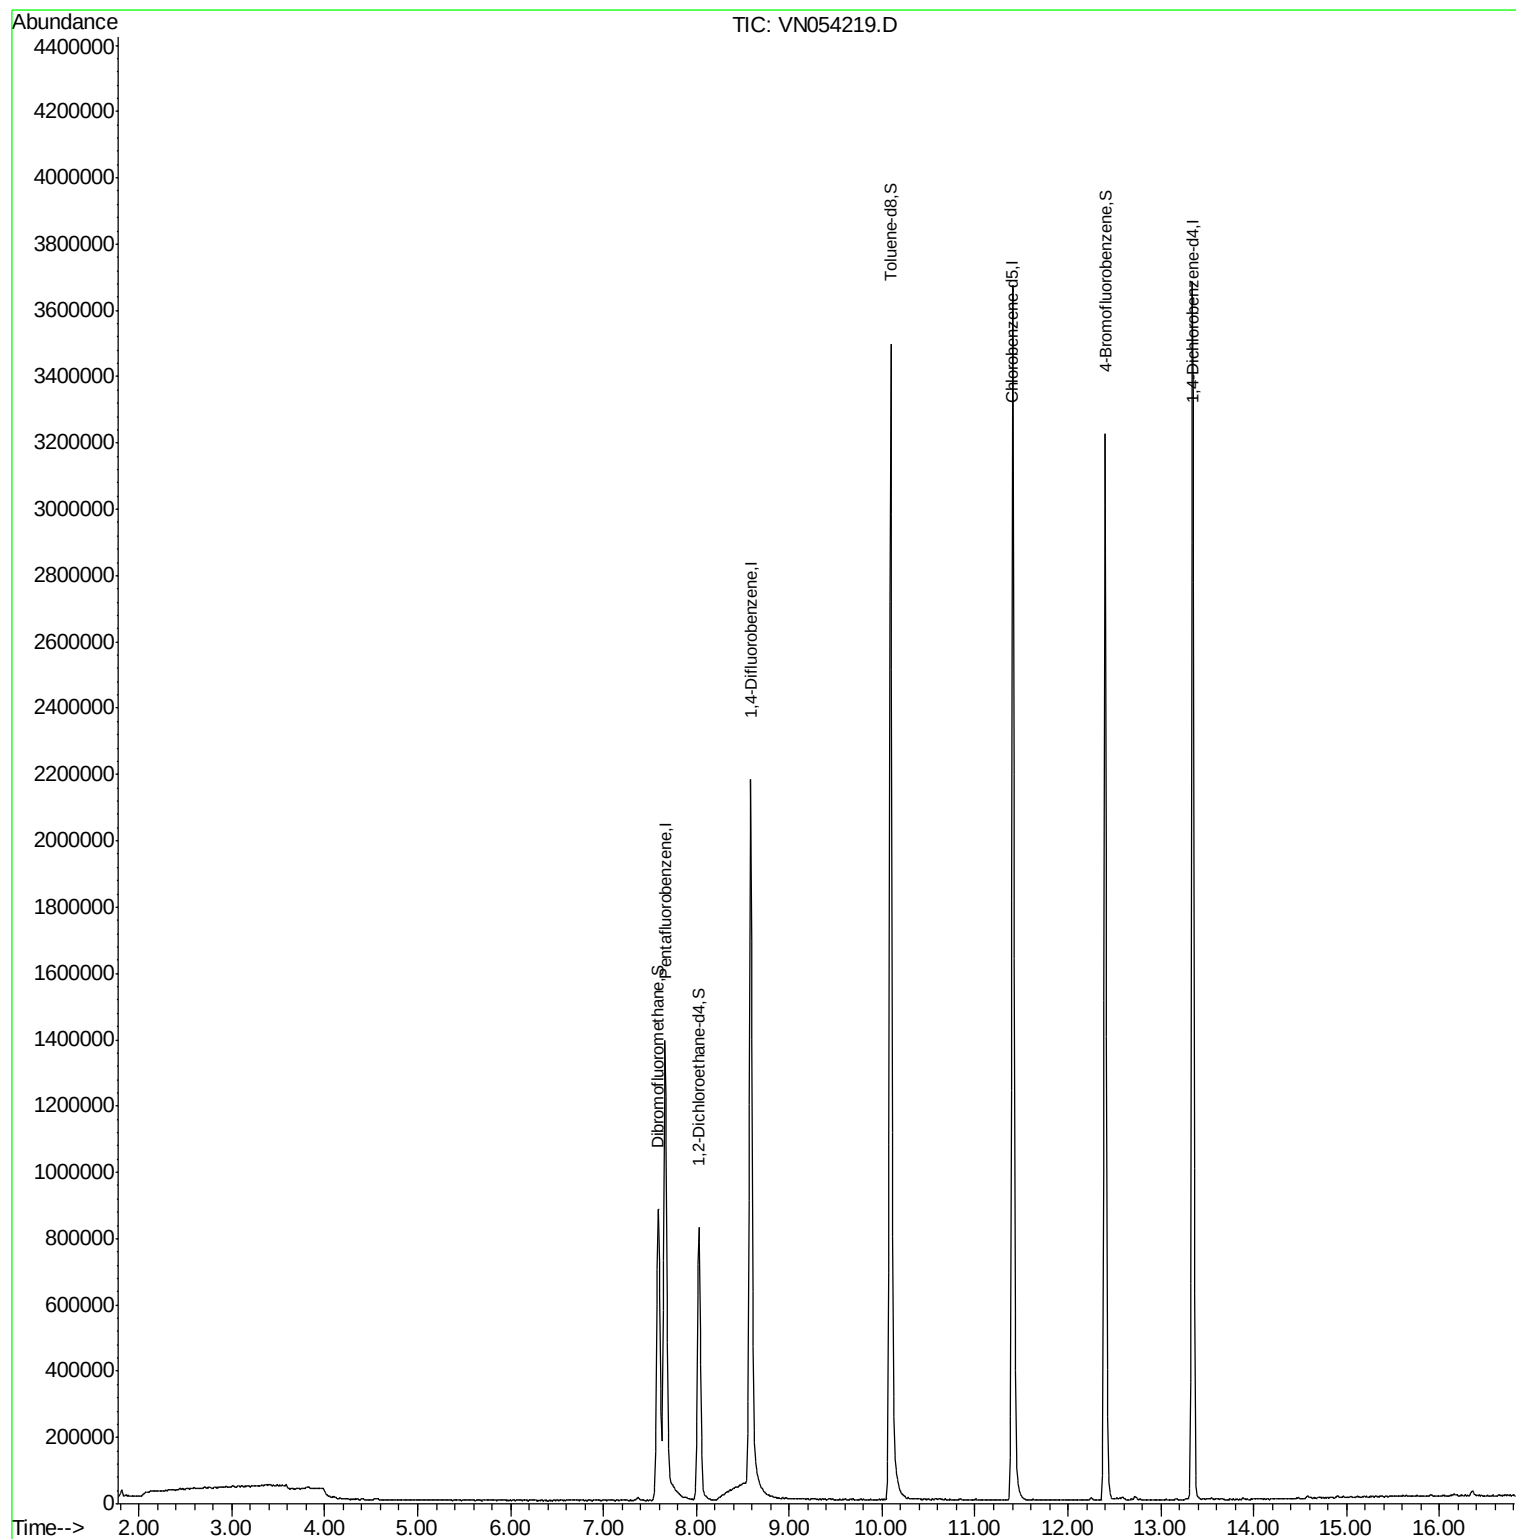

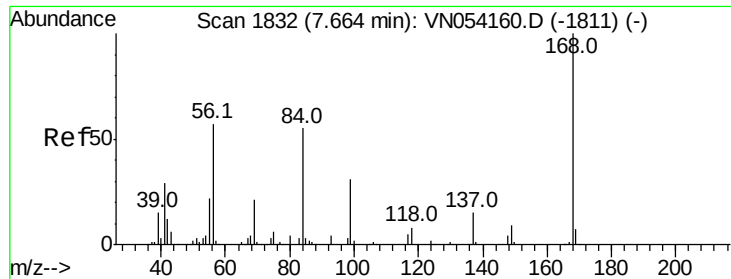

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. 0.00 min

Lab File: VN054219.D

Acq: 13 Mar 2019 18:18

Instrument :

MSVOA_N

ClientSampleId :


PR-MW-04_030819

Tot Ion:168 Resp: 1375228

Ion Ratio Lower Upper

168 100

99 47.4 37.1 55.7

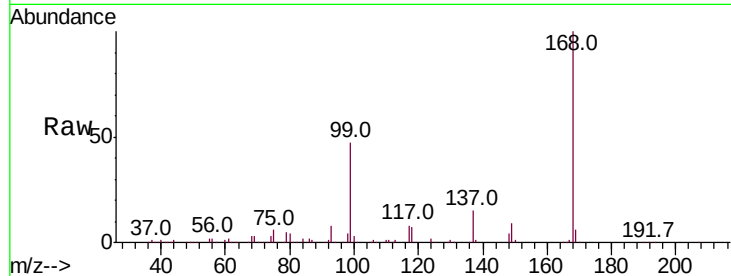

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

7.67

600000

500000

400000



300000

200000

100000

0

Time--> 7.50 7.60 7.70 7.80 7.90

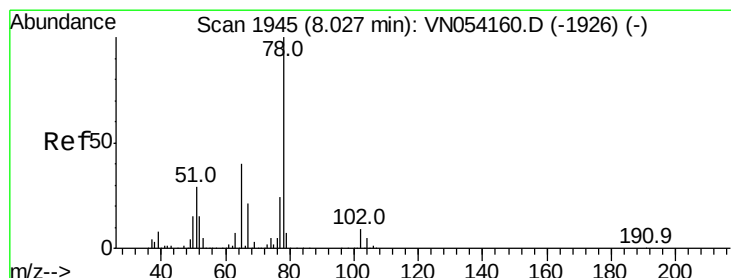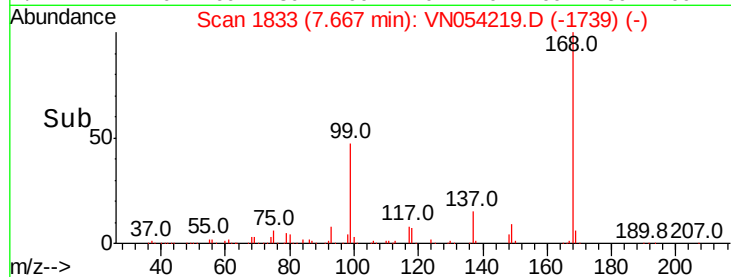

#33

1,2-Dichloroethane-d4

Concen: 50.094 ug/l

RT: 8.03 min Scan# 1945

Delta R.T. -0.00 min

Lab File: VN054219.D


Acq: 13 Mar 2019 18:18

Tgt Ion: 65 Resp: 731622

Ion Ratio Lower Upper

65 100

67 51.8 0.0 104.6

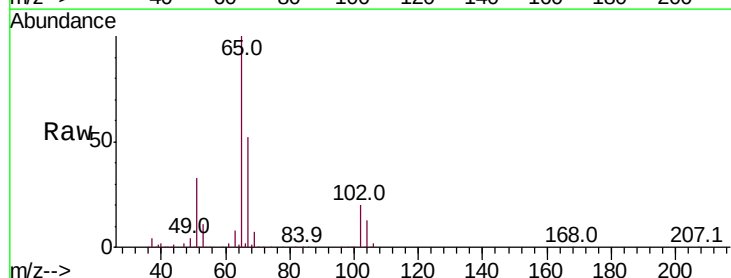

Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

8.03


300000


200000

100000

0

Time--> 7.90 8.00 8.10 8.20

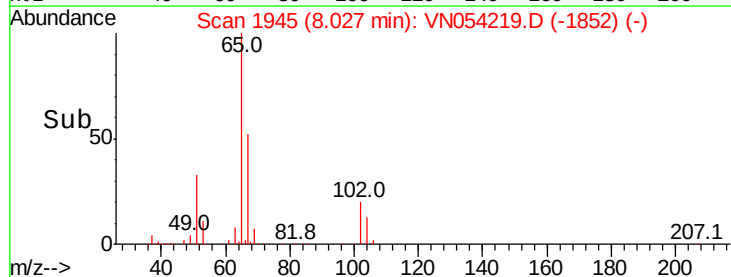


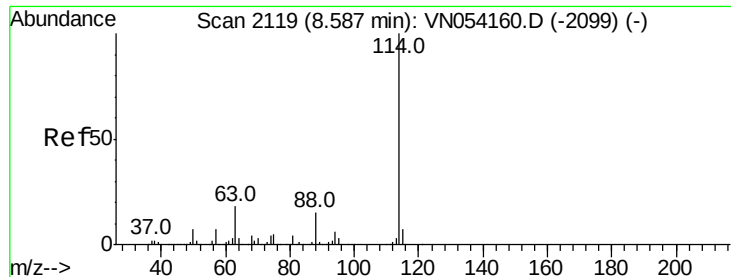




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.59 min Scan# 2119
Delta R.T. -0.00 min
Lab File: VN054219.D
Acq: 13 Mar 2019 18:18

Instrument :
MSVOA_N
ClientSampleId :
PR-MW-04_030819

Tot Ion:114 Resp: 2229193
Ion Ratio Lower Upper
114 100
63 18.0 0.0 35.2
88 15.0 0.0 30.2

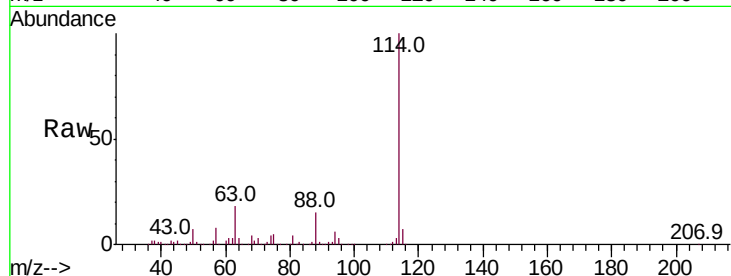


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VN
Ion 87.90 (87.60 to 88.60): VN

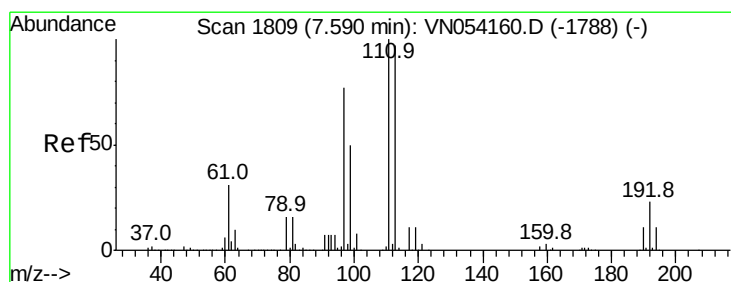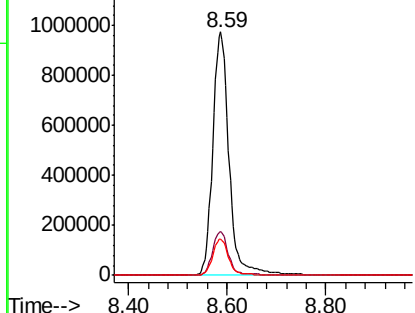
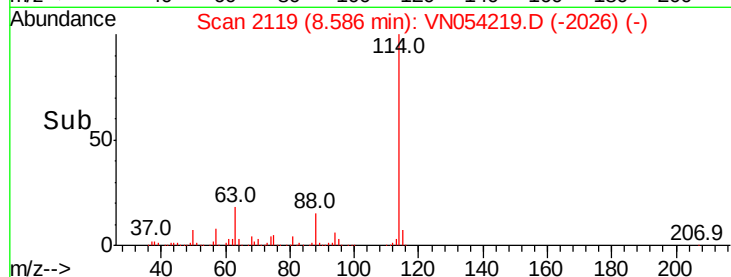



#35
Dibromofluoromethane
Concen: 47.431 ug/l
RT: 7.59 min Scan# 1809
Delta R.T. -0.00 min
Lab File: VN054219.D
Acq: 13 Mar 2019 18:18

Tgt Ion:113 Resp: 681938
Ion Ratio Lower Upper
113 100
111 102.7 82.2 123.4
192 23.7 19.2 28.8

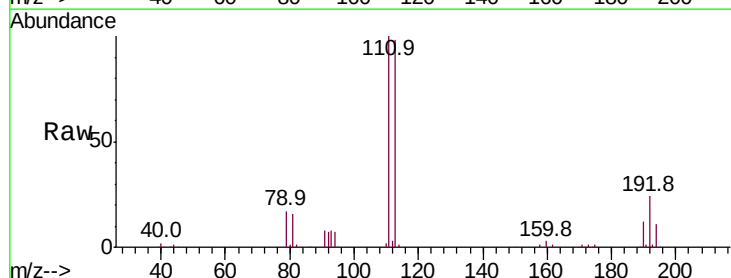

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

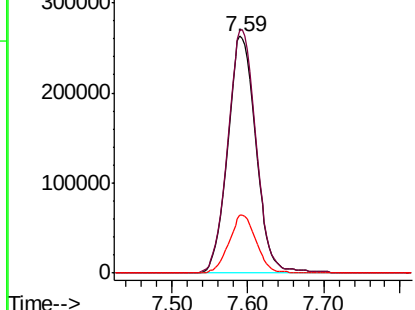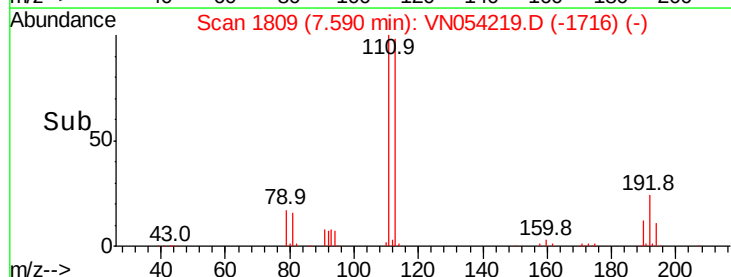

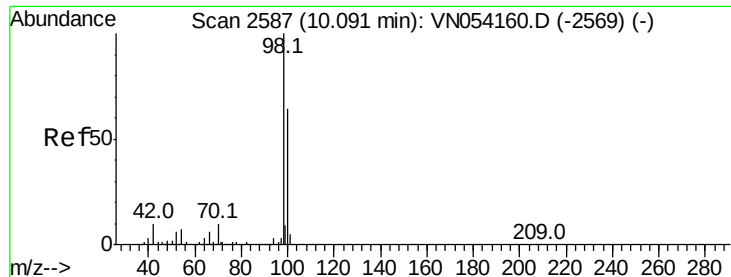

#50

Toluene-d8

Concen: 53.192 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN054219.D

Acq: 13 Mar 2019 18:18

Instrument :

MSVOA_N

ClientSampleId :





PR-MW-04_030819

Tot Ion: 98 Resp: 2824389

Ion Ratio Lower Upper

98 100

100 63.8 51.2 76.8

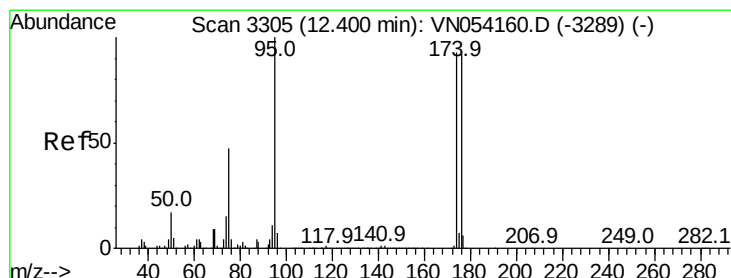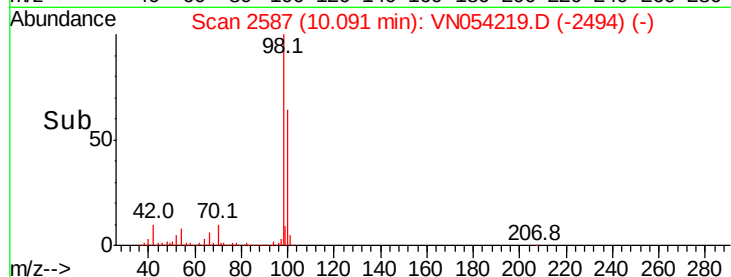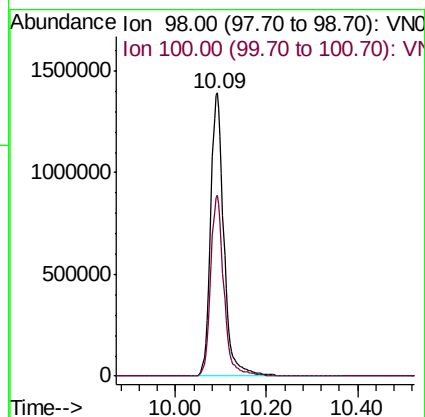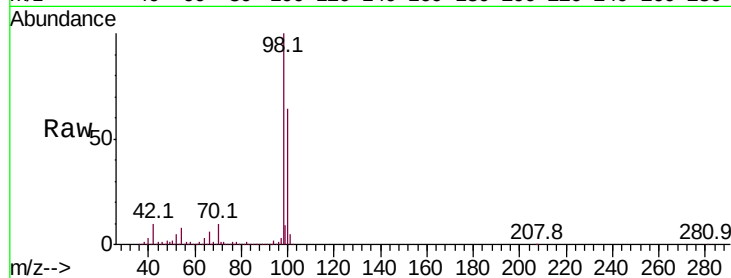

#62

4-Bromofluorobenzene

Concen: 60.204 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.00 min

Lab File: VN054219.D

Acq: 13 Mar 2019 18:18




Tgt Ion: 95 Resp: 1118524


Ion Ratio Lower Upper

95 100

174 97.4 0.0 191.0

176 94.9 0.0 187.4


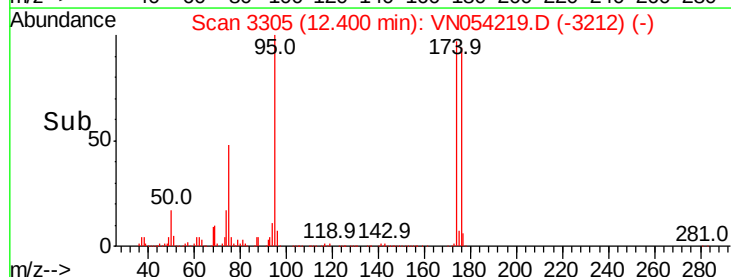
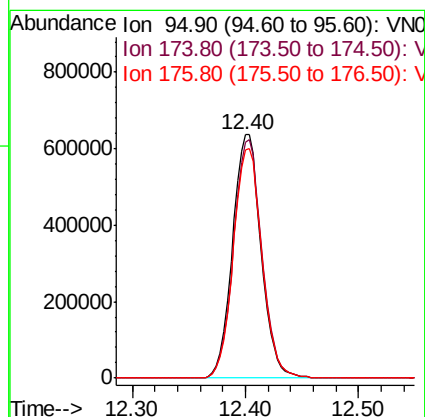
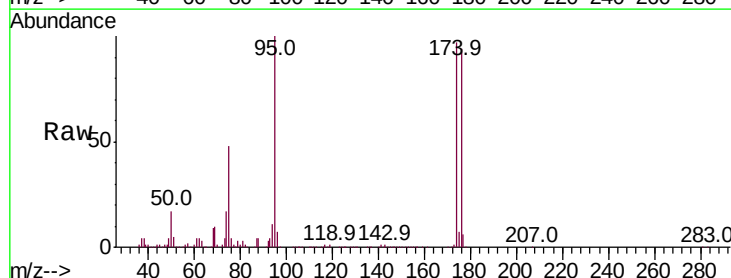


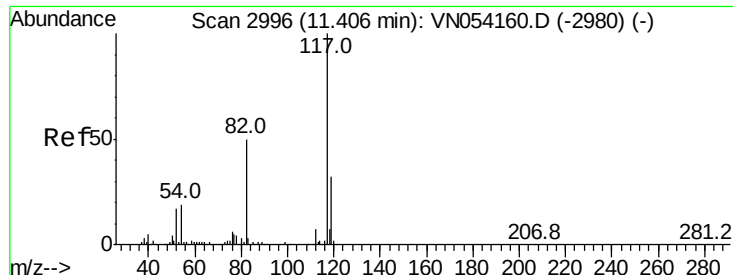

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. -0.00 min
Lab File: VN054219.D
Acq: 13 Mar 2019 18:18

Instrument :
MSVOA_N
ClientSampleId :
PR-MW-04_030819

Tot Ion:117 Resp: 2408832
Ion Ratio Lower Upper
117 100
82 51.0 40.0 60.0
119 32.1 25.8 38.6

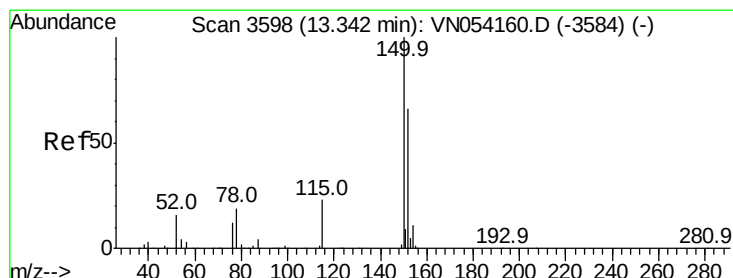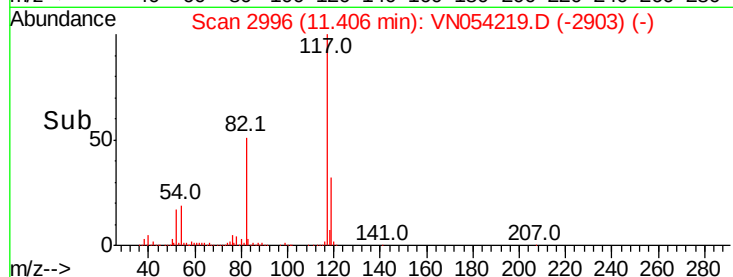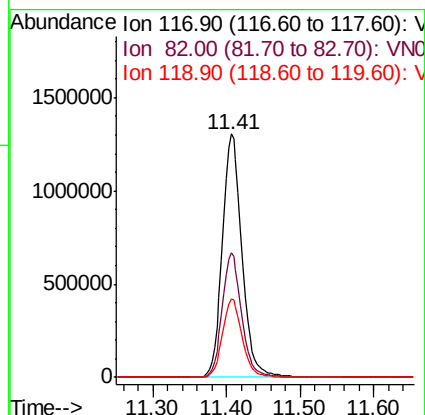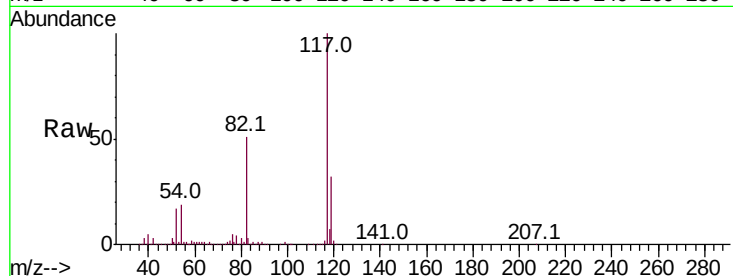

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3598
Delta R.T. -0.00 min
Lab File: VN054219.D
Acq: 13 Mar 2019 18:18

Tgt Ion:152 Resp: 1093265
Ion Ratio Lower Upper
152 100
115 54.4 27.2 81.6
150 157.8 0.0 349.2

