


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN031319\
 Data File : VN054226.D
 Acq On : 13 Mar 2019 21:49
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
 Title : SW846 8260
 Last Update : Wed Mar 13 03:33:31 2019

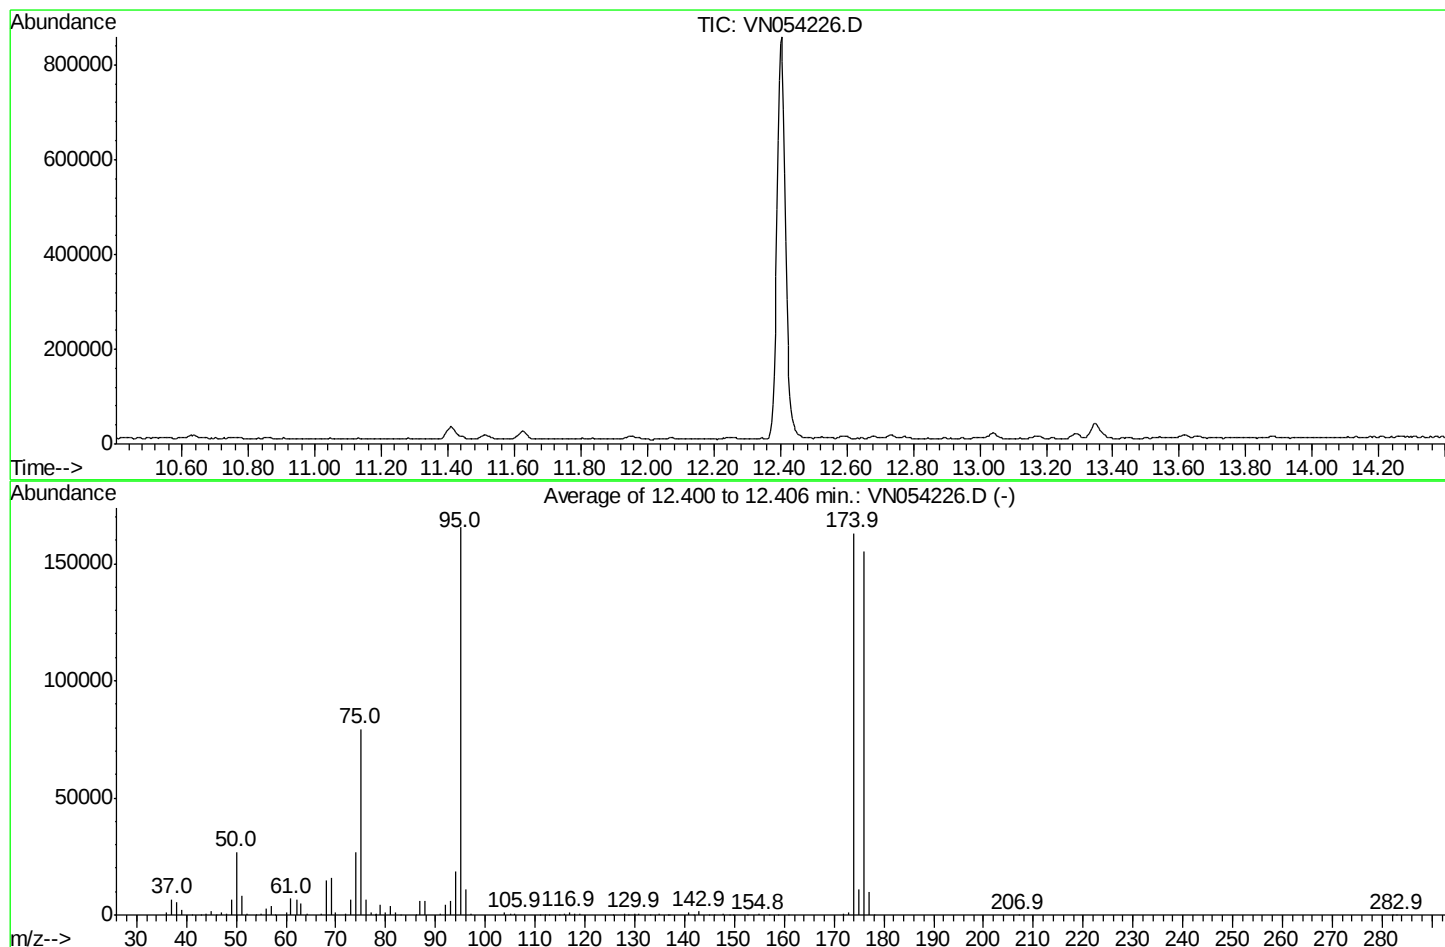

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3289

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	26824	PASS
75	95	30	60	47.9	79277	PASS
95	95	100	100	100.0	165482	PASS
96	95	5	9	6.6	10955	PASS
173	174	0.00	2	0.6	1054	PASS
174	95	50	100	98.5	163029	PASS
175	174	5	9	6.8	11128	PASS
176	174	95	101	95.1	155029	PASS
177	176	5	9	6.2	9640	PASS