


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN031320\
 Data File : VN060487.D
 Acq On : 13 Mar 2020 8:37
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
 Title : SW846 8260
 Last Update : Thu Feb 27 13:52:50 2020

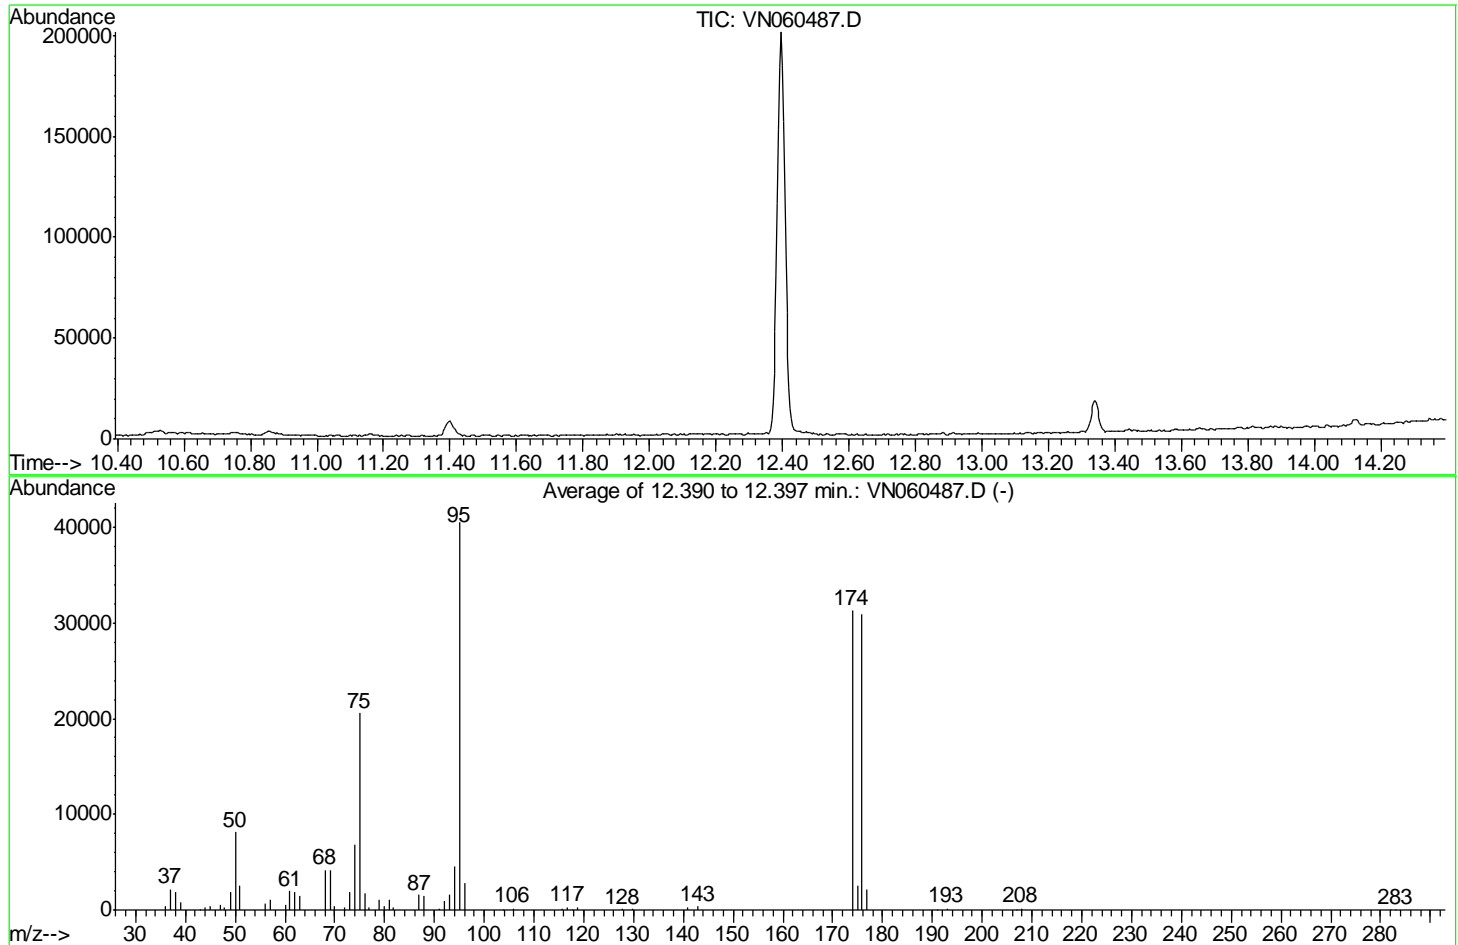

AutoFind: Scans 3302, 3303, 3304; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	8159	PASS
75	95	30	60	50.8	20586	PASS
95	95	100	100	100.0	40517	PASS
96	95	5	9	6.8	2761	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	77.1	31245	PASS
175	174	5	9	8.3	2601	PASS
176	174	95	101	98.8	30869	PASS
177	176	5	9	7.1	2177	PASS