

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031323\
 Data File : VN076957.D
 Acq On : 13 Mar 2023 13:19
 Operator : JC\MD
 Sample : 01854-02DL 4X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 33907DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031023W.M
 Title : SW846 8260

Signal : TIC: VN076957.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.678	118	126	133	rBV2	15223	28265	1.29%	0.074%
2	3.801	308	317	338	rBV	162088	445164	20.27%	1.172%
3	4.448	418	427	438	rBV	12379	39253	1.79%	0.103%
4	5.813	649	659	667	rBV5	14628	47881	2.18%	0.126%
5	7.436	925	935	941	rBV	12258	29454	1.34%	0.078%
6	8.172	1049	1060	1065	rBV	302998	727760	33.14%	1.916%
7	8.230	1065	1070	1083	rVB	599114	1356806	61.79%	3.572%
8	8.583	1119	1130	1147	rBV2	339917	930349	42.37%	2.449%
9	9.107	1210	1219	1235	rBV	806061	1665129	75.83%	4.383%
10	10.571	1459	1468	1473	rBV	1156900	2148806	97.86%	5.657%
11	10.630	1473	1478	1488	rVB	637238	1207082	54.97%	3.178%
12	11.871	1680	1689	1698	rBV	1010606	1852229	84.35%	4.876%
13	11.965	1698	1705	1713	rVV	153745	259602	11.82%	0.683%
14	12.071	1715	1723	1734	rVV	649824	1231335	56.08%	3.241%
15	12.401	1767	1779	1788	rBV	598856	1029319	46.88%	2.710%
16	12.671	1819	1825	1827	rBV	55406	89439	4.07%	0.235%
17	12.854	1849	1856	1867	rVB	844488	1454419	66.23%	3.829%
18	13.036	1880	1887	1892	rBV	141561	238430	10.86%	0.628%
19	13.101	1892	1898	1901	rBV	642730	1035139	47.14%	2.725%
20	13.130	1901	1903	1907	rVV	179880	225174	10.25%	0.593%
21	13.171	1907	1910	1917	rVB	383415	639911	29.14%	1.685%
22	13.336	1929	1938	1945	rBV	373406	650368	29.62%	1.712%
23	13.395	1945	1948	1957	rBV10	15567	37546	1.71%	0.099%
24	13.483	1957	1963	1974	rVB	1365146	2195861	100.00%	5.780%
25	13.618	1976	1986	1991	rBV2	56894	116373	5.30%	0.306%
26	13.677	1991	1996	2001	rBV	118531	194040	8.84%	0.511%
27	13.730	2001	2005	2010	rBV3	48237	77473	3.53%	0.204%
28	13.795	2010	2016	2019	rBV	1017130	1841019	83.84%	4.846%
29	13.877	2027	2030	2035	rVB4	45260	72741	3.31%	0.191%
30	13.954	2037	2043	2044	rBV	126585	161821	7.37%	0.426%
31	13.995	2044	2050	2053	rBV3	432720	843956	38.43%	2.222%
32	14.112	2065	2070	2076	rBV3	158184	279438	12.73%	0.736%
33	14.183	2077	2082	2087	rVV	169353	267548	12.18%	0.704%
34	14.248	2087	2093	2095	rVV	259705	405571	18.47%	1.068%
35	14.277	2095	2098	2103	rVV	251750	385443	17.55%	1.015%
36	14.336	2103	2108	2113	rVB	391556	608443	27.71%	1.602%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031323\
 Data File : VN076957.D
 Acq On : 13 Mar 2023 13:19
 Operator : JC\MD
 Sample : 01854-02DL 4X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 33907DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031023W.M
 Title : SW846 8260

37	14.401	2114	2119	2121	rBV	82259	113010	5.15%	0.297%
38	14.448	2121	2127	2132	rVB3	306457	538847	24.54%	1.418%
39	14.518	2137	2139	2143	rVB2	23762	28947	1.32%	0.076%
40	14.577	2143	2149	2154	rBV	167554	273879	12.47%	0.721%
41	14.659	2154	2163	2166	rBV	268096	529979	24.14%	1.395%
42	14.695	2166	2169	2173	rVB	368584	483743	22.03%	1.273%
43	14.736	2173	2176	2180	rVB2	121004	151050	6.88%	0.398%
44	14.777	2180	2183	2191	rVB2	75086	155888	7.10%	0.410%
45	14.877	2191	2200	2204	rBV3	105406	232364	10.58%	0.612%
46	14.930	2204	2209	2213	rBV2	392176	746029	33.97%	1.964%
47	15.054	2221	2230	2237	rBV3	777284	1928798	87.84%	5.077%
48	15.212	2250	2257	2264	rBV	607962	1107314	50.43%	2.915%
49	15.324	2264	2276	2280	rBV3	253965	660666	30.09%	1.739%
50	15.442	2288	2296	2304	rVB4	246352	653018	29.74%	1.719%
51	15.518	2304	2309	2316	rVB10	34223	82502	3.76%	0.217%
52	15.595	2316	2322	2325	rBV6	82938	163875	7.46%	0.431%
53	15.642	2325	2330	2335	rVV	220687	430343	19.60%	1.133%
54	15.701	2335	2340	2345	rVV2	184093	361311	16.45%	0.951%
55	15.753	2345	2349	2351	rVV3	120565	213464	9.72%	0.562%
56	15.783	2351	2354	2358	rVV3	145583	322738	14.70%	0.850%
57	15.836	2360	2363	2373	rVB2	206508	379931	17.30%	1.000%
58	15.948	2373	2382	2389	rBV	222788	493803	22.49%	1.300%
59	16.024	2392	2395	2400	rVB6	19429	29102	1.33%	0.077%
60	16.136	2405	2414	2415	rBV4	136418	284336	12.95%	0.748%
61	16.171	2415	2420	2431	rVB	498808	1022042	46.54%	2.690%
62	16.259	2431	2435	2440	rBV3	49307	87903	4.00%	0.231%
63	16.348	2441	2450	2458	rBV3	107179	278140	12.67%	0.732%
64	16.506	2466	2477	2490	rVB3	288076	779012	35.48%	2.051%
65	16.618	2491	2496	2501	rVB3	34183	58476	2.66%	0.154%
66	16.712	2504	2512	2518	rBV2	169133	374697	17.06%	0.986%
67	16.783	2518	2524	2525	rBV2	154384	204249	9.30%	0.538%


Sum of corrected areas: 37988043

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031323\
Data File : VN076957.D
Acq On : 13 Mar 2023 13:19
Operator : JC\MD
Sample : 01854-02DL 4X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
33907DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031023W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

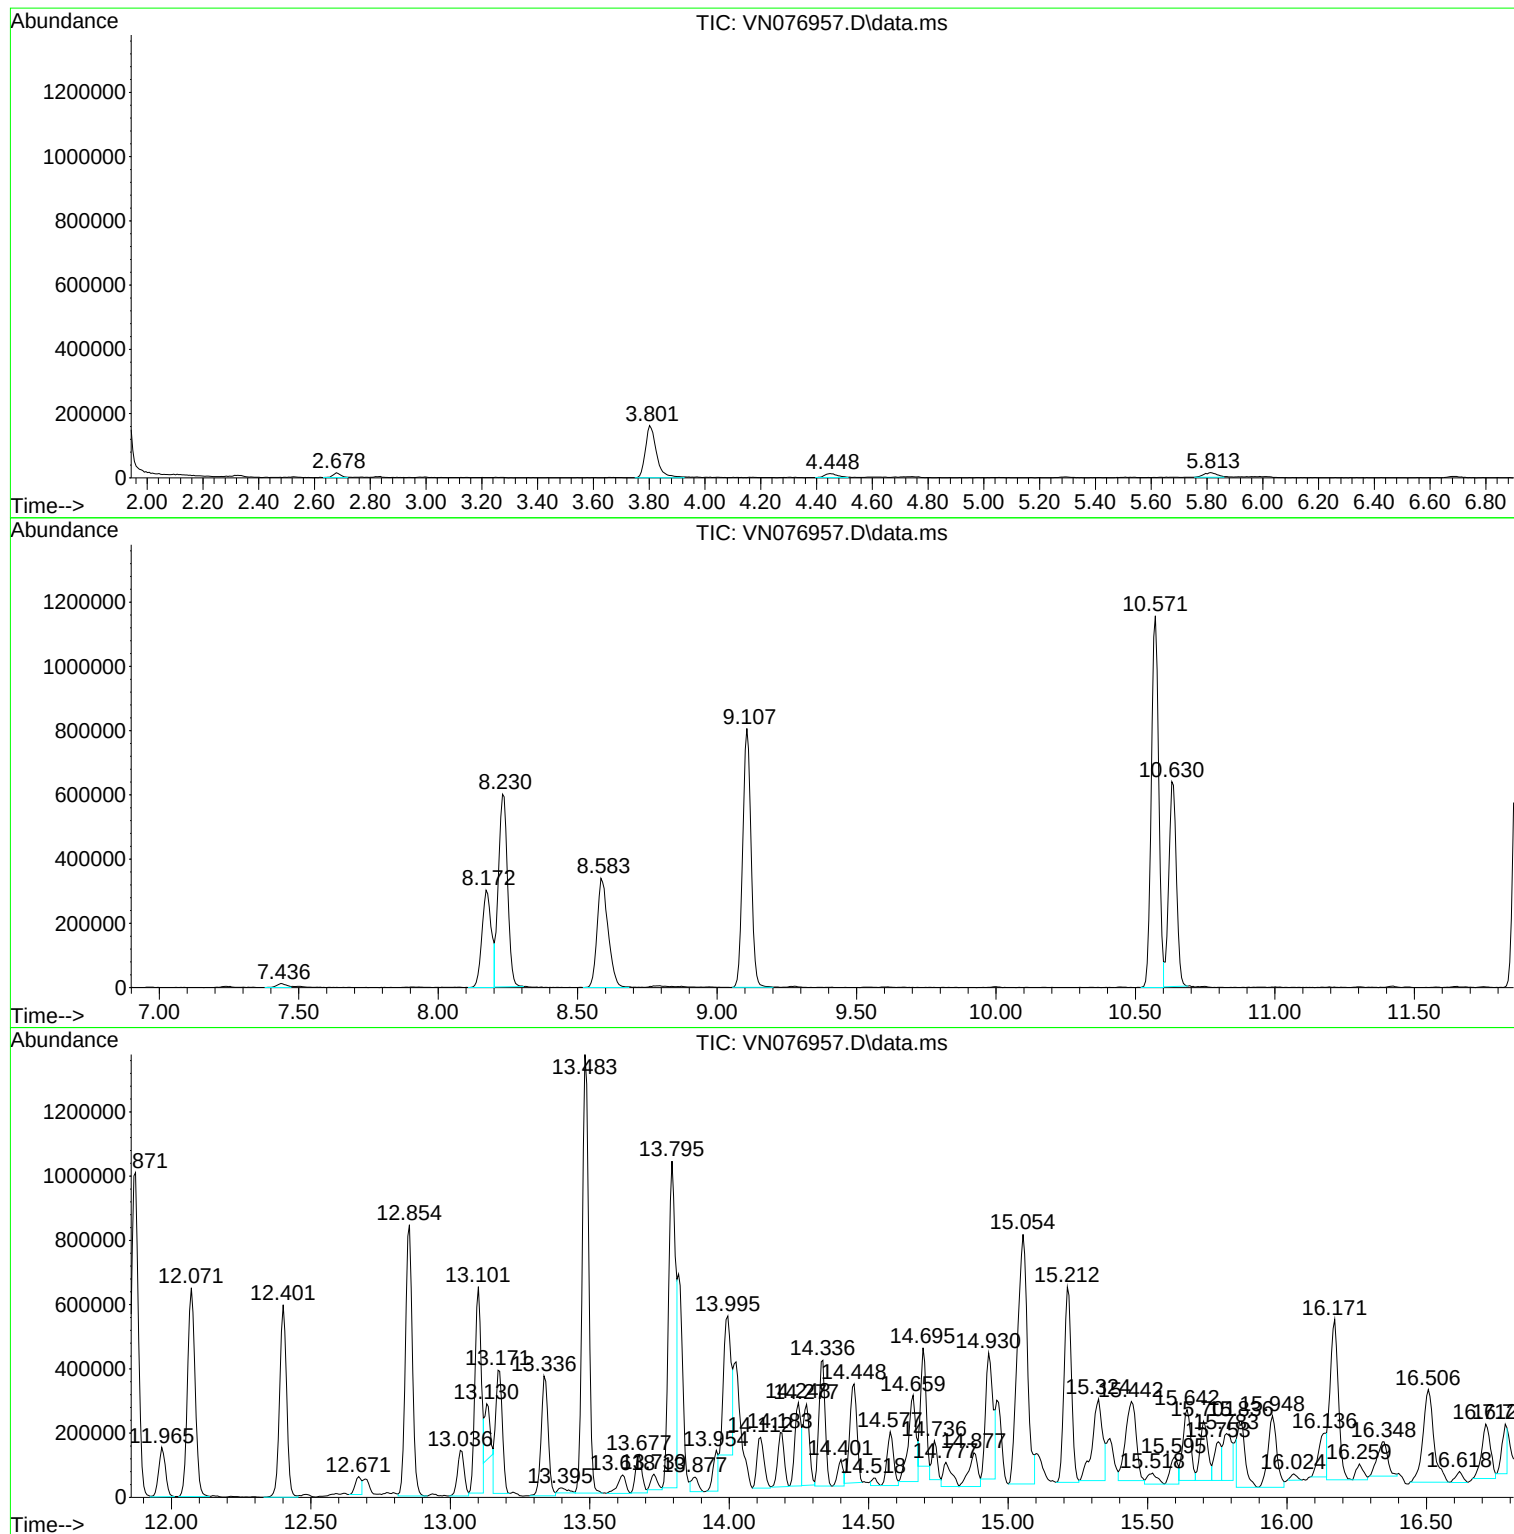

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031323\
Data File : VN076957.D
Acq On : 13 Mar 2023 13:19
Operator : JC\MD
Sample : 01854-02DL 4X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
33907DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031023W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031323\
Data File : VN076957.D
Acq On : 13 Mar 2023 13:19
Operator : JC\MD
Sample : 01854-02DL 4X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
33907DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031023W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc