
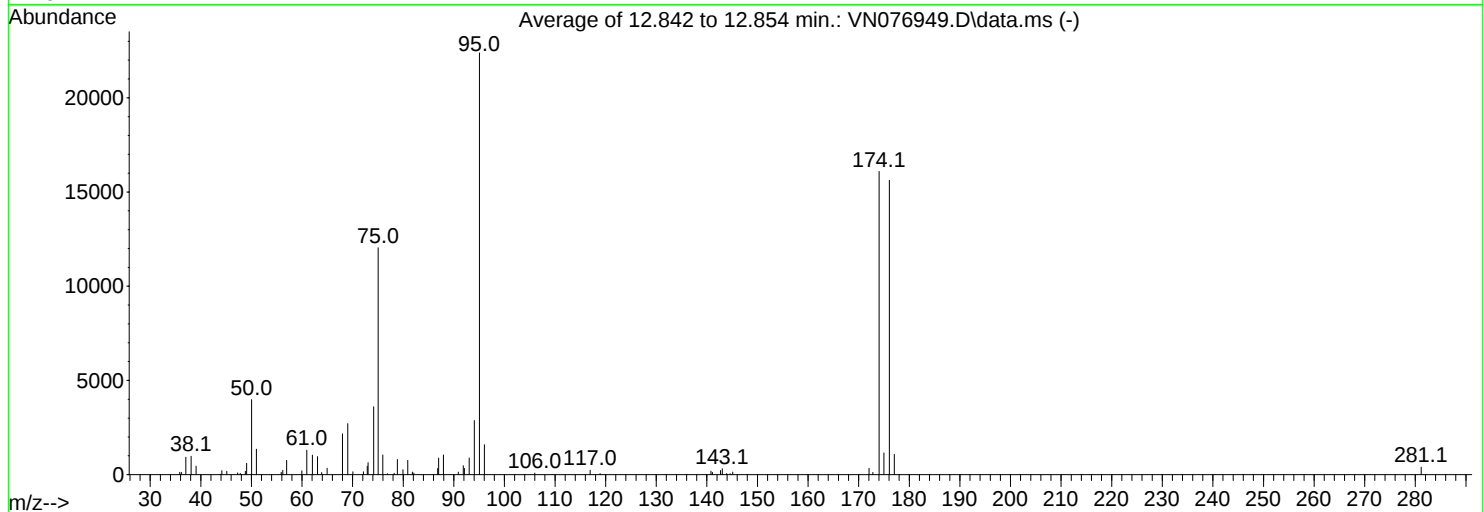


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031323\
Data File : VN076949.D
Acq On : 13 Mar 2023 09:37
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031023W.M
Title : SW846 8260
Last Update : Fri Mar 10 13:47:39 2023

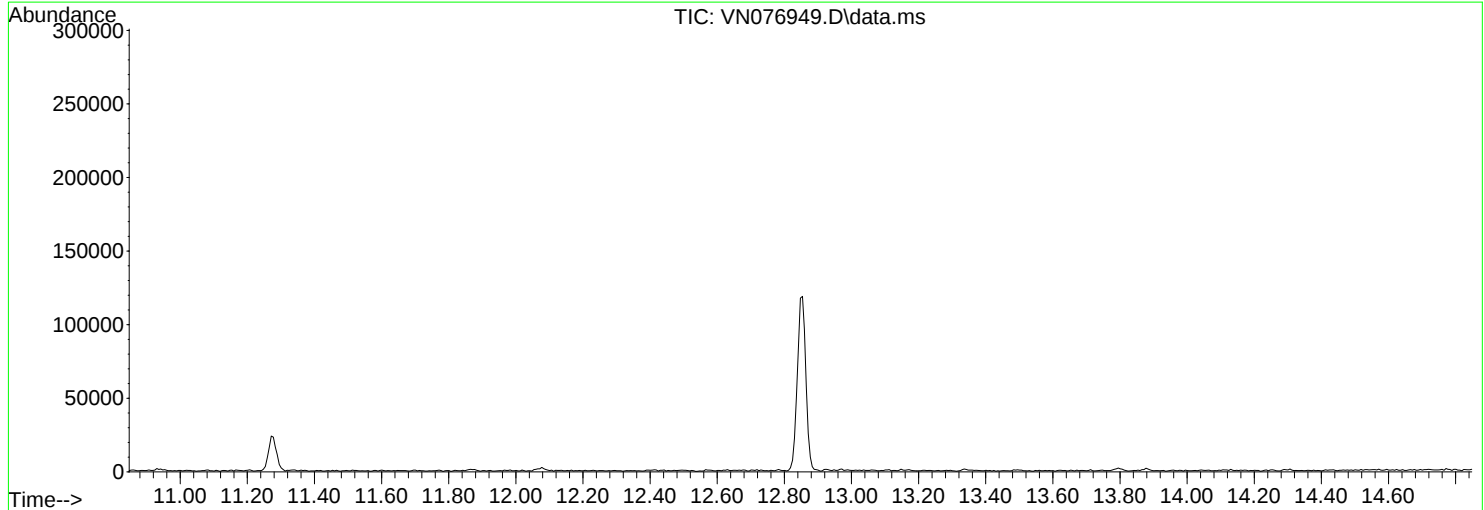

AutoFind: Scans 1854, 1855, 1856; Background Corrected with Scan 1847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	3984	PASS
75	95	30	60	53.8	12039	PASS
95	95	100	100	100.0	22387	PASS
96	95	5	9	7.1	1589	PASS
173	174	0.00	2	0.7	117	PASS
174	95	50	100	71.9	16090	PASS
175	174	5	9	7.2	1159	PASS
176	174	95	101	97.1	15624	PASS
177	176	5	9	6.9	1081	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	129	49.05	601	64.95	338	78.20	79
36.15	122	50.05	3984	68.00	2162	78.85	80
37.05	930	51.00	1354	69.05	2711	79.95	26
38.10	981	55.90	126	70.05	151	80.90	75
39.05	453	56.20	228	72.15	155	81.80	136
43.90	20	56.95	753	72.90	451	82.10	86
44.15	210	59.95	201	73.05	633	86.80	322
45.15	175	60.95	1297	74.15	3602	87.00	887
47.30	97	62.05	1033	75.05	12039	87.95	1042
47.80	68	63.05	957	75.95	1041	90.90	136
48.80	177	63.90	109	76.90	52	91.85	473

Average of 12.842 to 12.854 min.: VN076949.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.10	328	143.05	316				
93.05	882	143.90	59				
94.05	2868	144.60	51				
95.05	22387	145.10	134				
96.05	1589	172.05	336				
106.00	82	172.80	117				
116.95	241	174.05	16090				
118.90	58	175.00	1159				
140.80	190	176.05	15624				
141.10	116	177.05	1081				
142.70	222	281.15	400				

Instrument :

MSVOA_N

ClientSampleId :

BFB