

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031324\
 Data File : VN081396.D
 Acq On : 13 Mar 2024 16:29
 Operator : JC\MD
 Sample : P1734-08 10X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 1343

Quant Time: Mar 14 01:08:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030524W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 06 03:12:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	302371	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	586592	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	514462	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	225296	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	224837	51.427	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 102.860%			
35) Dibromofluoromethane	8.165	113	171998	47.859	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 95.720%			
50) Toluene-d8	10.565	98	643292	47.883	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 95.760%			
62) 4-Bromofluorobenzene	12.853	95	213669	44.999	ug/l	0.00
Spiked Amount 50.000	Range 64 - 133		Recovery = 90.000%			
Target Compounds						Qvalue
11) Tert butyl alcohol	5.506	59	776	1.015	ug/l #	72
13) Acrolein	4.165	56	612	0.676	ug/l	84
16) Acetone	4.430	43	8973	5.793	ug/l	89
18) Methyl Acetate	5.018	43	2994	0.675	ug/l #	76
20) Methylene Chloride	5.259	84	2404	Below Cal	#	61
25) 2-Butanone	7.494	43	2423	0.934	ug/l #	51
31) Cyclohexane	8.218	56	10405	1.572	ug/l #	1
36) 1,1-Dichloropropene	8.230	75	28856	4.977	ug/l #	50
38) Carbon Tetrachloride	8.224	117	34777	5.960	ug/l #	19
39) Methylcyclohexane	9.606	83	9487	1.422	ug/l #	81
43) Isopropyl Acetate	8.653	43	138283	13.940	ug/l #	57
49) 1,4-Dioxane	9.694	88	54	0.559	ug/l #	1
51) 4-Methyl-2-Pentanone	10.447	43	1480	0.257	ug/l	98
52) Toluene	10.630	92	10398	0.995	ug/l	99
55) 1,1,2-Trichloroethane	11.012	97	1775	0.428	ug/l #	13
59) 2-Hexanone	11.194	43	2239	0.520	ug/l	82
67) Ethyl Benzene	12.071	91	89371	4.576	ug/l #	62
68) m/p-Xylenes	12.071	106	44917	6.112	ug/l	92
69) o-Xylene	12.400	106	24827	3.486	ug/l	97
74) N-amyl acetate	12.459	43	1576	0.206	ug/l #	52
76) 1,2,3-Trichloropropane	12.853	75	119284	22.416	ug/l #	1
78) n-propylbenzene	13.100	91	8730	0.406	ug/l #	1
79) 2-Chlorotoluene	13.100	91	8730	0.664	ug/l #	45
80) 1,3,5-Trimethylbenzene	13.176	105	38238	2.543	ug/l	95
81) trans-1,4-Dichloro-2-b...	12.853	75	119284	62.558	ug/l #	14
82) 4-Chlorotoluene	13.182	91	5138	0.395	ug/l #	44
83) tert-Butylbenzene	13.488	119	12232	0.949	ug/l #	78
84) 1,2,4-Trimethylbenzene	13.482	105	96769	6.351	ug/l	93
85) sec-Butylbenzene	13.482	105	96769	5.188	ug/l #	60
86) p-Isopropyltoluene	13.676	119	3765	0.252	ug/l	87
90) Hexachloroethane	14.329	117	3019	1.153	ug/l #	21


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031324\
Data File : VN081396.D
Acq On : 13 Mar 2024 16:29
Operator : JC\MD
Sample : P1734-08 10X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
1343

Quant Time: Mar 14 01:08:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030524W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 06 03:12:57 2024
Response via : Initial Calibration




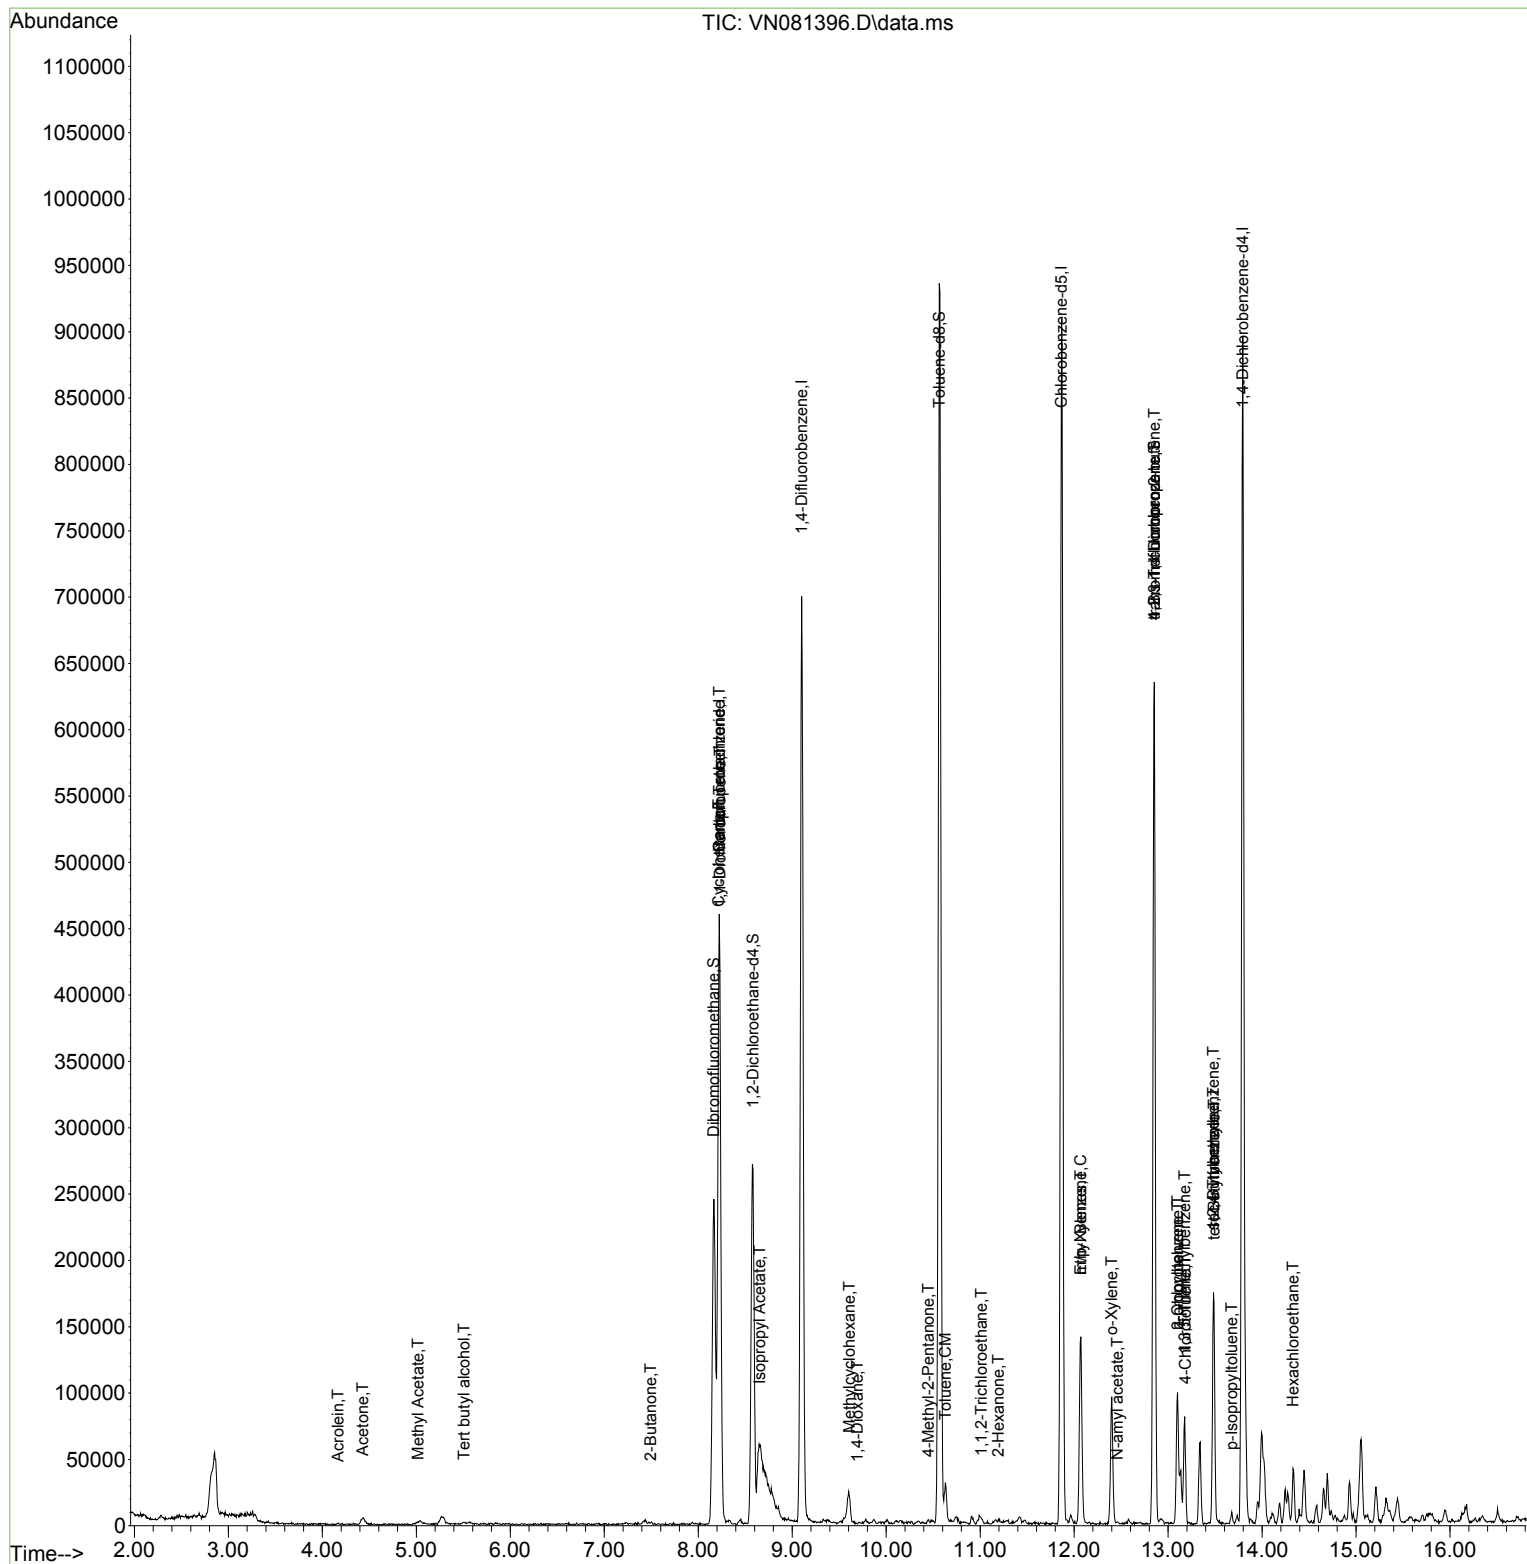




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29




Instrument :
MSVOA_N
ClientSampleId :
1343


Tgt Ion:168 Resp: 302371
Ion Ratio Lower Upper
168 100
99 68.3 59.9 89.9

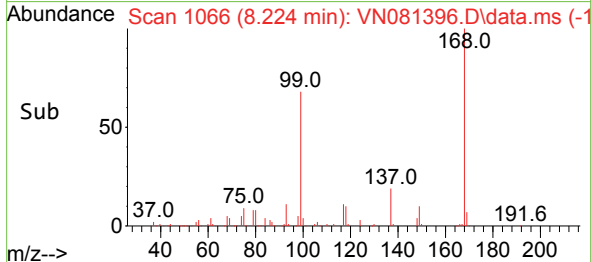

#11
Tert butyl alcohol
Concen: 1.015 ug/l
RT: 5.506 min Scan# 604
Delta R.T. -0.006 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29

Tgt Ion: 59 Resp: 776
Ion Ratio Lower Upper
59 100
57 0.0 8.6 12.8#

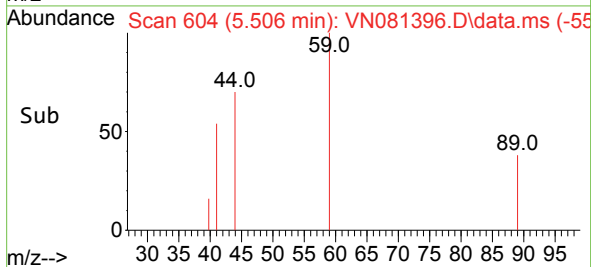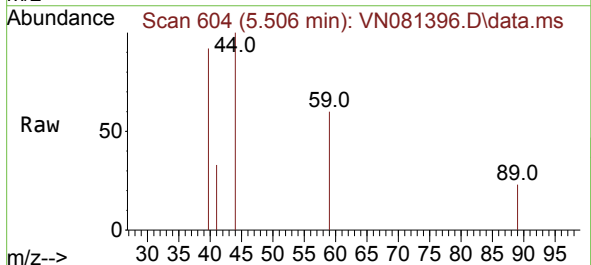



#13

Acrolein

Concen: 0.676 ug/l

RT: 4.165 min Scan# 31

Delta R.T. -0.012 min

Lab File: VN081396.D

Acq: 13 Mar 2024 16:29

Instrument :

MSVOA_N

ClientSampleId :





1343

Tgt Ion: 56 Resp: 612

Ion Ratio Lower Upper

56 100

55 82.2 55.3 82.9

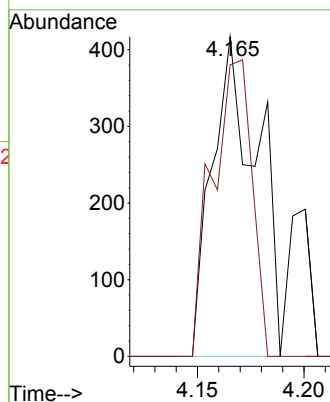

#16

Acetone

Concen: 5.793 ug/l

RT: 4.430 min Scan# 421

Delta R.T. 0.006 min

Lab File: VN081396.D




Acq: 13 Mar 2024 16:29


Tgt Ion: 43 Resp: 8973

Ion Ratio Lower Upper

43 100

58 37.2 24.8 37.2

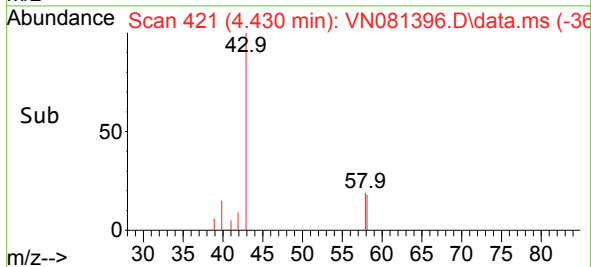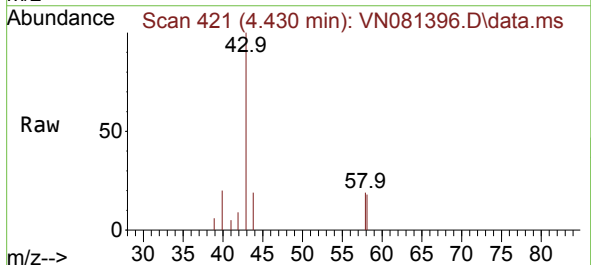



#18

Methyl Acetate

Concen: 0.675 ug/l

RT: 5.018 min Scan# 51

Delta R.T. 0.000 min

Lab File: VN081396.D

Acq: 13 Mar 2024 16:29

Instrument :

MSVOA_N

ClientSampleId :





1343

Tgt Ion: 43 Resp: 2994

Ion Ratio Lower Upper

43 100

74 10.3 17.3 25.9#

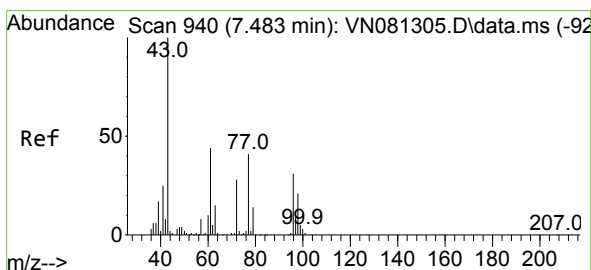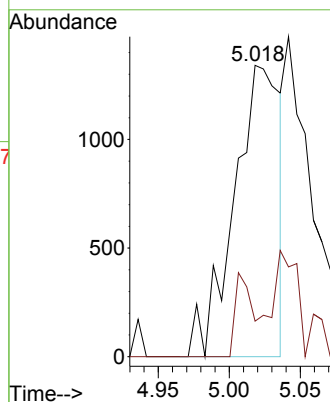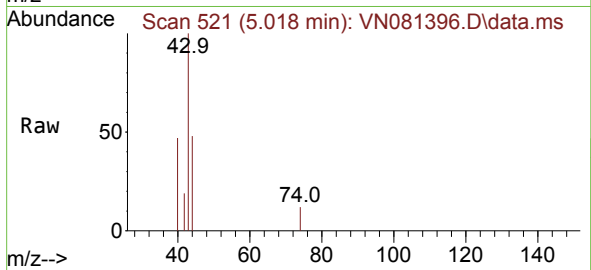

#25

2-Butanone

Concen: 0.934 ug/l

RT: 7.494 min Scan# 942

Delta R.T. 0.012 min

Lab File: VN081396.D




Acq: 13 Mar 2024 16:29


Tgt Ion: 43 Resp: 2423

Ion Ratio Lower Upper

43 100

72 0.0 19.5 29.3#




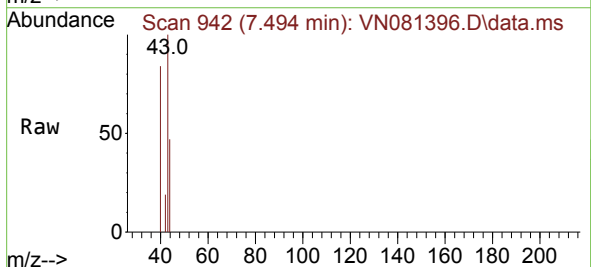




#31
Cyclohexane
Concen: 1.572 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.041 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29




Instrument :
MSVOA_N
ClientSampleId :
1343


Tgt Ion: 56 Resp: 10405
Ion Ratio Lower Upper
56 100
69 156.0 20.1 30.1#
84 106.7 56.9 85.3#

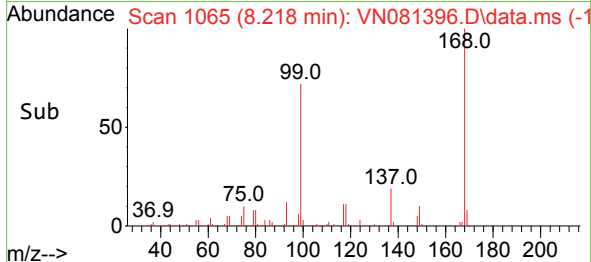

#33
1,2-Dichloroethane-d4
Concen: 51.427 ug/l
RT: 8.583 min Scan# 1127
Delta R.T. 0.006 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29

Tgt Ion: 65 Resp: 224837
Ion Ratio Lower Upper
65 100
67 51.6 0.0 102.4

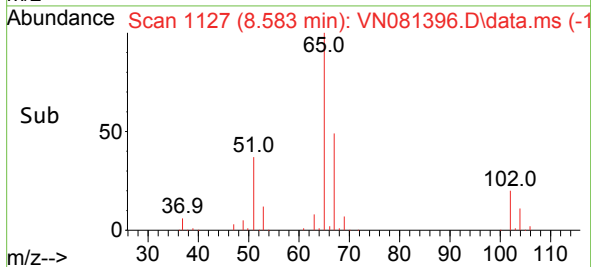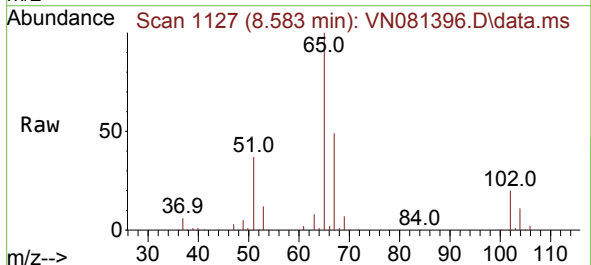



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 114

Delta R.T. -0.006 min

Lab File: VN081396.D

Acq: 13 Mar 2024 16:29

Instrument :

MSVOA_N

ClientSampleId :

1343





Tgt Ion:114 Resp: 586592

Ion Ratio Lower Upper

114 100

63 21.4 0.0 48.0

88 15.0 0.0 34.8



#35

Dibromofluoromethane

Concen: 47.859 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.000 min

Lab File: VN081396.D

Acq: 13 Mar 2024 16:29




Tgt Ion:113 Resp: 171998


Ion Ratio Lower Upper

113 100

111 103.6 82.2 123.4

192 16.0 12.5 18.7


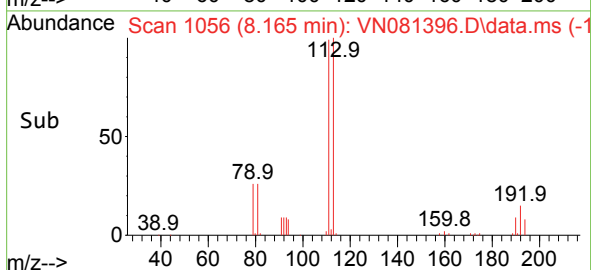






#36
1,1-Dichloropropene
Concen: 4.977 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.147 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29




Instrument :
MSVOA_N
ClientSampleId :
1343


Tgt Ion: 75 Resp: 28856
Ion Ratio Lower Upper
75 100
110 8.2 16.0 48.0#
77 0.0 25.8 38.6#

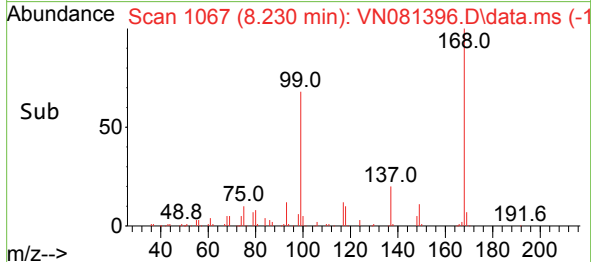

#38
Carbon Tetrachloride
Concen: 5.960 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.141 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29

Tgt Ion: 117 Resp: 34777
Ion Ratio Lower Upper
117 100
119 7.2 73.4 110.2#
121 0.0 24.4 36.6#


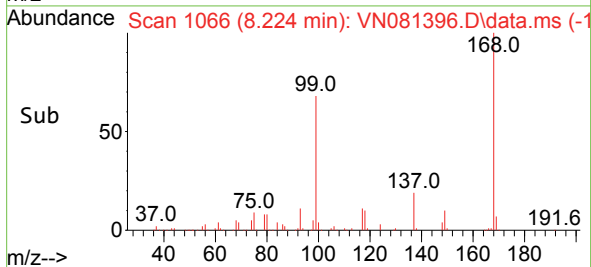

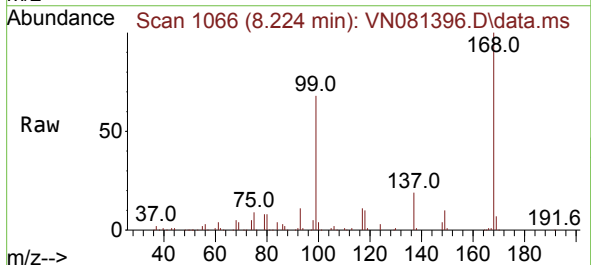




#39
Methylcyclohexane
Concen: 1.422 ug/l
RT: 9.606 min Scan# 1139
Delta R.T. 0.006 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29




Instrument :
MSVOA_N
ClientSampleId :
1343


Tgt Ion: 83 Resp: 9487
Ion Ratio Lower Upper
83 100
55 57.6 65.7 98.5#
98 44.1 33.8 50.6

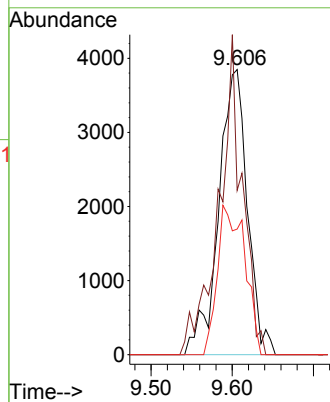

#43
Isopropyl Acetate
Concen: 13.940 ug/l
RT: 8.653 min Scan# 1139
Delta R.T. -0.035 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29

Tgt Ion: 43 Resp: 138283
Ion Ratio Lower Upper
43 100
61 0.6 19.9 29.9#
87 0.0 9.0 13.6#

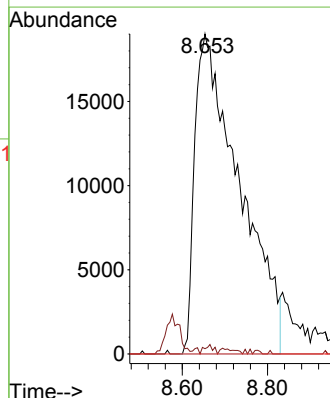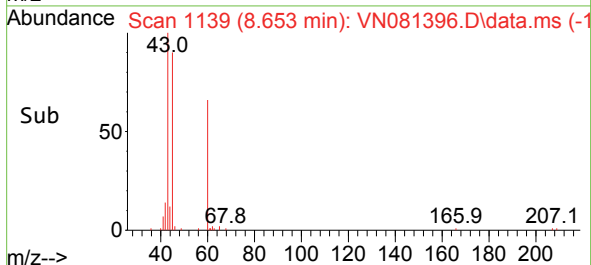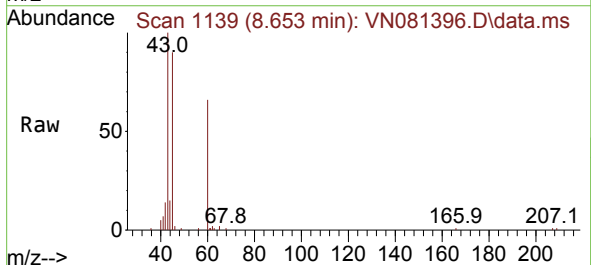



#49

1,4-Dioxane

Concen: 0.559 ug/l

RT: 9.694 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN081396.D

Acq: 13 Mar 2024 16:29

Instrument :

MSVOA_N

ClientSampleId :

1343





Tgt Ion: 88 Resp: 54

Ion Ratio Lower Upper

88 100

43 674.1 30.1 45.1#

58 0.0 63.9 95.9#

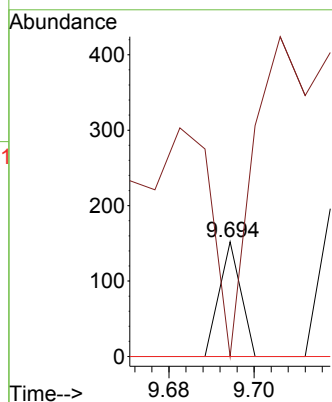

#50

Toluene-d8

Concen: 47.883 ug/l

RT: 10.565 min Scan# 1464

Delta R.T. -0.006 min

Lab File: VN081396.D




Acq: 13 Mar 2024 16:29


Tgt Ion: 98 Resp: 643292

Ion Ratio Lower Upper

98 100

100 64.9 51.4 77.0


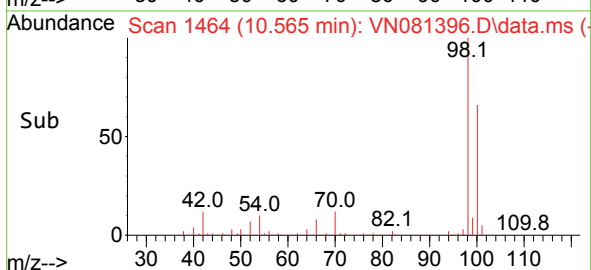






#51
4-Methyl-2-Pentanone
Concen: 0.257 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29




Instrument :
MSVOA_N
ClientSampleId :
1343


Tgt Ion: 43 Resp: 1480
Ion Ratio Lower Upper
43 100
58 35.5 29.4 44.0

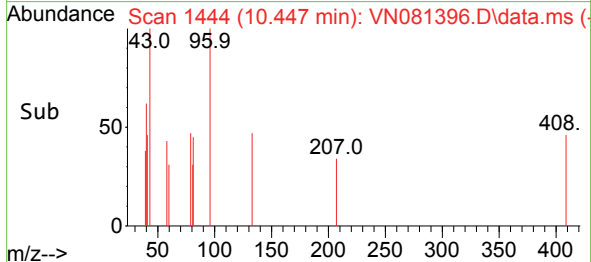

#52
Toluene
Concen: 0.995 ug/l
RT: 10.630 min Scan# 1475
Delta R.T. -0.006 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29


Tgt Ion: 92 Resp: 10398
Ion Ratio Lower Upper
92 100
91 175.6 139.4 209.0

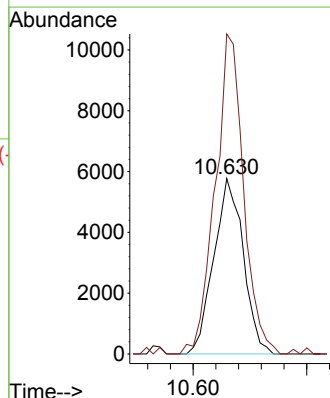






#55
1,1,2-Trichloroethane
Concen: 0.428 ug/l
RT: 11.012 min Scan# 1143
Delta R.T. -0.006 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29

Instrument :
MSVOA_N
ClientSampleId :
1343







Tgt Ion	Resp		
97	1775		
Ion	Ratio	Lower	Upper
97	100		
83	0.0	72.9	109.3#
85	0.0	50.2	75.2#
99	0.0	49.6	74.4#

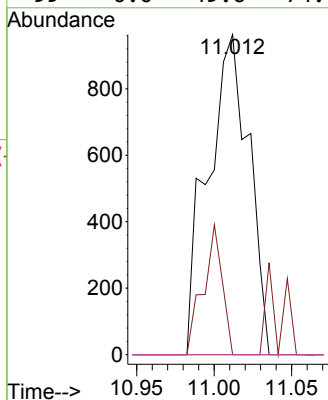

#59
2-Hexanone
Concen: 0.520 ug/l
RT: 11.194 min Scan# 1571
Delta R.T. 0.000 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29

Tgt Ion	Resp		
43	2239		
Ion	Ratio	Lower	Upper
43	100		
58	39.3	25.9	77.8


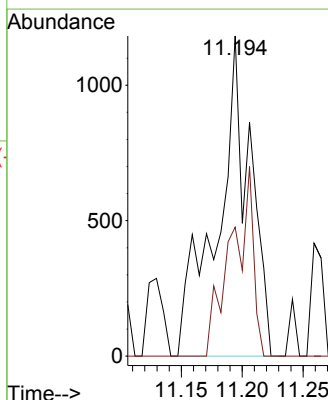
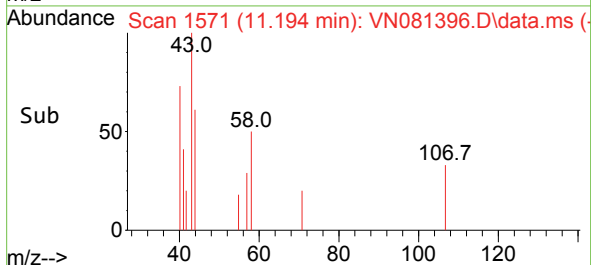
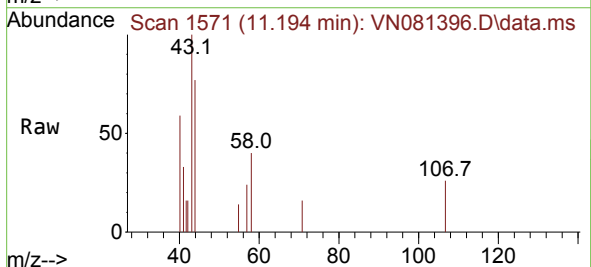




#62
4-Bromofluorobenzene
Concen: 44.999 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29




Instrument :
MSVOA_N
ClientSampleId :
1343


Tgt Ion: 95 Resp: 213669
Ion Ratio Lower Upper
95 100
174 69.9 0.0 120.4
176 67.2 0.0 121.0



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. -0.006 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29

Tgt Ion: 117 Resp: 514462
Ion Ratio Lower Upper
117 100
82 56.4 52.7 79.1
119 31.0 25.3 37.9


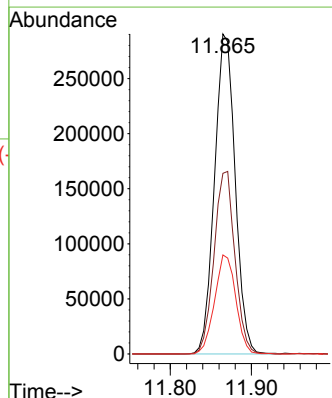




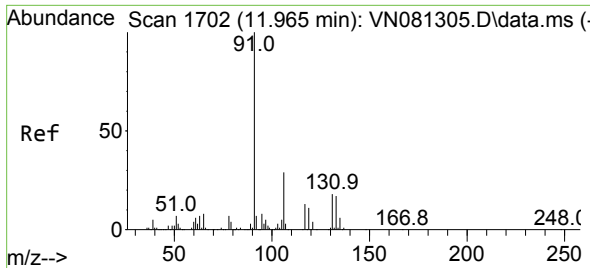

#67
Ethyl Benzene
Concen: 4.576 ug/l
RT: 12.071 min Scan# 1720
Delta R.T. 0.106 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29




Instrument :
MSVOA_N
ClientSampleId :
1343


Tgt Ion: 91 Resp: 89371
Ion Ratio Lower Upper
91 100
106 50.4 23.8 35.6#

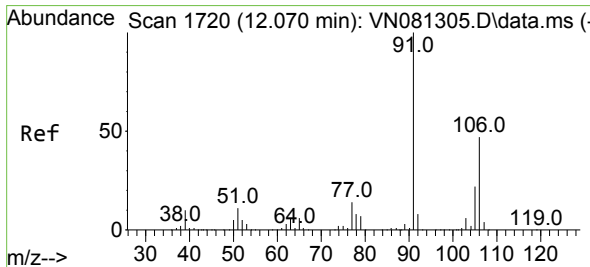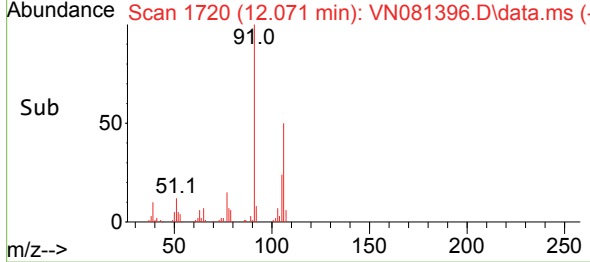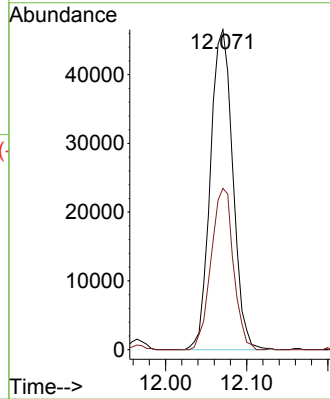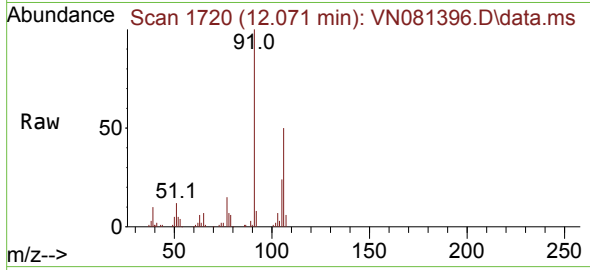

#68
m/p-Xylenes
Concen: 6.112 ug/l
RT: 12.071 min Scan# 1720
Delta R.T. 0.000 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29

Tgt Ion: 106 Resp: 44917
Ion Ratio Lower Upper
106 100
91 199.0 169.0 253.6


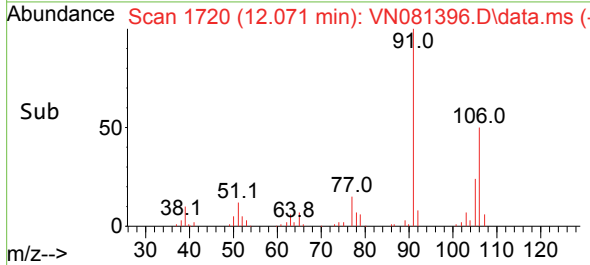

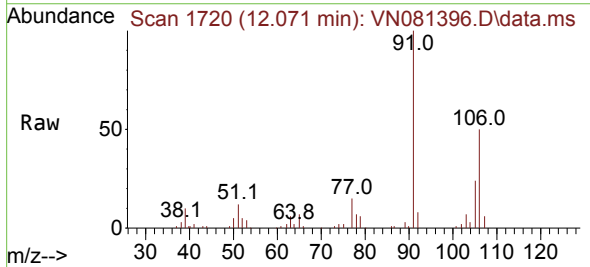




#69
o-Xylene
Concen: 3.486 ug/l
RT: 12.400 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29




Instrument :
MSVOA_N
ClientSampleId :
1343


Tgt Ion:106 Resp: 24827
Ion Ratio Lower Upper
106 100
91 219.0 112.1 336.3



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29

Tgt Ion:152 Resp: 225296
Ion Ratio Lower Upper
152 100
115 65.1 32.3 96.8
150 154.4 0.0 339.8

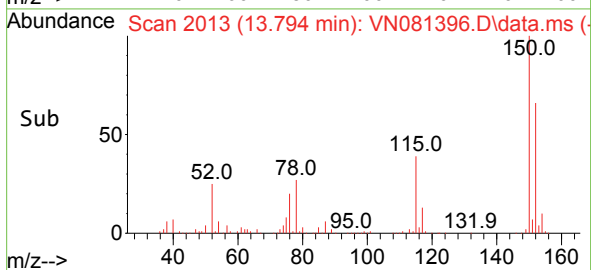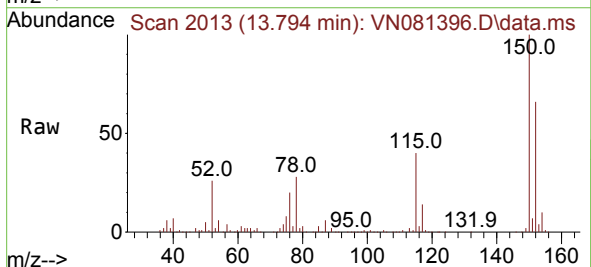



#74

N-amy1 acetate

Concen: 0.206 ug/l

RT: 12.459 min Scan# 1

Delta R.T. -0.035 min

Lab File: VN081396.D

Acq: 13 Mar 2024 16:29

Instrument :

MSVOA_N

ClientSampleId :

1343

Tgt Ion: 43 Resp: 1576





Ion Ratio Lower Upper

43 100

70 3.9 30.1 45.1#

55 5.1 17.0 25.4#

61 0.0 17.5 26.3#

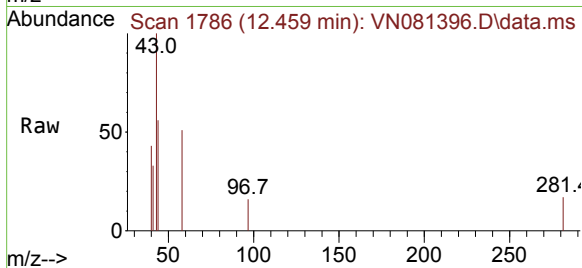

#76

1,2,3-Trichloropropane

Concen: 22.416 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.147 min

Lab File: VN081396.D




Acq: 13 Mar 2024 16:29


Tgt Ion: 75 Resp: 119284

Ion Ratio Lower Upper

75 100

77 1.5 91.0 272.8#

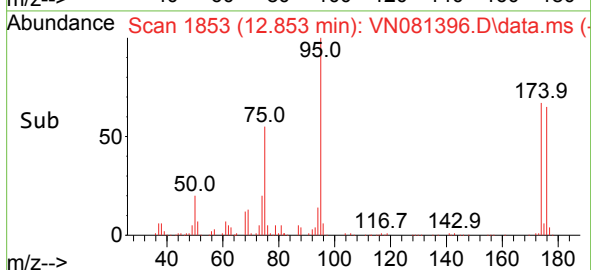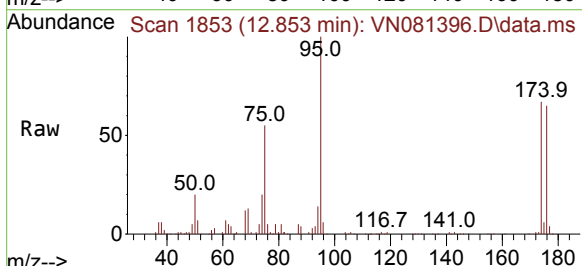

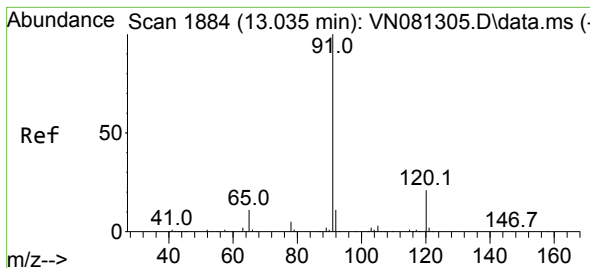

#78

n-propylbenzene

Concen: 0.406 ug/l

RT: 13.100 min Scan# 1895

Delta R.T. 0.065 min

Lab File: VN081396.D

Acq: 13 Mar 2024 16:29

Instrument :

MSVOA_N

ClientSampleId :





1343

Tgt Ion: 91 Resp: 8730

Ion Ratio Lower Upper

91 100

120 280.1 10.3 30.9#

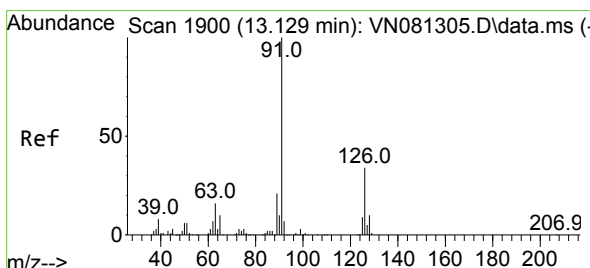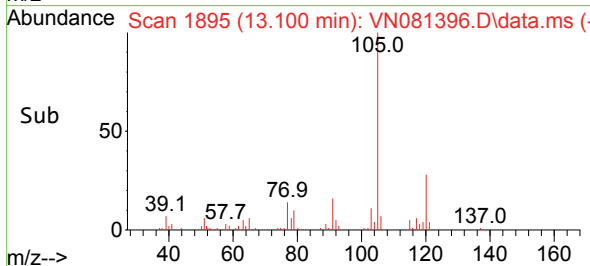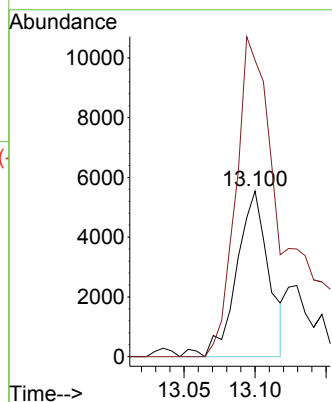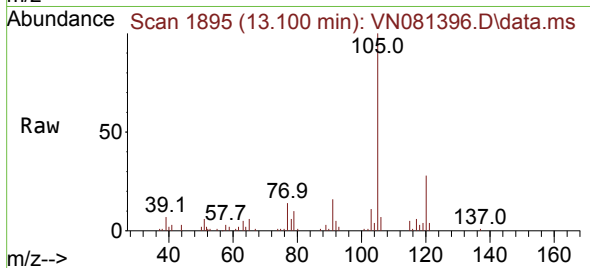

#79

2-Chlorotoluene

Concen: 0.664 ug/l

RT: 13.100 min Scan# 1895

Delta R.T. -0.029 min

Lab File: VN081396.D




Acq: 13 Mar 2024 16:29


Tgt Ion: 91 Resp: 8730

Ion Ratio Lower Upper

91 100

126 0.0 14.8 44.4#


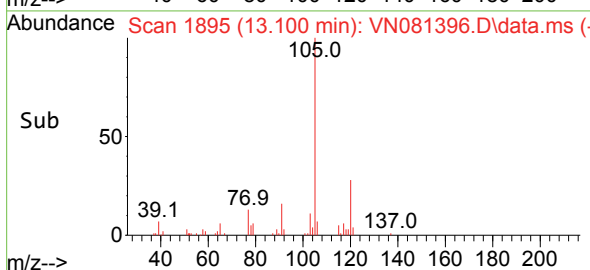

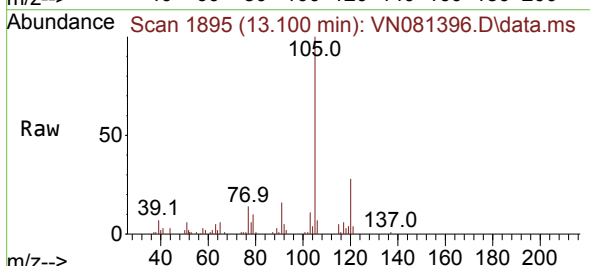




#80
1,3,5-Trimethylbenzene
Concen: 2.543 ug/l
RT: 13.176 min Scan# 1908
Delta R.T. 0.000 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29




Instrument :
MSVOA_N
ClientSampleId :
1343


Tgt Ion:105 Resp: 38238
Ion Ratio Lower Upper
105 100
120 49.6 23.0 69.0



#81
trans-1,4-Dichloro-2-butene
Concen: 62.558 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.112 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29

Tgt Ion: 75 Resp: 119284
Ion Ratio Lower Upper
75 100
53 0.2 71.4 107.2#
89 0.0 33.4 50.0#


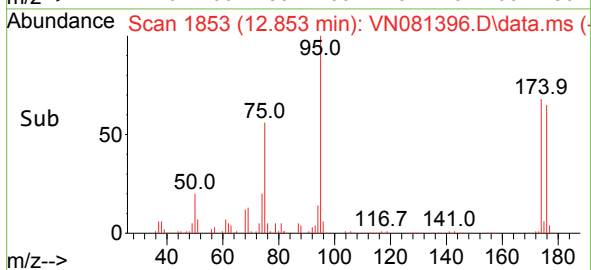

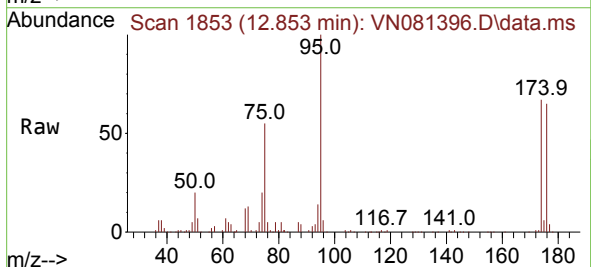


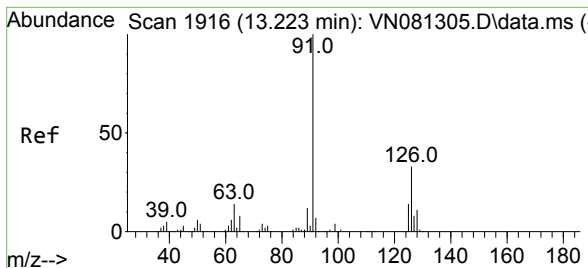

#82
4-Chlorotoluene
Concen: 0.395 ug/l
RT: 13.182 min Scan# 1909
Delta R.T. -0.041 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29




Instrument :
MSVOA_N
ClientSampleId :
1343


Tgt Ion: 91 Resp: 5138
Ion Ratio Lower Upper
91 100
126 0.0 15.3 45.9#

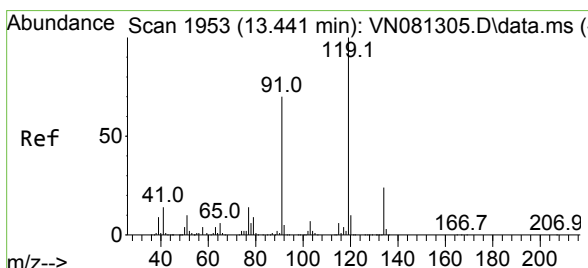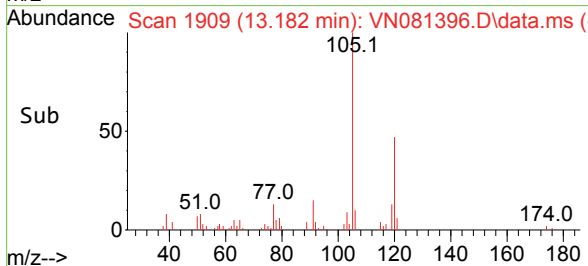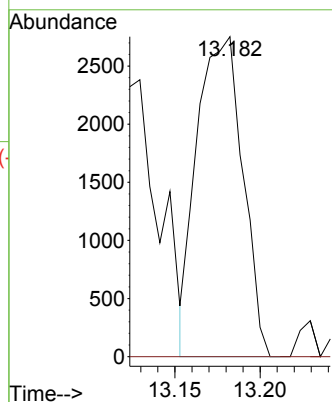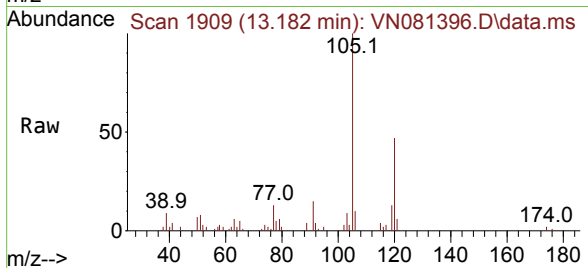

#83
tert-Butylbenzene
Concen: 0.949 ug/l
RT: 13.488 min Scan# 1961
Delta R.T. 0.047 min
Lab File: VN081396.D
Acq: 13 Mar 2024 16:29

Tgt Ion: 119 Resp: 12232
Ion Ratio Lower Upper
119 100
91 84.7 36.8 110.4
134 0.0 12.4 37.4#

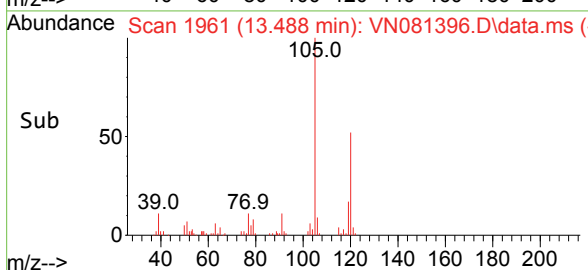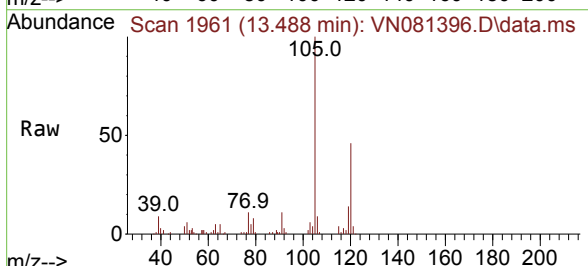



#84

1,2,4-Trimethylbenzene

Concen: 6.351 ug/l

RT: 13.482 min Scan# 1960

Delta R.T. 0.000 min

Lab File: VN081396.D

Acq: 13 Mar 2024 16:29

Instrument :

MSVOA_N

ClientSampleId :





1343

Tgt Ion:105 Resp: 96769

Ion Ratio Lower Upper

105 100

120 46.3 20.9 62.7

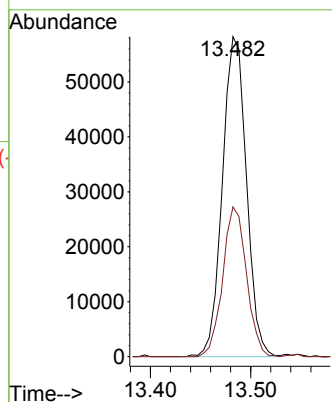

#85

sec-Butylbenzene

Concen: 5.188 ug/l

RT: 13.482 min Scan# 1960

Delta R.T. -0.135 min

Lab File: VN081396.D




Acq: 13 Mar 2024 16:29


Tgt Ion:105 Resp: 96769

Ion Ratio Lower Upper

105 100

134 0.0 8.6 25.8#

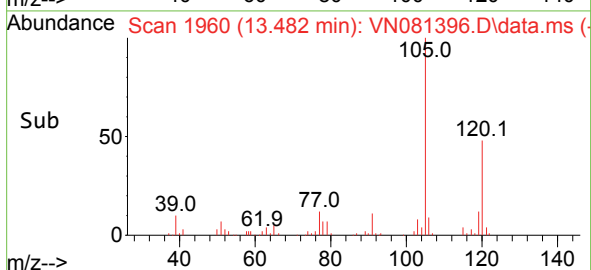

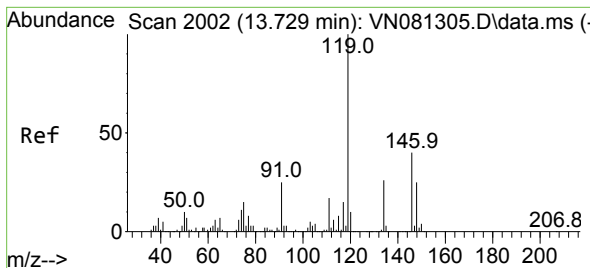

#86

p-Isopropyltoluene

Concen: 0.252 ug/l

RT: 13.676 min Scan# 1993

Delta R.T. -0.053 min

Lab File: VN081396.D

Acq: 13 Mar 2024 16:29

Instrument :

MSVOA_N

ClientSampleId :

1343





Tgt Ion:119 Resp: 3765

Ion Ratio Lower Upper

119 100

134 35.7 12.4 37.2

91 29.3 13.5 40.4

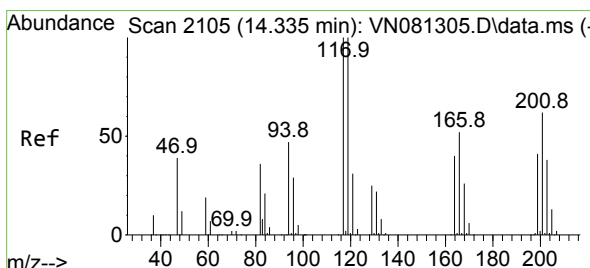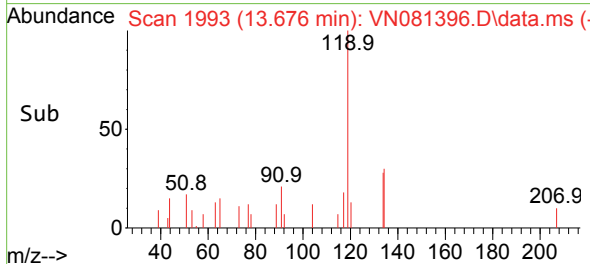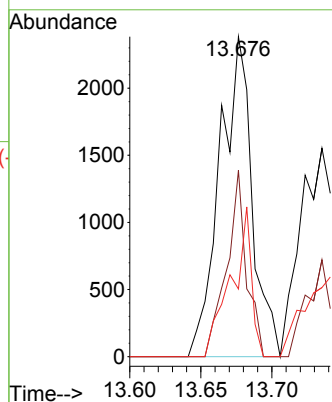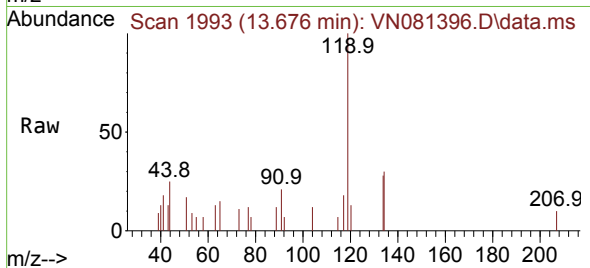

#90

Hexachloroethane

Concen: 1.153 ug/l

RT: 14.329 min Scan# 2104

Delta R.T. -0.006 min

Lab File: VN081396.D

Acq: 13 Mar 2024 16:29

Tgt Ion:117 Resp: 3019

Ion Ratio Lower Upper

117 100

201 0.0 30.0 90.0#

