
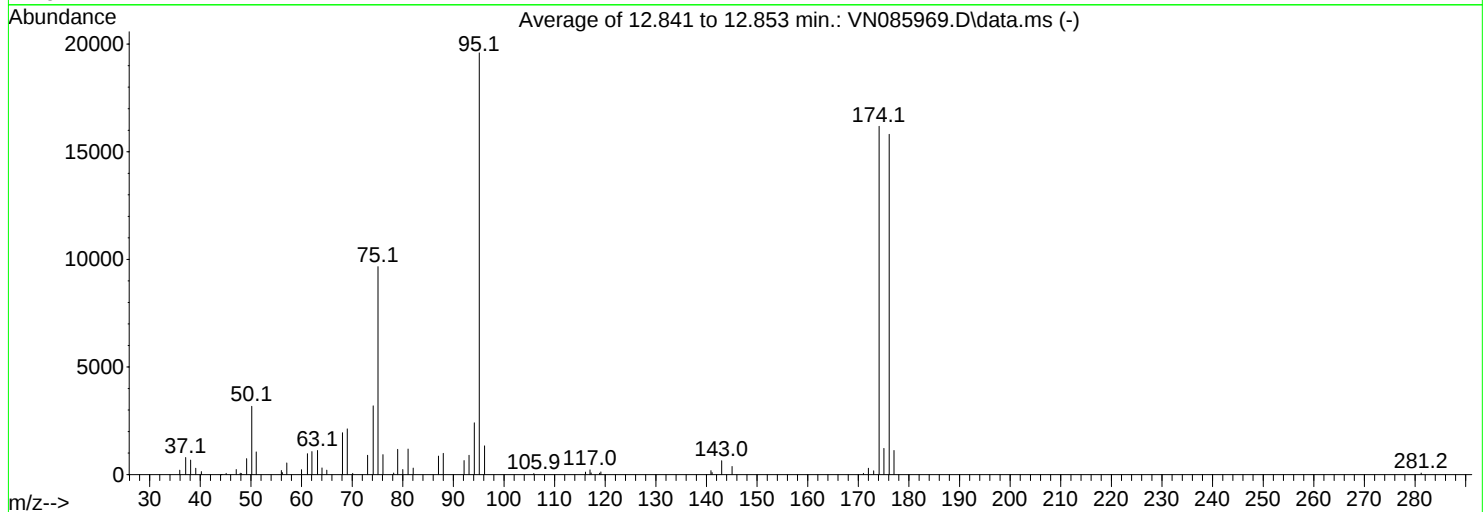


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031325\
Data File : VN085969.D
Acq On : 13 Mar 2025 10:06
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Title : SW846 8260
Last Update : Wed Feb 19 03:43:32 2025

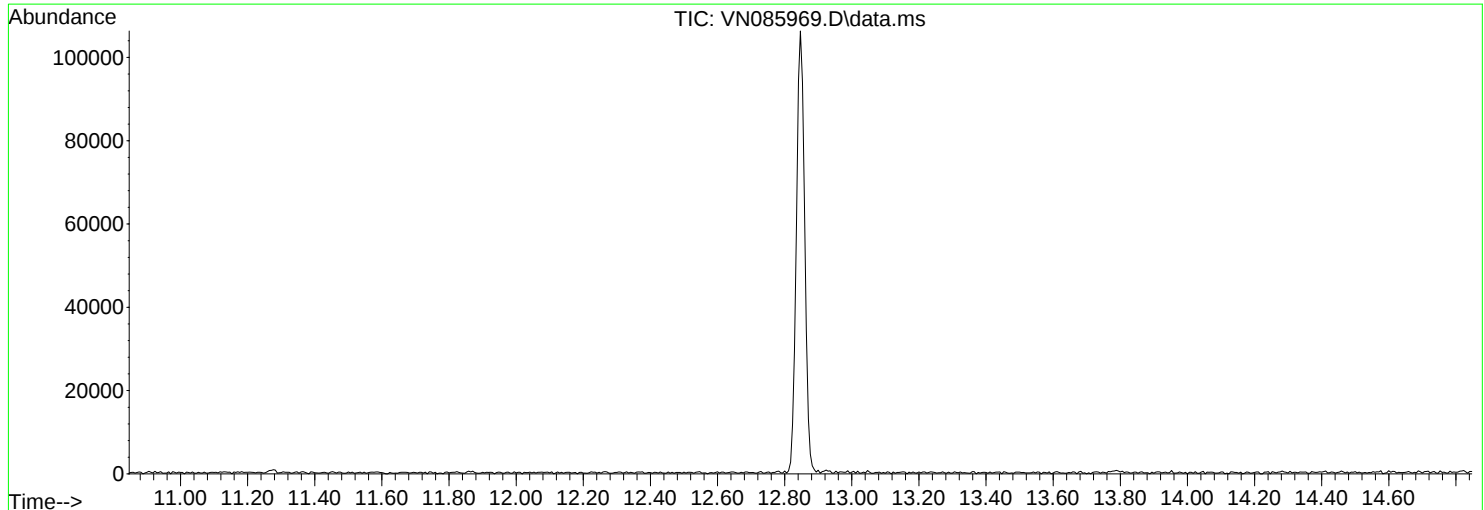

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	3175	PASS
75	95	30	60	49.3	9666	PASS
95	95	100	100	100.0	19595	PASS
96	95	5	9	6.8	1336	PASS
173	174	0.00	2	1.1	176	PASS
174	95	50	100	82.6	16179	PASS
175	174	5	9	7.5	1220	PASS
176	174	95	101	97.7	15813	PASS
177	176	5	9	7.1	1119	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	205	50.15	3175	68.10	1946	82.05	301
37.10	796	51.05	1059	69.05	2125	87.05	86
38.10	673	56.00	196	70.10	62	88.00	98
39.10	301	56.20	99	73.05	901	92.10	65
40.20	143	57.10	544	74.15	3195	93.10	899
44.10	3	60.00	234	75.10	9666	94.15	2405
45.10	56	61.15	973	76.10	928	95.10	19595
47.10	235	62.05	1073	78.20	73	96.15	1336
47.90	70	63.15	1122	79.00	1174	105.90	52
48.10	52	64.05	313	80.00	239	116.10	116
49.15	747	65.00	209	81.05	1190	117.00	222

Average of 12.841 to 12.853 min.: VN085969.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
117.20	81	175.05	1220				
118.90	67	176.10	15813				
119.15	123	177.05	1119				
140.90	189	281.20	72				
141.10	100						
143.00	645						
145.05	378						
171.00	61						
172.00	297						
173.05	176						
174.10	16179						

Instrument :

MSVOA_N

ClientSampleId :

BFB