


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031419\
 Data File : VN054252.D
 Acq On : 14 Mar 2019 9:53
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
 Title : SW846 8260
 Last Update : Wed Mar 13 03:33:31 2019

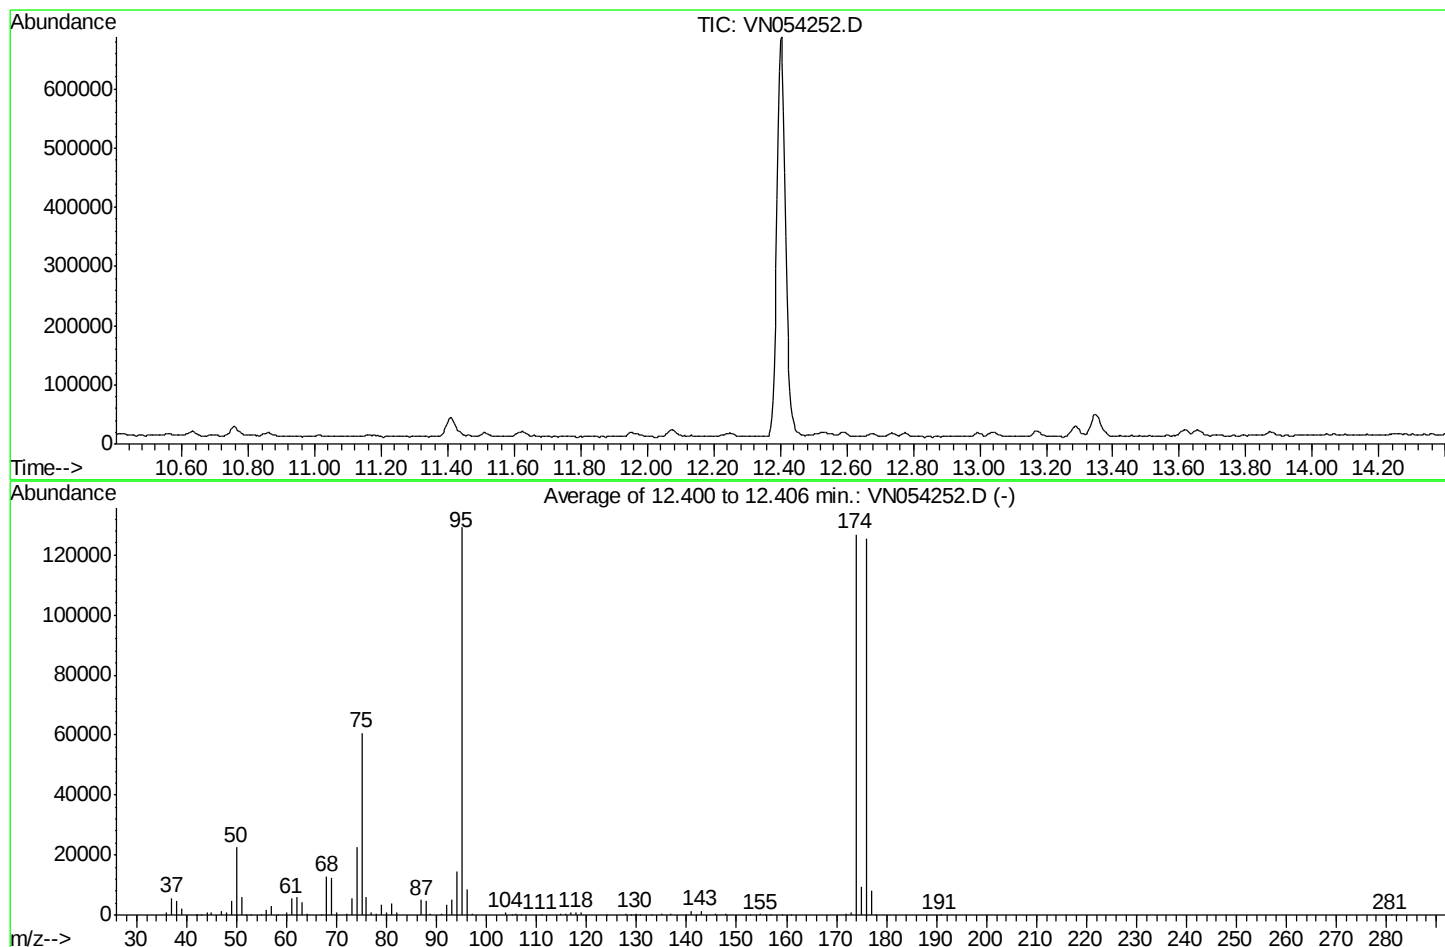

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	22576	PASS
75	95	30	60	47.0	60741	PASS
95	95	100	100	100.0	129226	PASS
96	95	5	9	6.5	8337	PASS
173	174	0.00	2	0.8	1057	PASS
174	95	50	100	98.2	126904	PASS
175	174	5	9	7.4	9361	PASS
176	174	95	101	98.7	125264	PASS
177	176	5	9	6.6	8329	PASS