


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031419\
 Data File : VN054278.D
 Acq On : 14 Mar 2019 23:05
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
 Title : SW846 8260
 Last Update : Wed Mar 13 03:33:31 2019

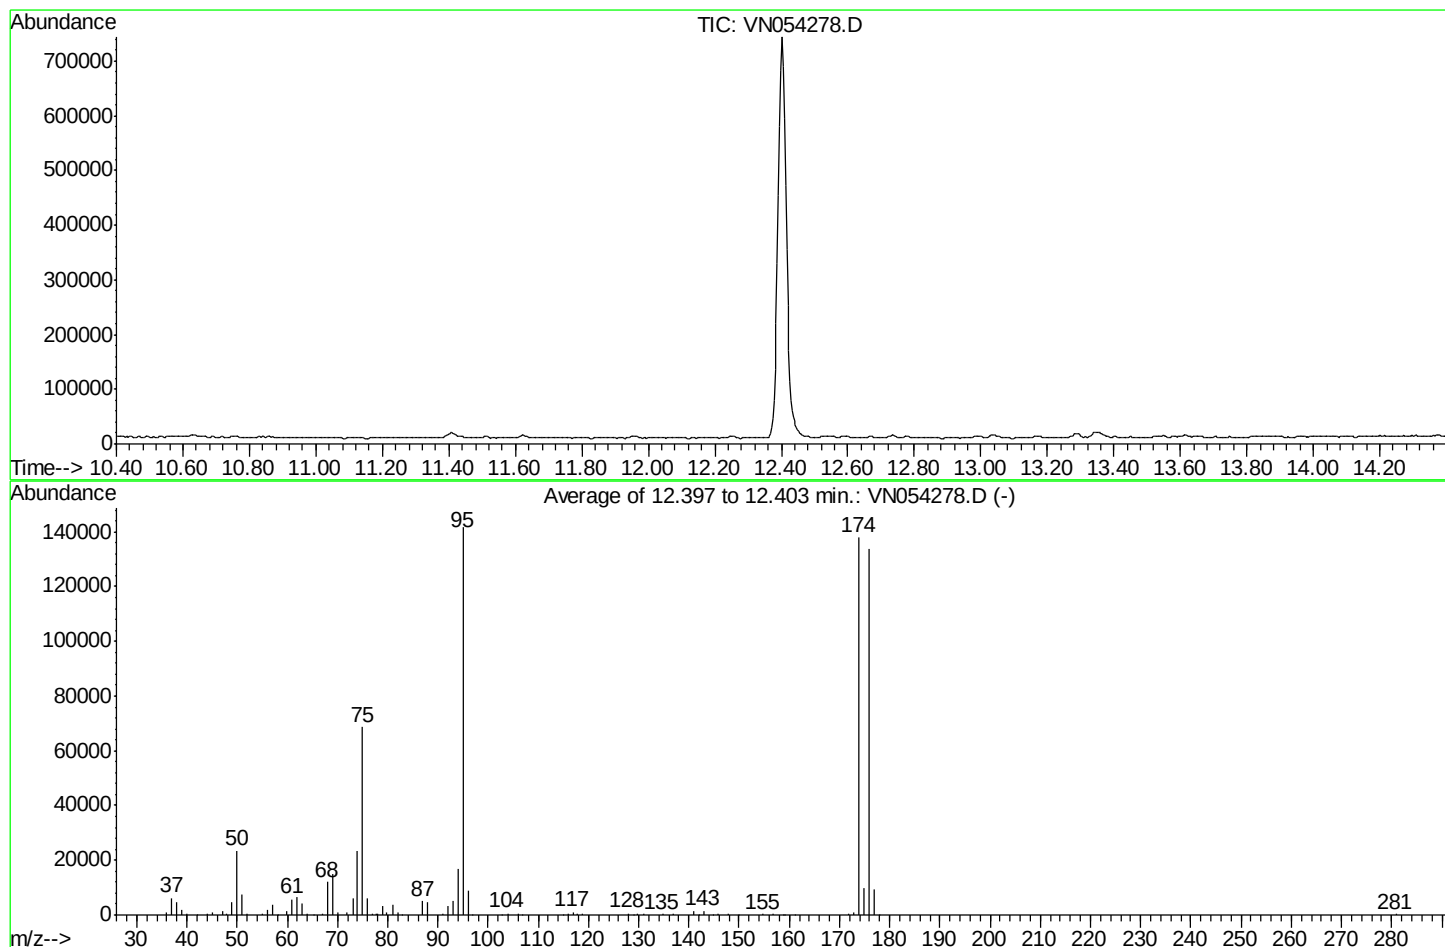

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	23418	PASS
75	95	30	60	48.5	68685	PASS
95	95	100	100	100.0	141632	PASS
96	95	5	9	6.4	9072	PASS
173	174	0.00	2	0.7	934	PASS
174	95	50	100	97.3	137829	PASS
175	174	5	9	7.1	9725	PASS
176	174	95	101	96.9	133549	PASS
177	176	5	9	6.9	9270	PASS