

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031422\
 Data File : VN071265.D
 Acq On : 14 Mar 2022 14:50
 Operator : JC\MD
 Sample : N1905-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 WC-14A-1A-3-(3.0-3.5)

Quant Time: Mar 15 02:52:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 08 06:52:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.081	168	714236	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1172682	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1062988	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.669	152	383920	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	448196	45.786	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	91.580%
35) Dibromofluoromethane	8.016	113	341982	46.214	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	92.420%
50) Toluene-d8	10.439	98	1440813	48.358	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	96.720%
62) 4-Bromofluorobenzene	12.727	95	510085	50.557	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	101.120%
Target Compounds						
					Qvalue	
3) Chloromethane	2.299	50	3251	0.275	ug/l	96
5) Bromomethane	2.852	94	1896	Below Cal	#	78
13) Acrolein	4.040	56	1087	0.534	ug/l #	78
15) Acrylonitrile	5.551	53	1705	0.299	ug/l #	55
16) Acetone	4.287	43	97807	20.535	ug/l	94
17) Carbon Disulfide	4.534	76	5589	0.274	ug/l #	91
18) Methyl Acetate	4.857	43	33523	3.066	ug/l	92
20) Methylene Chloride	5.087	84	19121	2.562	ug/l	90
25) 2-Butanone	7.334	43	29433	3.836	ug/l	95
29) Tetrahydrofuran	7.687	42	1965	0.370	ug/l #	62
31) Cyclohexane	8.087	56	16244	1.039	ug/l #	7
36) 1,1-Dichloropropene	8.081	75	54297	4.580	ug/l #	49
37) Ethyl Acetate	7.334	43	29433	1.804	ug/l #	71
38) Carbon Tetrachloride	8.087	117	71244	6.212	ug/l #	16
43) Isopropyl Acetate	8.557	43	142477	5.839	ug/l #	76
48) Methyl methacrylate	9.539	41	23327	2.063	ug/l #	8
49) 1,4-Dioxane	9.569	88	415	2.111	ug/l #	27
51) 4-Methyl-2-Pentanone	10.322	43	17194	1.135	ug/l	99
54) cis-1,3-Dichloropropene	10.239	75	104488	7.273	ug/l #	61
57) 1,3-Dichloropropane	11.086	76	54353	3.435	ug/l #	43
58) 2-Chloroethyl Vinyl ether	10.045	63	69	27.885	ug/l #	45
59) 2-Hexanone	11.086	43	850361	82.299	ug/l #	50
74) N-amyl acetate	12.386	43	4335	0.312	ug/l #	94
75) 1,1,2,2-Tetrachloroethane	12.810	83	1140	Below Cal	#	88
76) 1,2,3-Trichloropropane	12.727	75	262893	26.952	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.727	75	262893	74.022	ug/l #	5
89) n-Butylbenzene	13.939	91	5048	0.240	ug/l	87
92) 1,2-Dibromo-3-Chloropr...	14.598	75	651	0.302	ug/l #	54
93) 1,2,4-Trichlorobenzene	15.257	180	3078	3.449	ug/l	98
95) Naphthalene	15.504	128	11315	5.645	ug/l	100
96) 1,2,3-Trichlorobenzene	15.692	180	3439	3.271	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031422\
Data File : VN071265.D
Acq On : 14 Mar 2022 14:50
Operator : JC\MD
Sample : N1905-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-3-(3.0-3.5)

Quant Time: Mar 15 02:52:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 08 06:52:46 2022
Response via : Initial Calibration




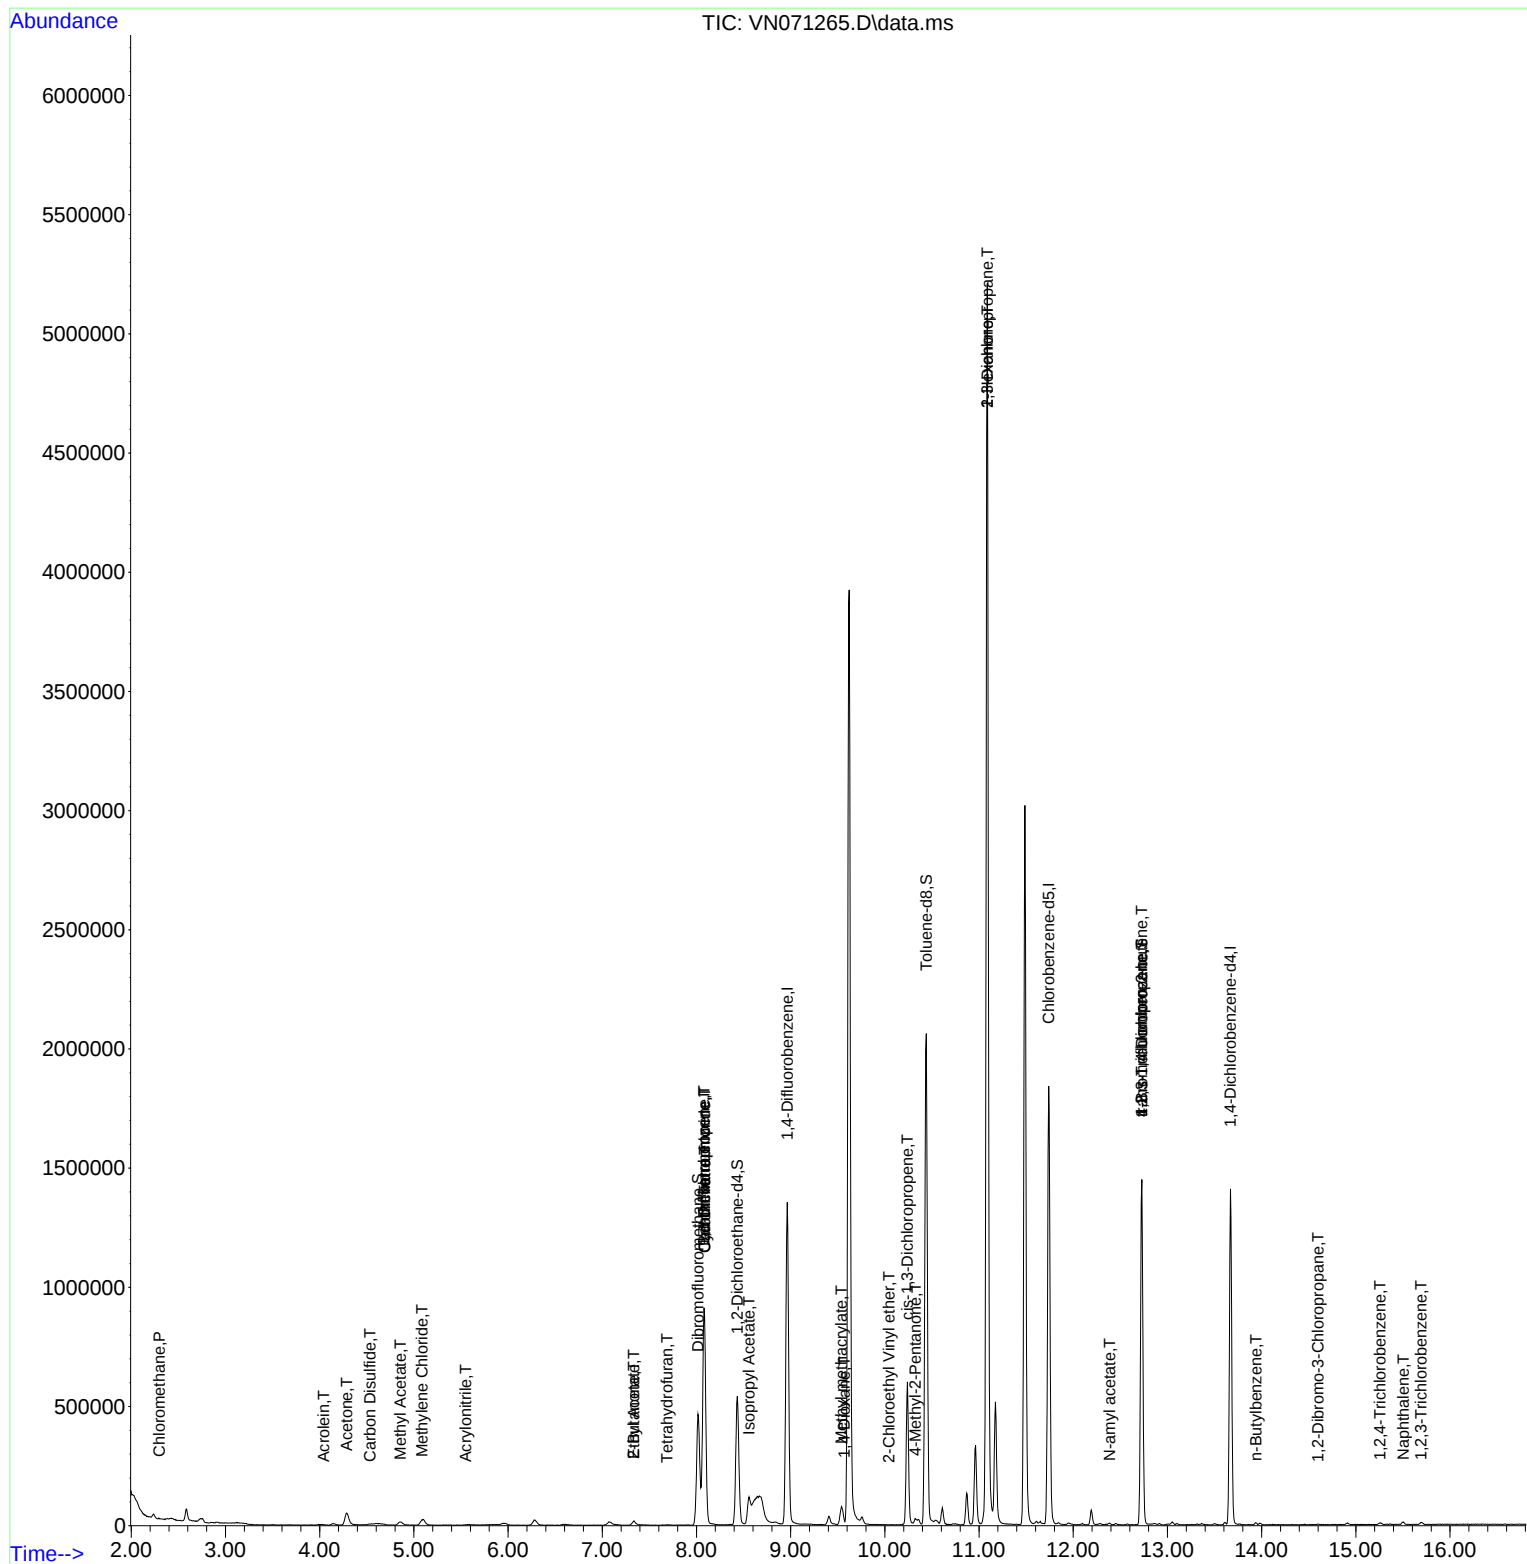




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 10
Delta R.T. -0.005 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-3(3.0-3.5)


Tgt Ion:168 Resp: 714236
Ion Ratio Lower Upper
168 100
99 57.0 41.3 61.9



#3
Chloromethane
Concen: 0.275 ug/l
RT: 2.299 min Scan# 53
Delta R.T. -0.000 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50

Tgt Ion: 50 Resp: 3251
Ion Ratio Lower Upper
50 100
52 29.6 25.4 38.0


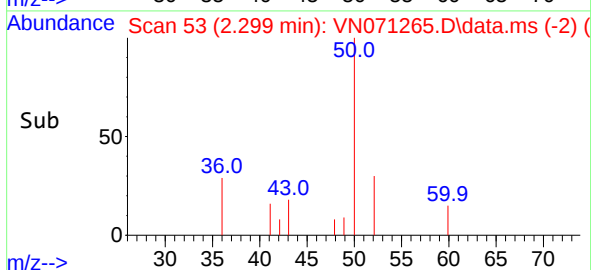






#5
Bromomethane
Concen: Below Cal
RT: 2.852 min Scan# 144
Delta R.T. 0.018 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-3-(3.0-3.5)


Tgt Ion: 94 Resp: 1896
Ion Ratio Lower Upper
94 100
96 71.0 73.8 110.8#

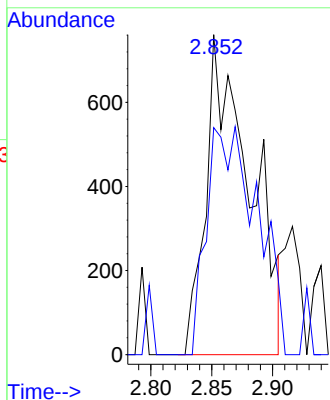

#13
Acrolein
Concen: 0.534 ug/l
RT: 4.040 min Scan# 349
Delta R.T. 0.000 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50

Tgt Ion: 56 Resp: 1087
Ion Ratio Lower Upper
56 100
55 52.4 56.6 85.0#


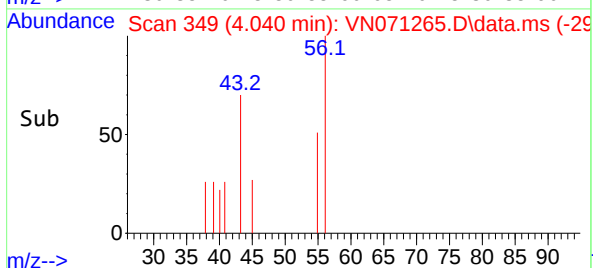
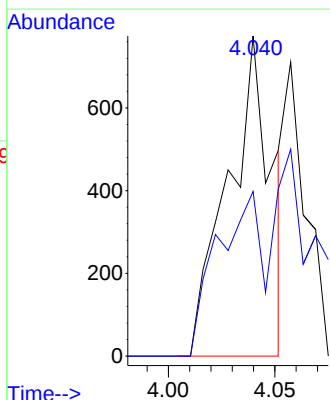





#15
Acrylonitrile
Concen: 0.299 ug/l
RT: 5.551 min Scan# 606
Delta R.T. 0.000 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-3-(3.0-3.5)


Tgt Ion: 53 Resp: 1705
Ion Ratio Lower Upper
53 100
52 46.6 66.2 99.2#
51 3.6 29.6 44.4#

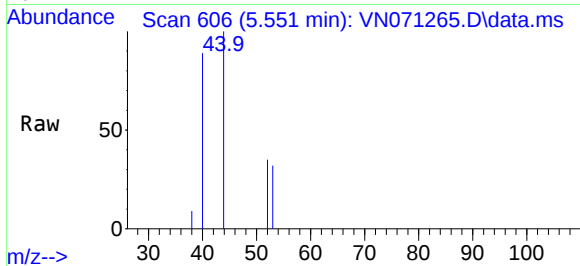

#16
Acetone
Concen: 20.535 ug/l
RT: 4.287 min Scan# 391
Delta R.T. 0.000 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50

Tgt Ion: 43 Resp: 97807
Ion Ratio Lower Upper
43 100
58 31.9 23.1 34.7


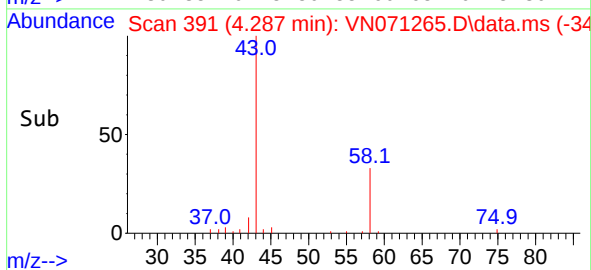

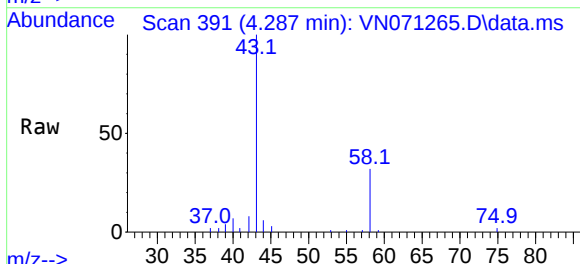




#17
Carbon Disulfide
Concen: 0.274 ug/l
RT: 4.534 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-3-(3.0-3.5)


Tgt Ion: 76 Resp: 5589
Ion Ratio Lower Upper
76 100
78 12.7 7.5 11.3#

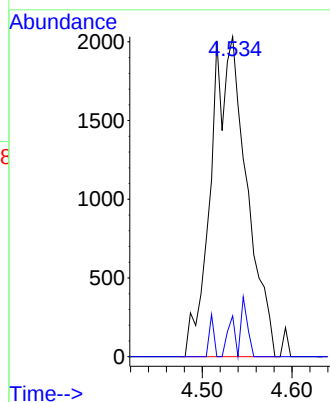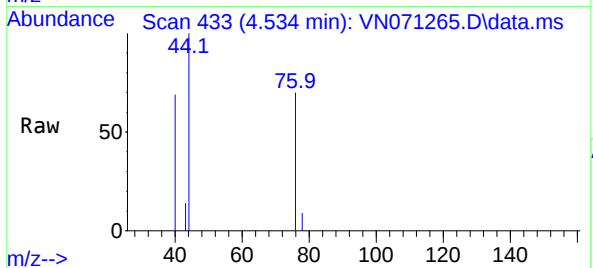

#18
Methyl Acetate
Concen: 3.066 ug/l
RT: 4.857 min Scan# 488
Delta R.T. 0.006 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50

Tgt Ion: 43 Resp: 33523
Ion Ratio Lower Upper
43 100
74 20.5 19.4 29.2


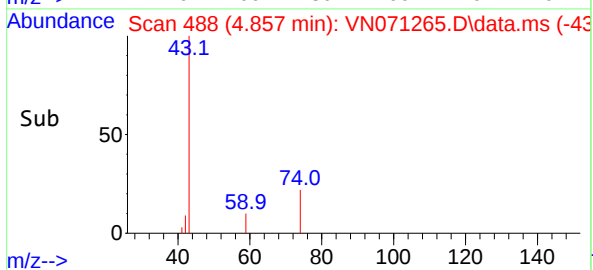
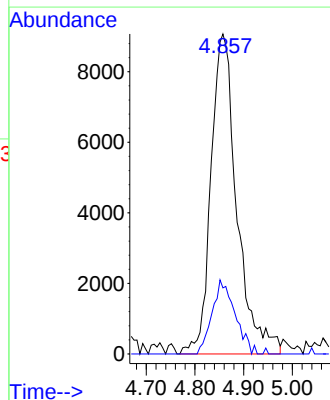





#20
Methylene Chloride
Concen: 2.562 ug/l
RT: 5.087 min Scan# 51
Delta R.T. -0.006 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-3-(3.0-3.5)


Tgt Ion:	84	Resp:	19121
Ion	Ratio	Lower	Upper
84	100		
49	131.8	93.5	140.3
51	39.9	29.4	44.2
86	60.9	53.0	79.4

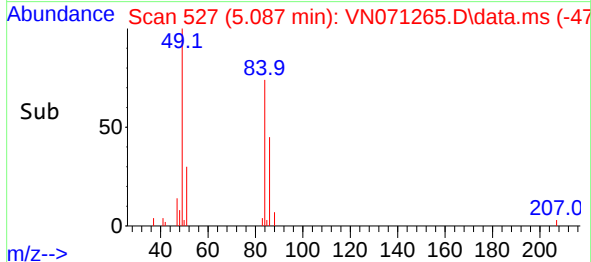

#25
2-Butanone
Concen: 3.836 ug/l
RT: 7.334 min Scan# 909
Delta R.T. 0.000 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50

Tgt Ion:	43	Resp:	29433
Ion	Ratio	Lower	Upper
43	100		
72	24.3	21.7	32.5

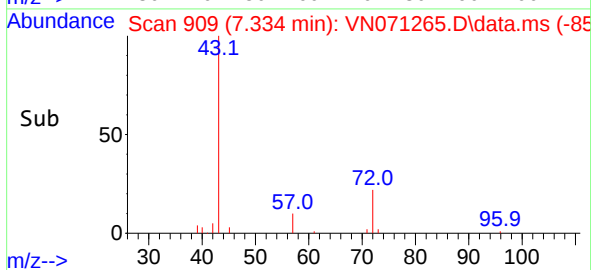



#29

Tetrahydrofuran

Concen: 0.370 ug/l

RT: 7.687 min Scan# 91

Delta R.T. 0.006 min

Lab File: VN071265.D


Acq: 14 Mar 2022 14:50

Instrument :

MSVOA_N

ClientSampleId :

WC-14A-1A-3-(3.0-3.5)

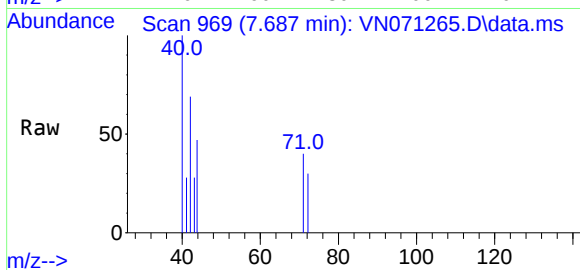




Tgt Ion: 42 Resp: 1965

Ion Ratio Lower Upper

42 100

72 30.8 36.3 54.5#

71 7.9 34.7 52.1#

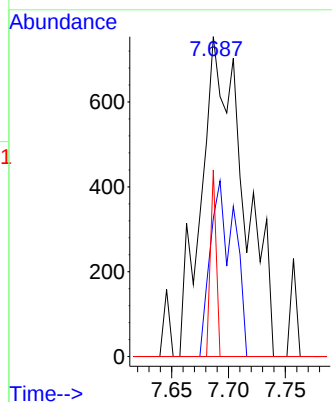

#31

Cyclohexane

Concen: 1.039 ug/l

RT: 8.087 min Scan# 1037

Delta R.T. -0.006 min

Lab File: VN071265.D

Acq: 14 Mar 2022 14:50




Tgt Ion: 56 Resp: 16244


Ion Ratio Lower Upper

56 100

69 166.4 27.1 40.7#

84 132.1 73.4 110.0#

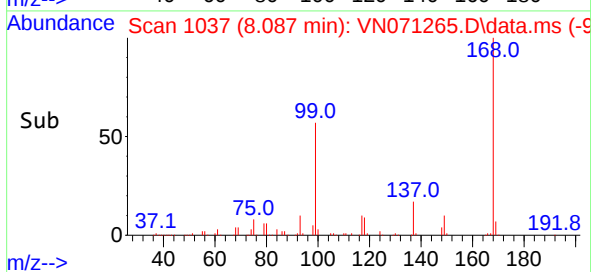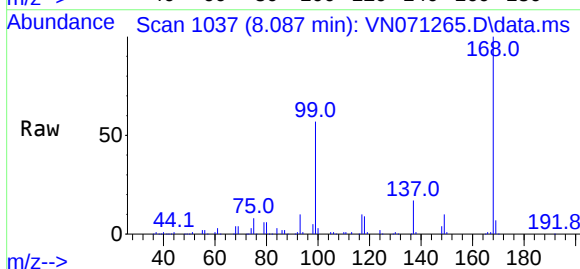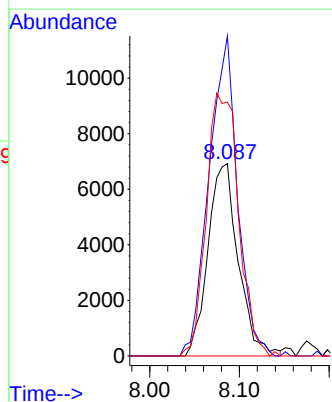



#33

1,2-Dichloroethane-d4

Concen: 45.786 ug/l

RT: 8.434 min Scan# 1096

Delta R.T. -0.006 min

Lab File: VN071265.D

Acq: 14 Mar 2022 14:50

Instrument :

MSVOA_N

ClientSampleId :





WC-14A-1A-3-(3.0-3.5)

Tgt Ion: 65 Resp: 448196

Ion Ratio Lower Upper

65 100

67 52.8 0.0 103.0

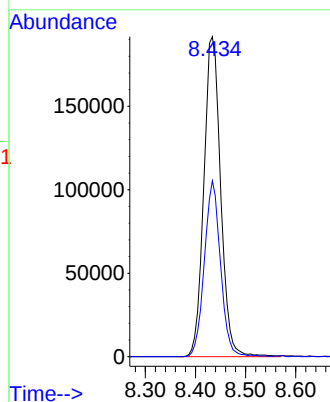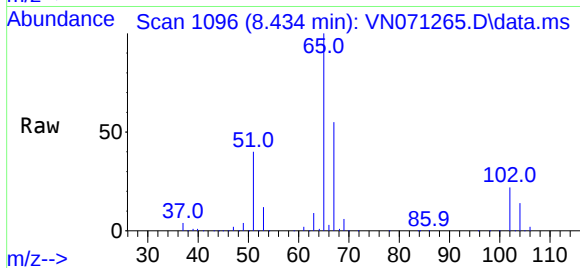

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN071265.D

Acq: 14 Mar 2022 14:50




Tgt Ion:114 Resp: 1172682


Ion Ratio Lower Upper

114 100

63 21.6 0.0 37.8


88 15.7 0.0 27.4

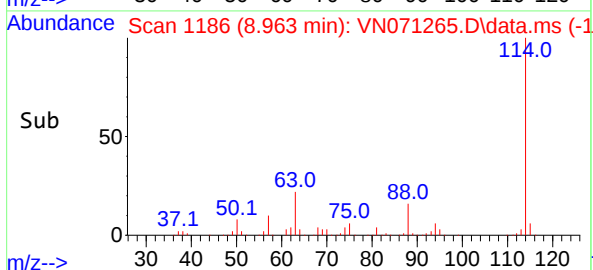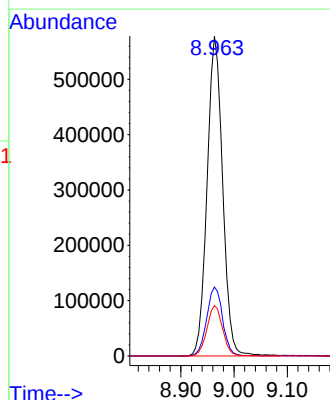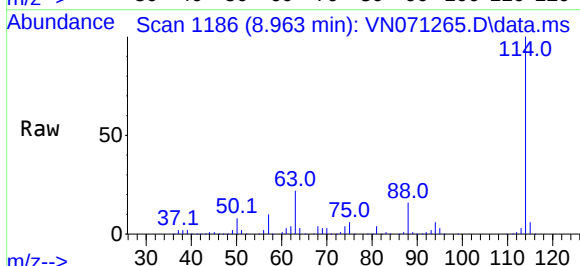






#35
Dibromofluoromethane
Concen: 46.214 ug/l
RT: 8.016 min Scan# 1025
Delta R.T. -0.006 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50

Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-3(3.0-3.5)



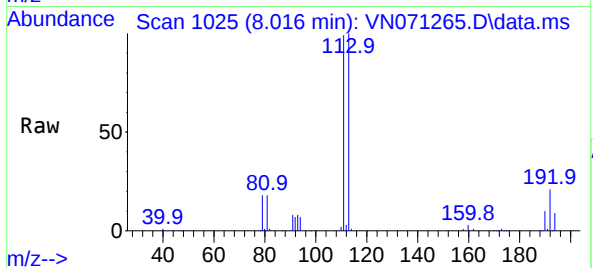



Tgt Ion:113 Resp: 341982
Ion Ratio Lower Upper
113 100
111 102.5 82.2 123.2
192 20.7 16.9 25.3



#36
1,1-Dichloropropene
Concen: 4.580 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.135 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50

Tgt Ion: 75 Resp: 54297
Ion Ratio Lower Upper
75 100
110 8.9 18.4 55.2#
77 0.0 24.4 36.6#


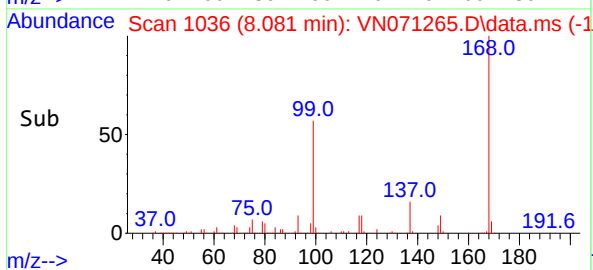






#37
Ethyl Acetate
Concen: 1.804 ug/l
RT: 7.334 min Scan# 909
Delta R.T. -0.076 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-3-(3.0-3.5)


Tgt Ion: 43 Resp: 29433
Ion Ratio Lower Upper
43 100
61 1.6 11.5 17.3#
70 0.2 7.9 11.9#



#38
Carbon Tetrachloride
Concen: 6.212 ug/l
RT: 8.087 min Scan# 1037
Delta R.T. -0.117 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50

Tgt Ion: 117 Resp: 71244
Ion Ratio Lower Upper
117 100
119 5.1 76.1 114.1#
121 0.0 24.2 36.2#


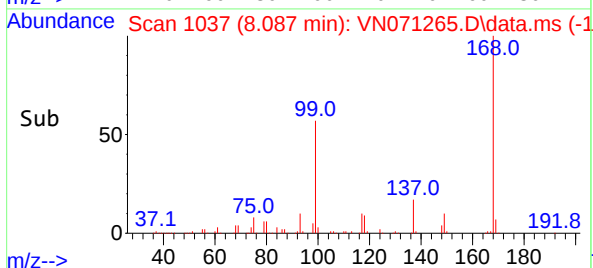
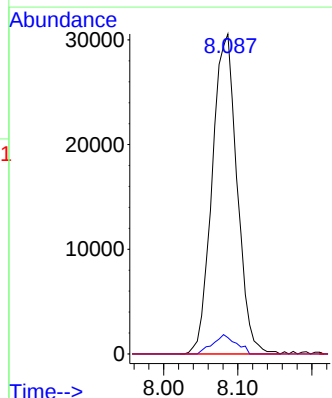





#43
Isopropyl Acetate
Concen: 5.839 ug/l
RT: 8.557 min Scan# 1117
Delta R.T. 0.000 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-3-(3.0-3.5)


Tgt Ion: 43 Resp: 142477
Ion Ratio Lower Upper
43 100
61 11.6 20.4 30.6#
87 6.6 11.2 16.8#



#48
Methyl methacrylate
Concen: 2.063 ug/l
RT: 9.539 min Scan# 1284
Delta R.T. -0.018 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50

Tgt Ion: 41 Resp: 23327
Ion Ratio Lower Upper
41 100
69 0.0 72.4 108.6#
39 0.0 58.4 87.6#


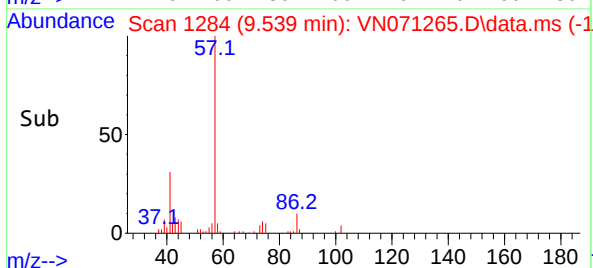
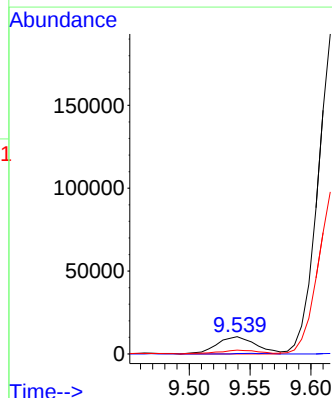





#49
1,4-Dioxane
Concen: 2.111 ug/l
RT: 9.569 min Scan# 1288
Delta R.T. 0.006 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-3-(3.0-3.5)


Tgt Ion: 88 Resp: 415
Ion Ratio Lower Upper
88 100
43 0.0 23.4 35.2#
58 0.0 50.6 75.8#

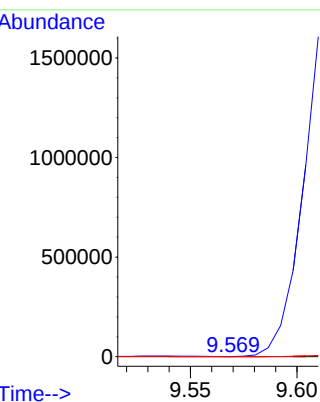

#50
Toluene-d8
Concen: 48.358 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50

Tgt Ion: 98 Resp: 1440813
Ion Ratio Lower Upper
98 100
100 65.6 50.4 75.6

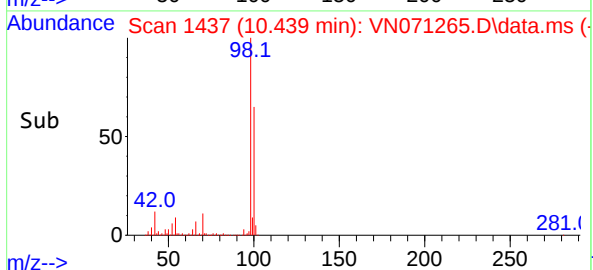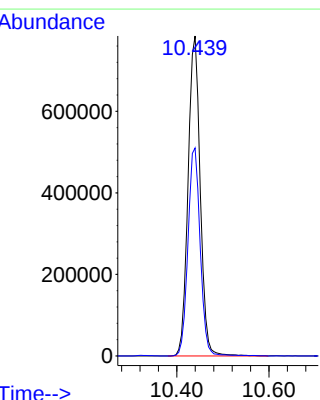



#51

4-Methyl-2-Pentanone

Concen: 1.135 ug/l

RT: 10.322 min Scan# 1418

Delta R.T. -0.005 min

Lab File: VN071265.D

Acq: 14 Mar 2022 14:50

Instrument :

MSVOA_N

ClientSampleId :





WC-14A-1A-3-(3.0-3.5)

Tgt Ion: 43 Resp: 17194

Ion Ratio Lower Upper

43 100

58 38.3 30.4 45.6

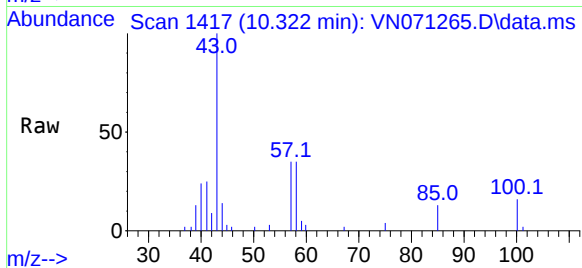

#54

cis-1,3-Dichloropropene

Concen: 7.273 ug/l

RT: 10.239 min Scan# 1403

Delta R.T. 0.053 min

Lab File: VN071265.D

Acq: 14 Mar 2022 14:50




Tgt Ion: 75 Resp: 104488


Ion Ratio Lower Upper

75 100

77 0.5 26.4 39.6#

39 33.4 42.5 63.7#

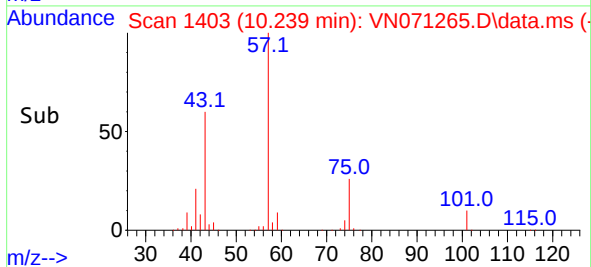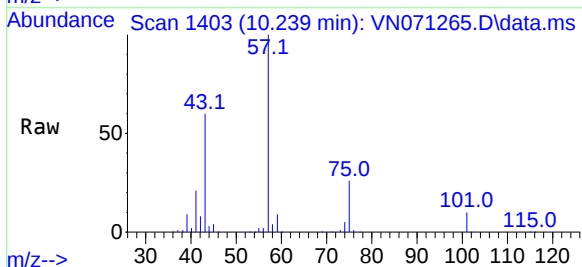



#57

1,3-Dichloropropane

Concen: 3.435 ug/l

RT: 11.086 min Scan# 11

Delta R.T. 0.047 min

Lab File: VN071265.D

Acq: 14 Mar 2022 14:50

Instrument :

MSVOA_N

ClientSampleId :





WC-14A-1A-3-(3.0-3.5)

Tgt Ion: 76 Resp: 54353

Ion Ratio Lower Upper

76 100

78 0.2 25.7 38.5#

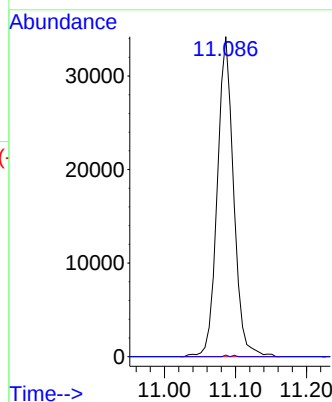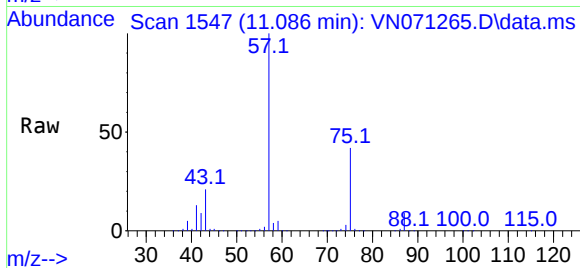

#58

2-Chloroethyl Vinyl ether

Concen: 27.885 ug/l

RT: 10.045 min Scan# 1370

Delta R.T. 0.006 min

Lab File: VN071265.D




Acq: 14 Mar 2022 14:50


Tgt Ion: 63 Resp: 69

Ion Ratio Lower Upper

63 100

106 0.0 23.9 35.9#




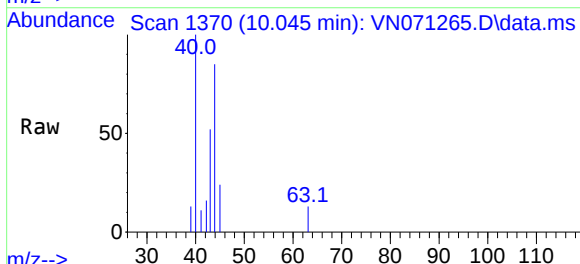




#59
2-Hexanone
Concen: 82.299 ug/l
RT: 11.086 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-3-(3.0-3.5)


Tgt Ion: 43 Resp: 850361
Ion Ratio Lower Upper
43 100
58 17.8 26.9 80.7#

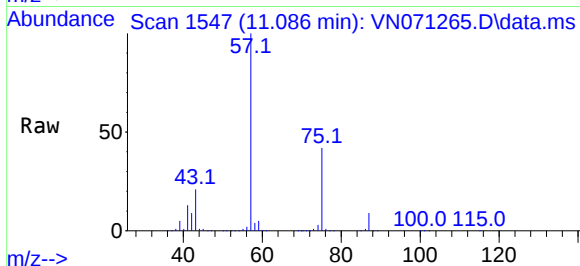

#62
4-Bromofluorobenzene
Concen: 50.557 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50

Tgt Ion: 95 Resp: 510085
Ion Ratio Lower Upper
95 100
174 79.6 0.0 187.2
176 76.1 0.0 181.4



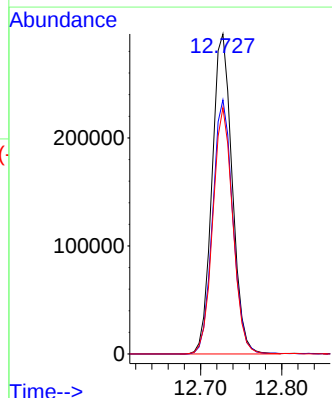
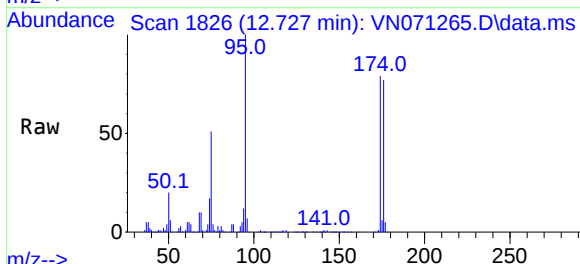




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1177
Delta R.T. 0.000 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-3-(3.0-3.5)


Tgt Ion:117 Resp: 1062988
Ion Ratio Lower Upper
117 100
82 57.8 42.4 63.6
119 32.4 25.4 38.2

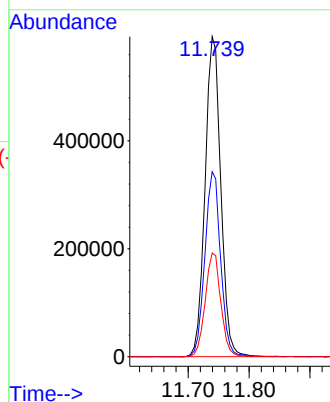

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.669 min Scan# 1986
Delta R.T. 0.001 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50

Tgt Ion:152 Resp: 383920
Ion Ratio Lower Upper
152 100
115 59.5 27.5 82.5
150 157.9 0.0 344.4



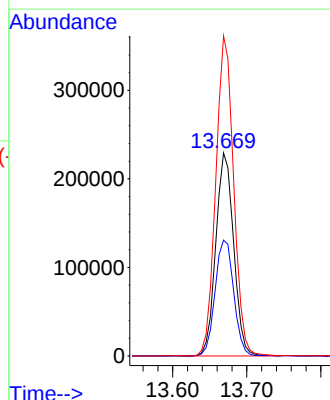





#74
N-amy1 acetate
Concen: 0.312 ug/l
RT: 12.386 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-3-(3.0-3.5)


Tgt Ion:	43	Resp:	4335
Ion	Ratio	Lower	Upper
43	100		
70	40.0	33.4	50.0
55	26.3	19.3	28.9
61	15.7	18.5	27.7#

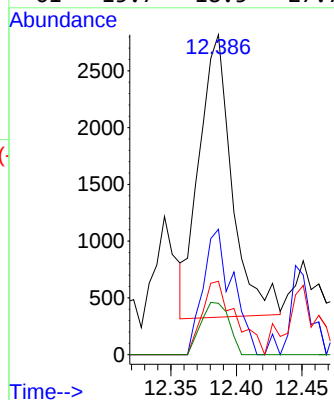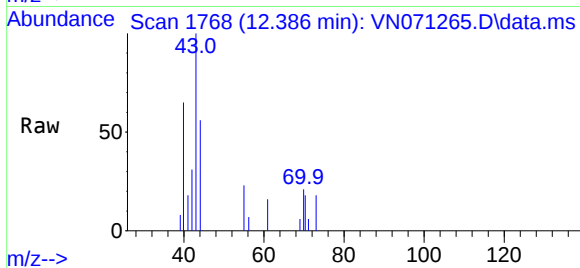

#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.810 min Scan# 1840
Delta R.T. -0.011 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50

Tgt Ion:	83	Resp:	1140
Ion	Ratio	Lower	Upper
83	100		
131	0.0	5.5	16.5#
85	57.5	32.4	97.2


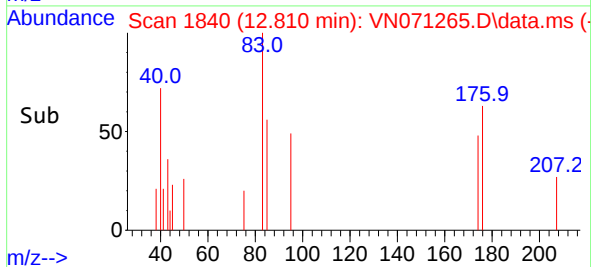
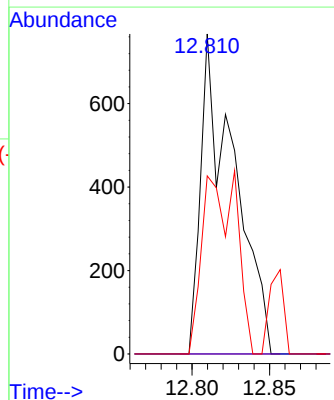
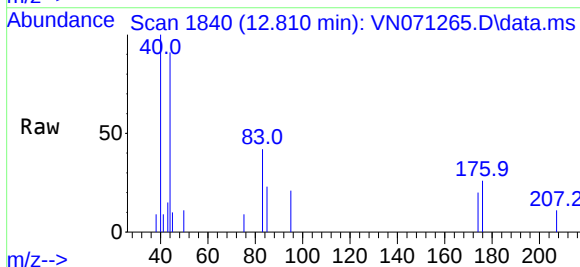




#76
1,2,3-Trichloropropane
Concen: 26.952 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-3-(3.0-3.5)


Tgt Ion: 75 Resp: 262893
Ion Ratio Lower Upper
75 100
77 1.1 82.6 247.8#

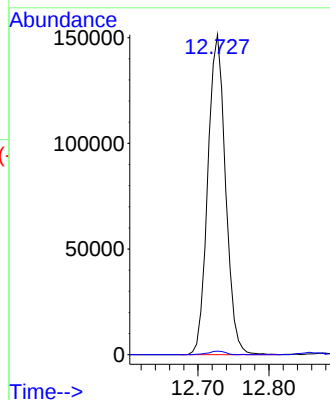

#81
trans-1,4-Dichloro-2-butene
Concen: 74.022 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.106 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50

Tgt Ion: 75 Resp: 262893
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#



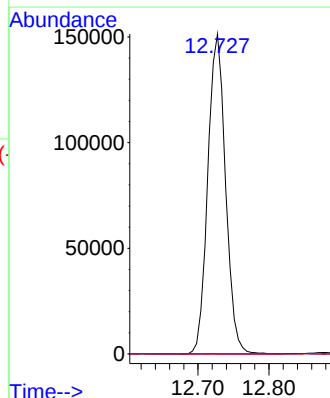





#89
n-Butylbenzene
Concen: 0.240 ug/l
RT: 13.939 min Scan# 2032
Delta R.T. 0.000 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-3-(3.0-3.5)


Tgt Ion:	91	Resp:	5048
Ion	Ratio	Lower	Upper
91	100		
92	57.4	25.4	76.0
134	17.8	13.6	40.8

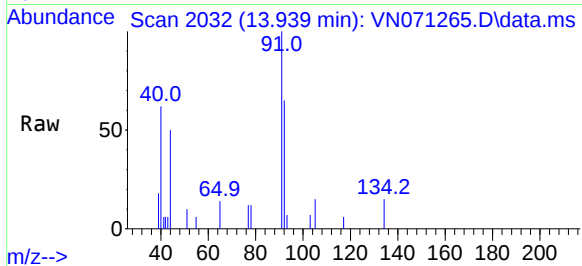

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.302 ug/l
RT: 14.598 min Scan# 2144
Delta R.T. 0.000 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50

Tgt Ion:	75	Resp:	651
Ion	Ratio	Lower	Upper
75	100		
155	31.8	46.9	140.7#
157	86.2	60.6	181.7



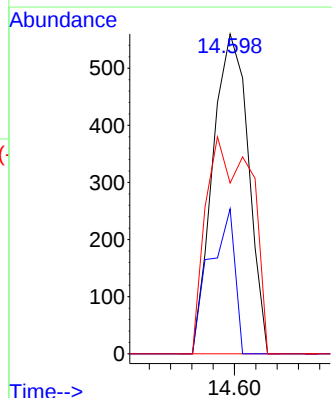
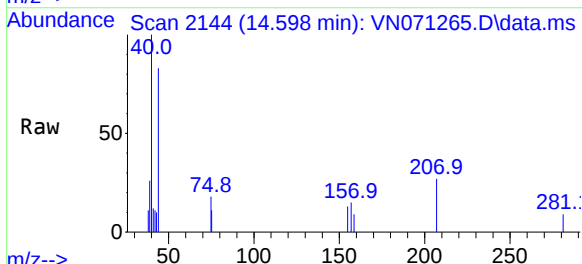




#93
1,2,4-Trichlorobenzene
Concen: 3.449 ug/l
RT: 15.257 min Scan# 21
Delta R.T. -0.005 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-3-(3.0-3.5)


Tgt Ion:180 Resp: 3078
Ion Ratio Lower Upper
180 100
182 99.3 48.3 144.9
145 28.2 14.5 43.5

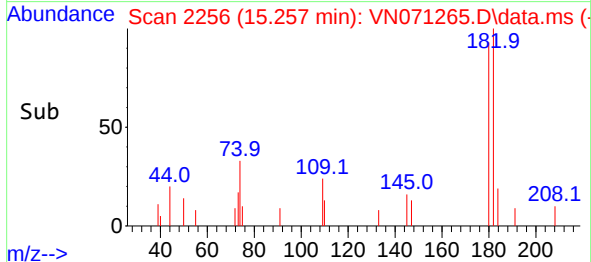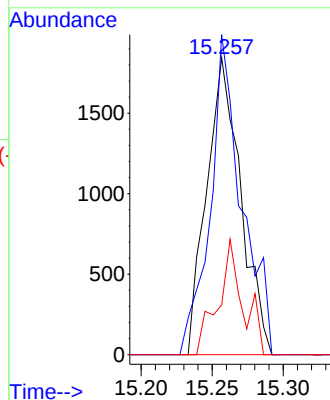

#95
Naphthalene
Concen: 5.645 ug/l
RT: 15.504 min Scan# 2298
Delta R.T. -0.000 min
Lab File: VN071265.D
Acq: 14 Mar 2022 14:50


Tgt Ion:128 Resp: 11315
Ion Ratio Lower Upper
128 100
127 13.1 10.5 15.7
129 10.5 8.7 13.1

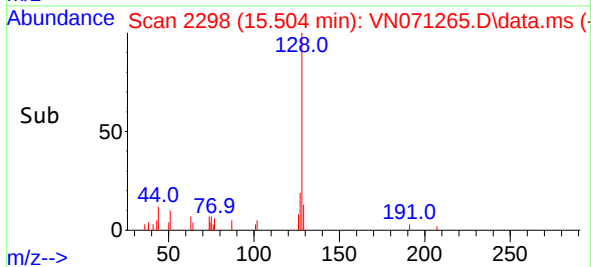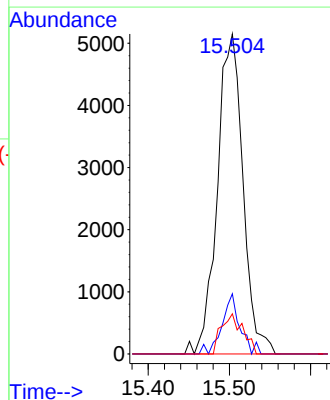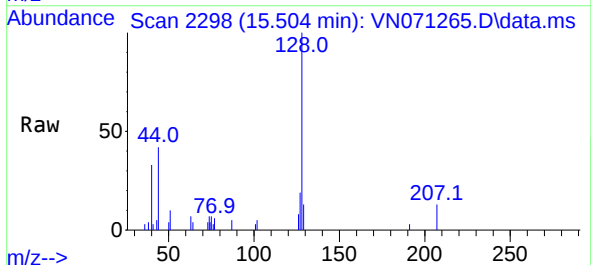



#96
 1,2,3-Trichlorobenzene
 Concen: 3.271 ug/l
 RT: 15.692 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: VN071265.D
 Acq: 14 Mar 2022 14:50

Instrument :
 MSVOA_N
 ClientSampleId :
 WC-14A-1A-3-(3.0-3.5)



Tgt Ion:	180	Resp:	3439
Ion	Ratio	Lower	Upper
180	100		
182	97.3	47.4	142.2
145	40.1	15.0	45.1

