


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031422\
 Data File : VN071256.D
 Acq On : 14 Mar 2022 09:50
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Title : SW846 8260
 Last Update : Tue Mar 08 06:52:46 2022

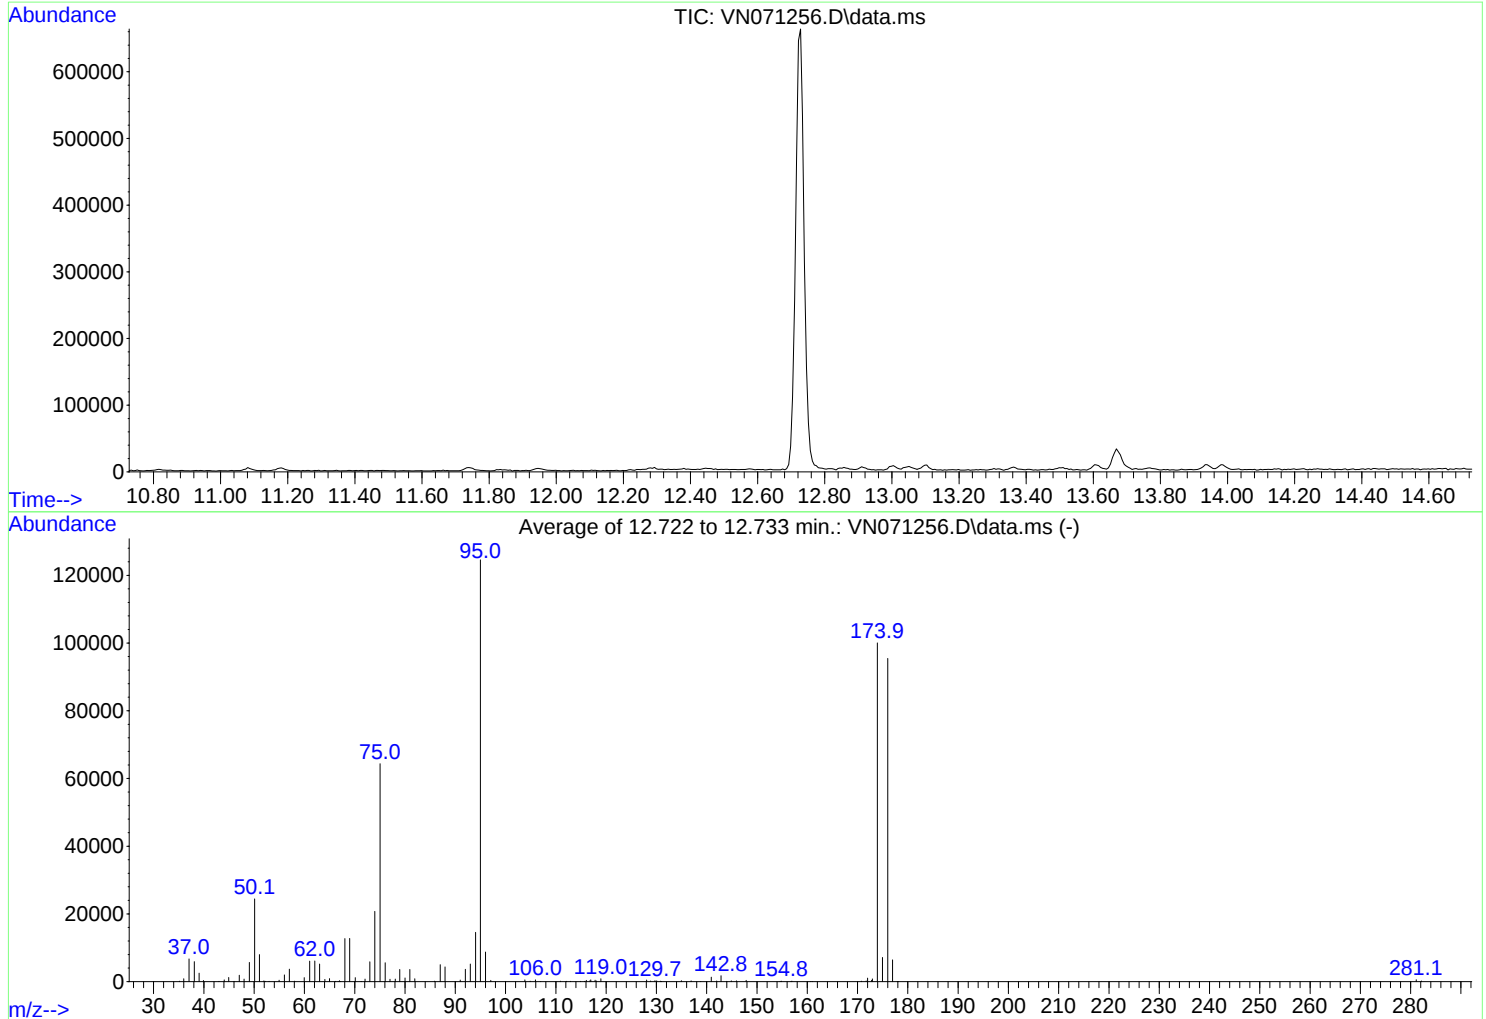

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1816

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	24429	PASS
75	95	30	60	51.7	64349	PASS
95	95	100	100	100.0	124568	PASS
96	95	5	9	7.0	8761	PASS
173	174	0.00	2	0.8	784	PASS
174	95	50	100	80.3	100021	PASS
175	174	5	9	7.1	7128	PASS
176	174	95	101	95.4	95451	PASS
177	176	5	9	6.7	6410	PASS