
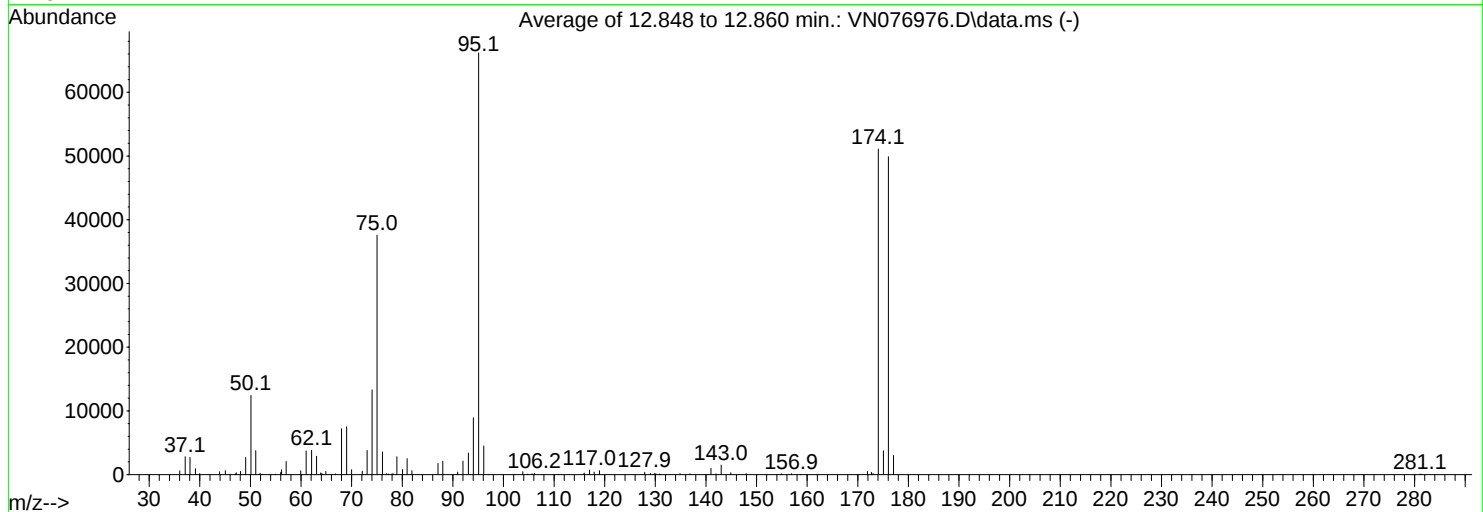


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031423\
Data File : VN076976.D
Acq On : 14 Mar 2023 08:33
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031023W.M
Title : SW846 8260
Last Update : Fri Mar 10 13:47:39 2023

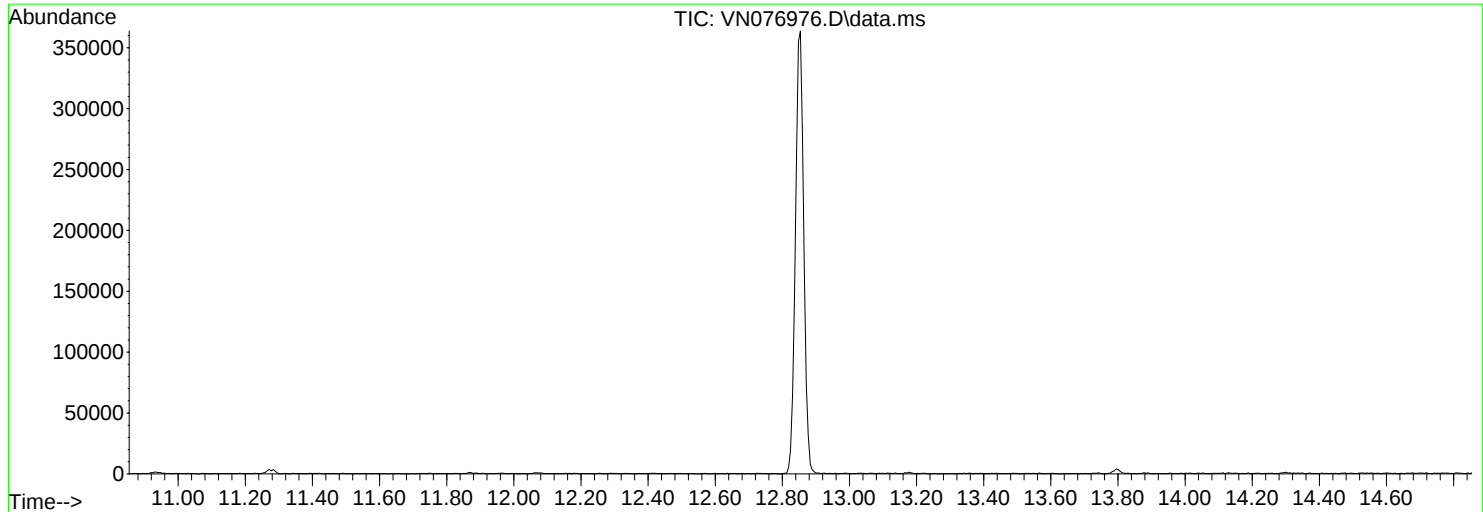

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.8	12433	PASS
75	95	30	60	56.8	37581	PASS
95	95	100	100	100.0	66187	PASS
96	95	5	9	6.8	4484	PASS
173	174	0.00	2	0.7	350	PASS
174	95	50	100	77.2	51104	PASS
175	174	5	9	7.3	3742	PASS
176	174	95	101	97.6	49891	PASS
177	176	5	9	6.0	3006	PASS

Average of 12.848 to 12.860 min.: VN076976.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	601	50.10	12433	63.05	2894	73.05	378
37.10	2812	51.05	3761	63.90	291	74.05	1331
38.05	2721	51.90	219	64.10	186	75.00	3758
39.15	930	52.20	52	64.30	68	76.10	356
40.00	172	54.90	69	64.90	515	76.90	151
43.90	445	56.00	345	66.00	52	77.30	111
45.05	636	56.15	758	66.80	119	78.00	145
47.00	138	57.05	2056	68.00	7209	78.20	138
47.20	296	59.95	600	69.00	7507	78.95	2827
48.05	500	61.00	3730	70.00	780	80.05	792
49.05	2693	62.10	3821	72.10	549	80.95	2527

Average of 12.848 to 12.860 min.: VN076976.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.90	628	104.80	73	129.05	172	147.95	187
87.05	1748	105.65	155	129.90	217	154.80	77
88.00	2117	106.15	204	130.10	133	154.95	135
90.95	405	110.90	54	130.80	93	156.90	150
92.00	2126	113.00	56	131.00	56	158.70	55
93.05	3396	115.80	111	134.90	145	171.90	494
94.05	8919	115.95	266	136.85	149	172.70	350
95.10	66187	117.00	726	141.00	1000	173.00	173
96.10	4484	117.90	399	142.00	118	174.05	51104
97.00	62	118.95	623	143.00	1501	175.05	3742
103.80	461	127.90	372	144.90	298	176.05	49891

Average of 12.848 to 12.860 min.: VN076976.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
177.05	3006						
281.10	107						
281.30	65						

Instrument :

MSVOA_N

ClientSampleId :

BFB