

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031424\
 Data File : VN081417.D
 Acq On : 14 Mar 2024 18:05
 Operator : JC\MD
 Sample : P1749-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-2A

Quant Time: Mar 15 01:16:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030524W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 06 03:12:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	299220	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	555208	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	470684	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	182718	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	231838	53.587	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	107.180%
35) Dibromofluoromethane	8.171	113	175520	51.600	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	103.200%
50) Toluene-d8	10.571	98	656245	51.608	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	103.220%
62) 4-Bromofluorobenzene	12.847	95	204267	45.450	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	=	90.900%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031424\
Data File : VN081417.D
Acq On : 14 Mar 2024 18:05
Operator : JC\MD
Sample : P1749-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-2A

Quant Time: Mar 15 01:16:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030524W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 06 03:12:57 2024
Response via : Initial Calibration




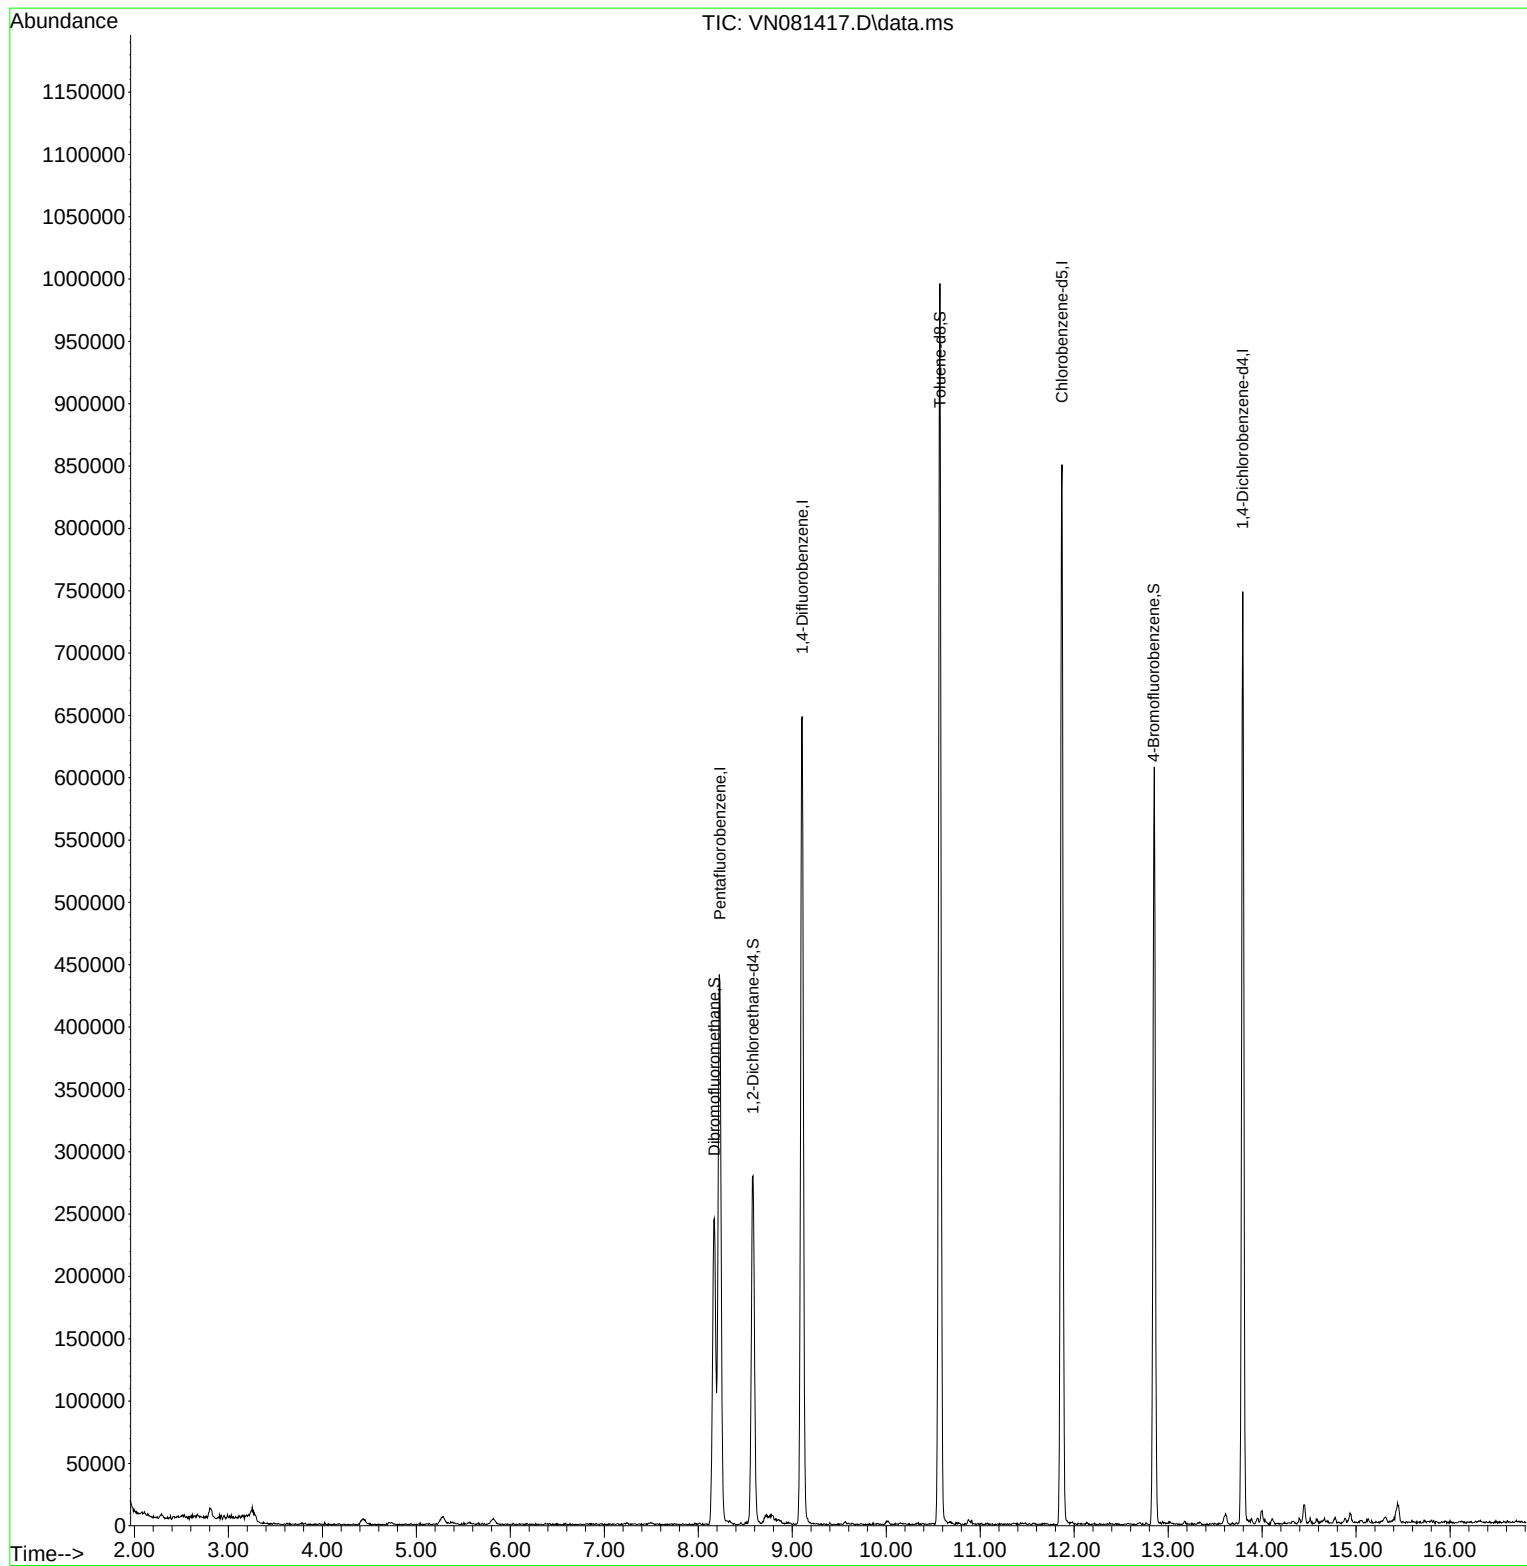


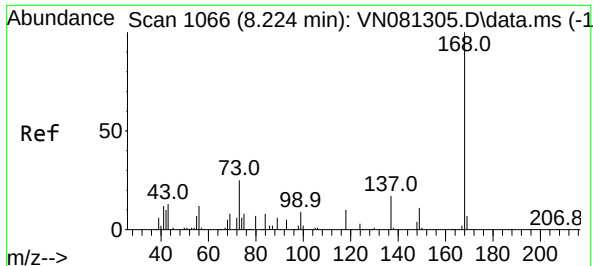

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VN081417.D
Acq: 14 Mar 2024 18:05




Instrument :
MSVOA_N
ClientSampleId :
MW-2A


Tgt Ion:168 Resp: 299220
Ion Ratio Lower Upper
168 100
99 65.8 59.9 89.9

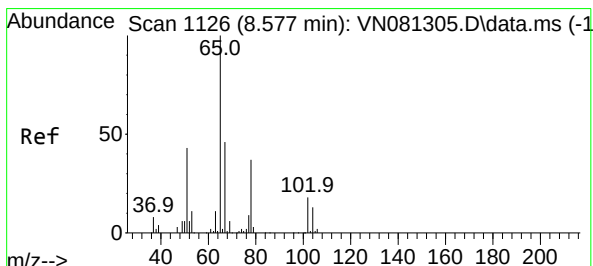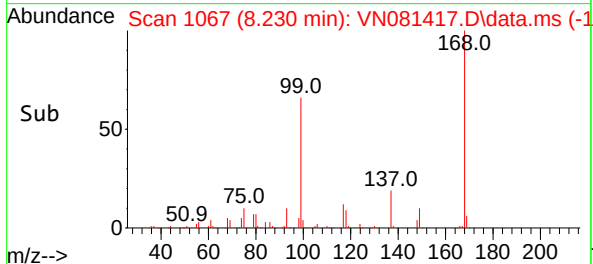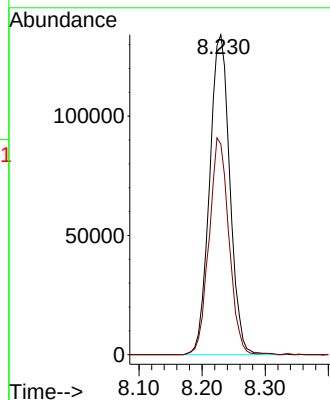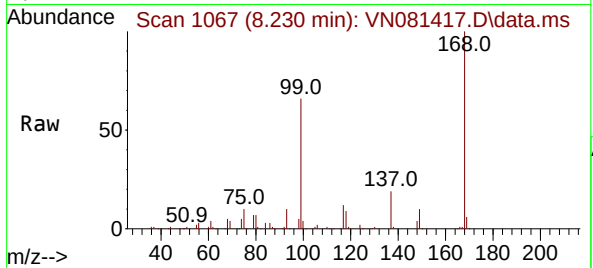

#33
1,2-Dichloroethane-d4
Concen: 53.587 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. 0.006 min
Lab File: VN081417.D
Acq: 14 Mar 2024 18:05

Tgt Ion: 65 Resp: 231838
Ion Ratio Lower Upper
65 100
67 52.5 0.0 102.4


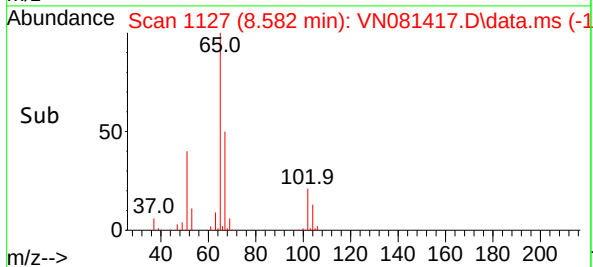
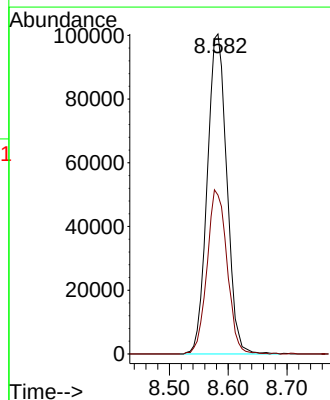
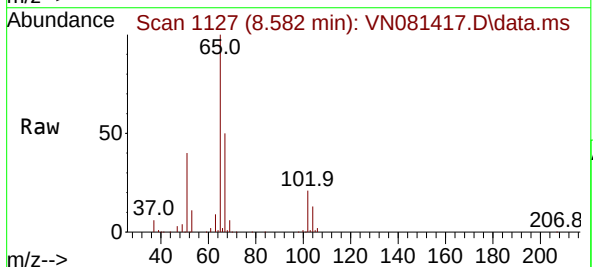


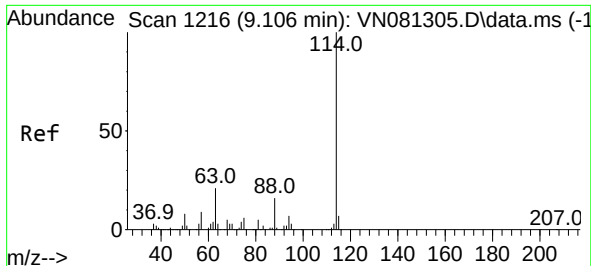

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN081417.D
Acq: 14 Mar 2024 18:05




Instrument :
MSVOA_N
ClientSampleId :
MW-2A


Tgt Ion:114 Resp: 555208
Ion Ratio Lower Upper
114 100
63 18.0 0.0 48.0
88 14.9 0.0 34.8

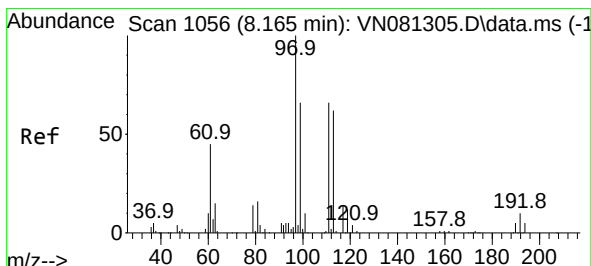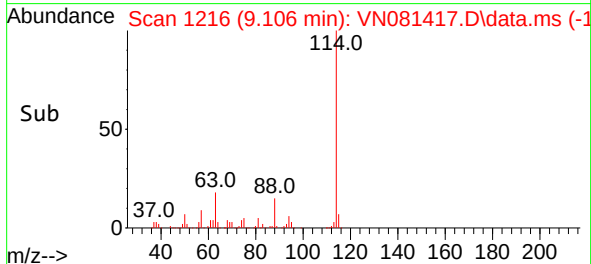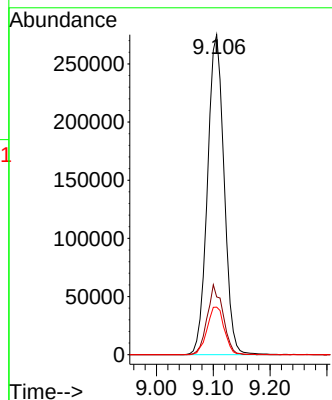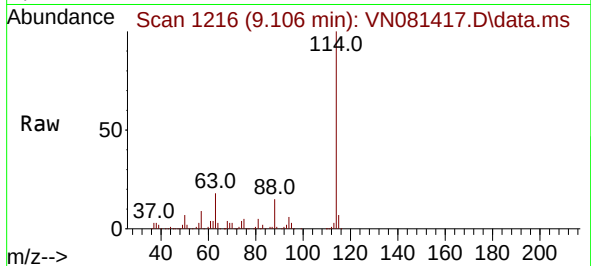

#35
Dibromofluoromethane
Concen: 51.600 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. 0.006 min
Lab File: VN081417.D
Acq: 14 Mar 2024 18:05

Tgt Ion:113 Resp: 175520
Ion Ratio Lower Upper
113 100
111 103.2 82.2 123.4
192 15.7 12.5 18.7


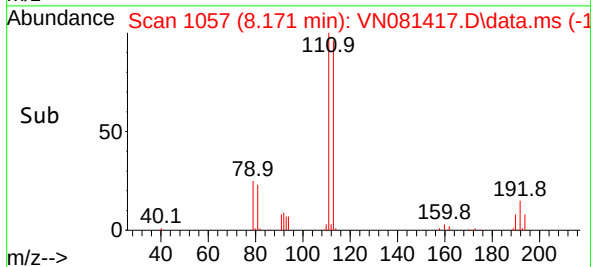
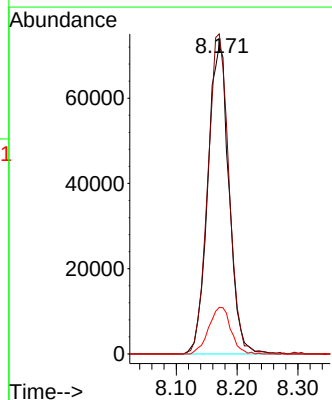
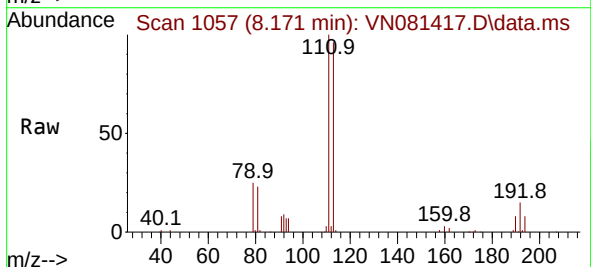


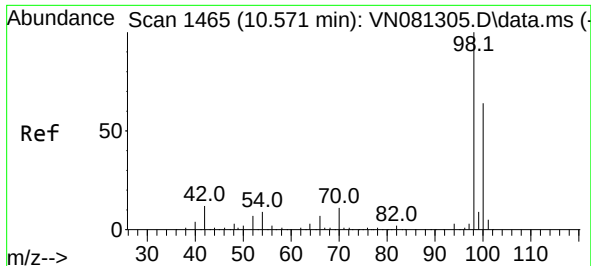

#50
Toluene-d8
Concen: 51.608 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN081417.D
Acq: 14 Mar 2024 18:05




Instrument :
MSVOA_N
ClientSampleId :
MW-2A


Tgt Ion: 98 Resp: 656245
Ion Ratio Lower Upper
98 100
100 65.4 51.4 77.0

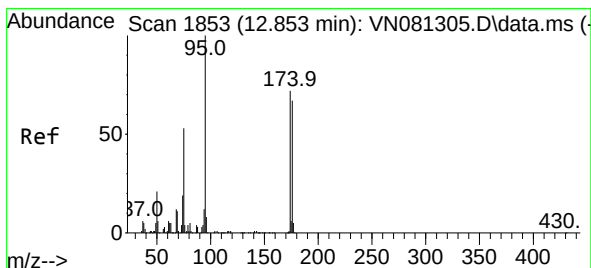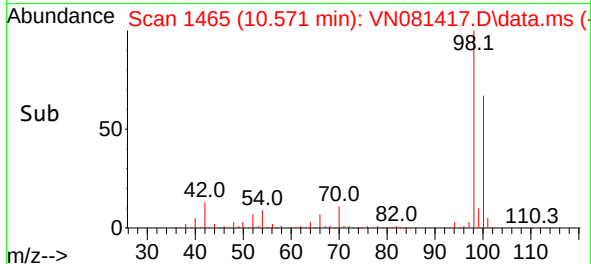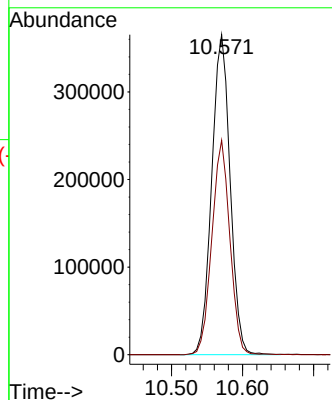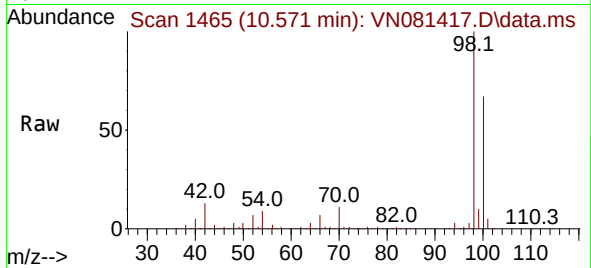

#62
4-Bromofluorobenzene
Concen: 45.450 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.006 min
Lab File: VN081417.D
Acq: 14 Mar 2024 18:05

Tgt Ion: 95 Resp: 204267
Ion Ratio Lower Upper
95 100
174 69.8 0.0 120.4
176 66.1 0.0 121.0


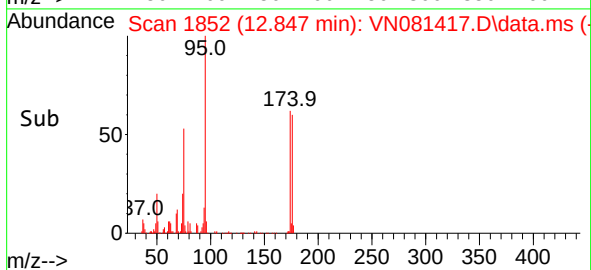
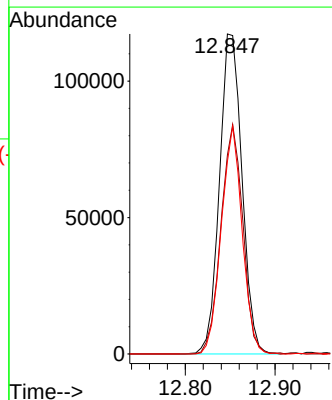
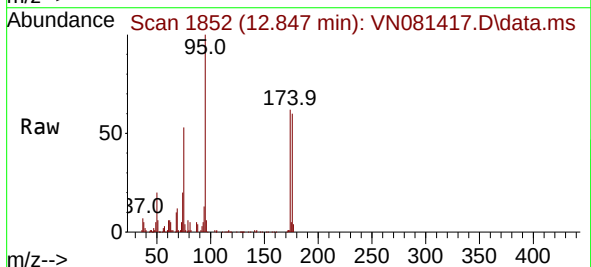


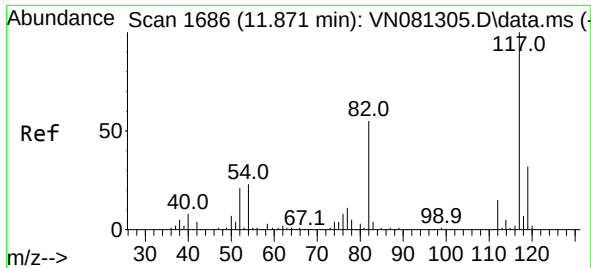

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN081417.D
Acq: 14 Mar 2024 18:05

Instrument :
MSVOA_N
ClientSampleId :
MW-2A

Tgt Ion:117 Resp: 470684
Ion Ratio Lower Upper
117 100
82 56.8 52.7 79.1
119 32.3 25.3 37.9

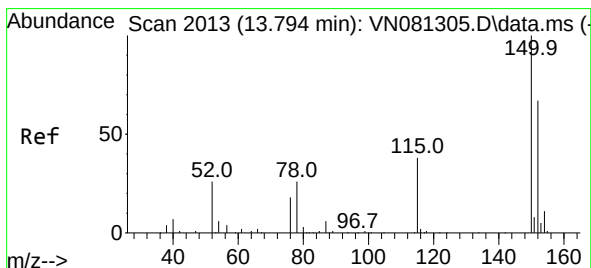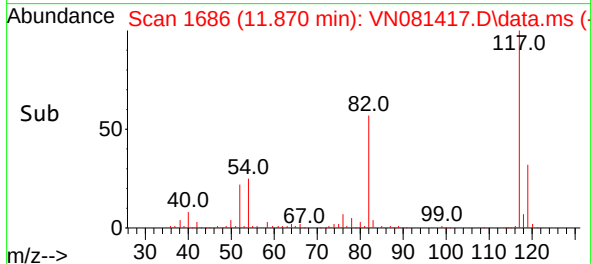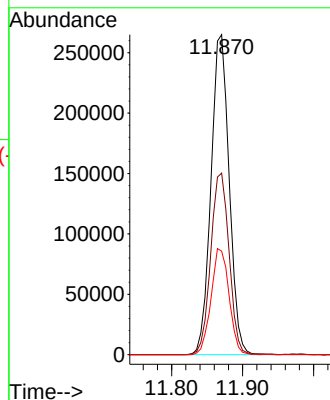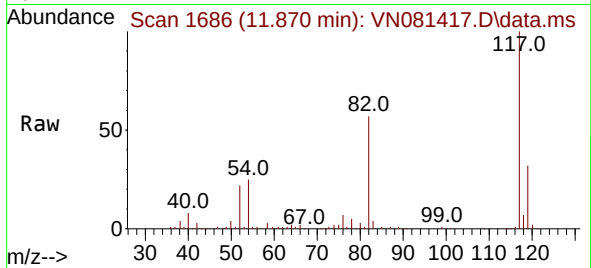

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN081417.D
Acq: 14 Mar 2024 18:05

Tgt Ion:152 Resp: 182718
Ion Ratio Lower Upper
152 100
115 63.9 32.3 96.8
150 157.2 0.0 339.8

