
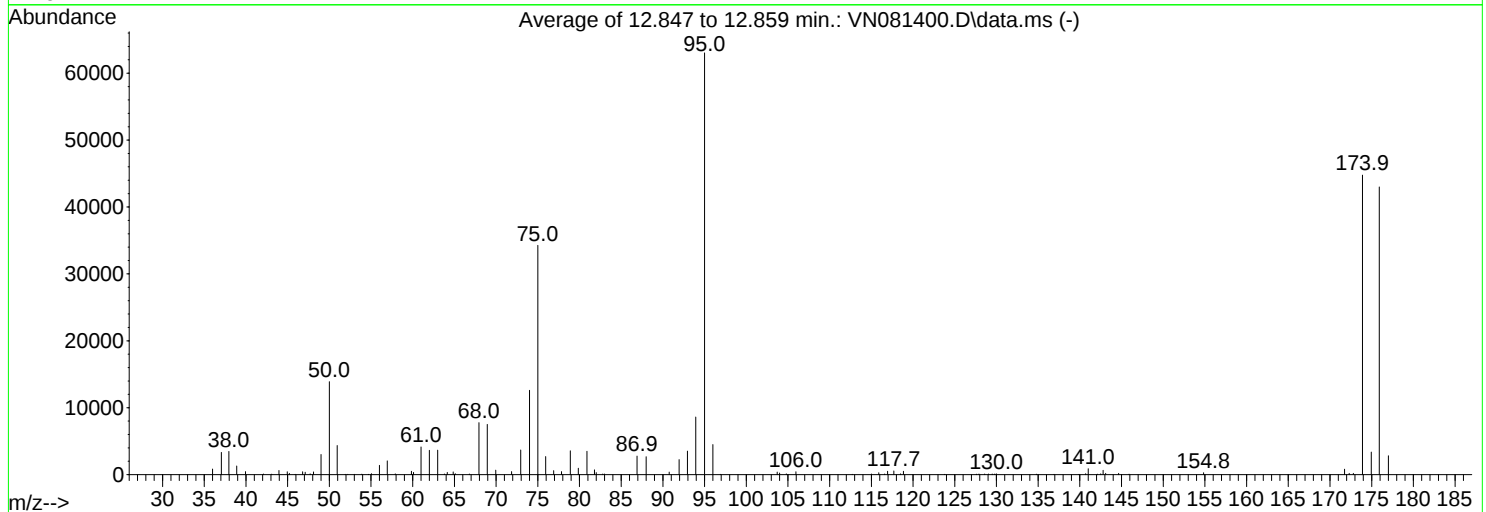


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031424\
Data File : VN081400.D
Acq On : 14 Mar 2024 10:49
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030524W.M
Title : SW846 8260
Last Update : Wed Mar 06 03:12:57 2024

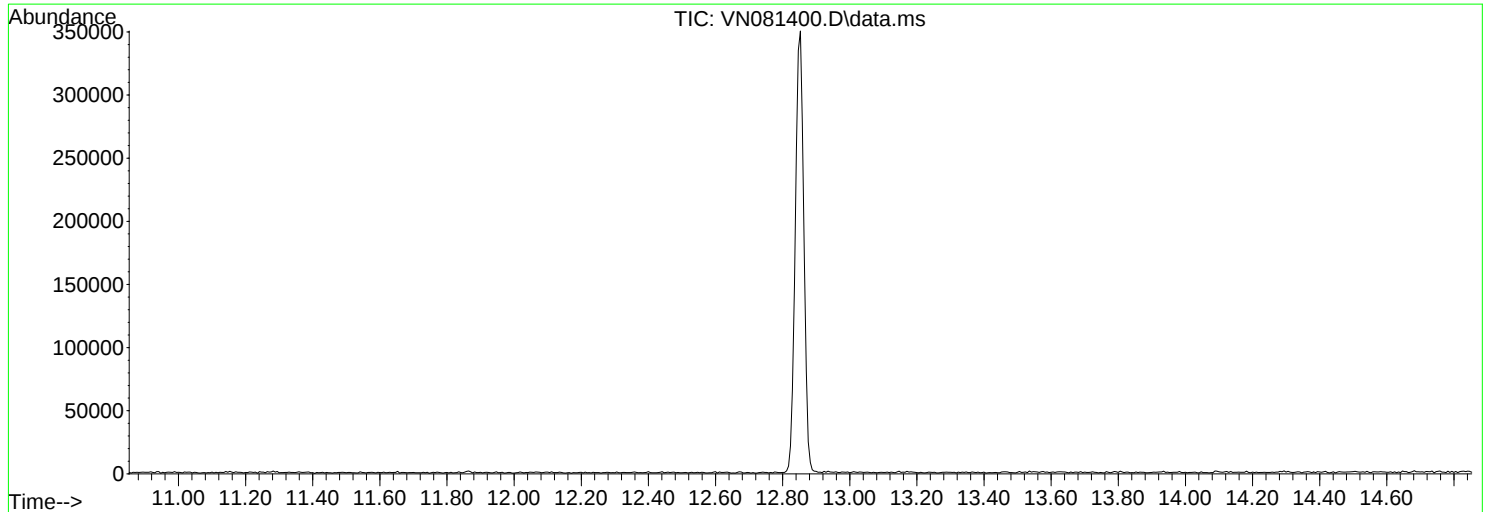

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	13902	PASS
75	95	30	60	54.4	34264	PASS
95	95	100	100	100.0	63043	PASS
96	95	5	9	7.1	4502	PASS
173	174	0.00	2	0.4	201	PASS
174	95	50	100	71.0	44757	PASS
175	174	5	9	7.5	3368	PASS
176	174	95	101	96.1	42997	PASS
177	176	5	9	6.6	2830	PASS

Average of 12.847 to 12.859 min.: VN081400.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	839	46.80	431	54.70	60	64.15	32
37.05	3338	47.10	350	55.05	147	64.85	40
37.95	3461	47.70	127	56.00	1377	65.10	14
38.90	1288	48.10	413	56.95	2058	66.80	10
39.95	455	49.00	3005	57.90	119	67.95	7782
42.10	95	50.00	13902	59.85	505	68.95	7521
43.10	79	50.95	4360	60.10	327	69.95	678
43.95	629	51.90	60	61.00	4146	71.85	453
44.95	425	52.20	55	62.00	3642	72.95	3687
45.20	207	53.00	51	63.00	3668	74.00	12611
45.90	57	53.90	84	63.80	90	75.00	34264

Average of 12.847 to 12.859 min.: VN081400.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.95	2700	88.00	2680	105.95	422	127.90	108
76.90	604	90.75	395	112.70	52	128.60	105
77.85	454	91.95	2240	115.00	97	129.05	106
78.90	3566	92.95	3527	115.90	283	129.50	93
79.85	968	93.95	8611	116.60	108	129.80	95
80.90	3499	95.00	63043	116.95	513	130.00	121
81.80	718	96.00	4502	117.70	560	134.80	64
82.00	301	96.90	58	118.50	126	136.90	62
82.80	102	103.70	379	118.85	499	139.90	52
83.00	106	104.00	239	123.80	55	140.70	155
86.90	2778	104.80	121	127.60	65	141.00	884

Average of 12.847 to 12.859 min.: VN081400.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
142.10	70	174.95	3368				
142.50	135	175.90	42997				
142.80	659	177.00	2830				
143.10	202						
144.65	201						
145.90	69						
154.85	276						
171.75	814						
172.30	188						
172.80	201						
173.90	44757						

Instrument :

MSVOA_N

ClientSampleId :

BFB