
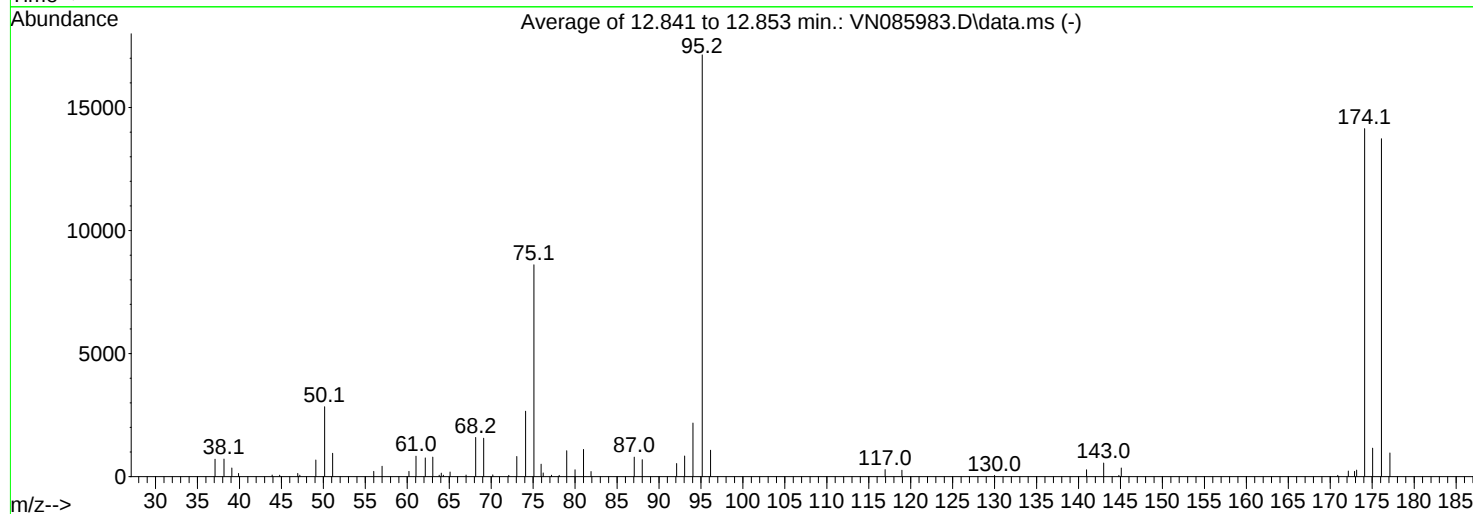


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031425\
Data File : VN085983.D
Acq On : 14 Mar 2025 09:42
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Title : SW846 8260
Last Update : Wed Feb 19 03:43:32 2025

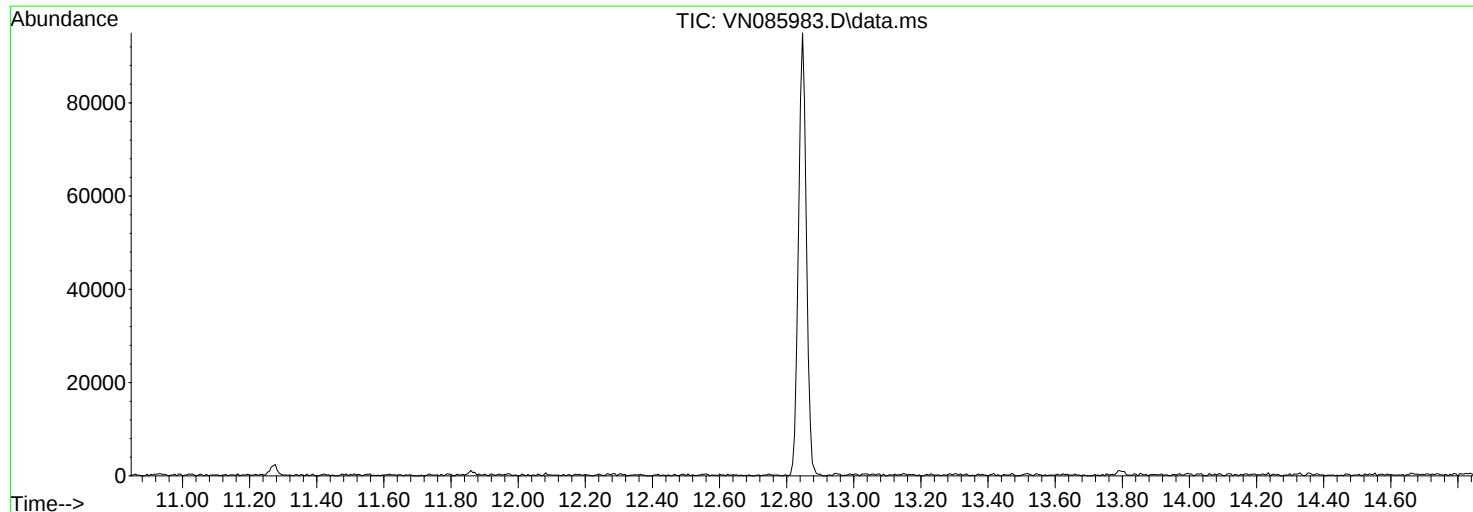

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.6	2844	PASS
75	95	30	60	50.2	8606	PASS
95	95	100	100	100.0	17140	PASS
96	95	5	9	6.2	1070	PASS
173	174	0.00	2	1.9	269	PASS
174	95	50	100	82.5	14141	PASS
175	174	5	9	8.2	1158	PASS
176	174	95	101	97.1	13732	PASS
177	176	5	9	7.0	963	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
37.10	711	56.00	215	68.15	1590	79.00	1051
38.15	714	57.00	424	69.10	1558	80.00	270
39.10	353	60.20	212	70.20	72	81.00	110
39.90	127	61.05	830	72.10	50	81.90	210
43.90	66	62.15	764	73.05	822	87.05	794
44.80	57	63.05	791	74.10	2657	88.00	687
46.95	128	63.80	56	75.10	8606	92.10	536
47.20	60	64.05	146	75.95	509	93.05	837
49.10	676	64.30	56	76.20	148	94.05	2179
50.15	2844	65.10	189	77.20	60	95.15	17140
51.10	951	67.00	65	78.10	55	96.15	1070

Average of 12.841 to 12.853 min.: VN085983.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.95	284	174.10	14141				
118.95	259	175.05	1158				
130.00	52	176.10	13732				
140.95	278	177.10	963				
143.00	556						
144.80	54						
145.10	354						
170.90	54						
172.15	226						
172.90	213						
173.15	269						

Instrument :

MSVOA_N

ClientSampleId :

BFB