


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031519\
Data File : VN054304.D
Acq On : 15 Mar 2019 12:02
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
Title : SW846 8260
Last Update : Wed Mar 13 03:33:31 2019

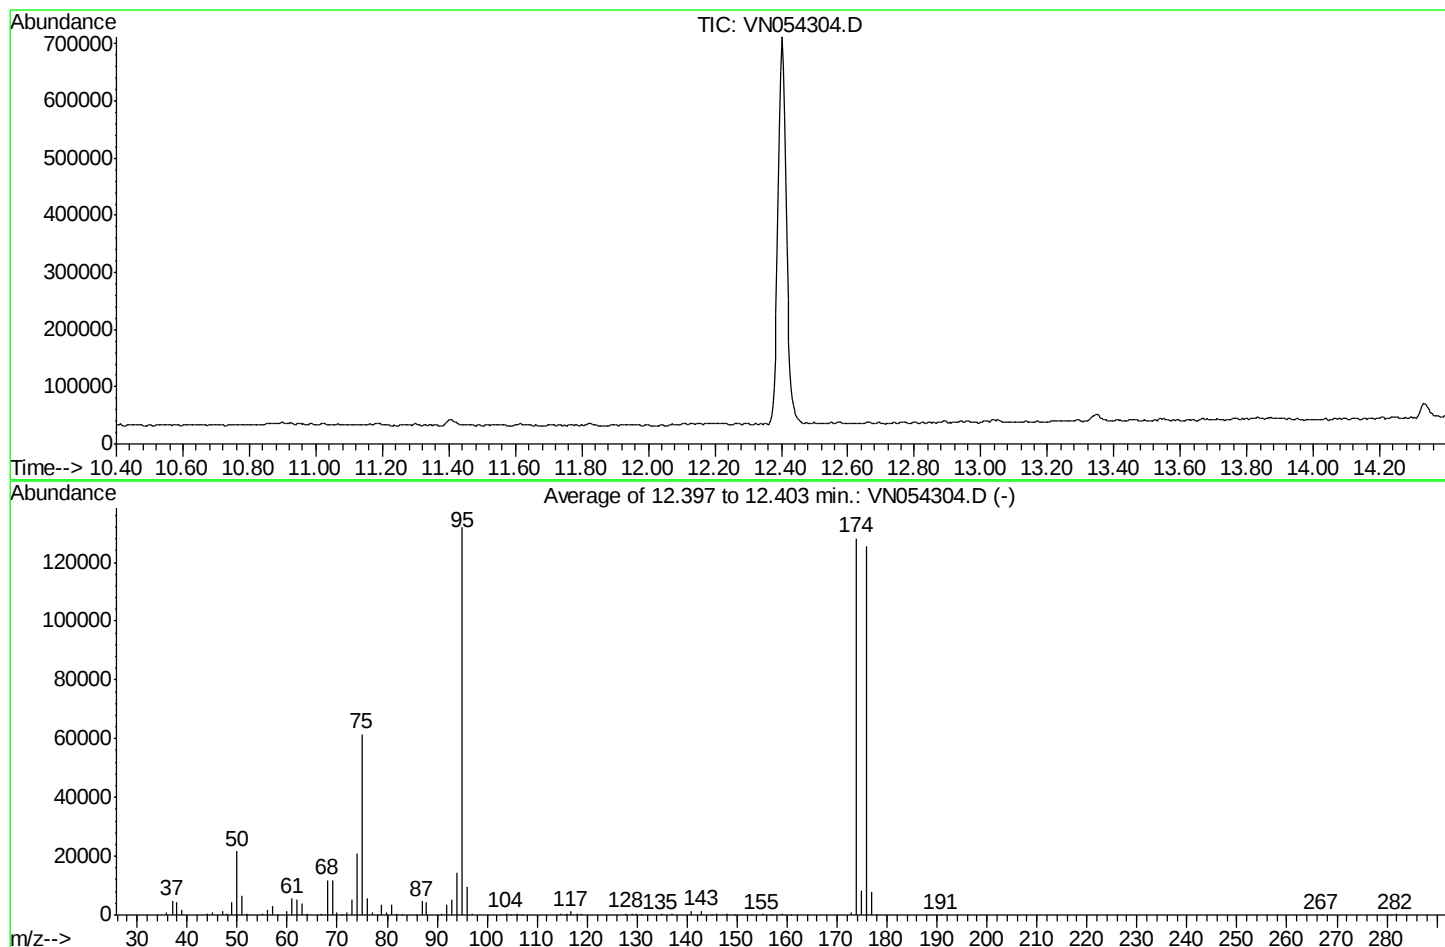

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	21746	PASS
75	95	30	60	46.7	61576	PASS
95	95	100	100	100.0	131936	PASS
96	95	5	9	7.4	9803	PASS
173	174	0.00	2	0.8	1070	PASS
174	95	50	100	97.1	128098	PASS
175	174	5	9	6.6	8476	PASS
176	174	95	101	98.1	125629	PASS
177	176	5	9	6.4	7978	PASS