


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031521\
 Data File : VN066197.D
 Acq On : 15 Mar 2021 9:09
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031221W.M
 Title : SW846 8260
 Last Update : Fri Mar 12 13:00:23 2021

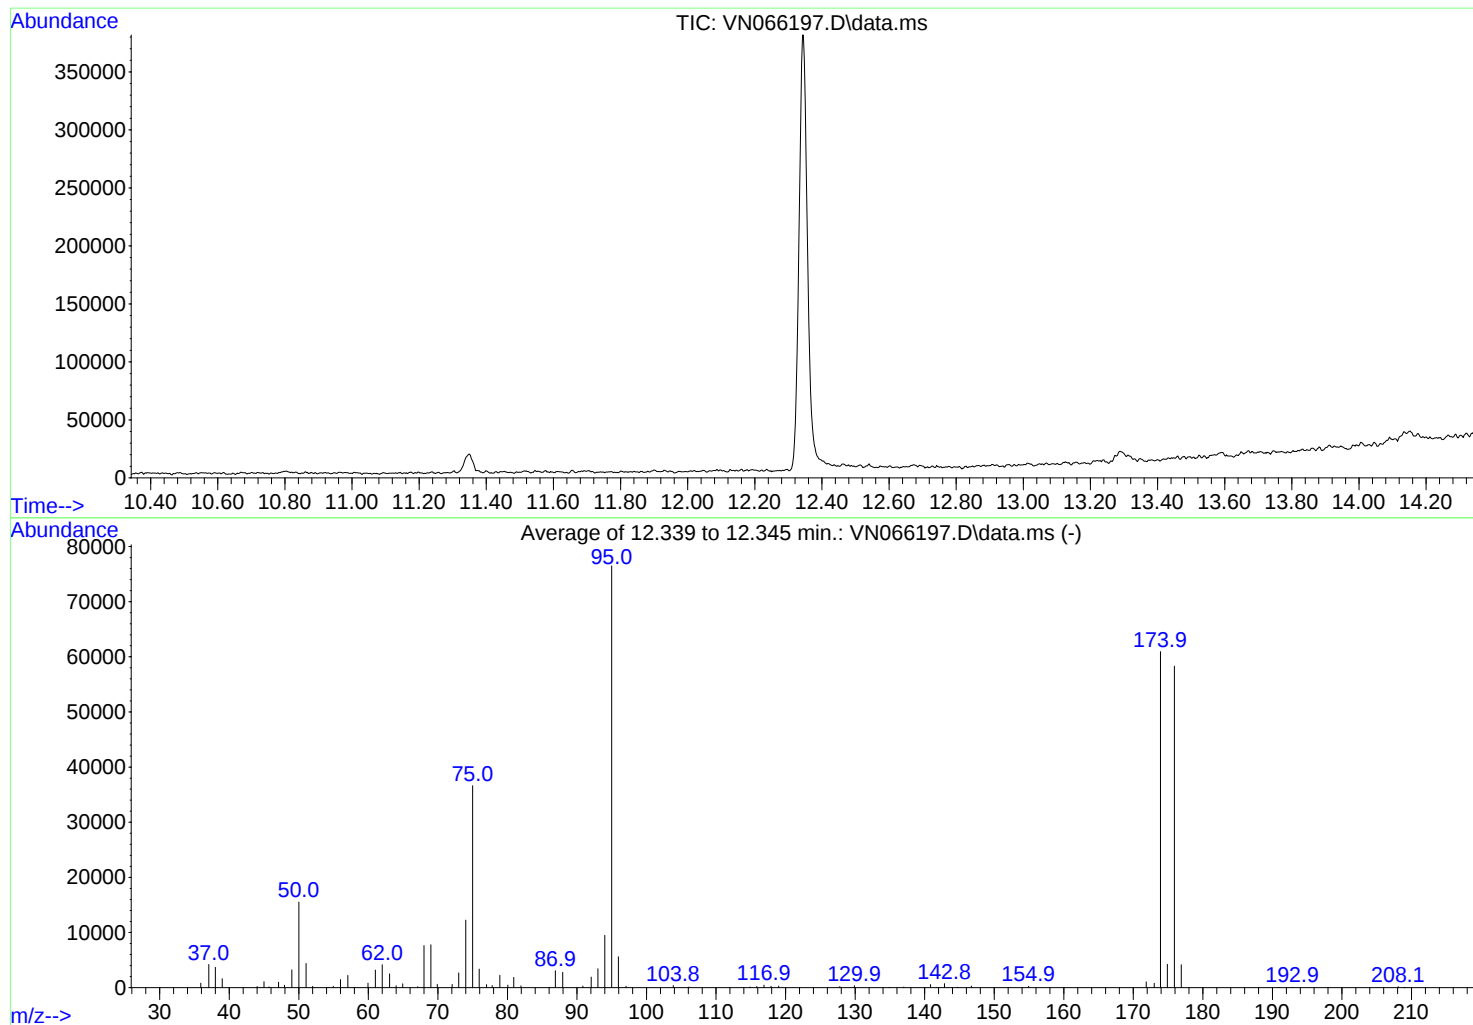

AutoFind: Scans 3971, 3972, 3973; Background Corrected with Scan 3956

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	15527	PASS
75	95	30	60	47.9	36637	PASS
95	95	100	100	100.0	76501	PASS
96	95	5	9	7.3	5595	PASS
173	174	0.00	2	1.3	785	PASS
174	95	50	100	79.7	60949	PASS
175	174	5	9	6.9	4225	PASS
176	174	95	101	95.7	58307	PASS
177	176	5	9	7.1	4161	PASS