

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031522\
 Data File : VN071296.D
 Acq On : 15 Mar 2022 16:52
 Operator : JC\MD
 Sample : PB143286ZHE#12
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB143286ZHE#12

Quant Time: Mar 16 08:02:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 08 06:52:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.087	168	767957	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1290470	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1196751	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.669	152	415617	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	492462	46.789	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	93.580%		
35) Dibromofluoromethane	8.022	113	375476	46.108	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	92.220%		
50) Toluene-d8	10.439	98	1603145	48.895	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	97.800%		
62) 4-Bromofluorobenzene	12.727	95	507851	45.742	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	91.480%		
Target Compounds						Qvalue
3) Chloromethane	2.299	50	2811	0.214	ug/l	95
5) Bromomethane	2.875	94	1954	Below Cal	#	57
13) Acrolein	4.052	56	912	0.417	ug/l #	71
15) Acrylonitrile	5.557	53	1615	0.263	ug/l #	24
16) Acetone	4.293	43	33056	6.455	ug/l	95
18) Methyl Acetate	4.857	43	23189	2.140	ug/l	94
20) Methylene Chloride	5.099	84	16235	2.103	ug/l	93
25) 2-Butanone	7.334	43	7787	0.944	ug/l	99
29) Tetrahydrofuran	7.698	42	1388	0.243	ug/l #	46
31) Cyclohexane	8.081	56	16265	0.968	ug/l #	1
36) 1,1-Dichloropropene	8.081	75	58678	4.497	ug/l #	49
38) Carbon Tetrachloride	8.081	117	75427	5.977	ug/l #	17
43) Isopropyl Acetate	8.563	43	129663	4.829	ug/l #	79
45) 1,2-Dichloropropane	9.616	63	5612	0.532	ug/l #	44
48) Methyl methacrylate	9.539	41	20854	1.676	ug/l #	9
49) 1,4-Dioxane	9.563	88	119	0.550	ug/l #	1
51) 4-Methyl-2-Pentanone	10.328	43	16192	0.972	ug/l	92
54) cis-1,3-Dichloropropene	10.239	75	119096	7.533	ug/l #	60
57) 1,3-Dichloropropane	11.086	76	76546	4.396	ug/l #	43
58) 2-Chloroethyl Vinyl ether	10.039	63	72	27.884	ug/l #	45
59) 2-Hexanone	11.086	43	1168972	102.808	ug/l #	49
74) N-amyl acetate	12.386	43	5152	0.342	ug/l #	87
75) 1,1,2,2-Tetrachloroethane	12.822	83	908	Below Cal	#	90
76) 1,2,3-Trichloropropane	12.727	75	263453	24.727	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.057	105	11643	0.374	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.727	75	263453	68.523	ug/l #	5
92) 1,2-Dibromo-3-Chloropr...	14.592	75	529	0.227	ug/l	72
93) 1,2,4-Trichlorobenzene	15.257	180	3084	3.415	ug/l	96
95) Naphthalene	15.498	128	9254	5.504	ug/l #	95
96) 1,2,3-Trichlorobenzene	15.698	180	3253	3.203	ug/l	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031522\
Data File : VN071296.D
Acq On : 15 Mar 2022 16:52
Operator : JC\MD
Sample : PB143286ZHE#12
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB143286ZHE#12

Quant Time: Mar 16 08:02:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 08 06:52:46 2022
Response via : Initial Calibration




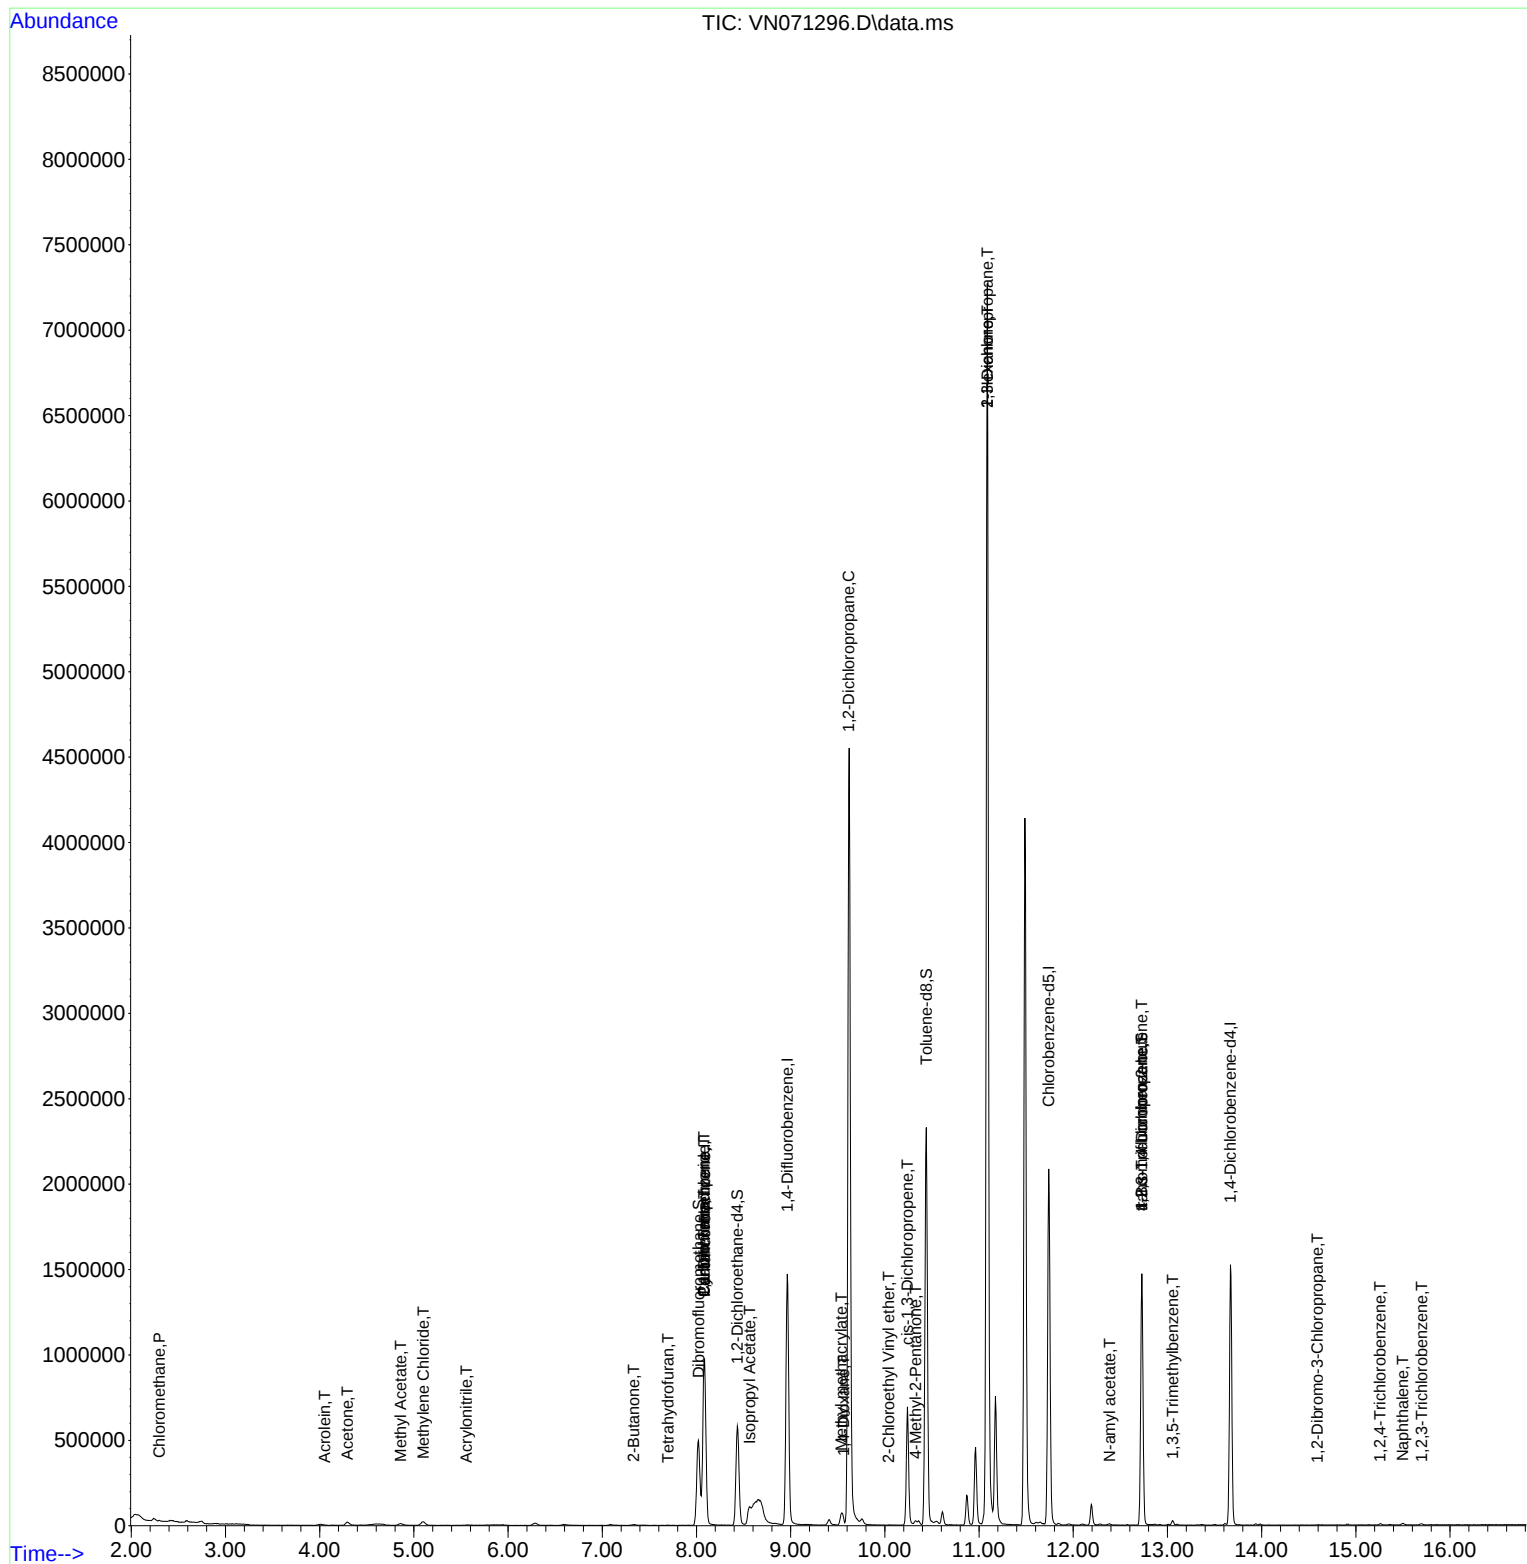




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.087 min Scan# 10
Delta R.T. 0.001 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52




Instrument :
MSVOA_N
ClientSampleId :
PB143286ZHE#12


Tgt Ion:168 Resp: 767957
Ion Ratio Lower Upper
168 100
99 56.6 41.3 61.9

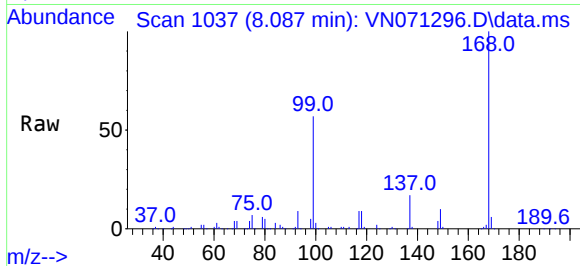

#3
Chloromethane
Concen: 0.214 ug/l
RT: 2.299 min Scan# 53
Delta R.T. -0.000 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52

Tgt Ion: 50 Resp: 2811
Ion Ratio Lower Upper
50 100
52 34.4 25.4 38.0




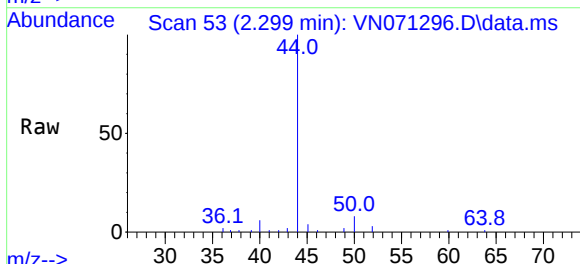




#5
Bromomethane
Concen: Below Cal
RT: 2.875 min Scan# 11
Delta R.T. 0.041 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52




Instrument :
MSVOA_N
ClientSampleId :
PB143286ZHE#12


Tgt Ion: 94 Resp: 1954
Ion Ratio Lower Upper
94 100
96 51.5 73.8 110.8#

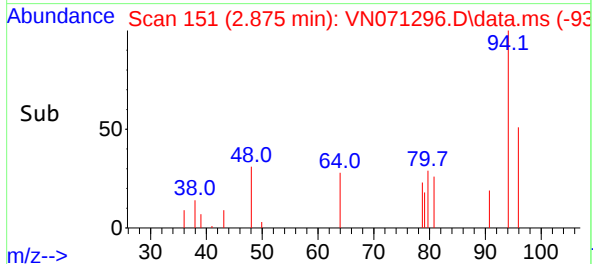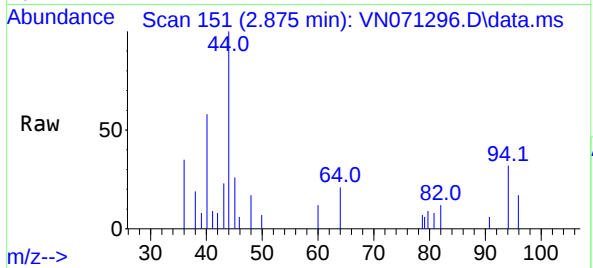

#13
Acrolein
Concen: 0.417 ug/l
RT: 4.052 min Scan# 351
Delta R.T. 0.012 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52

Tgt Ion: 56 Resp: 912
Ion Ratio Lower Upper
56 100
55 46.8 56.6 85.0#


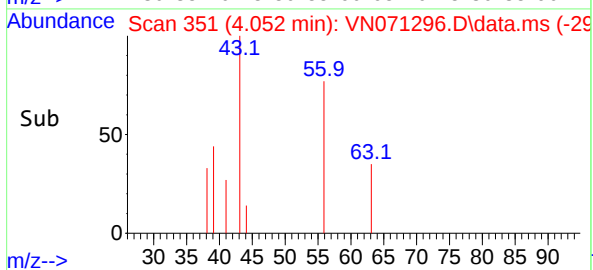

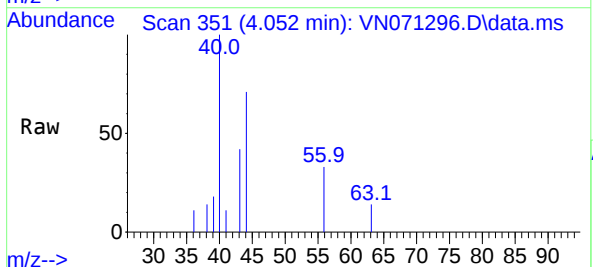




#15
Acrylonitrile
Concen: 0.263 ug/l
RT: 5.557 min Scan# 606
Delta R.T. 0.006 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52




Instrument :
MSVOA_N
ClientSampleId :
PB143286ZHE#12


Tgt Ion: 53 Resp: 1615
Ion Ratio Lower Upper
53 100
52 0.0 66.2 99.2#
51 13.2 29.6 44.4#



#16
Acetone
Concen: 6.455 ug/l
RT: 4.293 min Scan# 392
Delta R.T. 0.006 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52

Tgt Ion: 43 Resp: 33056
Ion Ratio Lower Upper
43 100
58 26.4 23.1 34.7


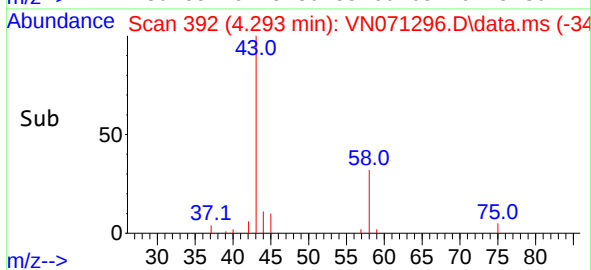






#18
Methyl Acetate
Concen: 2.140 ug/l
RT: 4.857 min Scan# 488
Delta R.T. 0.006 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52




Instrument :
MSVOA_N
ClientSampleId :
PB143286ZHE#12


Tgt Ion: 43 Resp: 23189
Ion Ratio Lower Upper
43 100
74 21.2 19.4 29.2



#20
Methylene Chloride
Concen: 2.103 ug/l
RT: 5.099 min Scan# 529
Delta R.T. 0.006 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52

Tgt Ion: 84 Resp: 16235
Ion Ratio Lower Upper
84 100
49 128.3 93.5 140.3
51 35.9 29.4 44.2
86 68.3 53.0 79.4

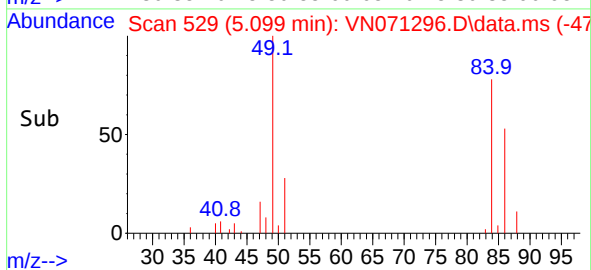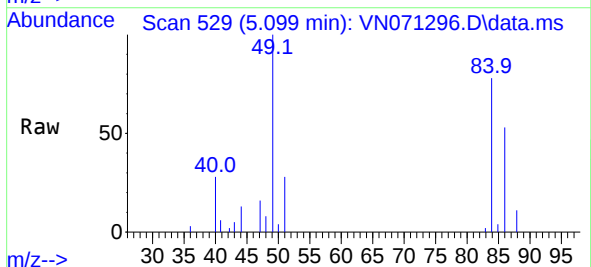



#25

2-Butanone

Concen: 0.944 ug/l

RT: 7.334 min Scan# 909

Delta R.T. 0.000 min

Lab File: VN071296.D

Acq: 15 Mar 2022 16:52

Instrument :

MSVOA_N

ClientSampleId :





PB143286ZHE#12

Tgt Ion: 43 Resp: 7787

Ion Ratio Lower Upper

43 100

72 26.5 21.7 32.5

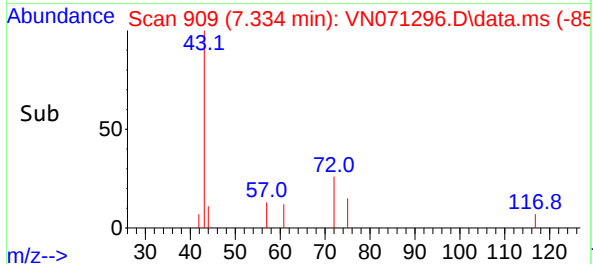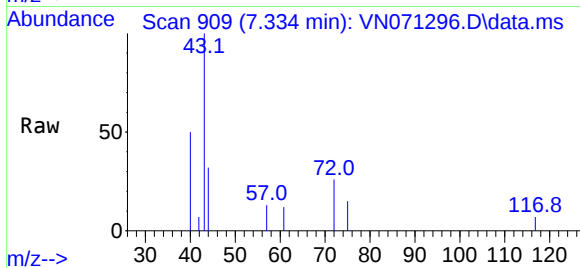

#29

Tetrahydrofuran

Concen: 0.243 ug/l

RT: 7.698 min Scan# 971

Delta R.T. 0.018 min

Lab File: VN071296.D

Acq: 15 Mar 2022 16:52




Tgt Ion: 42 Resp: 1388


Ion Ratio Lower Upper

42 100

72 0.0 36.3 54.5#

71 18.4 34.7 52.1#

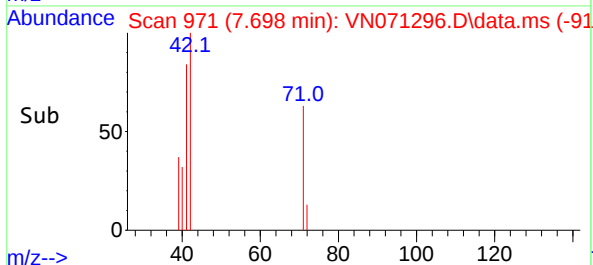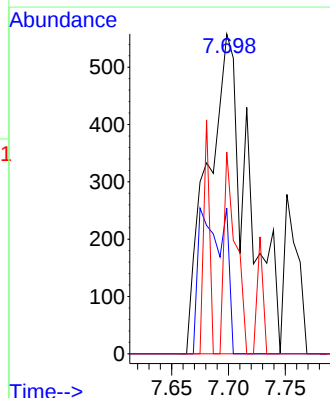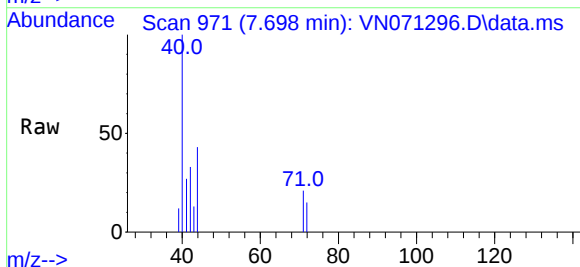



#31

Cyclohexane

Concen: 0.968 ug/l

RT: 8.081 min Scan# 1036

Delta R.T. -0.012 min

Lab File: VN071296.D

Acq: 15 Mar 2022 16:52

Instrument :

MSVOA_N

ClientSampleId :

PB143286ZHE#12





Tgt Ion: 56 Resp: 16265

Ion Ratio Lower Upper

56 100

69 166.3 27.1 40.7#

84 156.1 73.4 110.0#

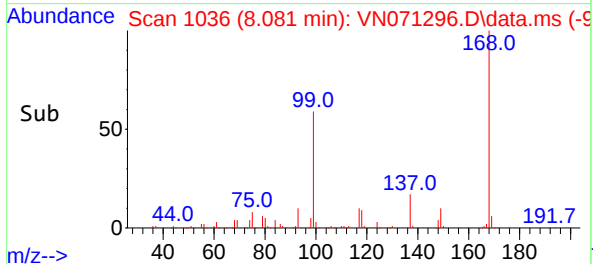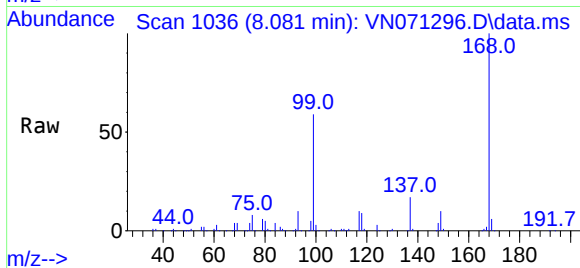

#33

1,2-Dichloroethane-d4

Concen: 46.789 ug/l

RT: 8.434 min Scan# 1096

Delta R.T. -0.006 min

Lab File: VN071296.D




Acq: 15 Mar 2022 16:52


Tgt Ion: 65 Resp: 492462

Ion Ratio Lower Upper

65 100

67 52.8 0.0 103.0

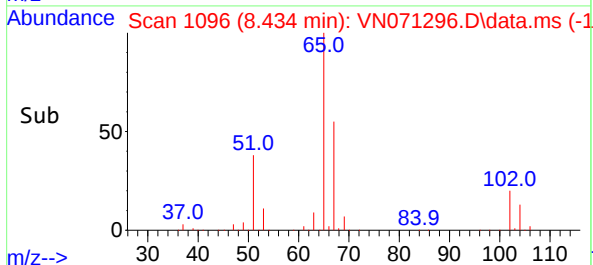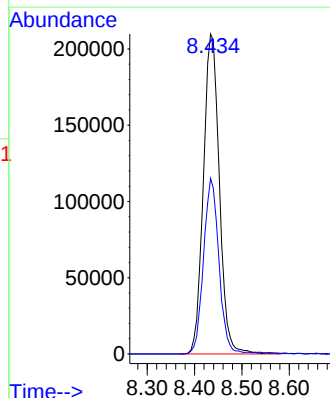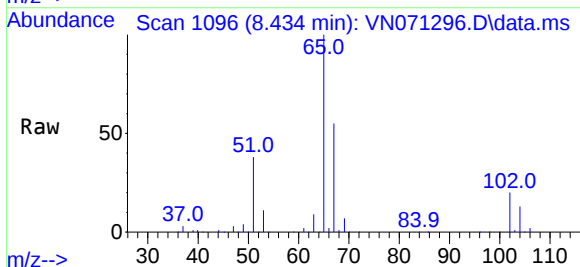



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. 0.000 min

Lab File: VN071296.D

Acq: 15 Mar 2022 16:52

Instrument :

MSVOA_N

ClientSampleId :

PB143286ZHE#12





Tgt Ion:114 Resp: 1290470

Ion Ratio Lower Upper

114 100

63 21.8 0.0 37.8

88 16.3 0.0 27.4

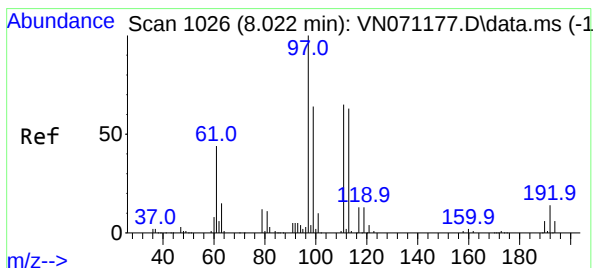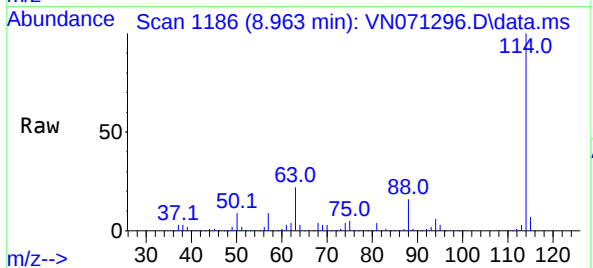

#35

Dibromofluoromethane

Concen: 46.108 ug/l

RT: 8.022 min Scan# 1026

Delta R.T. 0.000 min

Lab File: VN071296.D

Acq: 15 Mar 2022 16:52




Tgt Ion:113 Resp: 375476


Ion Ratio Lower Upper

113 100

111 102.9 82.2 123.2

192 20.1 16.9 25.3

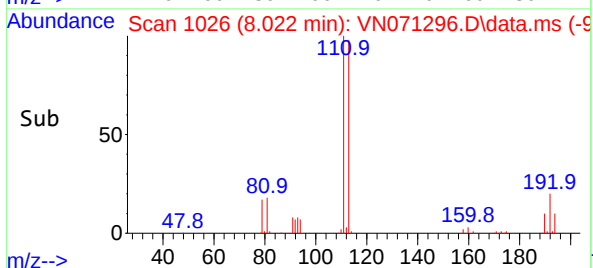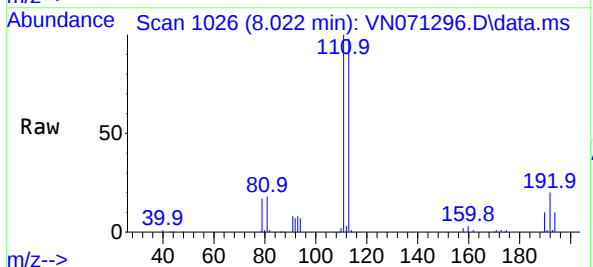

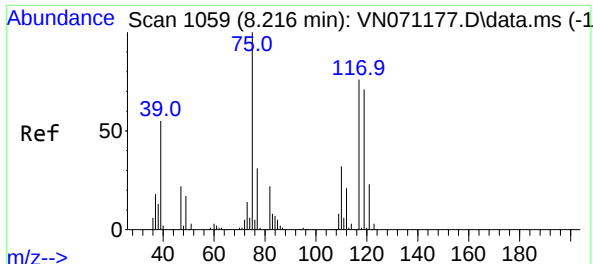

#36

1,1-Dichloropropene

Concen: 4.497 ug/l

RT: 8.081 min Scan# 1036

Delta R.T. -0.135 min

Lab File: VN071296.D

Acq: 15 Mar 2022 16:52

Instrument :

MSVOA_N

ClientSampleId :

PB143286ZHE#12





Tgt Ion: 75 Resp: 58678

Ion Ratio Lower Upper

75 100

110 9.3 18.4 55.2#

77 0.0 24.4 36.6#

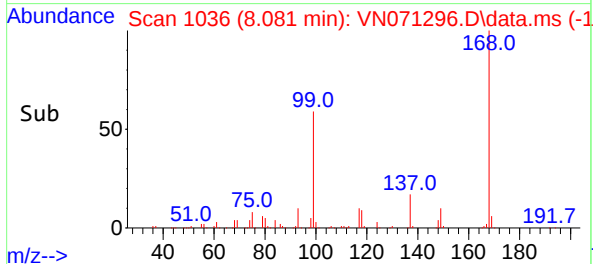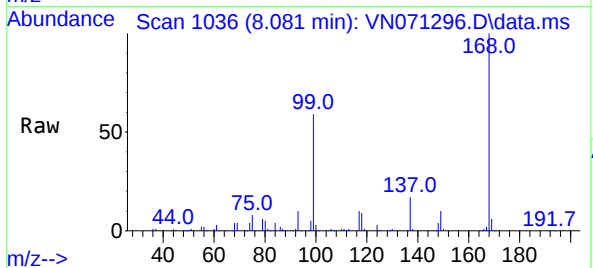

#38

Carbon Tetrachloride

Concen: 5.977 ug/l

RT: 8.081 min Scan# 1036

Delta R.T. -0.123 min

Lab File: VN071296.D

Acq: 15 Mar 2022 16:52




Tgt Ion: 117 Resp: 75427


Ion Ratio Lower Upper

117 100

119 5.7 76.1 114.1#

121 0.0 24.2 36.2#


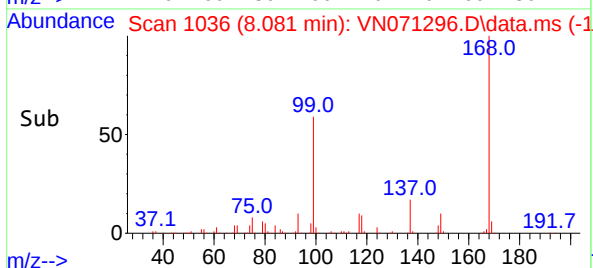
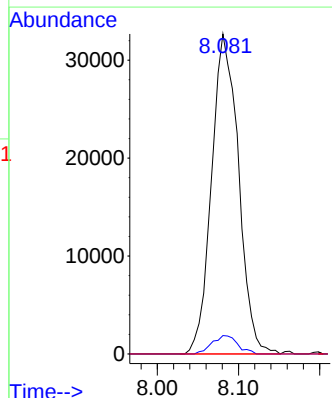
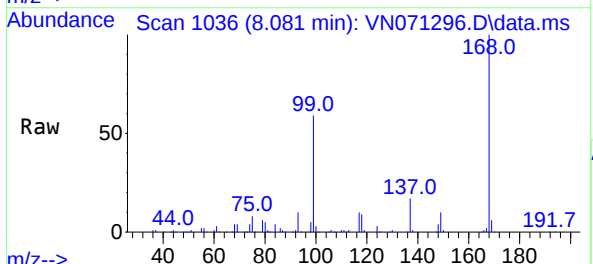




#43
Isopropyl Acetate
Concen: 4.829 ug/l
RT: 8.563 min Scan# 1117
Delta R.T. 0.006 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52




Instrument :
MSVOA_N
ClientSampleId :
PB143286ZHE#12


Tgt Ion: 43 Resp: 129663
Ion Ratio Lower Upper
43 100
61 13.7 20.4 30.6#
87 7.5 11.2 16.8#

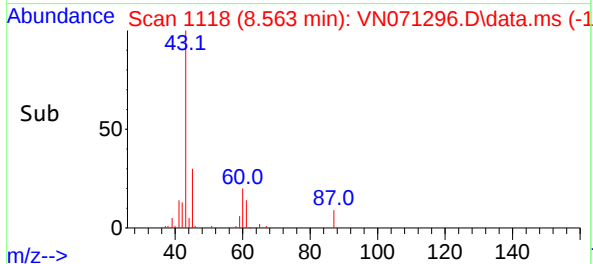

#45
1,2-Dichloropropane
Concen: 0.532 ug/l
RT: 9.616 min Scan# 1297
Delta R.T. 0.130 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52

Tgt Ion: 63 Resp: 5612
Ion Ratio Lower Upper
63 100
65 0.0 24.7 37.1#


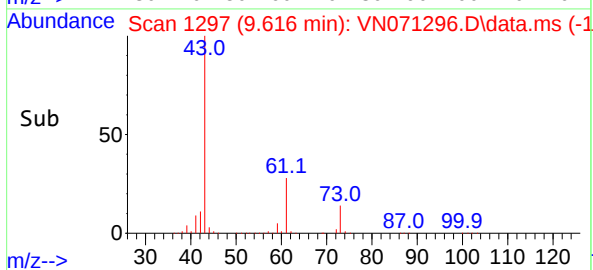

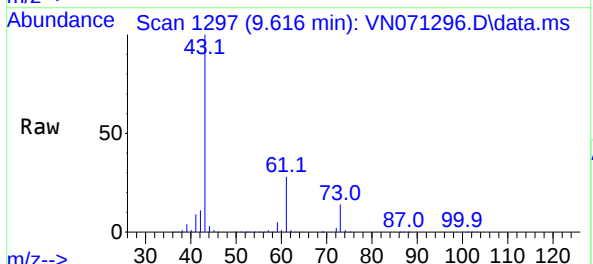




#48
Methyl methacrylate
Concen: 1.676 ug/l
RT: 9.539 min Scan# 1284
Delta R.T. -0.018 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52




Instrument :
MSVOA_N
ClientSampleId :
PB143286ZHE#12


Tgt Ion: 41 Resp: 20854
Ion Ratio Lower Upper
41 100
69 0.8 72.4 108.6#
39 0.0 58.4 87.6#

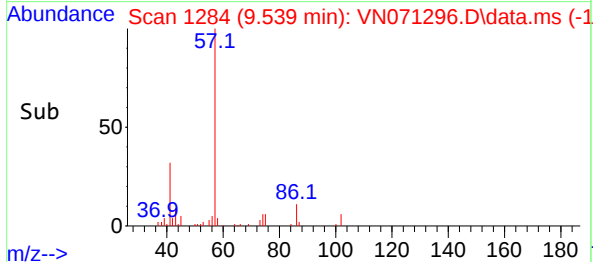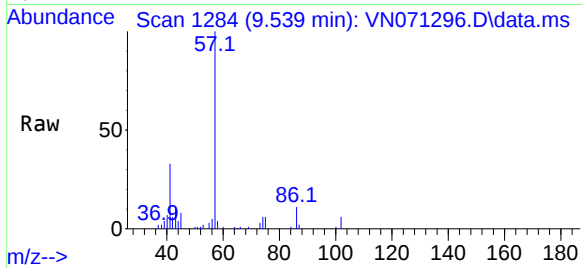

#49
1,4-Dioxane
Concen: 0.550 ug/l
RT: 9.563 min Scan# 1288
Delta R.T. -0.000 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52

Tgt Ion: 88 Resp: 119
Ion Ratio Lower Upper
88 100
43 0.0 23.4 35.2#
58 2885.7 50.6 75.8#


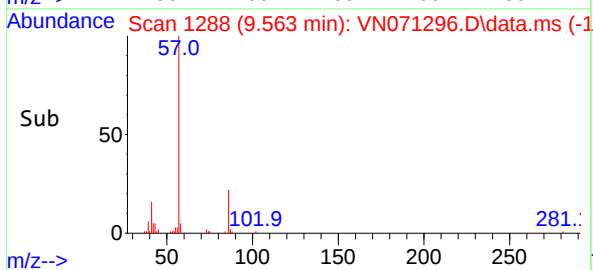

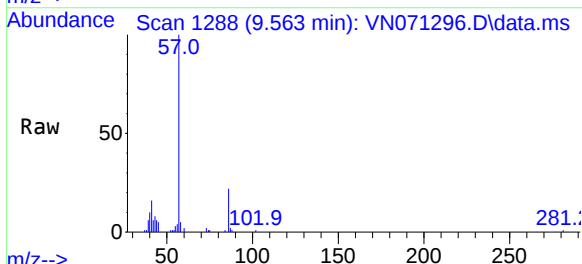




#50
Toluene-d8
Concen: 48.895 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52




Instrument :
MSVOA_N
ClientSampleId :
PB143286ZHE#12


Tgt Ion: 98 Resp: 1603145
Ion Ratio Lower Upper
98 100
100 65.4 50.4 75.6

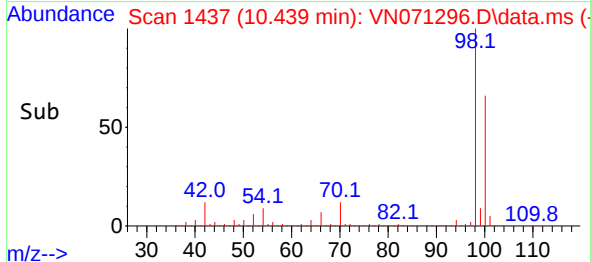

#51
4-Methyl-2-Pentanone
Concen: 0.972 ug/l
RT: 10.328 min Scan# 1418
Delta R.T. 0.001 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52

Tgt Ion: 43 Resp: 16192
Ion Ratio Lower Upper
43 100
58 43.0 30.4 45.6


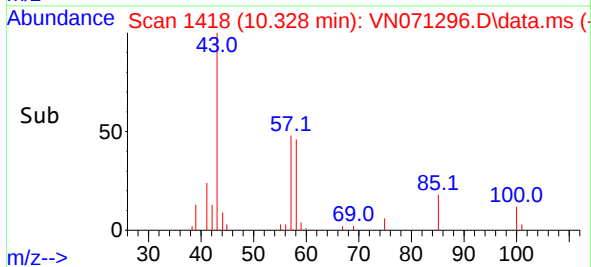

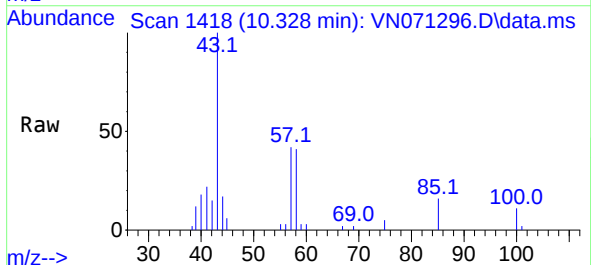




#54
 cis-1,3-Dichloropropene
 Concen: 7.533 ug/l
 RT: 10.239 min Scan# 1403
 Delta R.T. 0.053 min
 Lab File: VN071296.D
 Acq: 15 Mar 2022 16:52




Instrument :
 MSVOA_N
 ClientSampleId :
 PB143286ZHE#12


Tgt Ion: 75 Resp: 119096
 Ion Ratio Lower Upper
 75 100
 77 0.4 26.4 39.6#
 39 32.8 42.5 63.7#

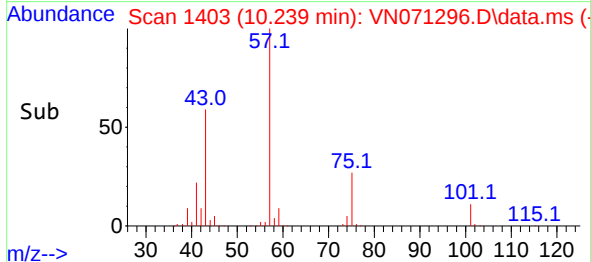

#57
 1,3-Dichloropropane
 Concen: 4.396 ug/l
 RT: 11.086 min Scan# 1547
 Delta R.T. 0.047 min
 Lab File: VN071296.D
 Acq: 15 Mar 2022 16:52

Tgt Ion: 76 Resp: 76546
 Ion Ratio Lower Upper
 76 100
 78 0.3 25.7 38.5#


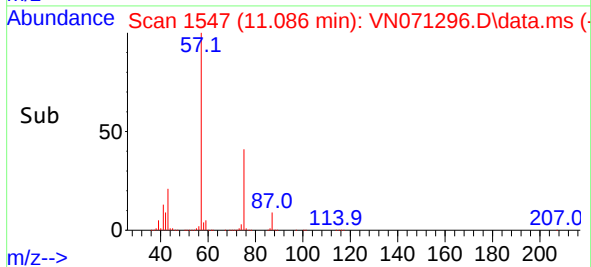

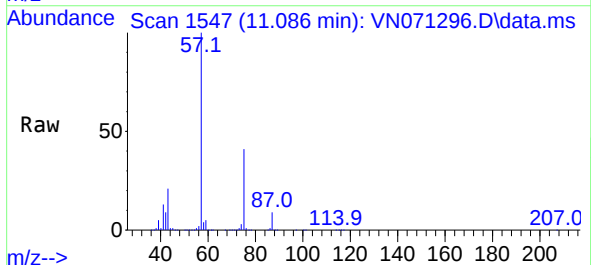




#58
2-Chloroethyl Vinyl ether
Concen: 27.884 ug/l
RT: 10.039 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52




Instrument :
MSVOA_N
ClientSampleId :
PB143286ZHE#12


Tgt Ion: 63 Resp: 72
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#

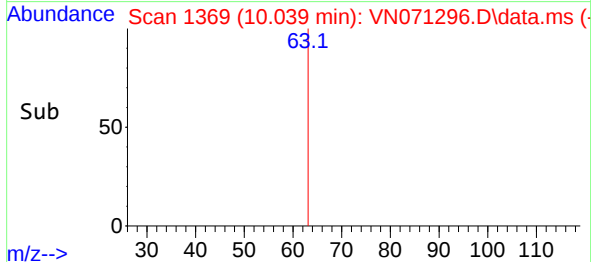

#59
2-Hexanone
Concen: 102.808 ug/l
RT: 11.086 min Scan# 1547
Delta R.T. 0.006 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52

Tgt Ion: 43 Resp: 1168972
Ion Ratio Lower Upper
43 100
58 17.5 26.9 80.7#


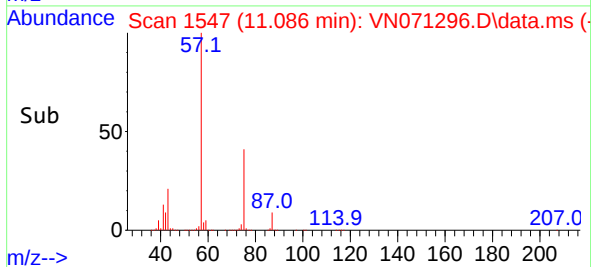

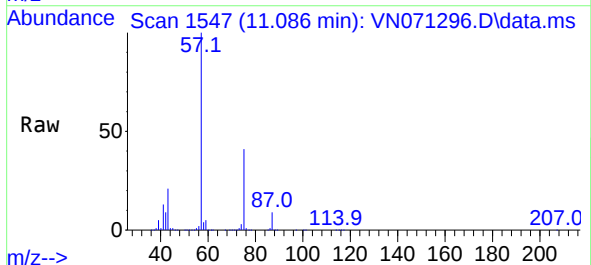




#62
4-Bromofluorobenzene
Concen: 45.742 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52




Instrument :
MSVOA_N
ClientSampleId :
PB143286ZHE#12


Tgt Ion: 95 Resp: 507851
Ion Ratio Lower Upper
95 100
174 79.6 0.0 187.2
176 75.9 0.0 181.4

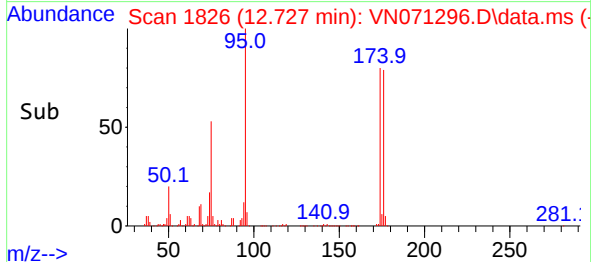

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1658
Delta R.T. 0.000 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52

Tgt Ion: 117 Resp: 1196751
Ion Ratio Lower Upper
117 100
82 59.7 42.4 63.6
119 31.5 25.4 38.2


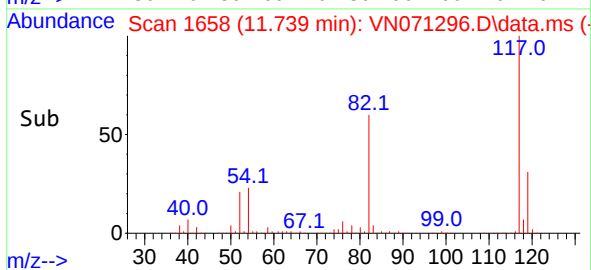






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.669 min Scan# 1986
Delta R.T. 0.001 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52




Instrument :
MSVOA_N
ClientSampleId :
PB143286ZHE#12


Tgt Ion:152 Resp: 415617
Ion Ratio Lower Upper
152 100
115 59.6 27.5 82.5
150 159.2 0.0 344.4



#74
N-ethyl acetate
Concen: 0.342 ug/l
RT: 12.386 min Scan# 1768
Delta R.T. 0.000 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52

Tgt Ion: 43 Resp: 5152
Ion Ratio Lower Upper
43 100
70 29.8 33.4 50.0#
55 26.2 19.3 28.9
61 17.3 18.5 27.7#


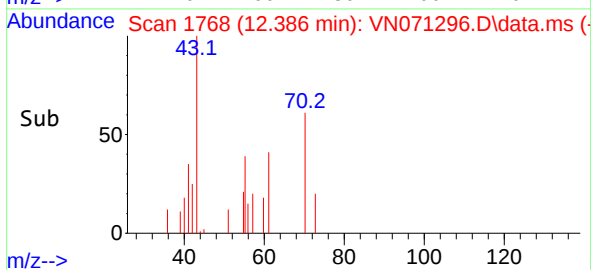






#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.822 min Scan# 1842
Delta R.T. 0.001 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52




Instrument :
MSVOA_N
ClientSampleId :
PB143286ZHE#12


Tgt Ion: 83 Resp: 908
Ion Ratio Lower Upper
83 100
131 0.0 5.5 16.5#
85 59.1 32.4 97.2

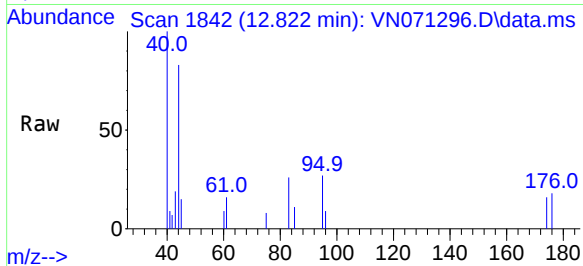

#76
1,2,3-Trichloropropane
Concen: 24.727 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52

Tgt Ion: 75 Resp: 263453
Ion Ratio Lower Upper
75 100
77 1.1 82.6 247.8#


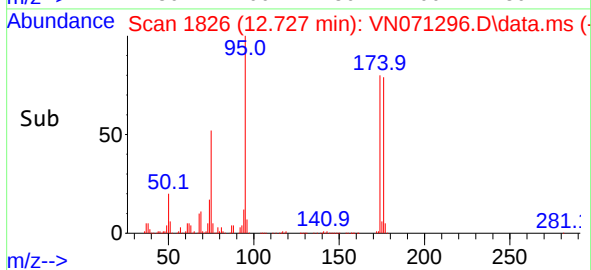

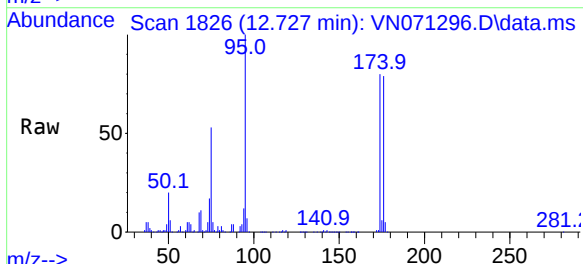




#80
1,3,5-Trimethylbenzene
Concen: 0.374 ug/l
RT: 13.057 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52




Instrument :
MSVOA_N
ClientSampleId :
PB143286ZHE#12


Tgt Ion:105 Resp: 11643
Ion Ratio Lower Upper
105 100
120 50.7 24.6 73.6



#81
trans-1,4-Dichloro-2-butene
Concen: 68.523 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.106 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52

Tgt Ion: 75 Resp: 263453
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#



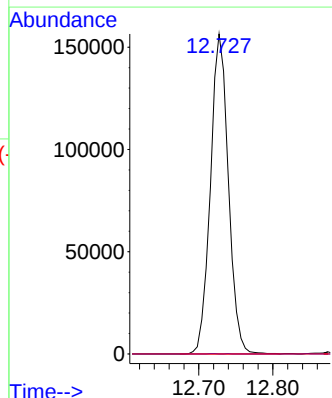



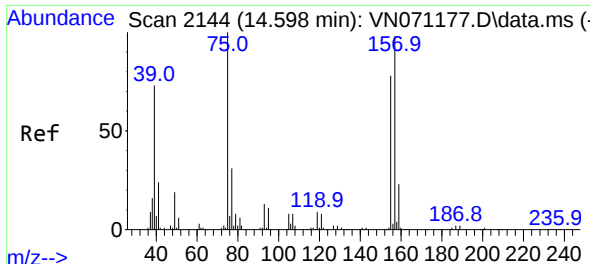

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.227 ug/l
 RT: 14.592 min Scan# 2143
 Delta R.T. -0.006 min
 Lab File: VN071296.D
 Acq: 15 Mar 2022 16:52




Instrument :
 MSVOA_N
 ClientSampleId :
 PB143286ZHE#12


Tgt Ion: 75 Resp: 529
 Ion Ratio Lower Upper
 75 100
 155 59.5 46.9 140.7
 157 95.5 60.6 181.7

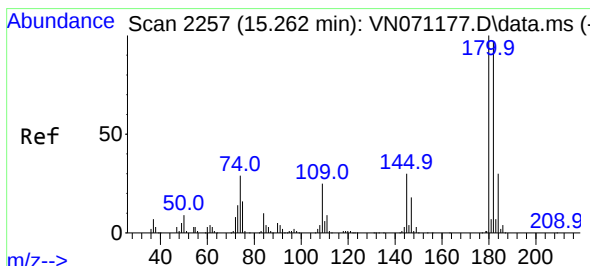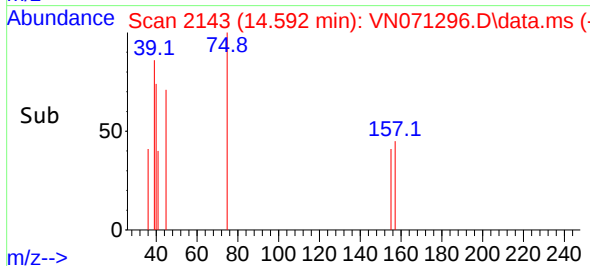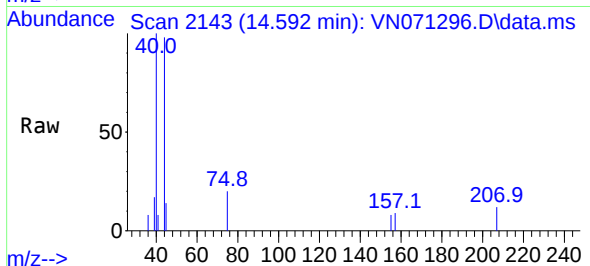

#93
 1,2,4-Trichlorobenzene
 Concen: 3.415 ug/l
 RT: 15.257 min Scan# 2256
 Delta R.T. -0.005 min
 Lab File: VN071296.D
 Acq: 15 Mar 2022 16:52

Tgt Ion: 180 Resp: 3084
 Ion Ratio Lower Upper
 180 100
 182 101.5 48.3 144.9
 145 30.4 14.5 43.5


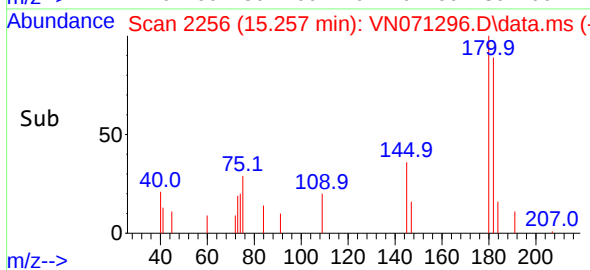

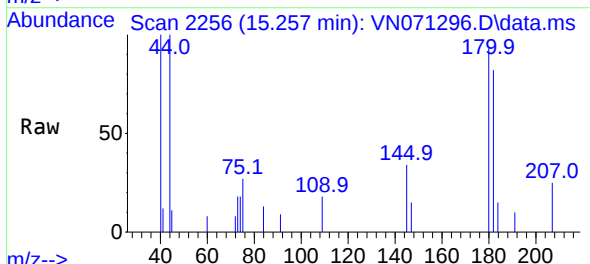




#95
Naphthalene
Concen: 5.504 ug/l
RT: 15.498 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52

Instrument :
MSVOA_N
ClientSampleId :
PB143286ZHE#12

Tgt Ion:128 Resp: 9254
Ion Ratio Lower Upper
128 100
127 11.5 10.5 15.7
129 8.4 8.7 13.1#

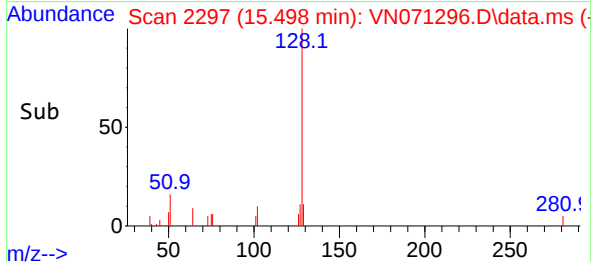

#96
1,2,3-Trichlorobenzene
Concen: 3.203 ug/l
RT: 15.698 min Scan# 2331
Delta R.T. -0.000 min
Lab File: VN071296.D
Acq: 15 Mar 2022 16:52

Tgt Ion:180 Resp: 3253
Ion Ratio Lower Upper
180 100
182 83.2 47.4 142.2
145 31.2 15.0 45.1

