


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031522\
Data File : VN071283.D
Acq On : 15 Mar 2022 11:04
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
Title : SW846 8260
Last Update : Tue Mar 08 06:52:46 2022

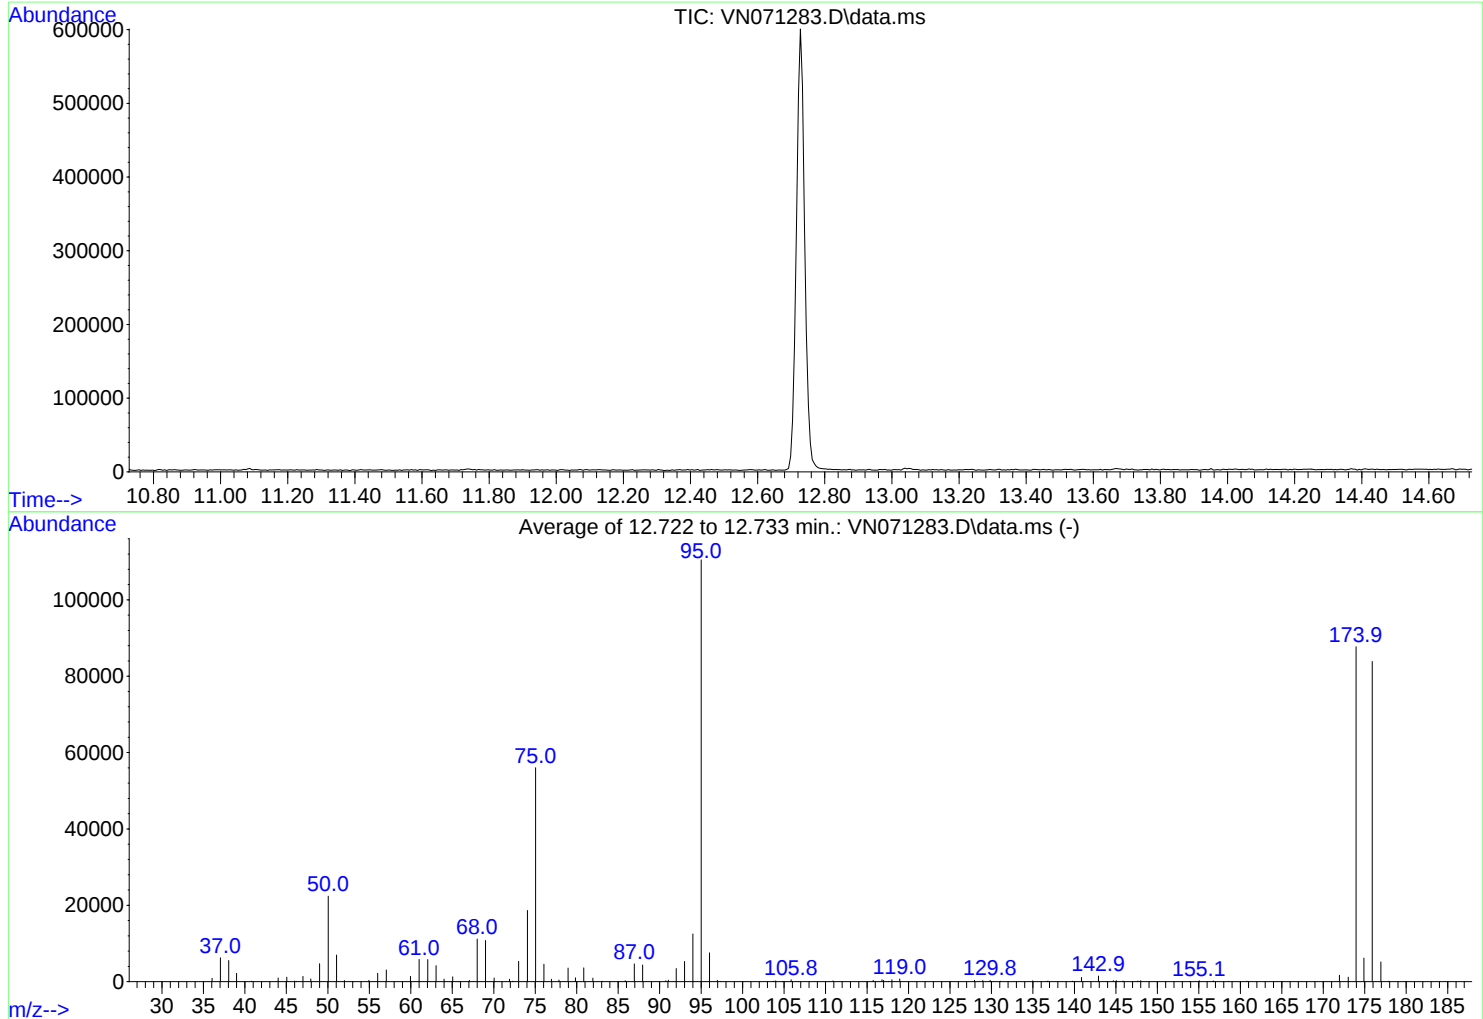

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1816

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	22365	PASS
75	95	30	60	50.7	56029	PASS
95	95	100	100	100.0	110483	PASS
96	95	5	9	6.8	7556	PASS
173	174	0.00	2	1.4	1187	PASS
174	95	50	100	79.4	87733	PASS
175	174	5	9	7.0	6173	PASS
176	174	95	101	95.6	83851	PASS
177	176	5	9	6.2	5179	PASS