
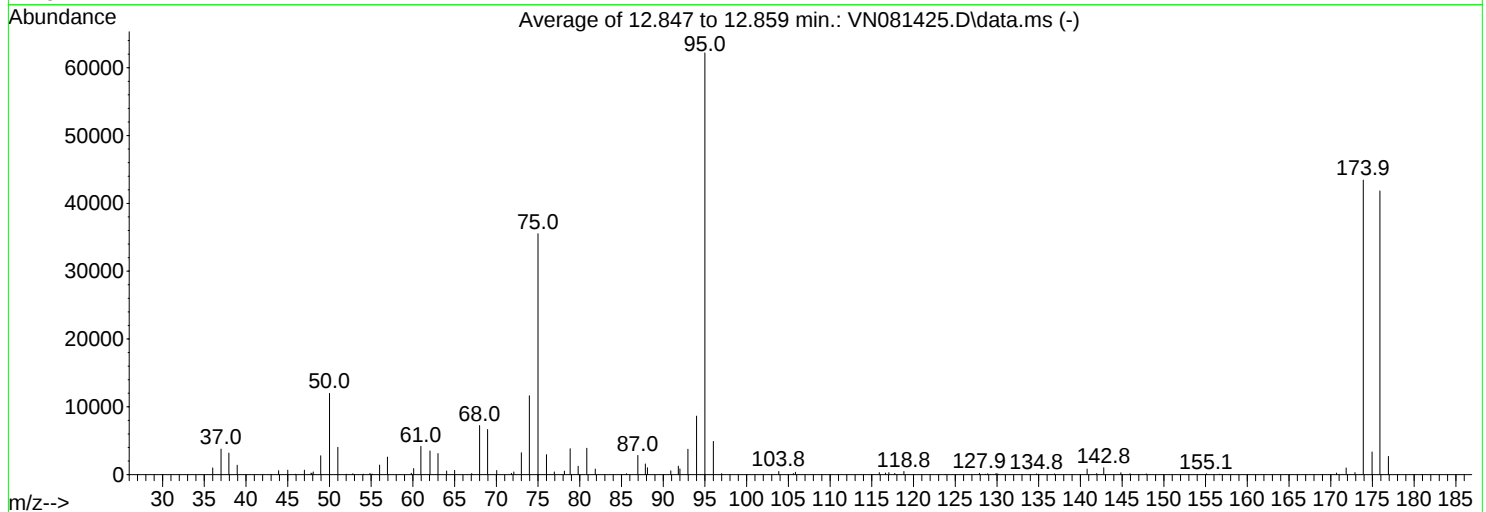


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031524\
Data File : VN081425.D
Acq On : 15 Mar 2024 13:10
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030524W.M
Title : SW846 8260
Last Update : Wed Mar 06 03:12:57 2024

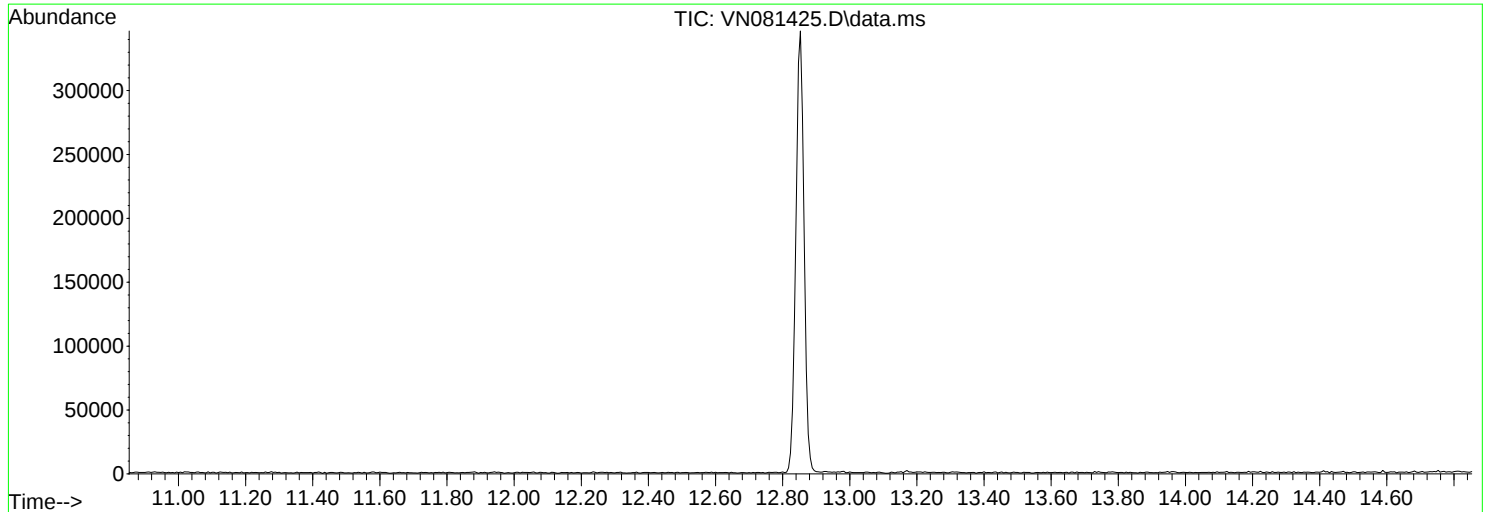

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	11990	PASS
75	95	30	60	57.1	35539	PASS
95	95	100	100	100.0	62192	PASS
96	95	5	9	7.9	4910	PASS
173	174	0.00	2	0.7	311	PASS
174	95	50	100	69.8	43440	PASS
175	174	5	9	7.7	3355	PASS
176	174	95	101	96.3	41827	PASS
177	176	5	9	6.4	2686	PASS

Average of 12.847 to 12.859 min.: VN081425.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	997	48.05	405	59.80	205	71.80	171
37.00	3765	48.95	2775	60.10	889	72.10	407
37.95	3197	50.00	11990	60.95	4166	73.00	323
38.95	1390	51.00	4039	62.05	3496	73.95	1164
43.00	56	52.00	62	63.00	3110	75.00	35539
43.90	596	52.80	135	64.05	547	76.00	2943
45.00	670	54.10	61	65.00	641	76.95	406
45.90	73	54.85	180	67.05	176	78.15	516
47.00	670	55.10	95	68.00	7251	78.85	3815
47.80	234	56.00	1411	68.95	6648	79.80	1245
47.90	165	56.95	2599	70.05	625	80.85	3890

Average of 12.847 to 12.859 min.: VN081425.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.85	828	96.00	4910	127.90	194	144.85	292
85.60	149	97.00	147	128.60	80	145.95	143
86.95	2827	103.85	485	128.90	132	147.00	55
87.85	1586	105.60	157	129.90	192	147.90	125
88.10	1026	105.85	360	130.10	117	155.10	119
90.90	565	115.90	318	134.75	129	156.70	81
91.80	1251	116.65	236	135.00	62	170.70	229
92.00	858	117.05	305	136.90	128	171.85	992
92.95	3744	117.75	182	140.80	818	172.90	311
94.00	8638	118.85	462	141.95	156	173.90	43440
95.00	62192	123.80	55	142.80	1017	174.95	3355

Average of 12.847 to 12.859 min.: VN081425.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
175.90	41827						
176.90	2686						

Instrument :

MSVOA_N

ClientSampleId :

BFB