


Chloromethane

Response Ratio

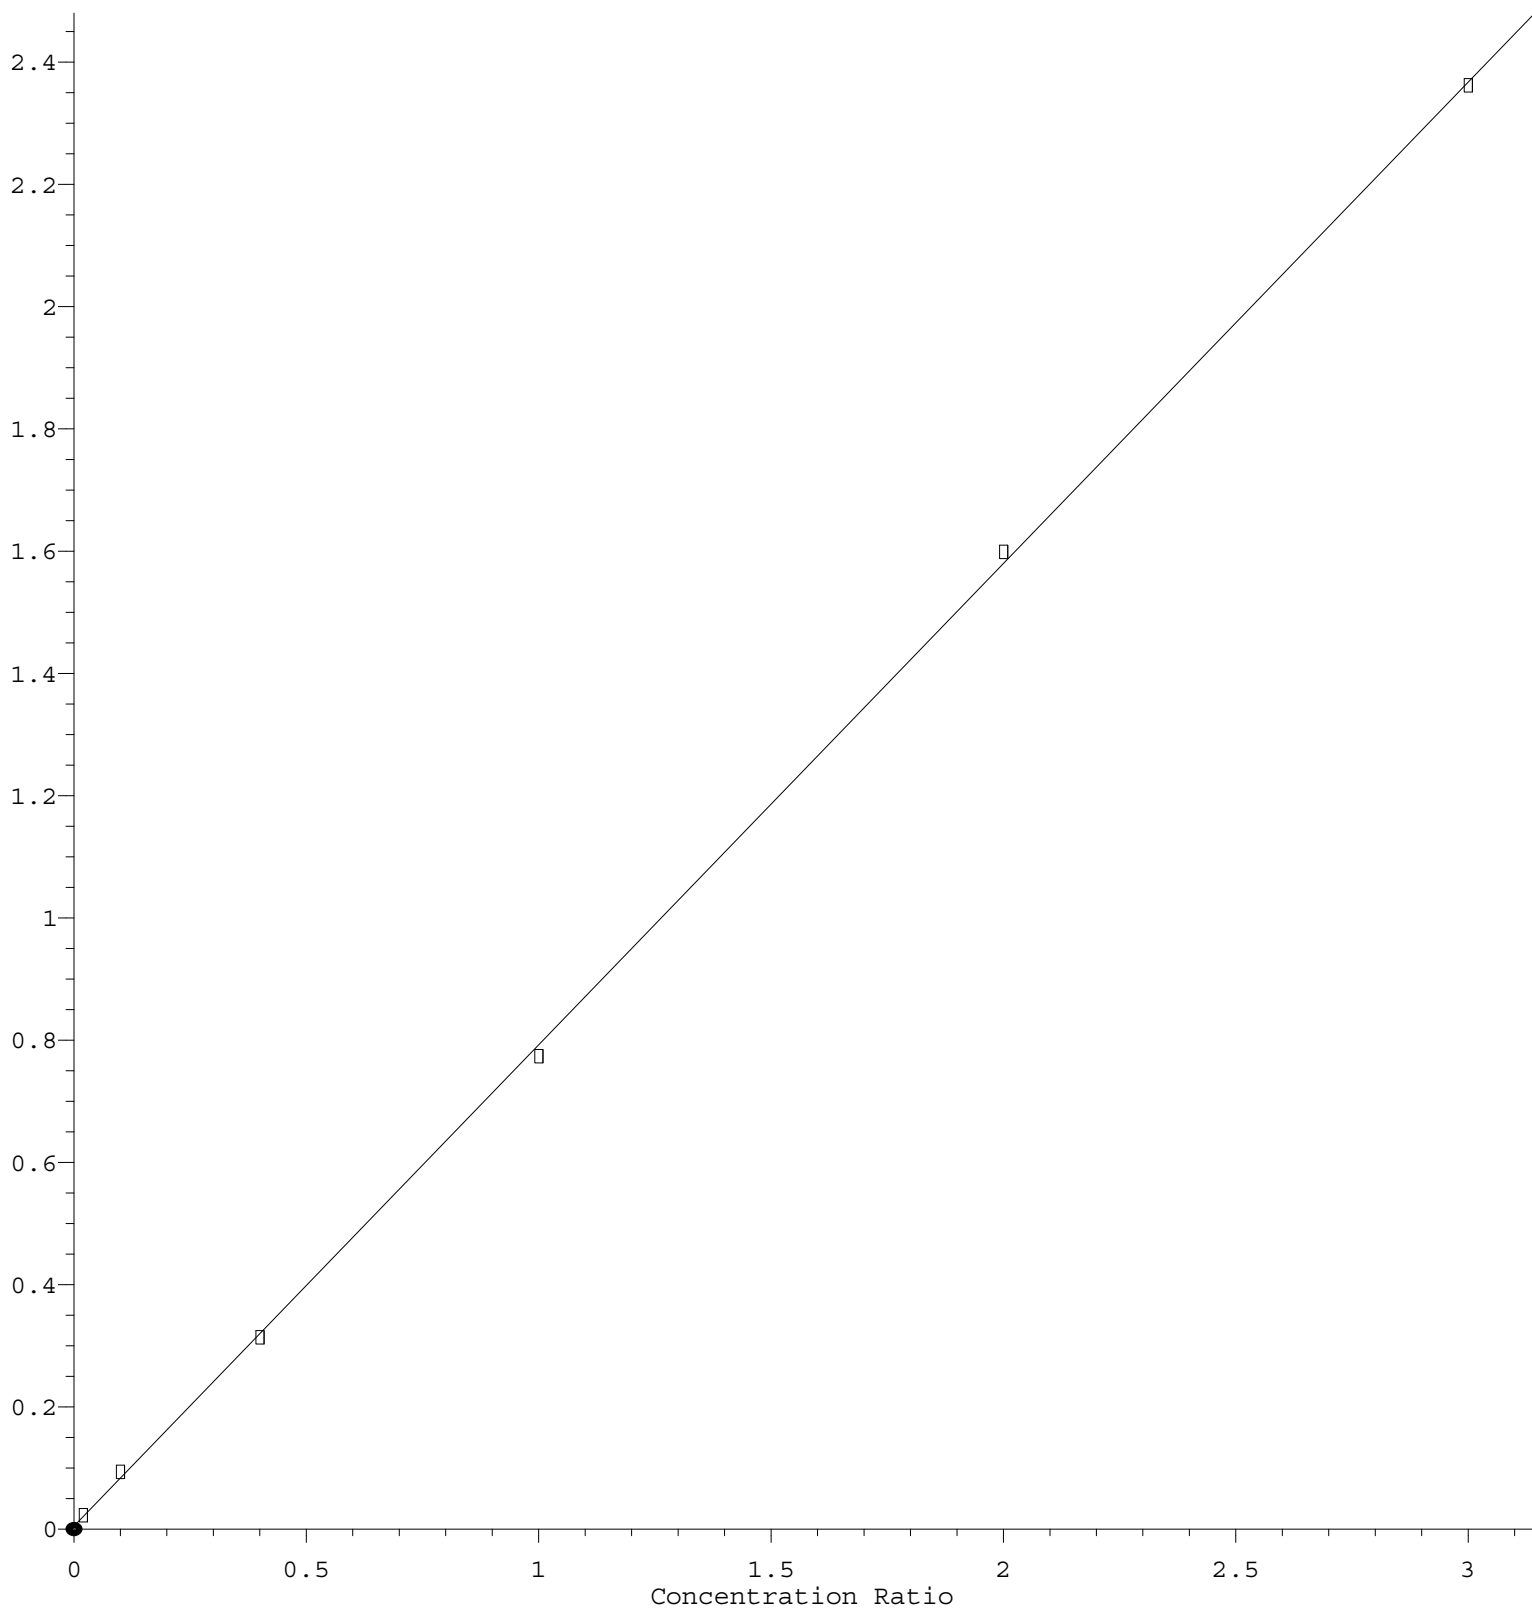

$$\text{Response} = 7.876\text{e-}001 * \text{Amt} + 4.928\text{e-}003$$


Coef of Det (r^2) = 0.999801 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031621W.M

Calibration Table Last Updated: Wed Mar 17 05:05:15 2021

Acrolein

Response Ratio

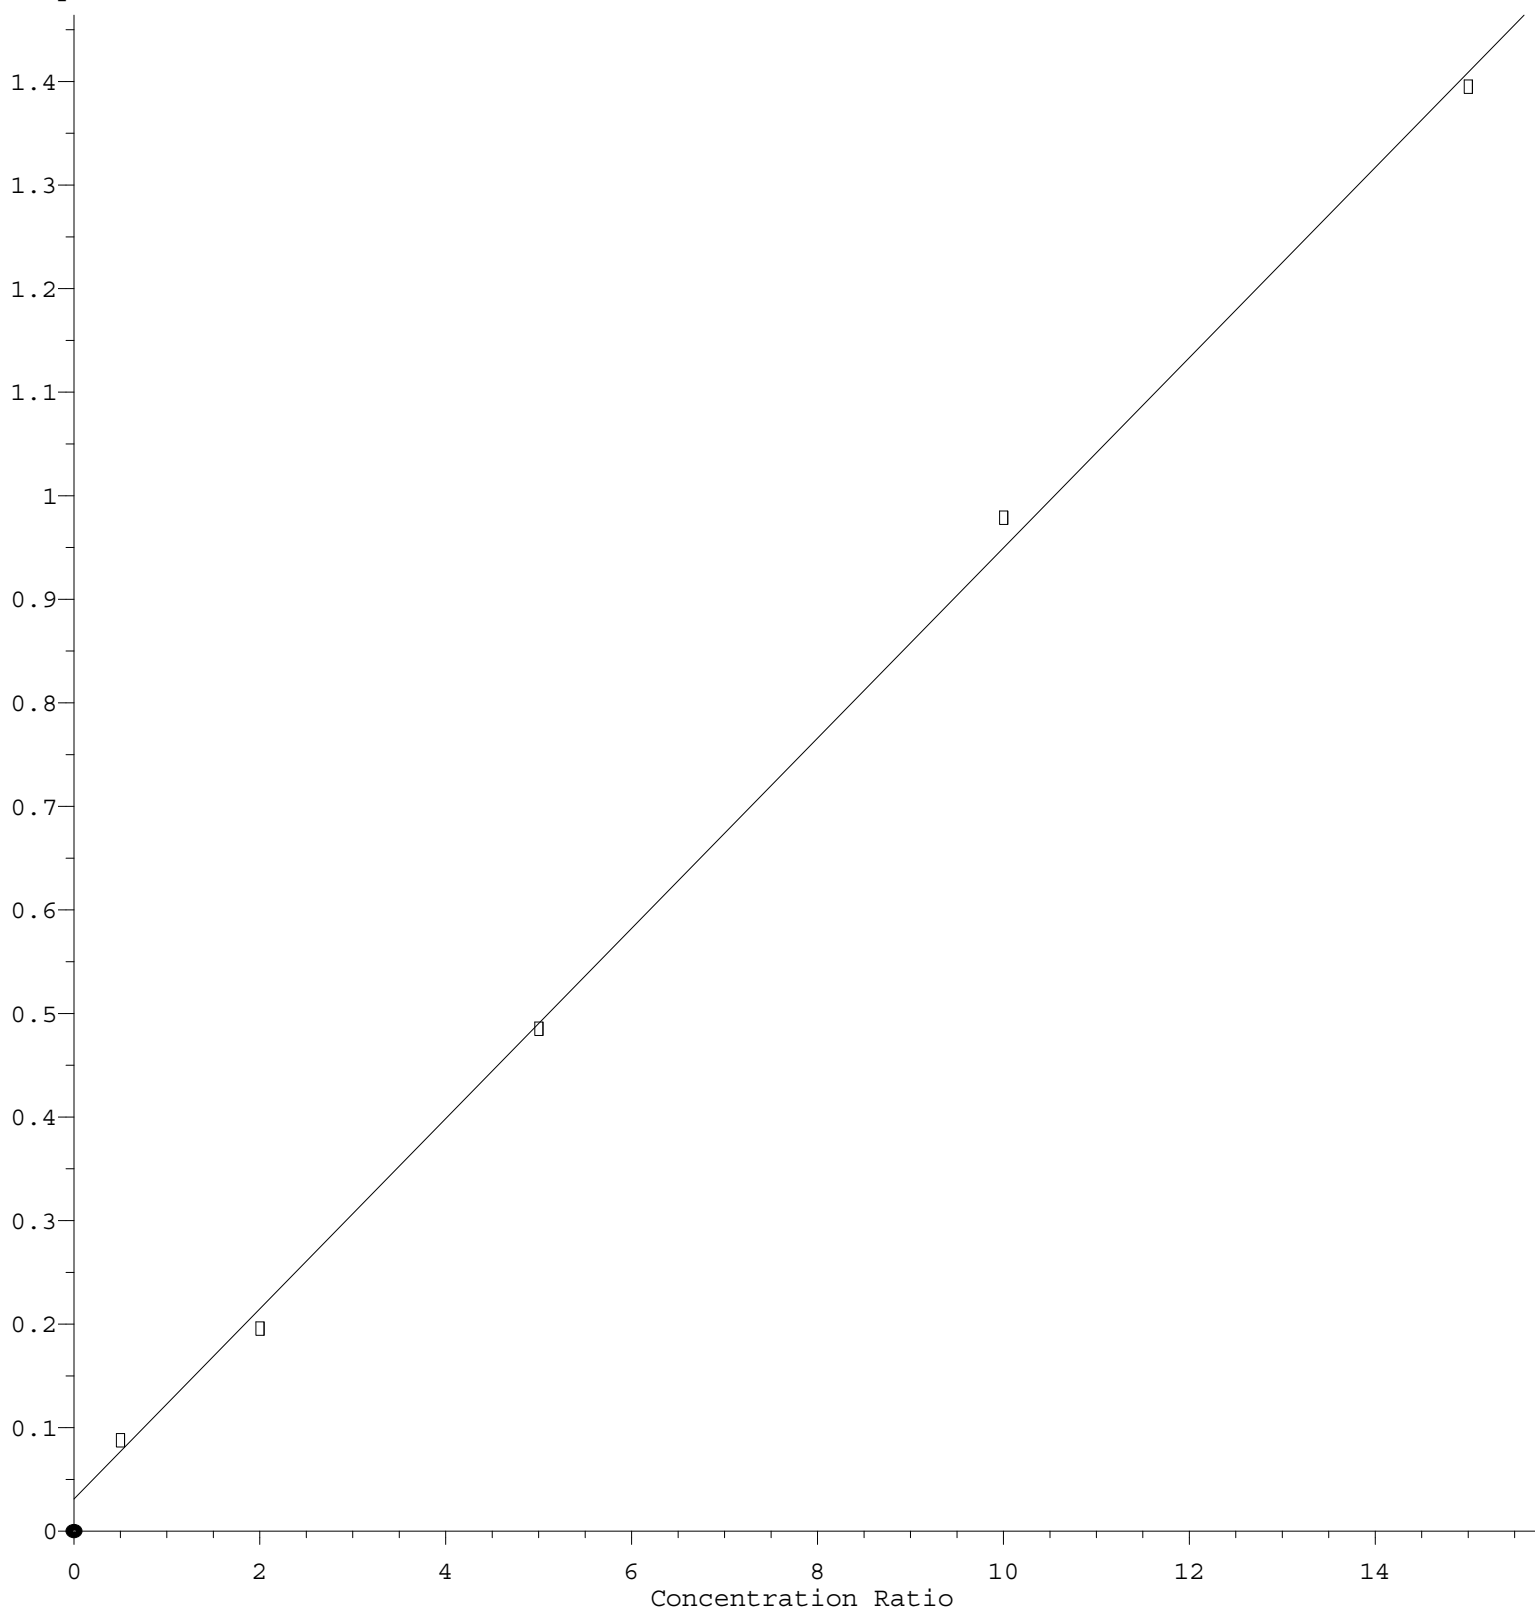

$$\text{Response} = 9.194\text{e-}002 * \text{Amt} + 3.084\text{e-}002$$


Coef of Det (r^2) = 0.998720 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031621W.M

Calibration Table Last Updated: Wed Mar 17 05:05:15 2021

Ethyl methacrylate

Response Ratio

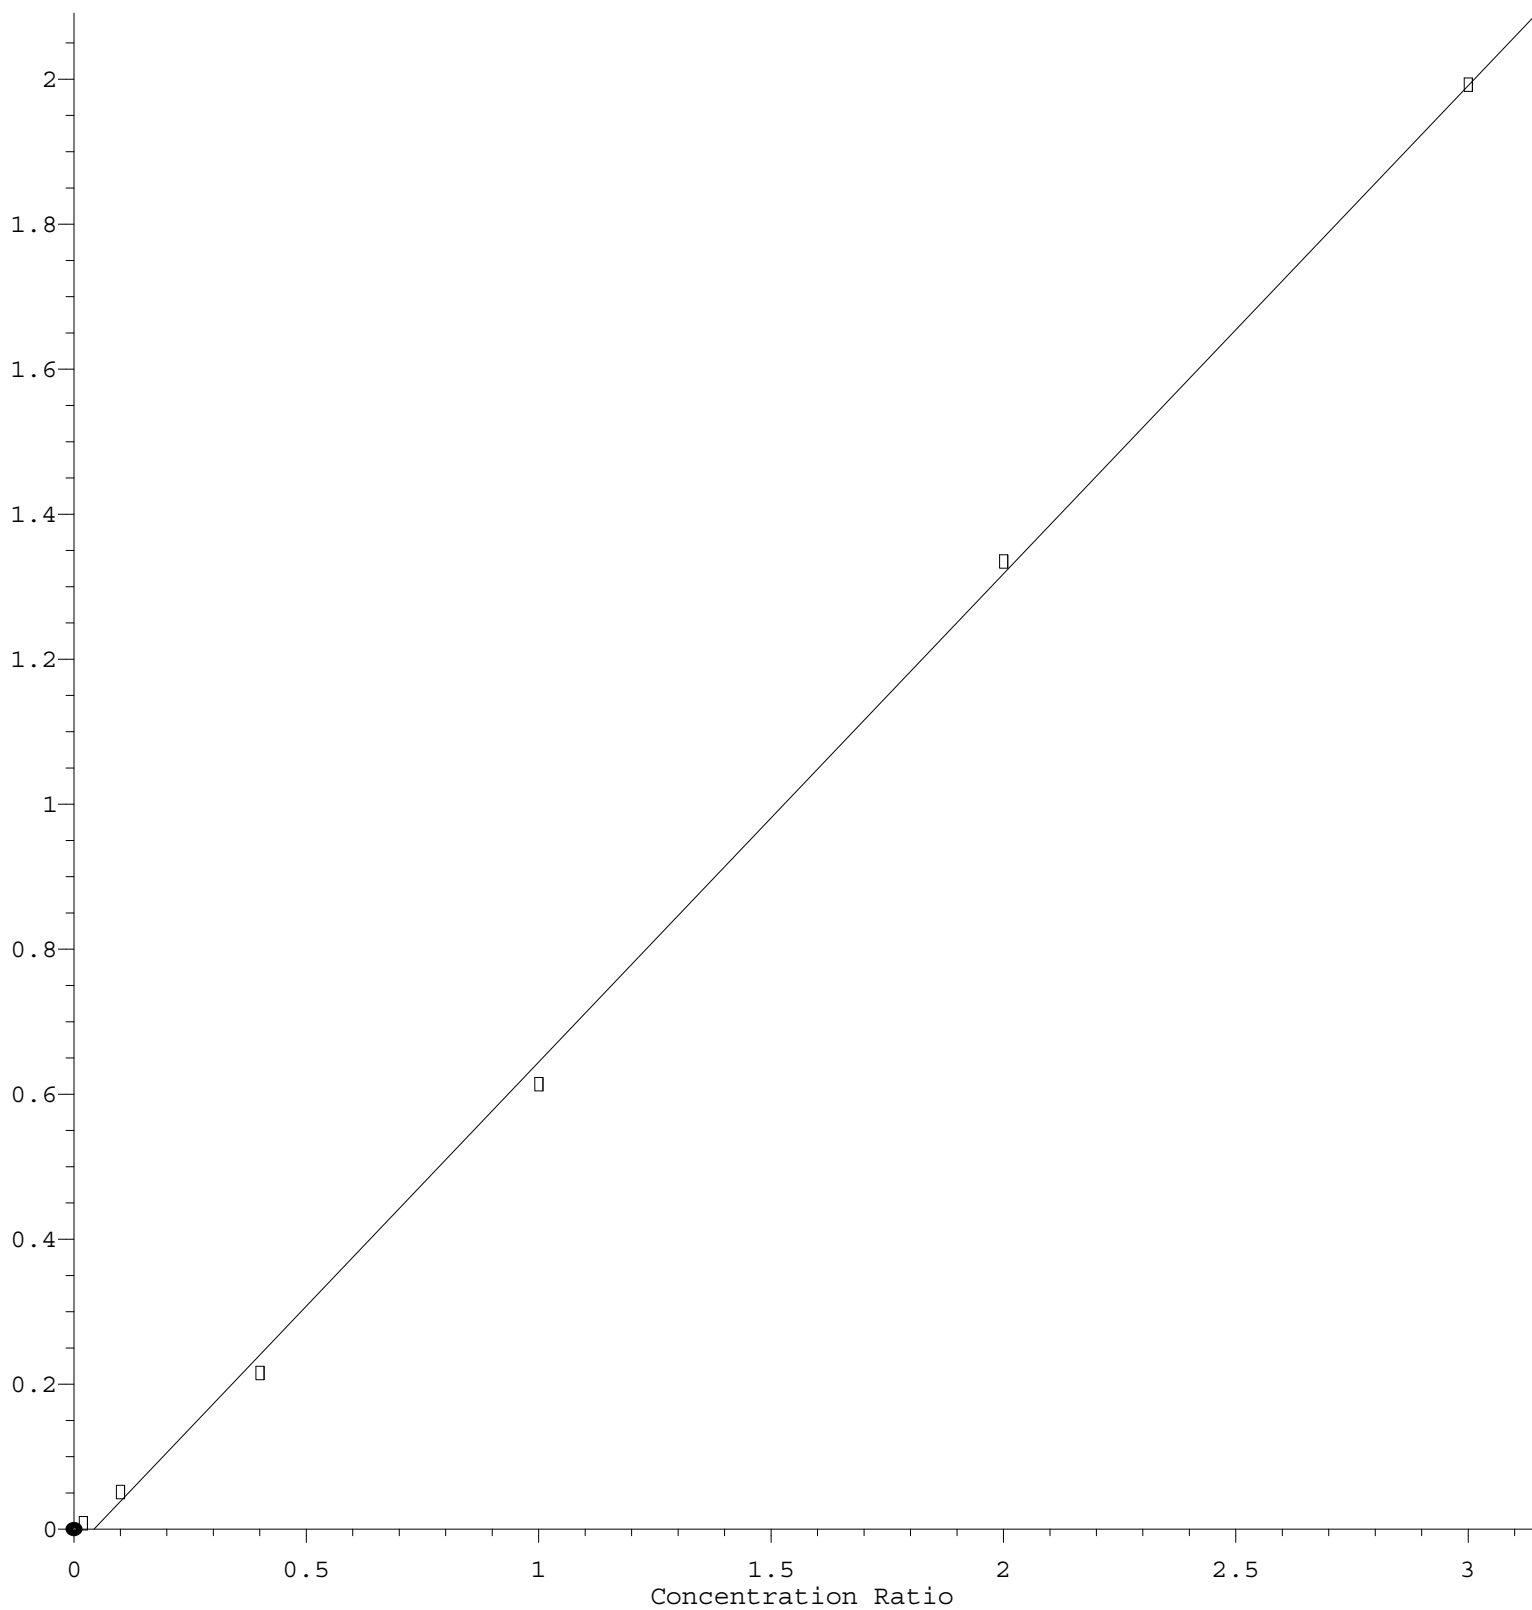

$$\text{Response} = 6.733\text{e-}001 * \text{Amt} - 2.910\text{e-}002$$


Coef of Det (r^2) = 0.999198 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031621W.M

Calibration Table Last Updated: Wed Mar 17 05:05:15 2021

2-Chloroethyl Vinyl ether

Response Ratio

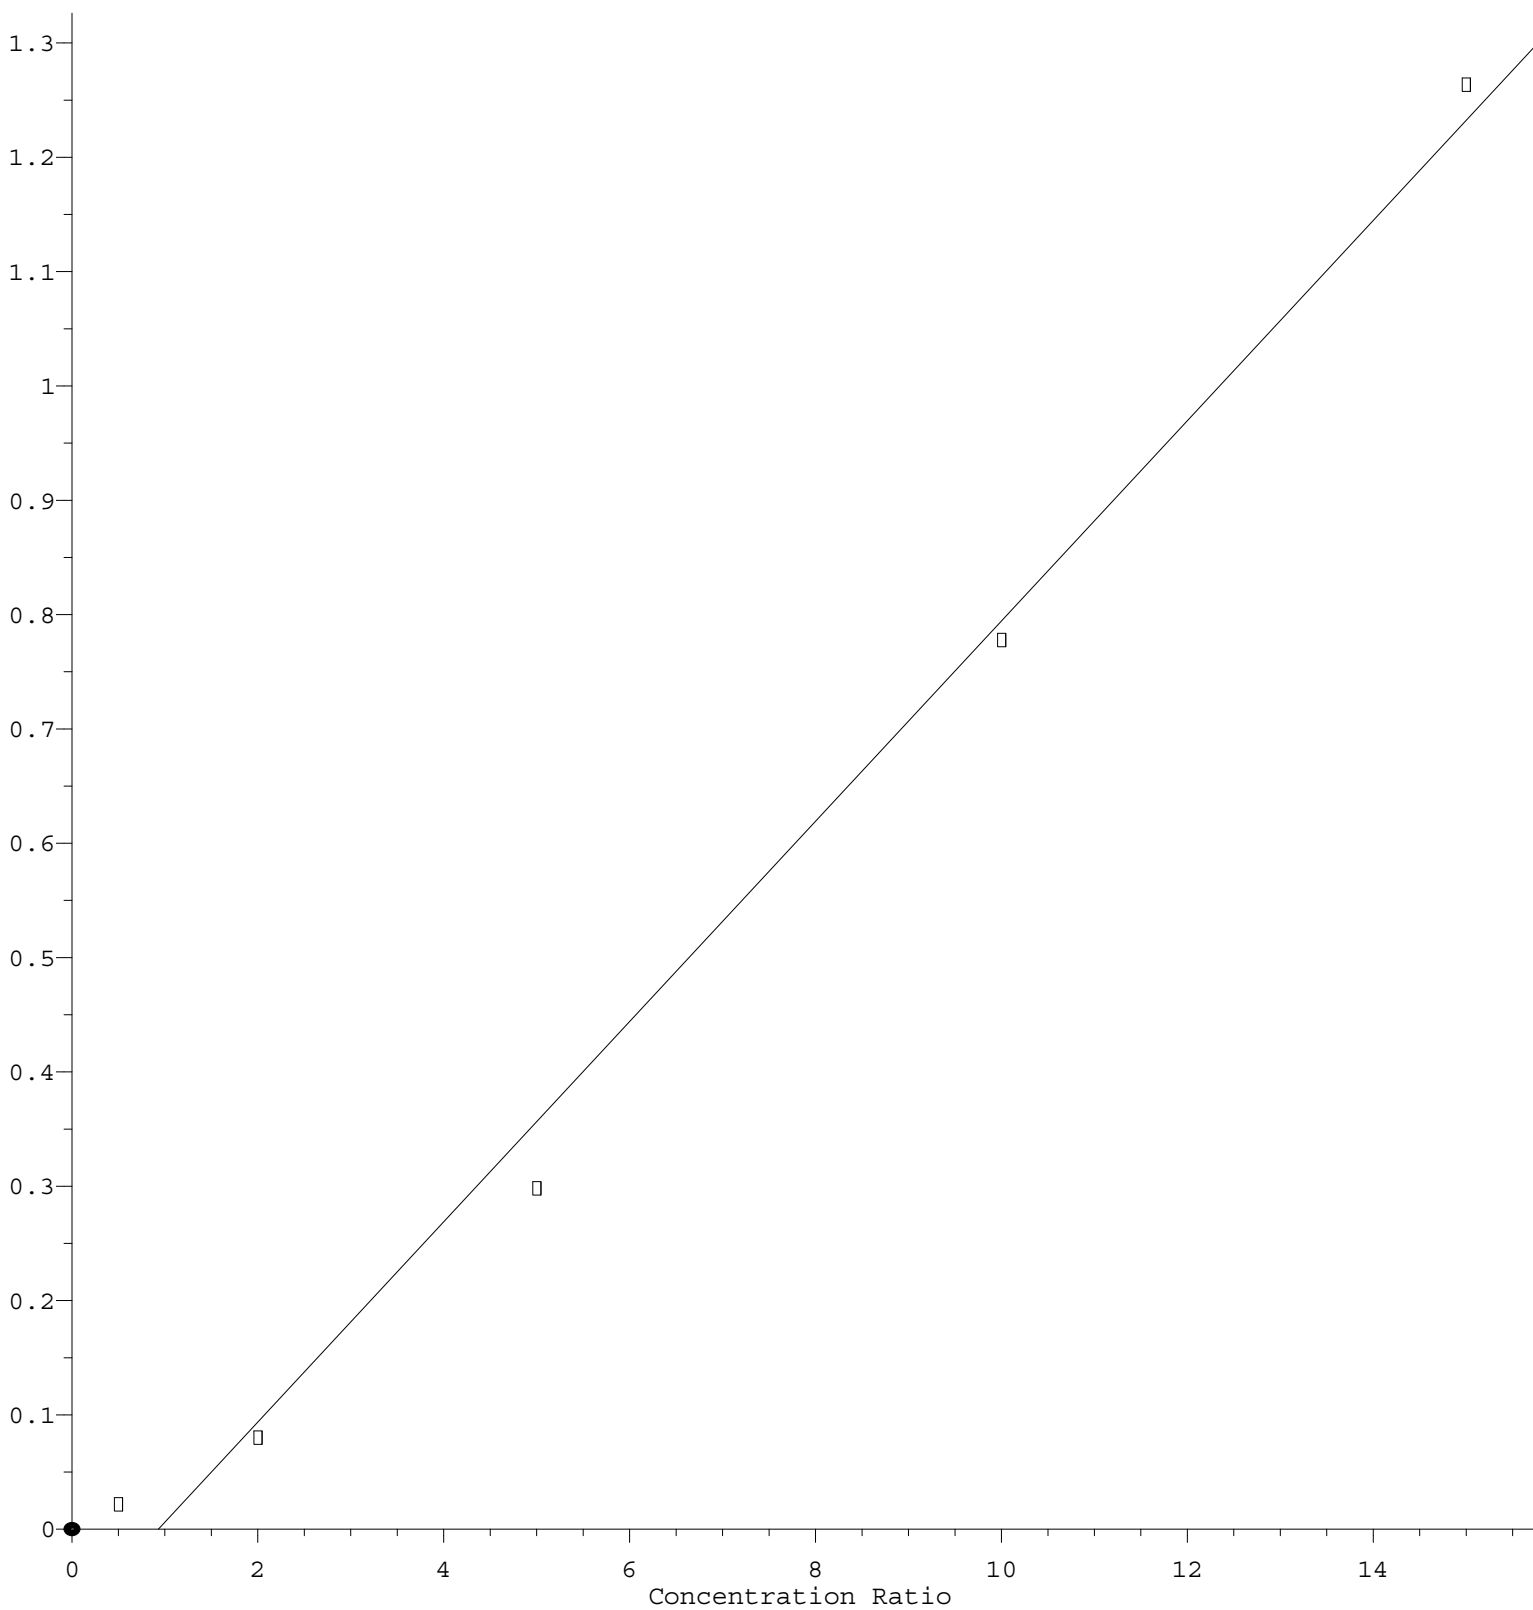

$$\text{Response} = 8.758\text{e-}002 * \text{Amt} - 8.108\text{e-}002$$


Coef of Det (r^2) = 0.992431 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031621W.M

Calibration Table Last Updated: Wed Mar 17 05:05:15 2021

2-Hexanone


Response Ratio

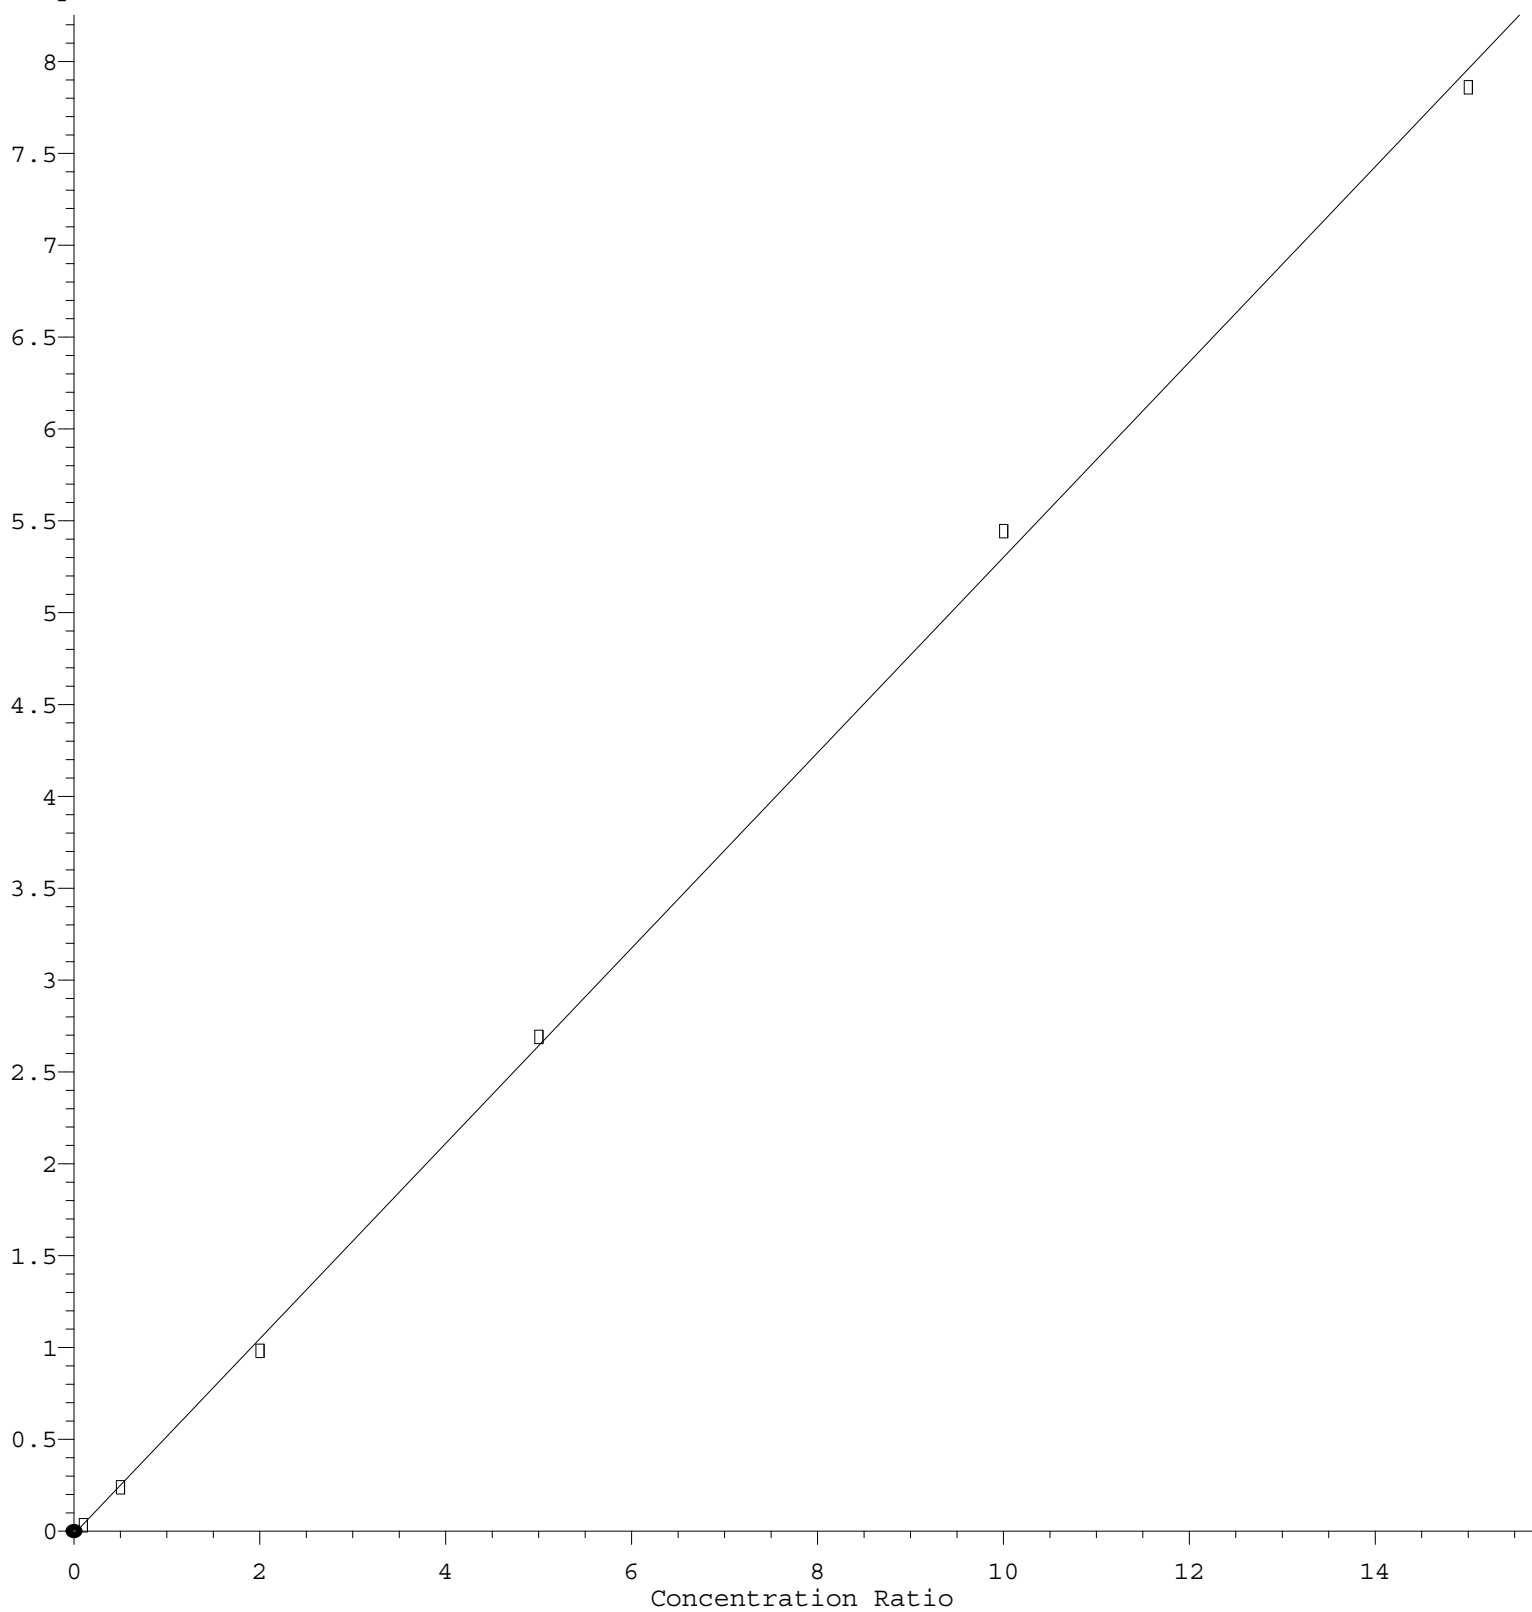

Response = 5.316e-001 * Amt - 1.420e-002
Coef of Det (r^2) = 0.999259 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031621W.M
Calibration Table Last Updated: Wed Mar 17 05:05:15 2021

Styrene

Response Ratio

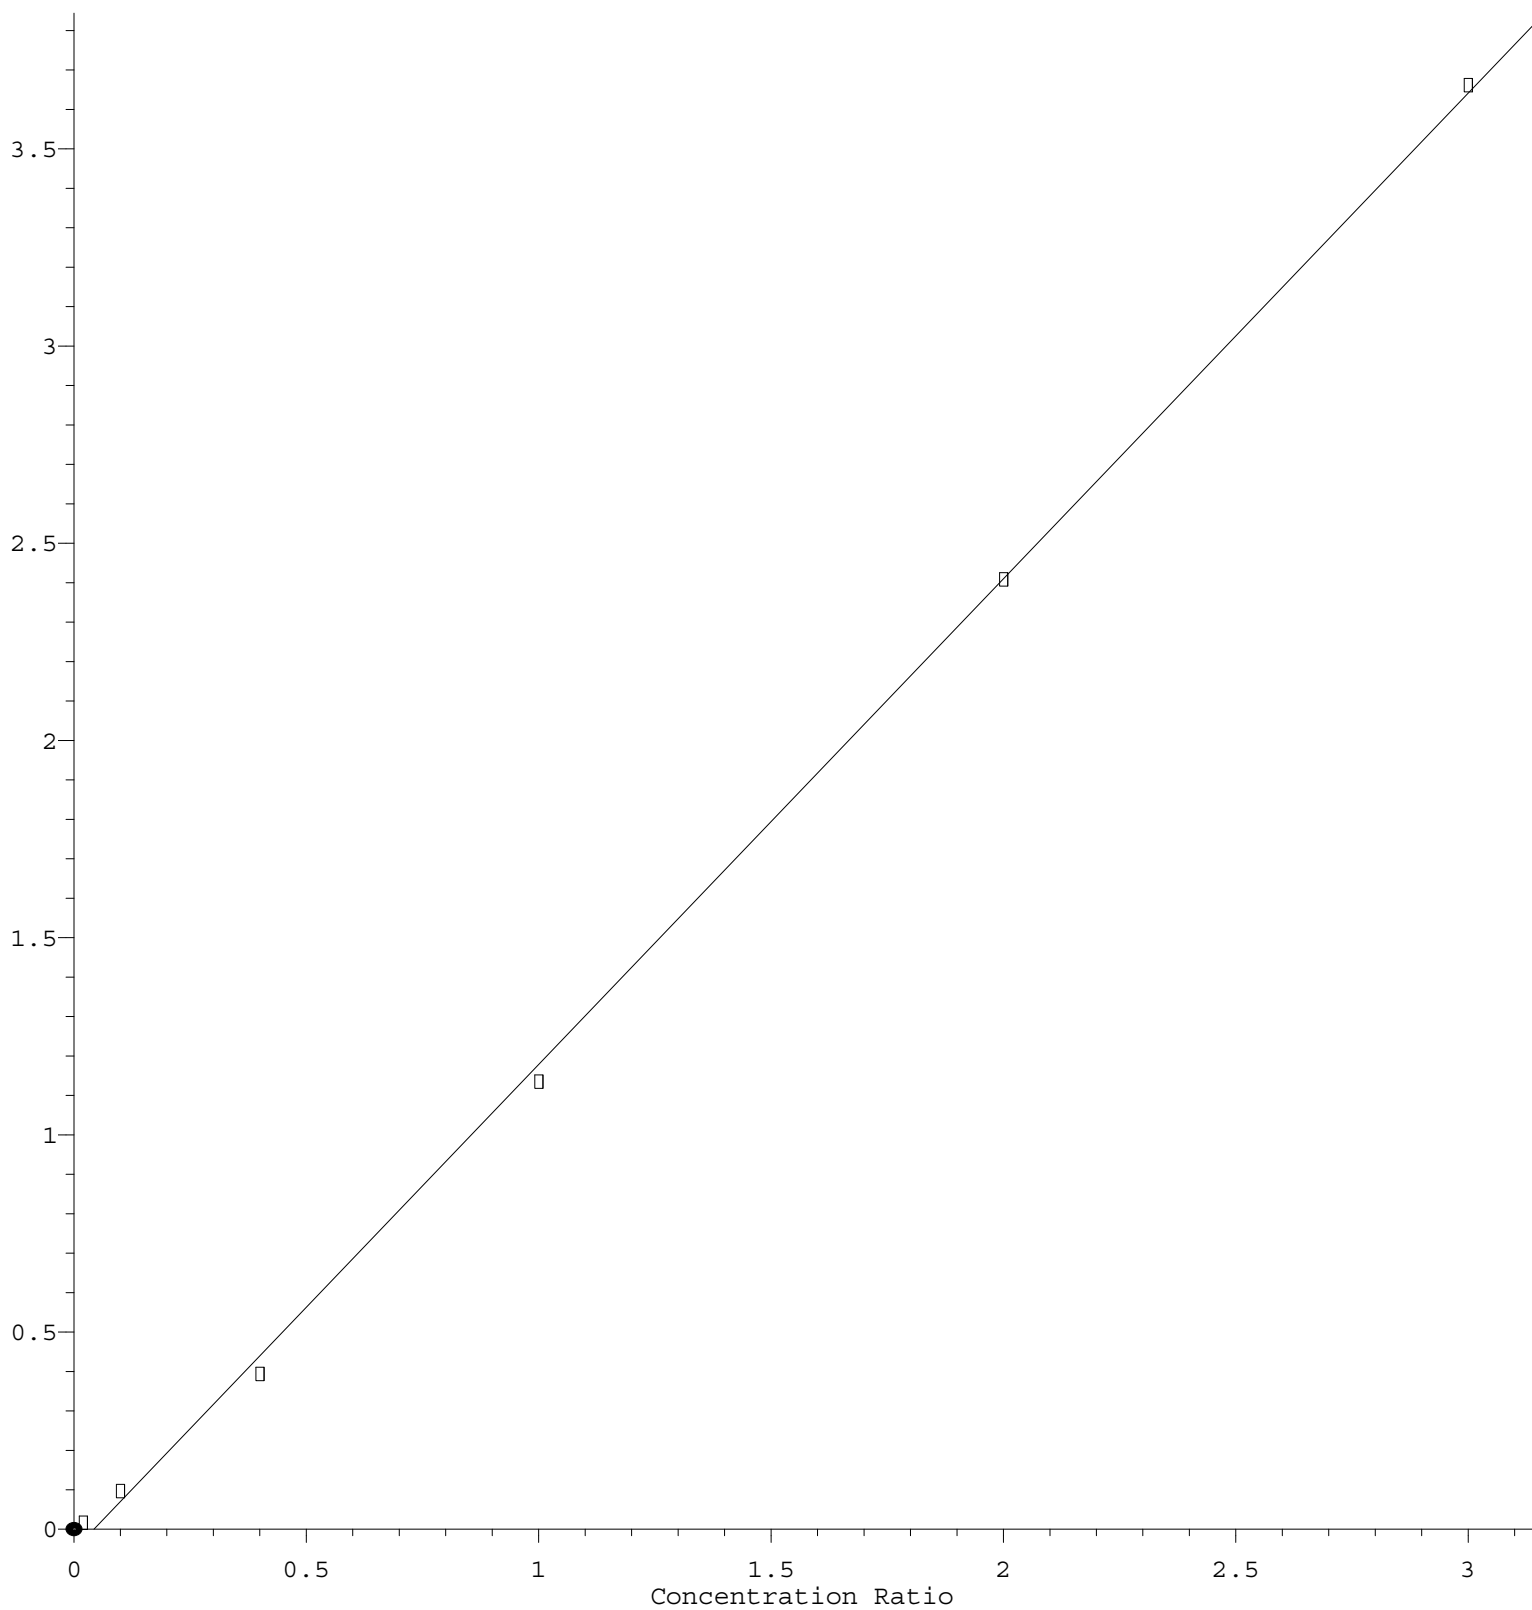

$$\text{Response} = 1.231\text{e}+000 * \text{Amt} - 5.294\text{e}-002$$


Coef of Det (r^2) = 0.999339 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031621W.M

Calibration Table Last Updated: Wed Mar 17 05:05:15 2021

N-amyl acetate

Response Ratio

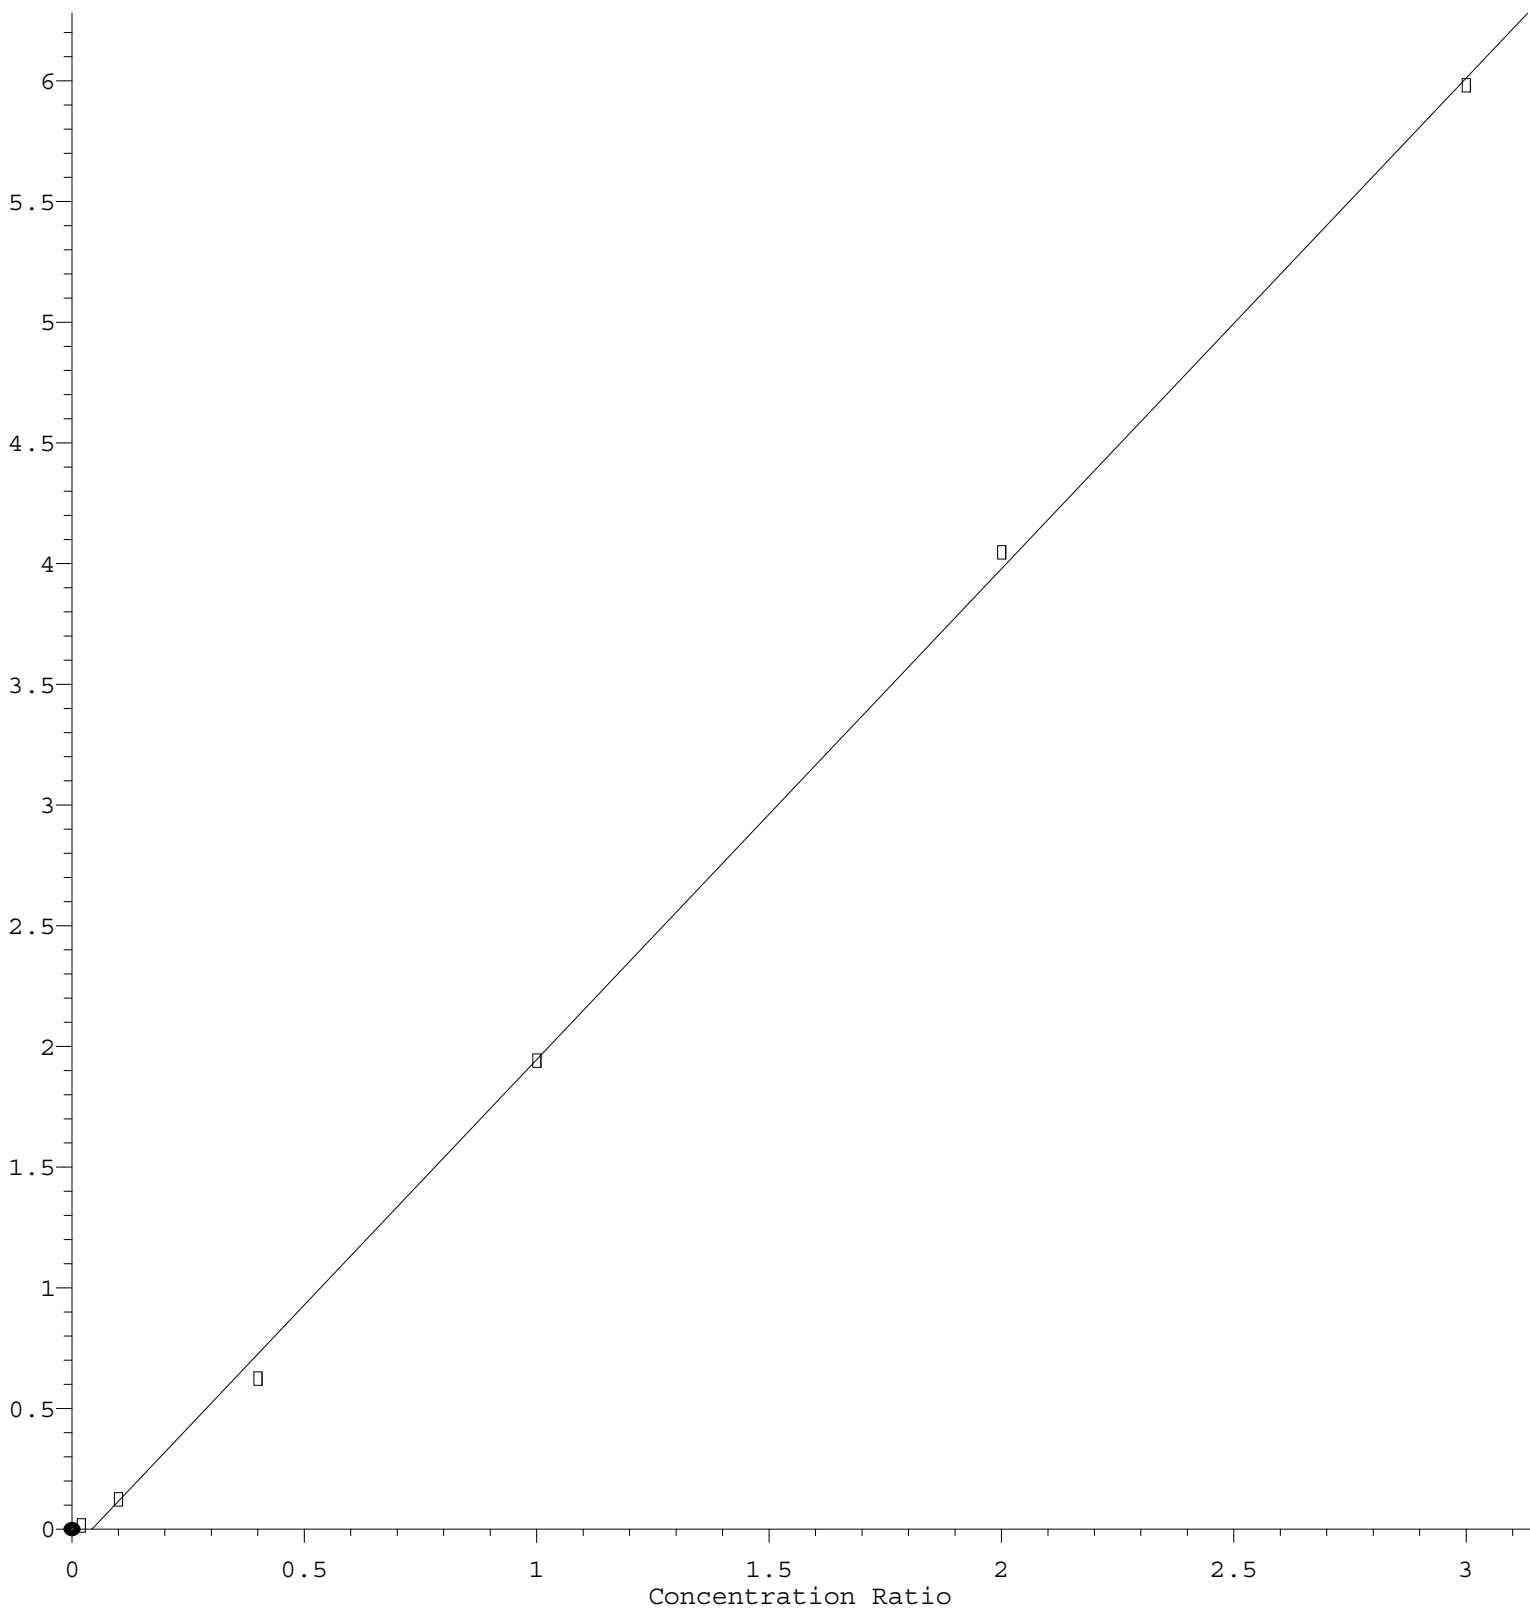

$$\text{Response} = 2.033\text{e}+000 * \text{Amt} - 8.781\text{e}-002$$


Coef of Det (r^2) = 0.999321 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031621W.M

Calibration Table Last Updated: Wed Mar 17 05:05:15 2021

4-Chlorotoluene

Response Ratio

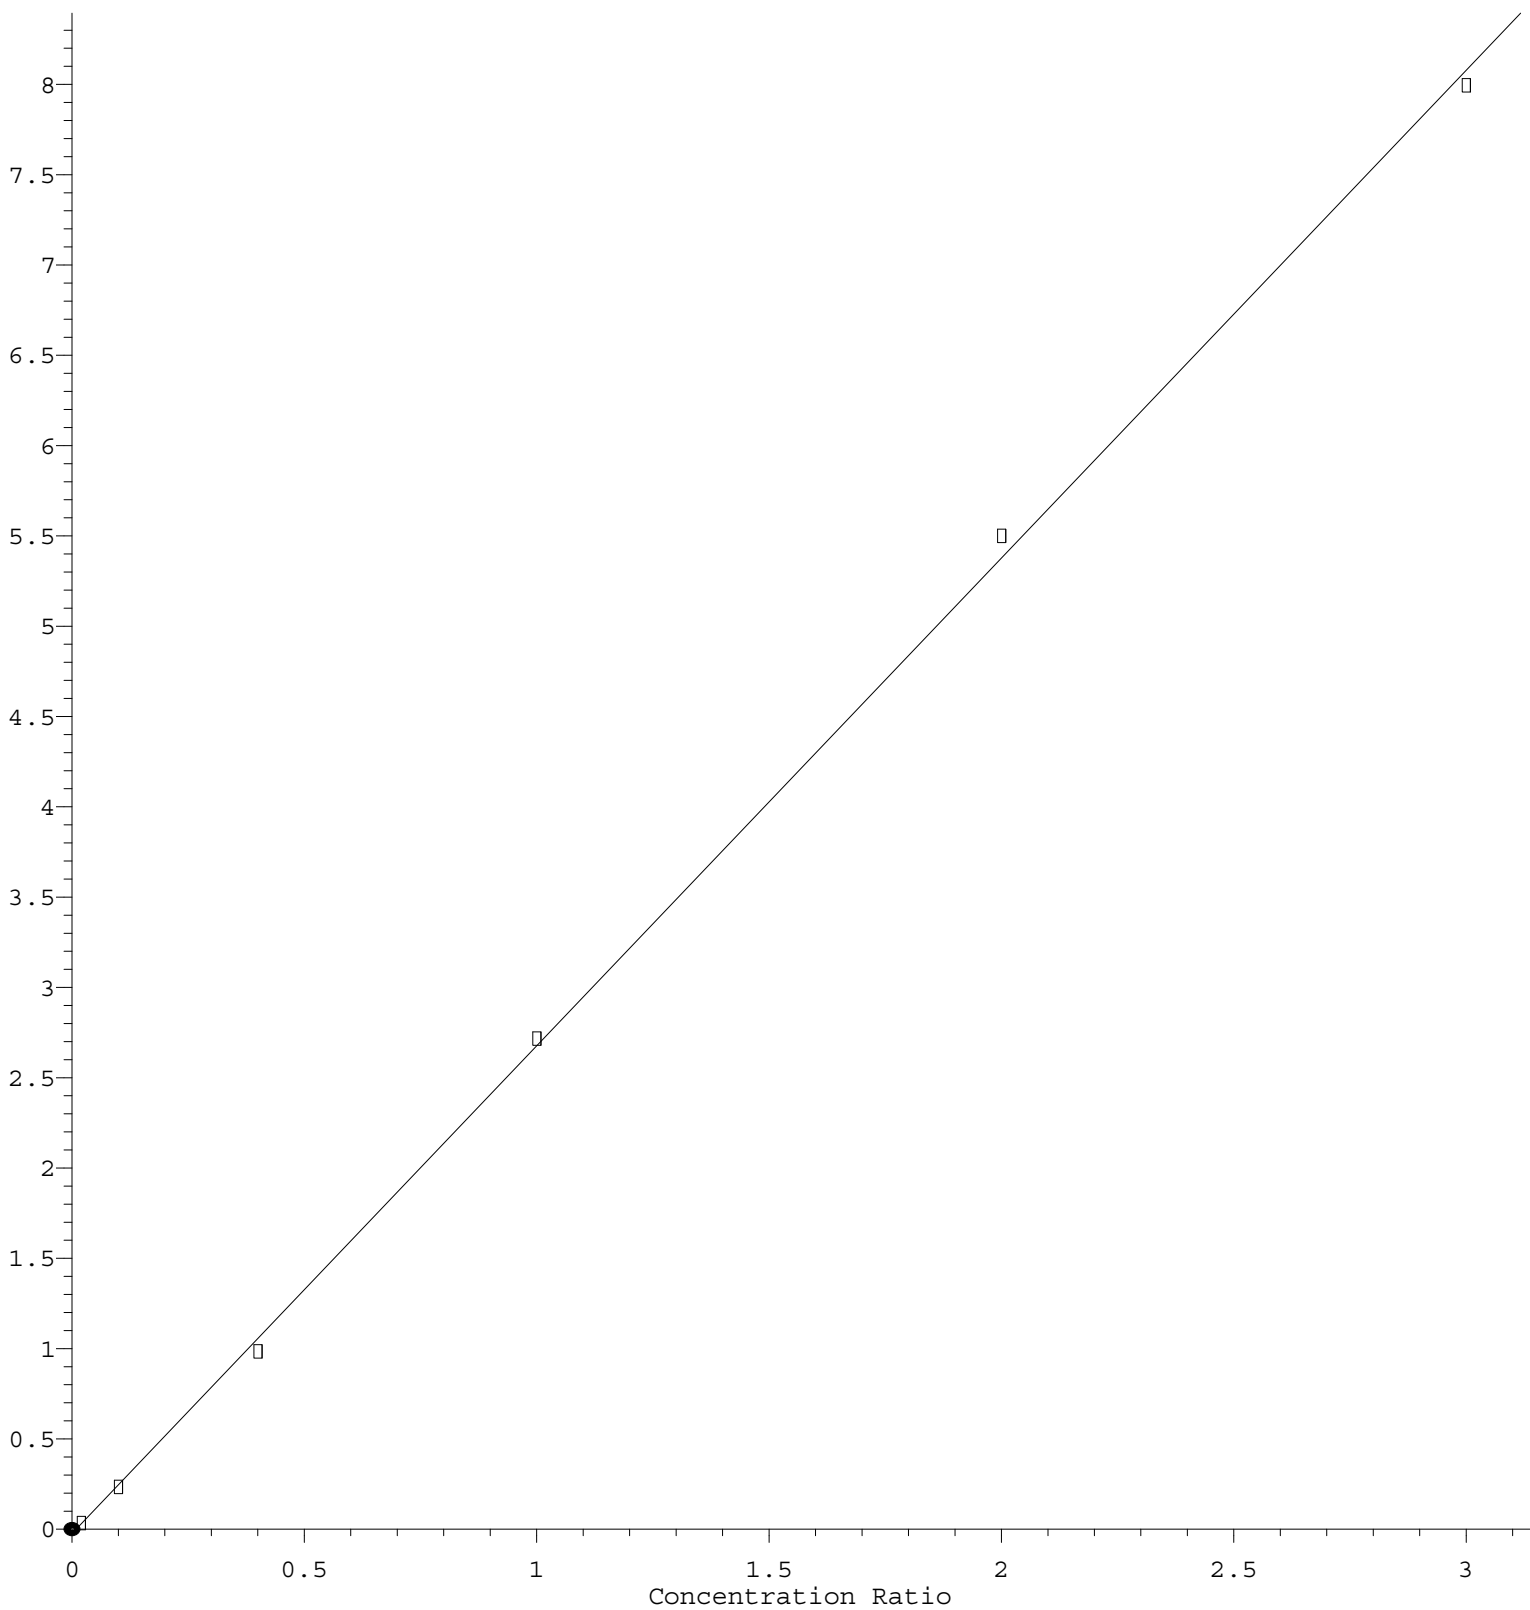

$$\text{Response} = 2.701\text{e}+000 * \text{Amt} - 2.530\text{e}-002$$


Coef of Det (r^2) = 0.999444 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031621W.M

Calibration Table Last Updated: Wed Mar 17 05:05:15 2021

n-Butylbenzene

Response Ratio

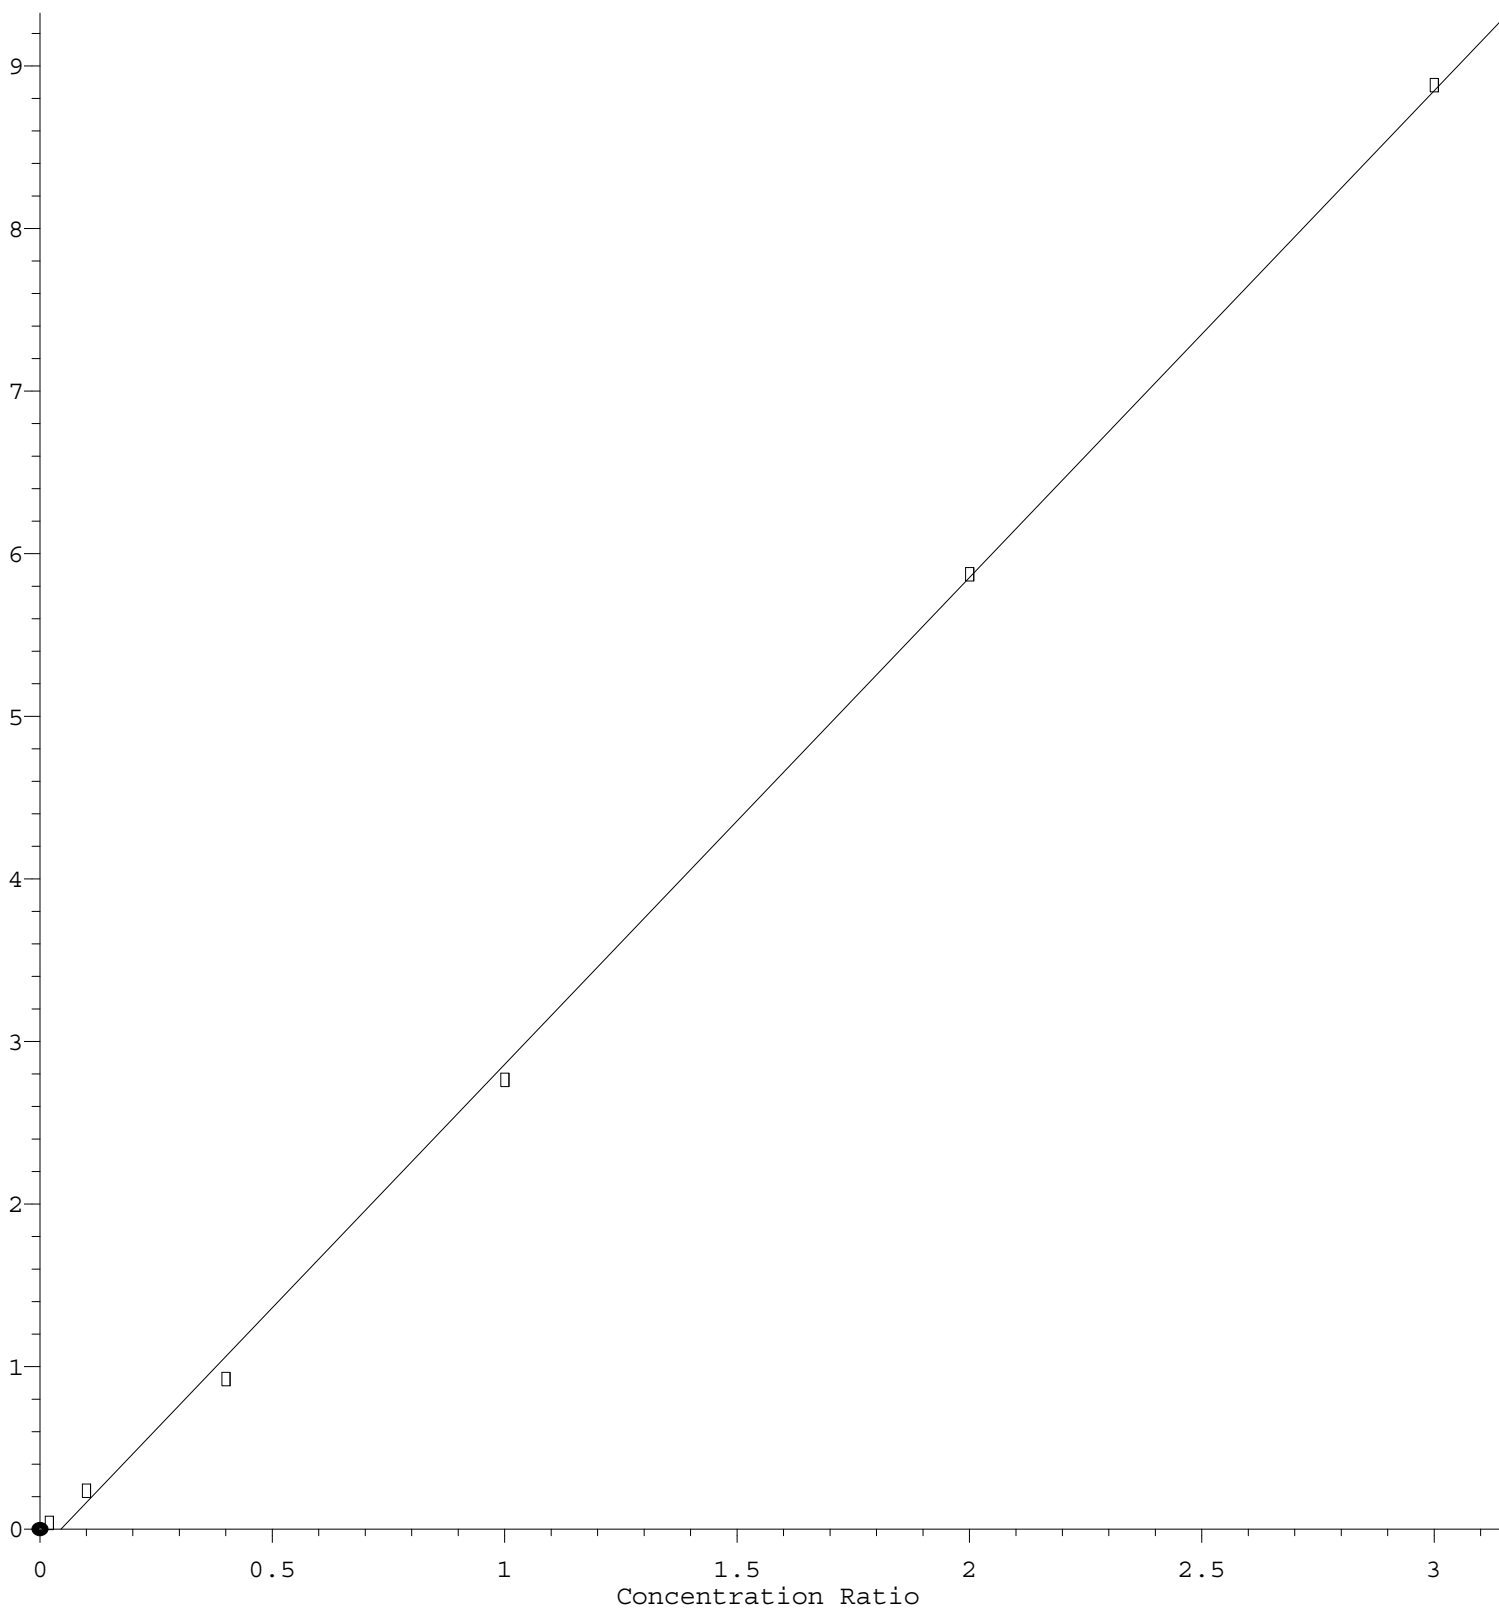


$$\text{Response} = 2.994\text{e}+000 * \text{Amt} - 1.340\text{e}-001$$

Coef of Det (r^2) = 0.999241 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031621W.M

Calibration Table Last Updated: Wed Mar 17 05:05:15 2021

1,2-Dibromo-3-Chloropropane

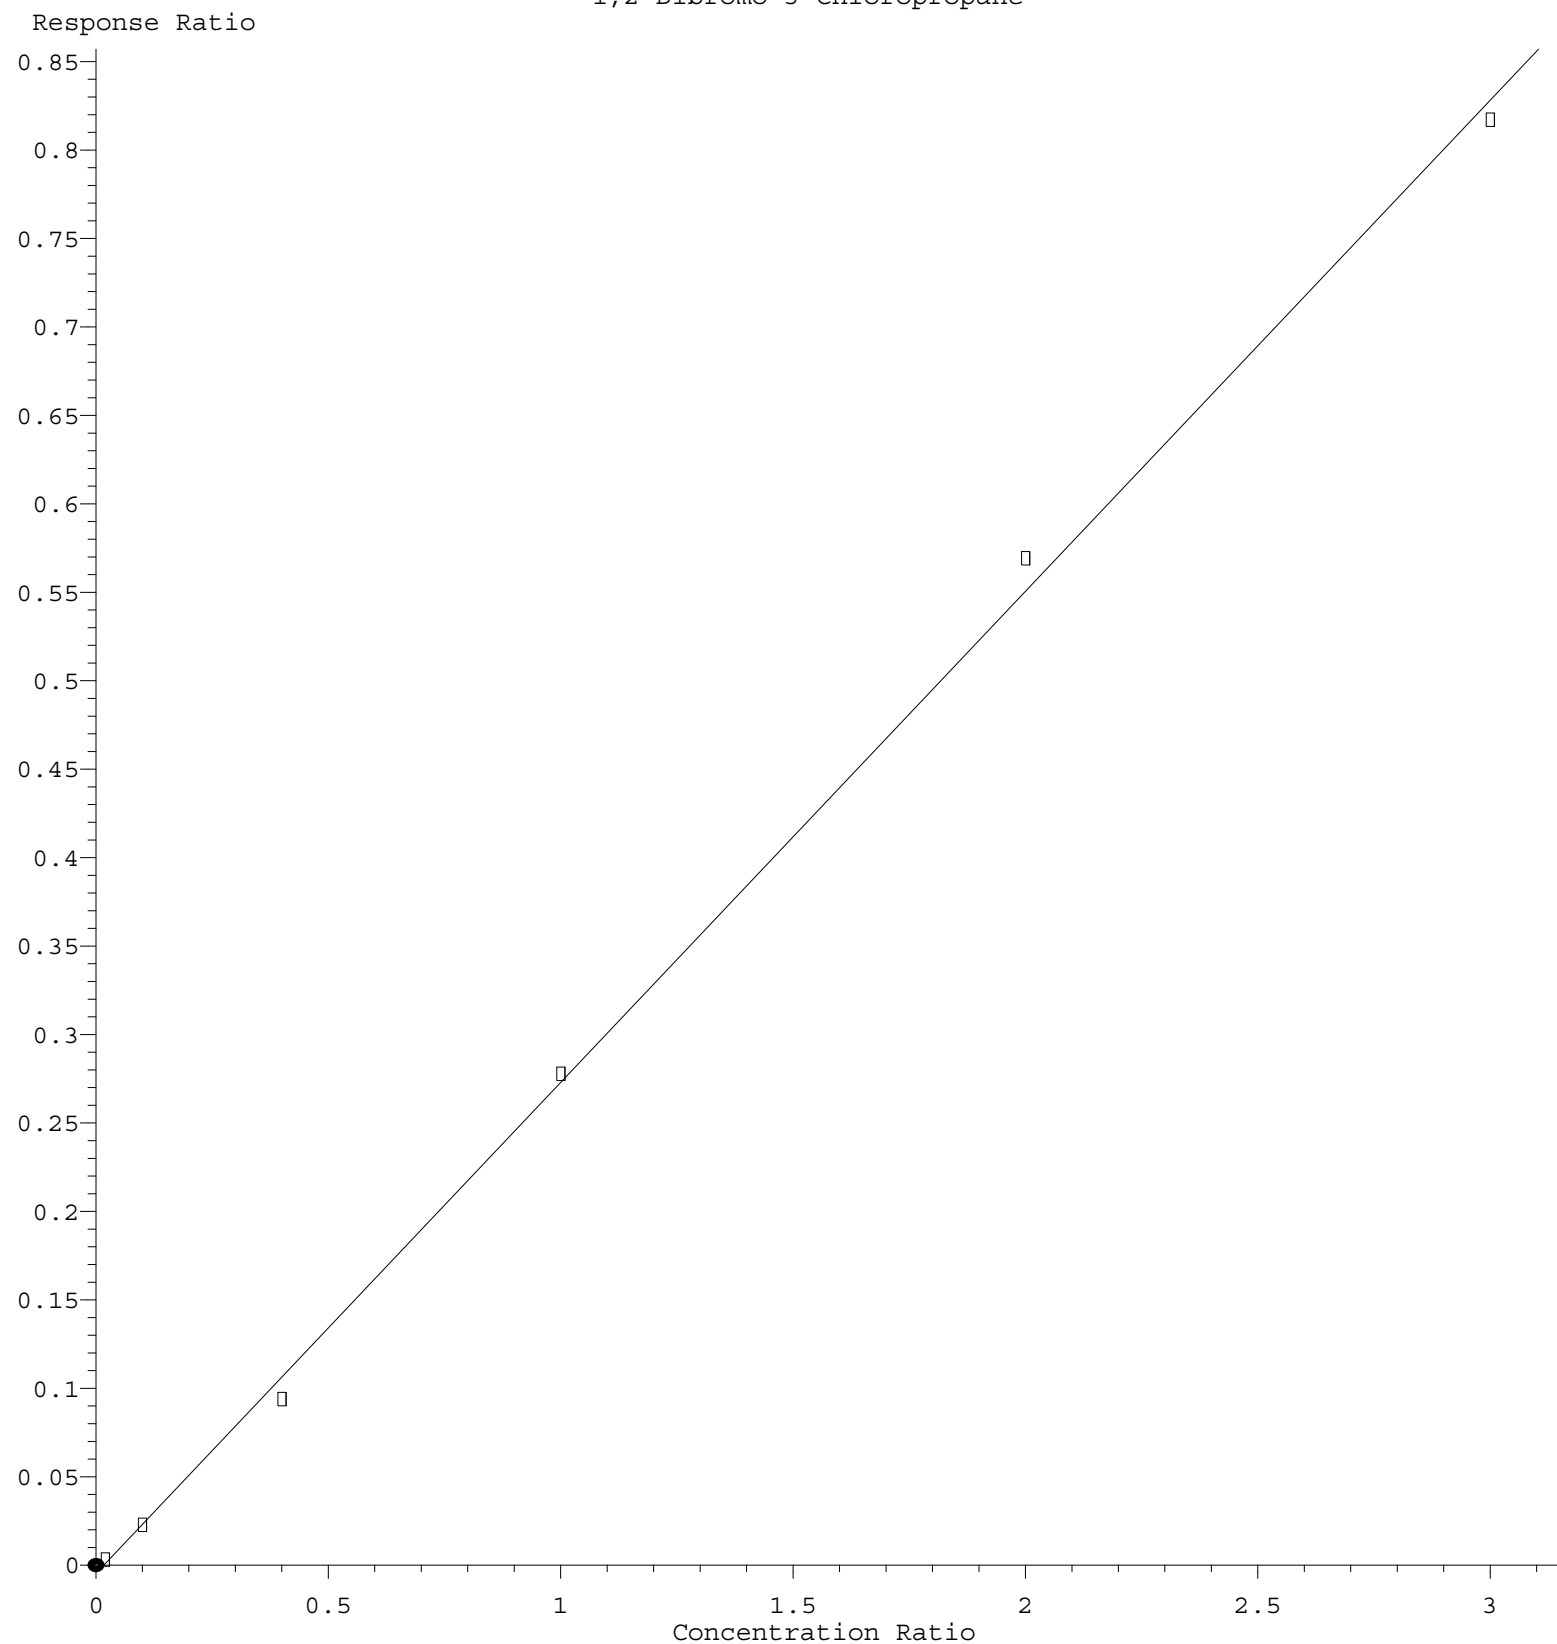

Response = 2.779e-001 * Amt - 4.638e-003
 Coef of Det (r^2) = 0.998808 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N031621W.M
 Calibration Table Last Updated: Wed Mar 17 05:05:15 2021